

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
 Data File : BGTEST04.D
 Acq On : 19 Jun 2015 22:01
 Operator : TP/IZ
 Sample : UNIT-3-SPOT-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 20 02:51:43 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 19 17:30:37 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	61147	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	273378	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	166119	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	372922	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	386319	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	356711	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.99	96	58	0.04	ng/uL	-0.15
5) Phenol-d5	6.79	99	671475	126.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	5923	1.93	ng/ul	-0.16
9) 2-Chlorophenol-d4	7.15	132	554527	127.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	413	0.09	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	181547	86.31	ng/ul	0.00
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	10.02	165	89	0.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	135	0.03	ng/ul	0.05
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.26	176	992	0.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.11	188	4659	0.27	ng/ul	0.00
78) Pyrene-d10	0.00	212	0	0.00	ng/ul	
89) Benzo(a)pyrene-d12	23.31	264	65	0.00	ng/ul	0.01


Target Compounds					Qvalue
44) Dimethylphthalate	13.73	163	113412	9.21 ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
Data File : BGTEST04.D
Acq On : 19 Jun 2015 22:01
Operator : TP/IZ
Sample : UNIT-3-SPOT-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 20 02:51:43 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 19 17:30:37 2015
Response via : Initial Calibration

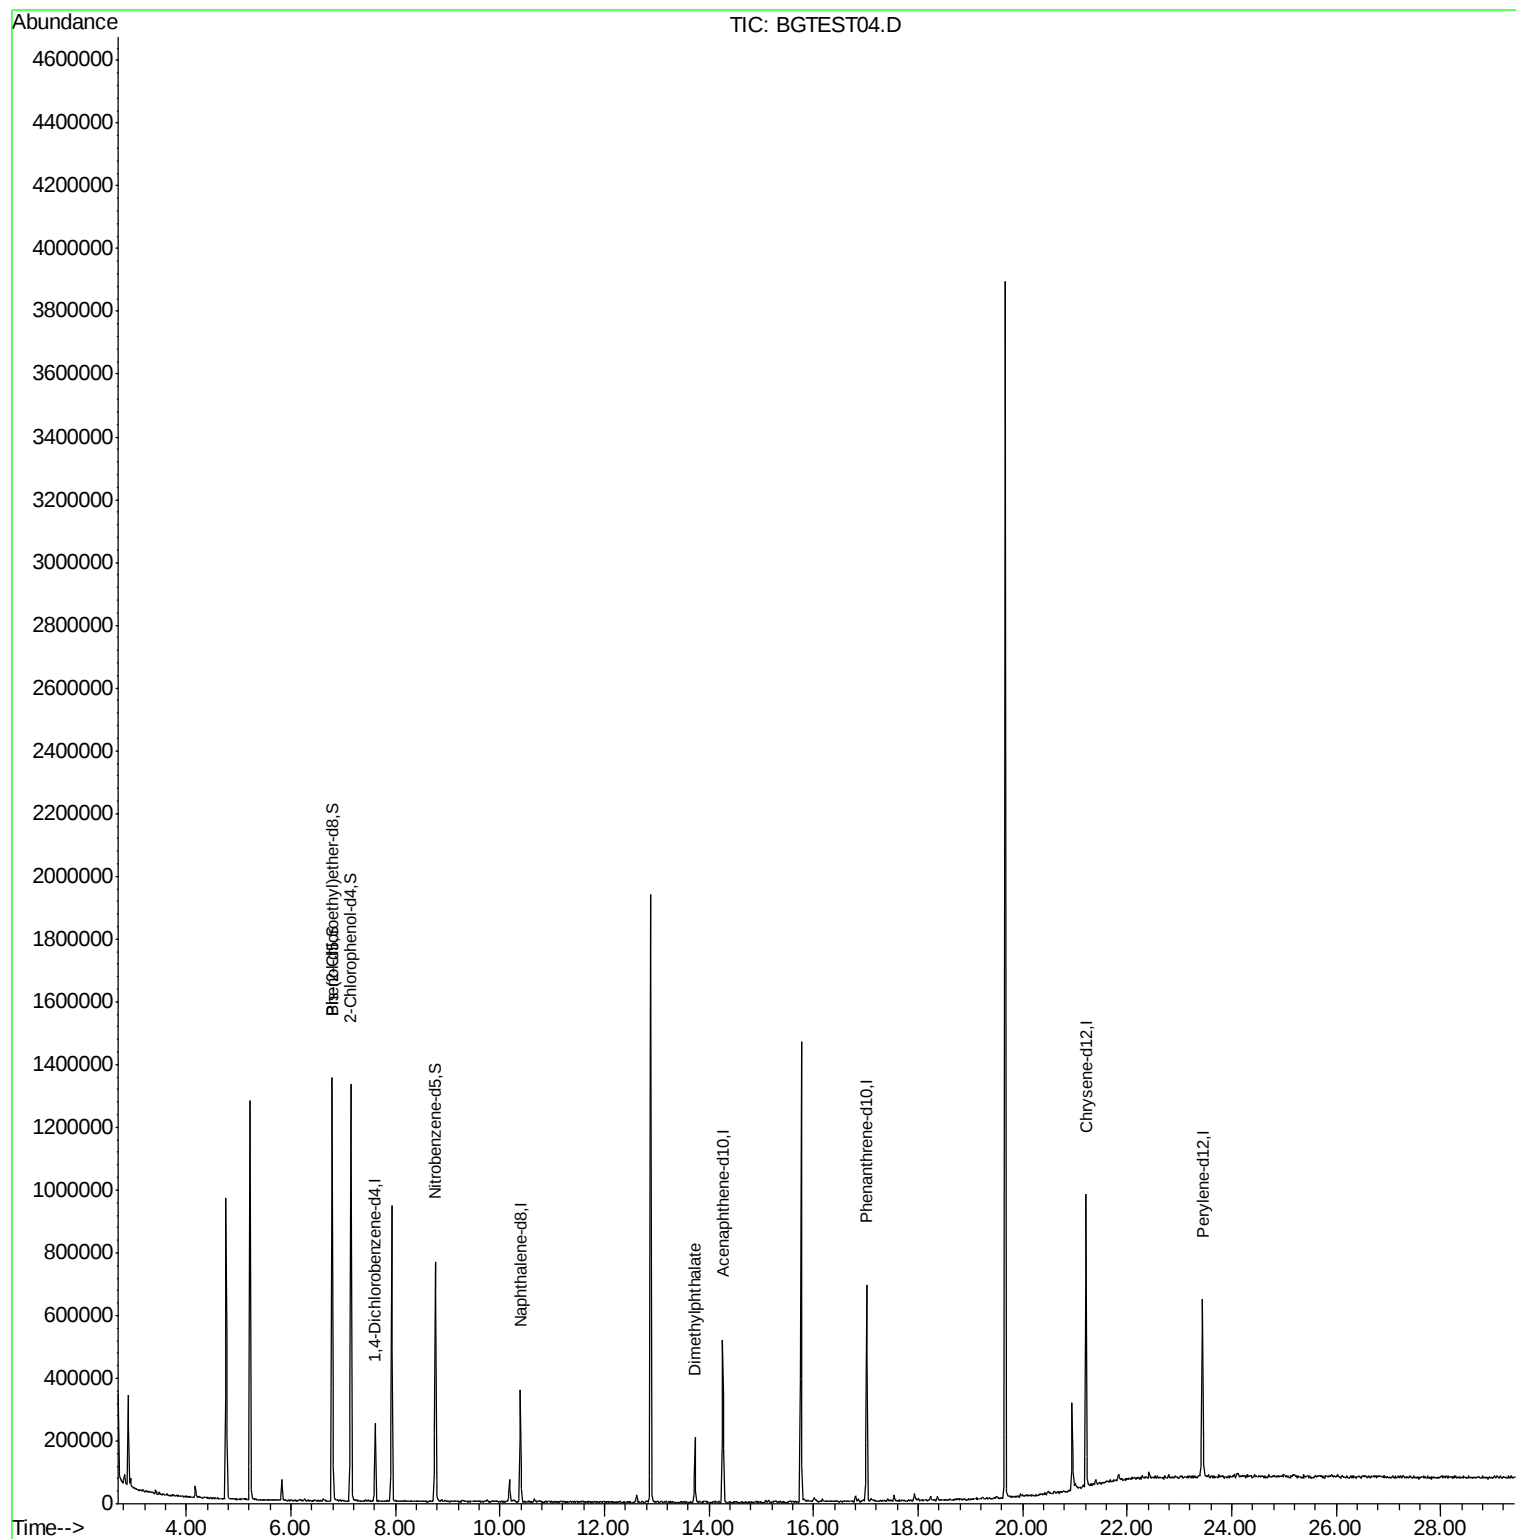

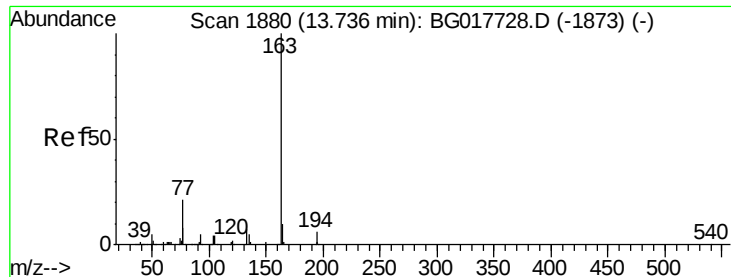

#44
 Dimethylphthalate
 Concen: 9.21 ng/ul
 RT: 13.73 min Scan# 1879
 Delta R.T. -0.01 min
 Lab File: BGTEST04.D
 Acq: 19 Jun 2015 22:01

Instrument :
 BNA_G
 ClientSampleId :

Tgt Ion	Ratio	Lower	Upper
163	100		
194	5.9	3.6	5.4#
164	11.2	8.0	12.0

