

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
 Data File : BGTEST05.D
 Acq On : 19 Jun 2015 22:36
 Operator : TP/IZ
 Sample : UNIT-3-SPOT-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 20 02:51:49 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 19 17:30:37 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	58026	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	265484	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	160719	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	360594	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	377035	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	357312	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.90	96	129	0.10	ng/uL	-0.24
5) Phenol-d5	6.79	99	697381	138.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	156	0.05	ng/ul	0.12
9) 2-Chlorophenol-d4	7.15	132	567775	137.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	465	0.11	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	189070	92.56	ng/ul	0.00
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.38	131	264	0.05	ng/ul	-0.15
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.25	176	979	0.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.11	188	5761	0.35	ng/ul	0.00
78) Pyrene-d10	0.00	212	0	0.00	ng/ul	
89) Benzo(a)pyrene-d12	23.28	264	262	0.02	ng/ul	-0.02


Target Compounds					Qvalue
44) Dimethylphthalate	13.73	163	134809	11.32 ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
Data File : BGTEST05.D
Acq On : 19 Jun 2015 22:36
Operator : TP/IZ
Sample : UNIT-3-SPOT-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 20 02:51:49 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 19 17:30:37 2015
Response via : Initial Calibration

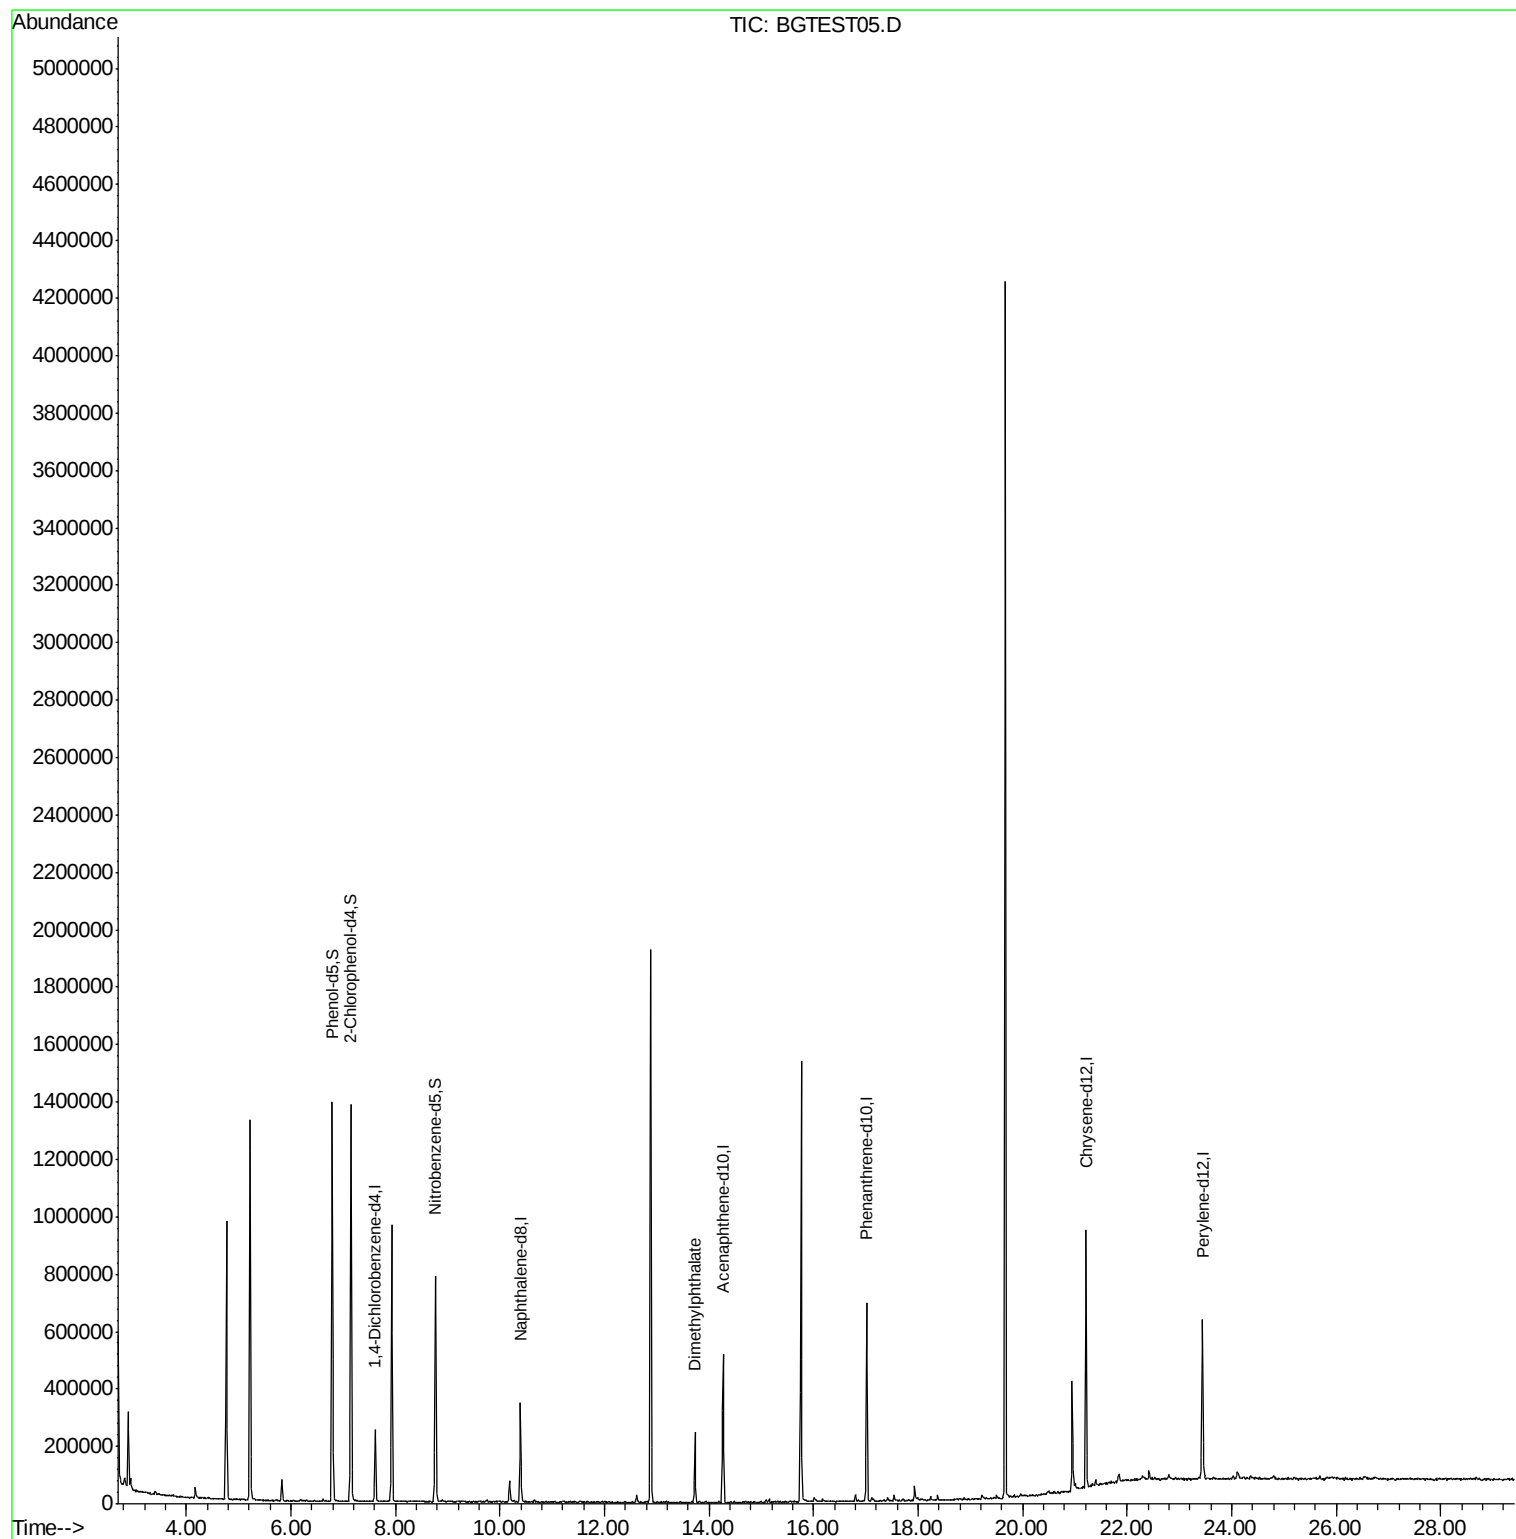

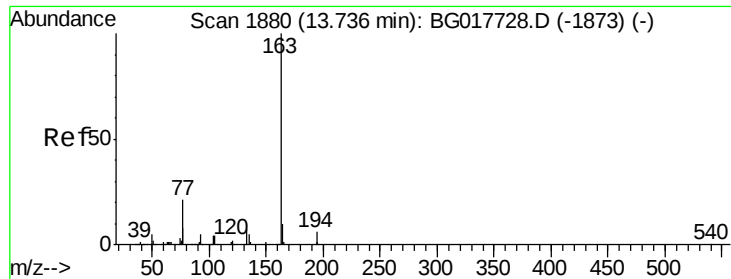

#44

Dimethylphthalate

Concen: 11.32 ng/ul

RT: 13.73 min Scan# 1879

Delta R.T. -0.01 min

Lab File: BGTEST05.D

Acq: 19 Jun 2015 22:36

Instrument :

BNA_G

ClientSampleId :


Tgt Ion:163 Resp: 134809

Ion Ratio Lower Upper

163 100

194 6.6 3.6 5.4#

164 9.0 8.0 12.0

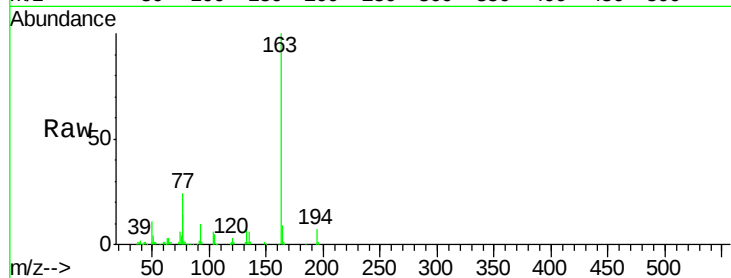

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

