

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
 Data File : BGTEST06.D
 Acq On : 19 Jun 2015 23:11
 Operator : TP/IZ
 Sample : UNIT-3-SPOT-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 20 02:51:54 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 19 17:30:37 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	61414	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	271991	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	166277	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.01	188	370254	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	384187	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	361680	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.40	96	73	0.05	ng/uL	0.26
5) Phenol-d5	6.79	99	682955	128.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	203	0.07	ng/ul	0.11
9) 2-Chlorophenol-d4	7.15	132	559918	128.06	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	470	0.11	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	183090	87.49	ng/ul	0.00
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.40	131	176	0.03	ng/ul	-0.13
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.26	176	599	0.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.11	188	5190	0.30	ng/ul	0.00
78) Pyrene-d10	0.00	212	0	0.00	ng/ul	
89) Benzo(a)pyrene-d12	23.30	264	152	0.01	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.73	163	118220	9.60	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
Data File : BGTEST06.D
Acq On : 19 Jun 2015 23:11
Operator : TP/IZ
Sample : UNIT-3-SPOT-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 20 02:51:54 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 19 17:30:37 2015
Response via : Initial Calibration

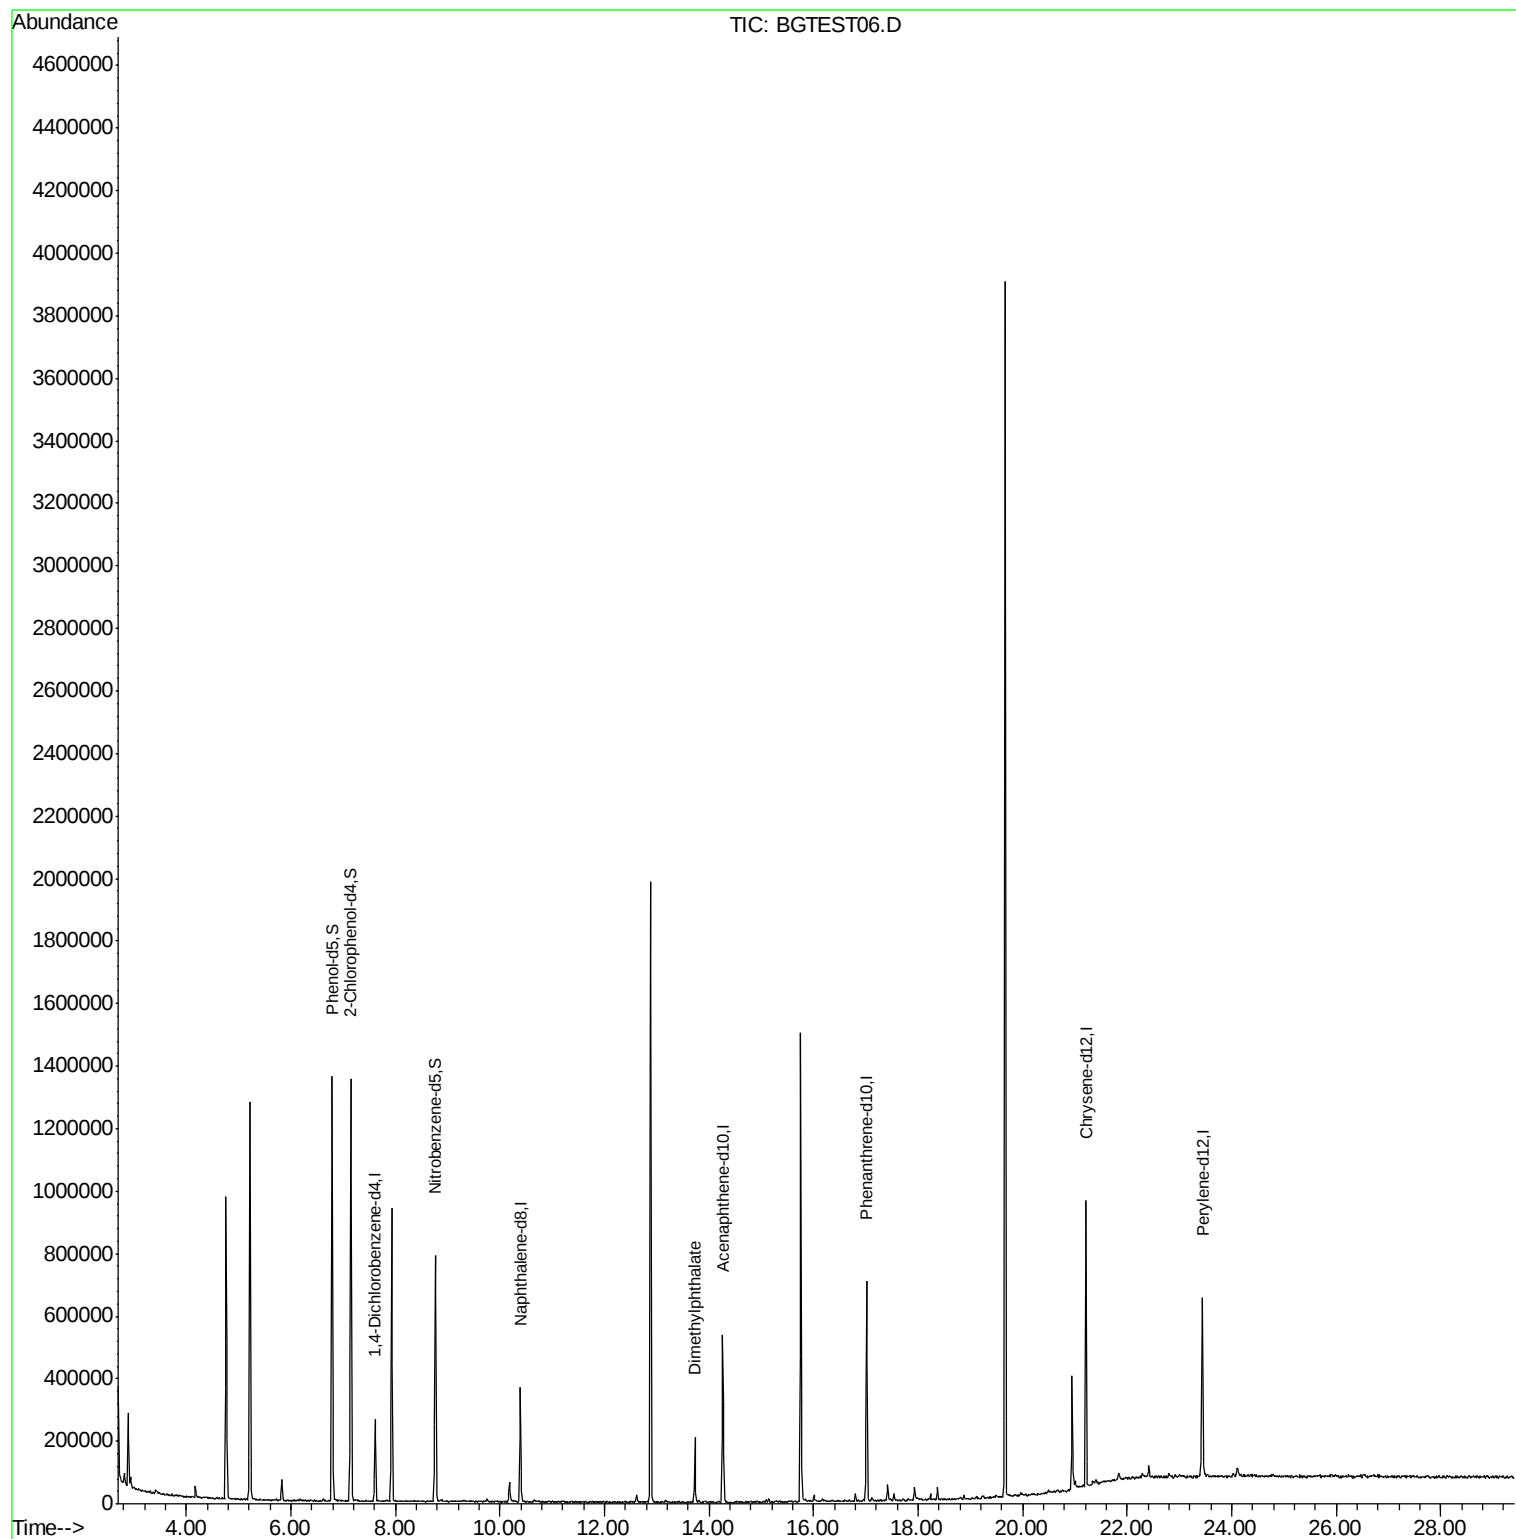

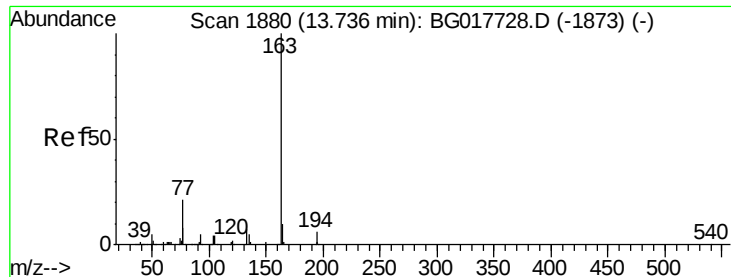

#44
 Dimethylphthalate
 Concen: 9.60 ng/ul
 RT: 13.73 min Scan# 1879
 Delta R.T. -0.01 min
 Lab File: BGTEST06.D
 Acq: 19 Jun 2015 23:11

Instrument :
 BNA_G
 ClientSampleId :

Tgt Ion	Ratio	Lower	Upper
163	100		
194	6.2	3.6	5.4#
164	10.1	8.0	12.0

