

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
 Data File : BGTEST07.D
 Acq On : 19 Jun 2015 23:46
 Operator : TP/IZ
 Sample : UNIT-3-SPOT-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 20 02:51:59 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 19 17:30:37 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	58254	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	259307	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	160564	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	357767	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	368114	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	344885	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	122	0.09	ng/uL	0.16
5) Phenol-d5	6.79	99	675653	133.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	6518	2.23	ng/ul	-0.17
9) 2-Chlorophenol-d4	7.14	132	550484	132.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	201	0.05	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	182715	91.58	ng/ul	0.00
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.39	131	415	0.08	ng/ul	-0.14
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.26	176	1027	0.10	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.11	188	6207	0.38	ng/ul	0.00
78) Pyrene-d10	0.00	212	0	0.00	ng/ul	
89) Benzo(a)pyrene-d12	23.30	264	54	0.00	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.73	163	117991	9.92	ng/ul#	97




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
Data File : BGTEST07.D
Acq On : 19 Jun 2015 23:46
Operator : TP/IZ
Sample : UNIT-3-SPOT-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 20 02:51:59 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 19 17:30:37 2015
Response via : Initial Calibration

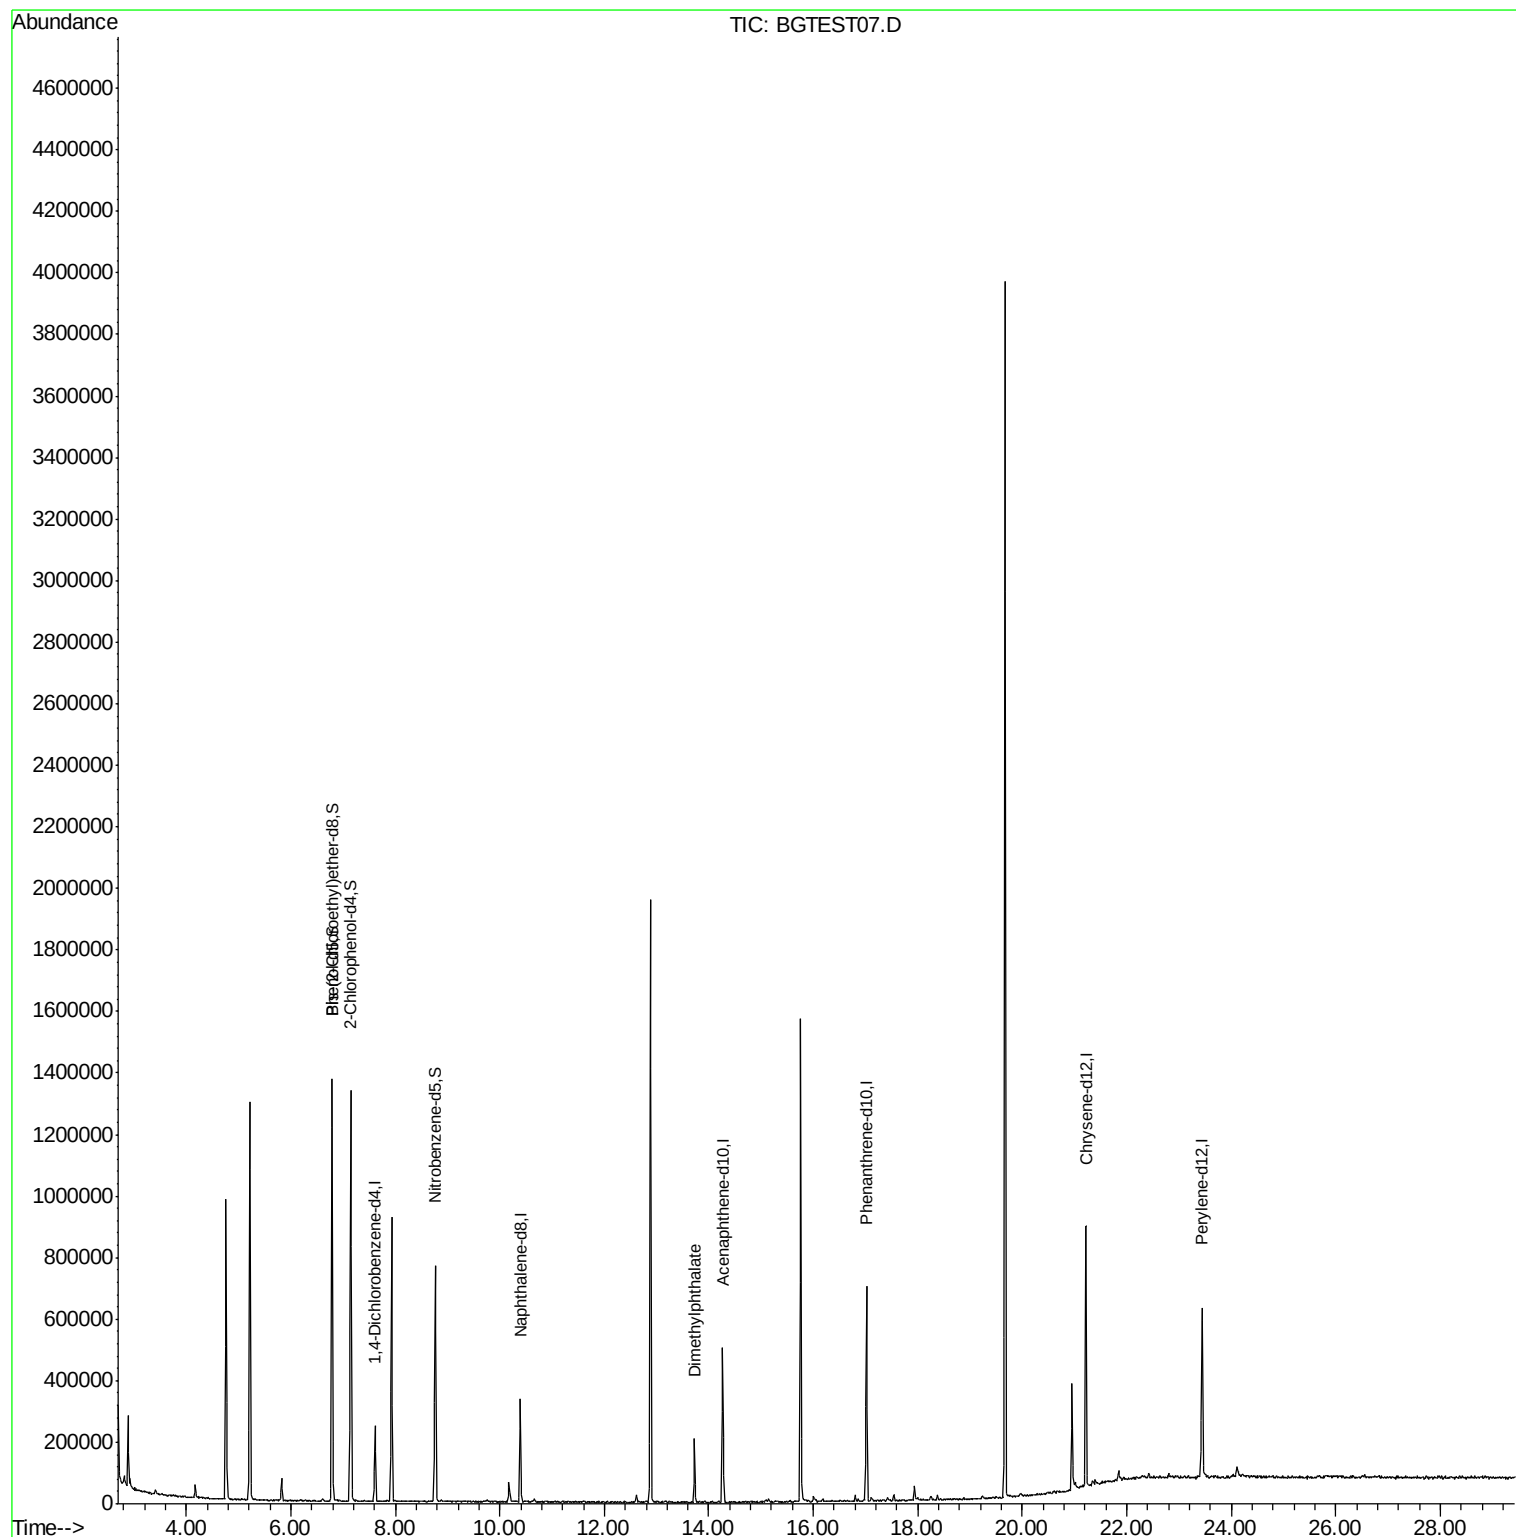

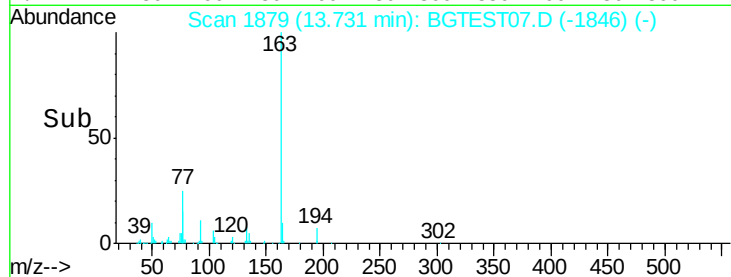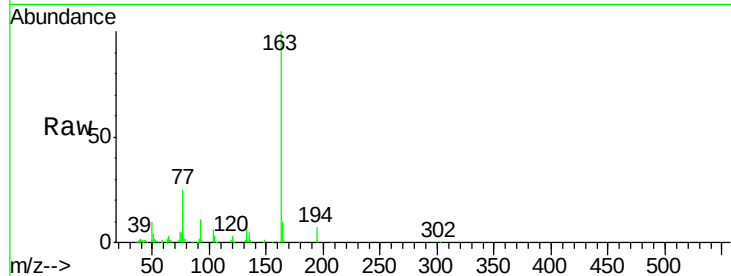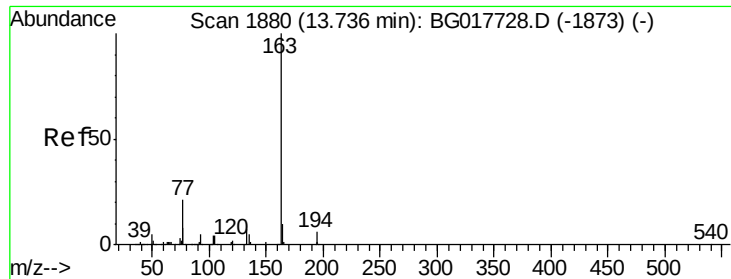

#44

Dimethylphthalate

Concen: 9.92 ng/ul

RT: 13.73 min Scan# 1879

Delta R.T. -0.01 min

Lab File: BGTEST07.D

Acq: 19 Jun 2015 23:46

Instrument :

BNA_G

ClientSampleId :

Tgt Ion:	163	Resp:	117991
Ion Ratio	Lower	Upper	
163	100		
194	6.7	3.6	5.4#
164	10.3	8.0	12.0

