

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
 Data File : BGTEST08.D
 Acq On : 20 Jun 2015 00:21
 Operator : TP/IZ
 Sample : UNIT-3-SPOT-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 20 02:52:04 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 19 17:30:37 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	62160	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	275793	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	173117	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	385857	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	400720	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	372562	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	109	0.08	ng/uL	0.16
5) Phenol-d5	6.80	99	802519	149.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.11	67	60	0.02	ng/ul	0.15
9) 2-Chlorophenol-d4	7.15	132	658942	148.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	122	0.03	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	217444	102.48	ng/ul	0.00
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.40	131	611	0.11	ng/ul	-0.14
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.26	176	1153	0.10	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.11	188	5793	0.33	ng/ul	0.00
78) Pyrene-d10	0.00	212	0	0.00	ng/ul	
89) Benzo(a)pyrene-d12	23.29	264	236	0.01	ng/ul	-0.01


Target Compounds					Qvalue
44) Dimethylphthalate	13.73	163	142686	11.12 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
Data File : BGTEST08.D
Acq On : 20 Jun 2015 00:21
Operator : TP/IZ
Sample : UNIT-3-SPOT-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 20 02:52:04 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 19 17:30:37 2015
Response via : Initial Calibration

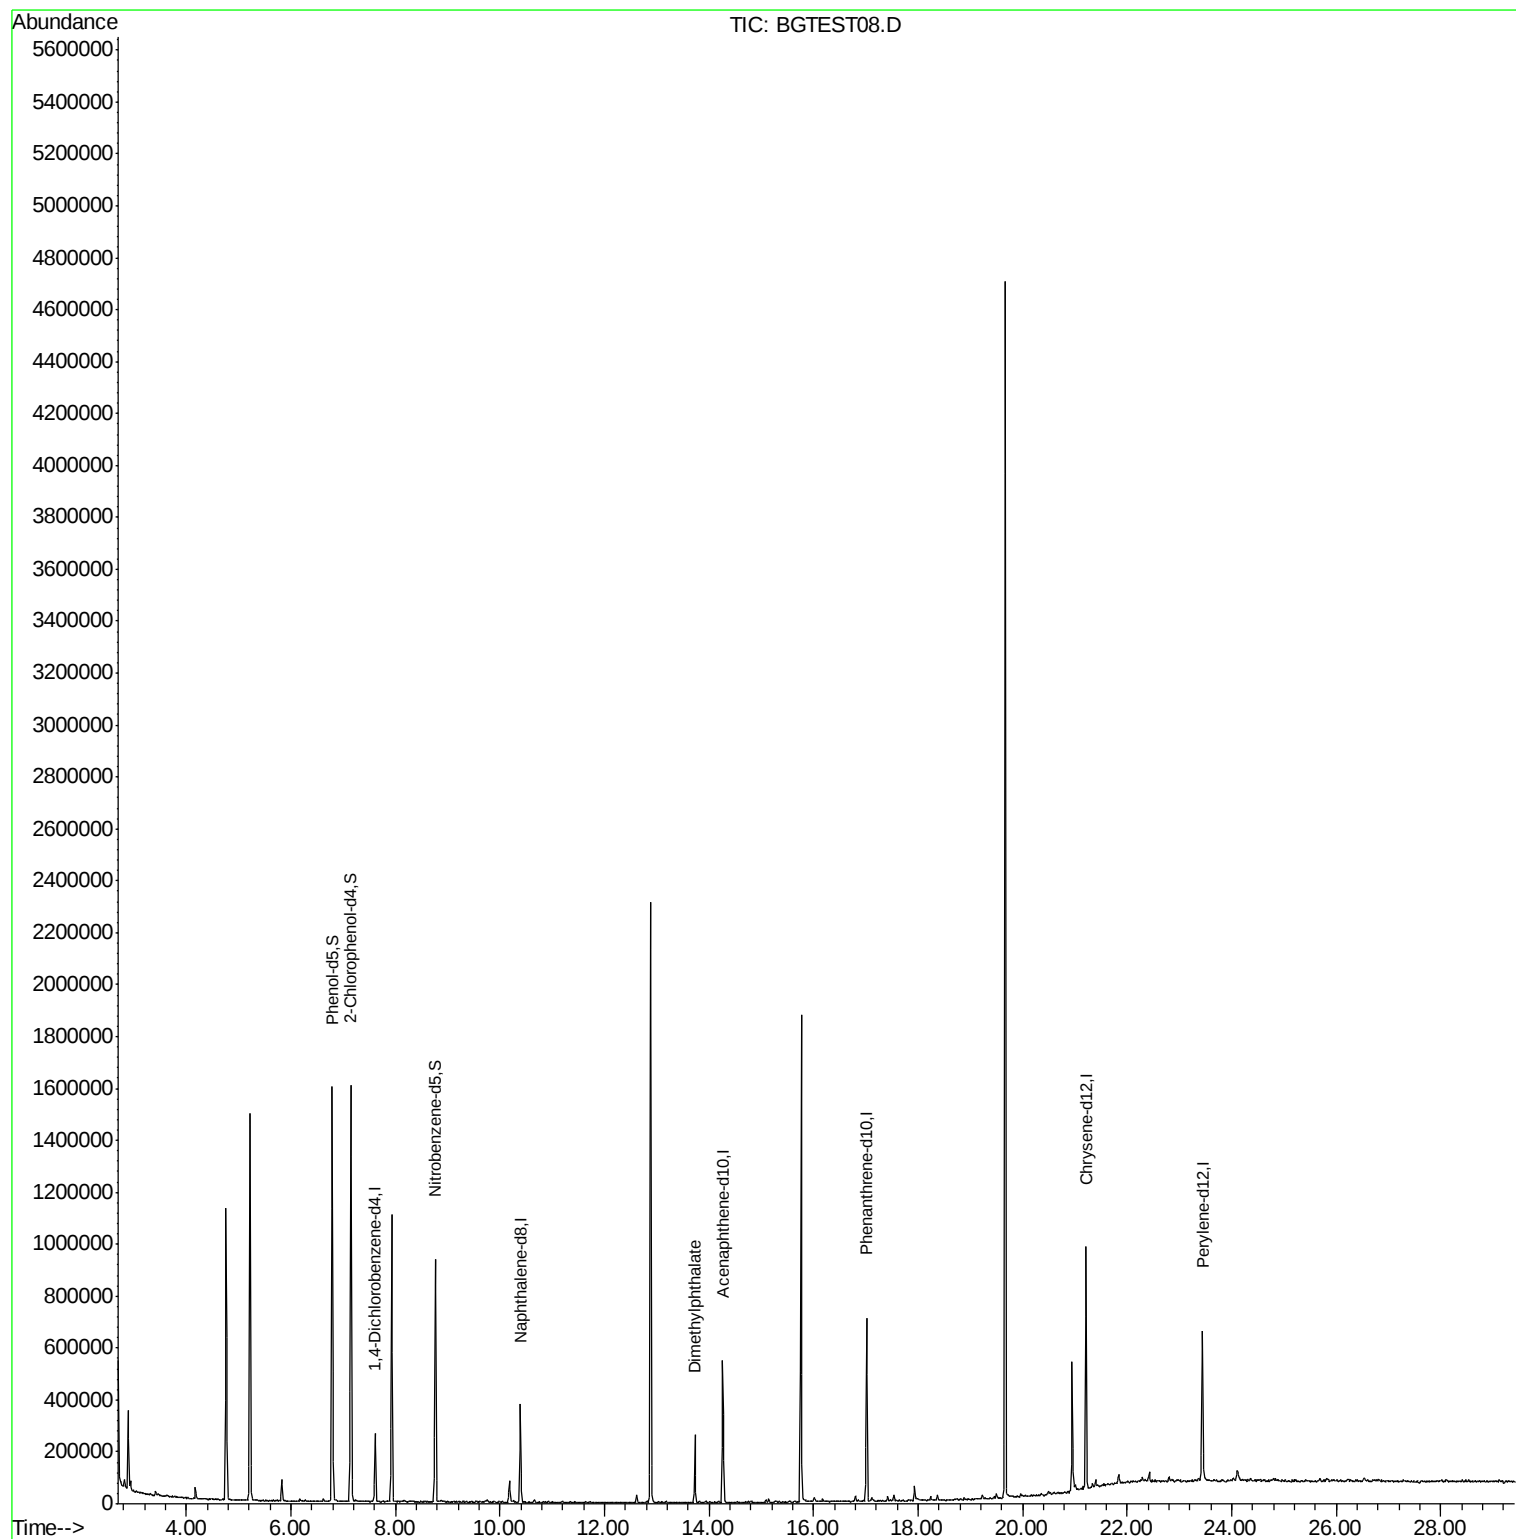

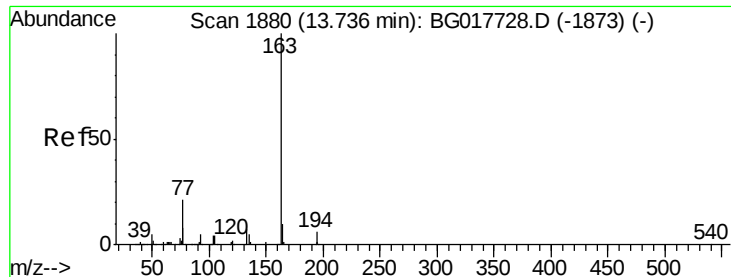

#44

Dimethylphthalate

Concen: 11.12 ng/ul

RT: 13.73 min Scan# 1879

Delta R.T. -0.01 min


Lab File: BGTEST08.D

Acq: 20 Jun 2015 00:21

Instrument :

BNA_G

ClientSampleId :

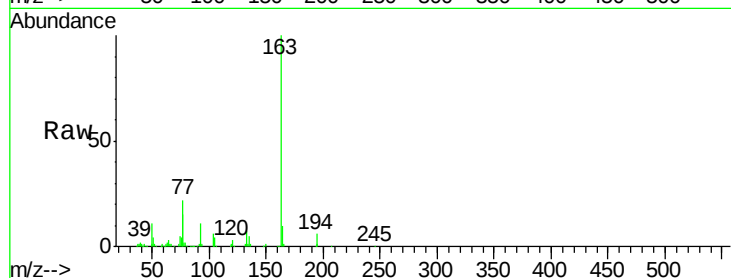

Tgt Ion:	163	Resp:	142686
Ion Ratio		Lower	Upper
163	100		
194	6.1	3.6	5.4#
164	9.7	8.0	12.0

