

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
 Data File : BGTEST09.D
 Acq On : 20 Jun 2015 00:55
 Operator : TP/IZ
 Sample : UNIT-3-SPOT-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 20 02:52:09 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 19 17:30:37 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	60492	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	263846	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	160089	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	359642	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	370944	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	347849	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.79	99	754855	144.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	167	0.06	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.15	132	620712	144.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	498	0.12	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	207202	102.07	ng/ul	0.00
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.41	131	161	0.03	ng/ul	-0.13
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.27	176	863	0.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.11	188	5904	0.36	ng/ul	0.00
78) Pyrene-d10	0.00	212	0	0.00	ng/ul	
89) Benzo(a)pyrene-d12	0.00	264	0	0.00	ng/ul	


Target Compounds					Qvalue
44) Dimethylphthalate	13.73	163	171199	14.43 ng/ul#	98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061915\
Data File : BGTEST09.D
Acq On : 20 Jun 2015 00:55
Operator : TP/IZ
Sample : UNIT-3-SPOT-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 20 02:52:09 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG061915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 19 17:30:37 2015
Response via : Initial Calibration

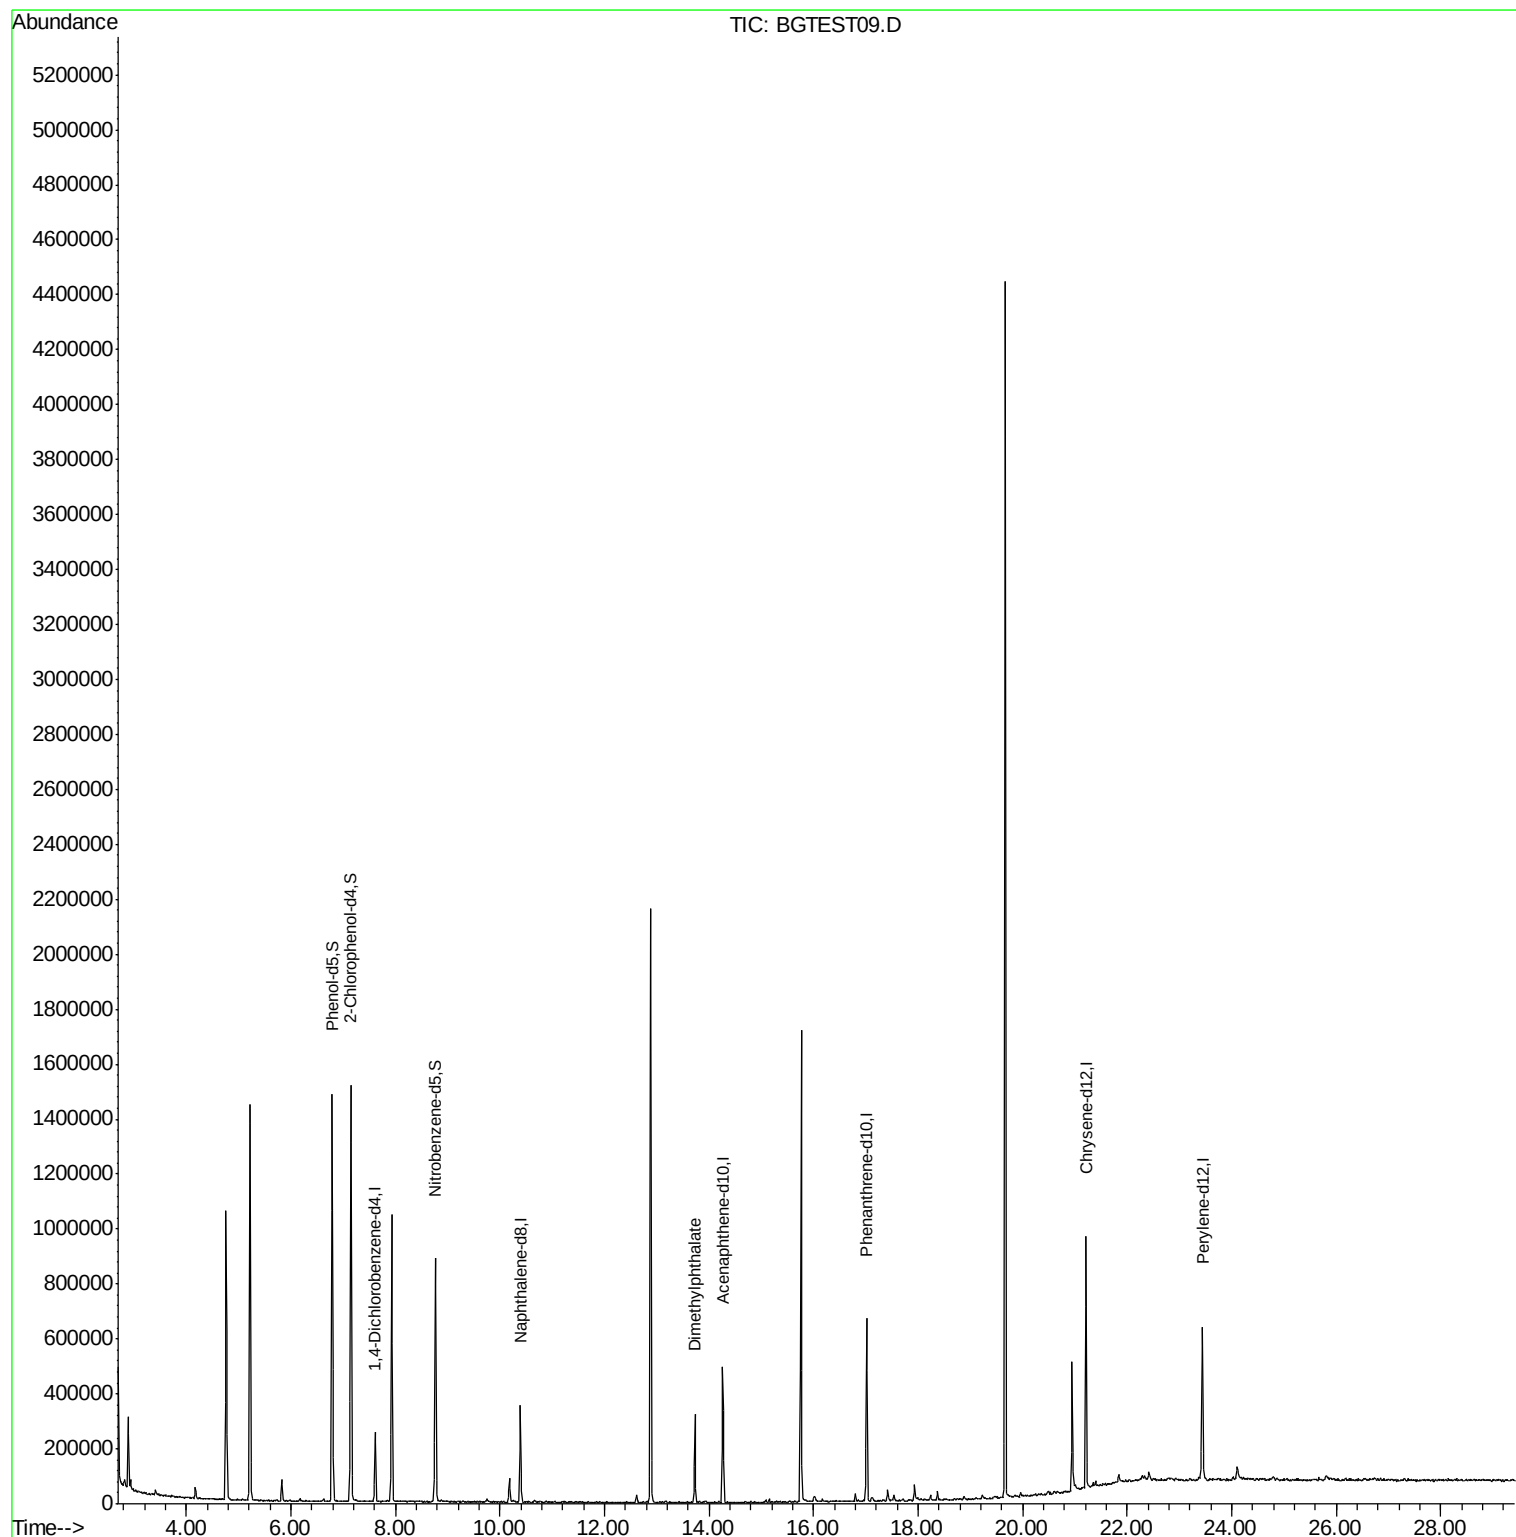

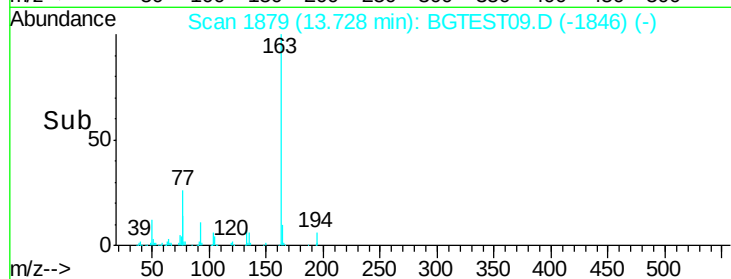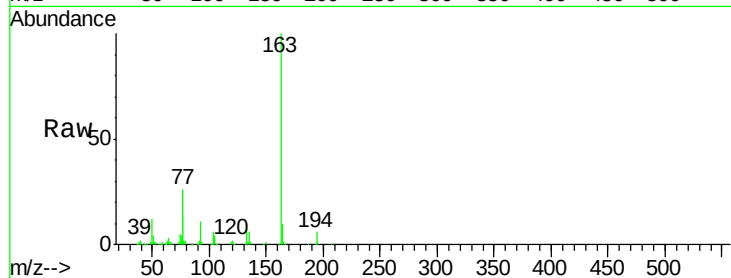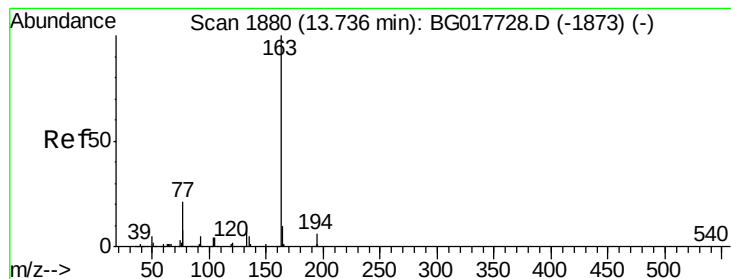

#44

Dimethylphthalate

Concen: 14.43 ng/ul

RT: 13.73 min Scan# 1879

Delta R.T. -0.01 min

Lab File: BGTEST09.D

Acq: 20 Jun 2015 00:55

Instrument :

BNA_G

ClientSampleId :

Tgt Ion:163 Resp: 171199

Ion Ratio Lower Upper

163 100

194 6.5 3.6 5.4#

164 10.3 8.0 12.0

