

Data File : BG027523.D
Acq On : 19 Jun 2017 11:01
Operator : SJ/MA
Sample : PB99876BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK76

Quant Time: Jun 20 01:01:06 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 20 01:01:03 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.52	152	32746	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	167736	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	111298	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.85	188	264034	20.00	ng/ul	0.00
75) Chrysene-d12	22.22	240	280521	20.00	ng/ul	0.00
83) Perylene-d12	25.88	264	270464	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	4.08	96	5965	7.29	ng/uL	0.00
5) Phenol-d5	7.65	99	124002	34.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.83	67	92210	38.10	ng/ul	0.00
9) 2-Chlorophenol-d4	8.05	132	89110	37.98	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	99718	35.92	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	45318	37.19	ng/ul	0.00
22) 2-Nitrophenol-d4	10.40	143	50641	39.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	87469	35.77	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	139021	44.90	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	338704	36.35	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	398625	37.14	ng/ul	0.00
51) 4-Nitrophenol-d4	15.27	143	50128	27.50	ng/ul	0.00
57) Fluorene-d10	16.09	176	304262	34.80	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.19	200	50225	30.63	ng/ul	0.00
70) Anthracene-d10	17.95	188	468255	38.03	ng/ul	0.00
76) Pyrene-d10	20.22	212	516913	37.73	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.63	264	460559	37.82	ng/ul	0.00

Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	9.20	70	2962	1.22 ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG027523.D

Acq On : 19 Jun 2017 11:01

Operator : SJ/MA

Sample : PB99876BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

SBLK76


Quant Time: Jun 20 01:01:06 2017




Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Jun 20 01:01:03 2017

Response via : Initial Calibration

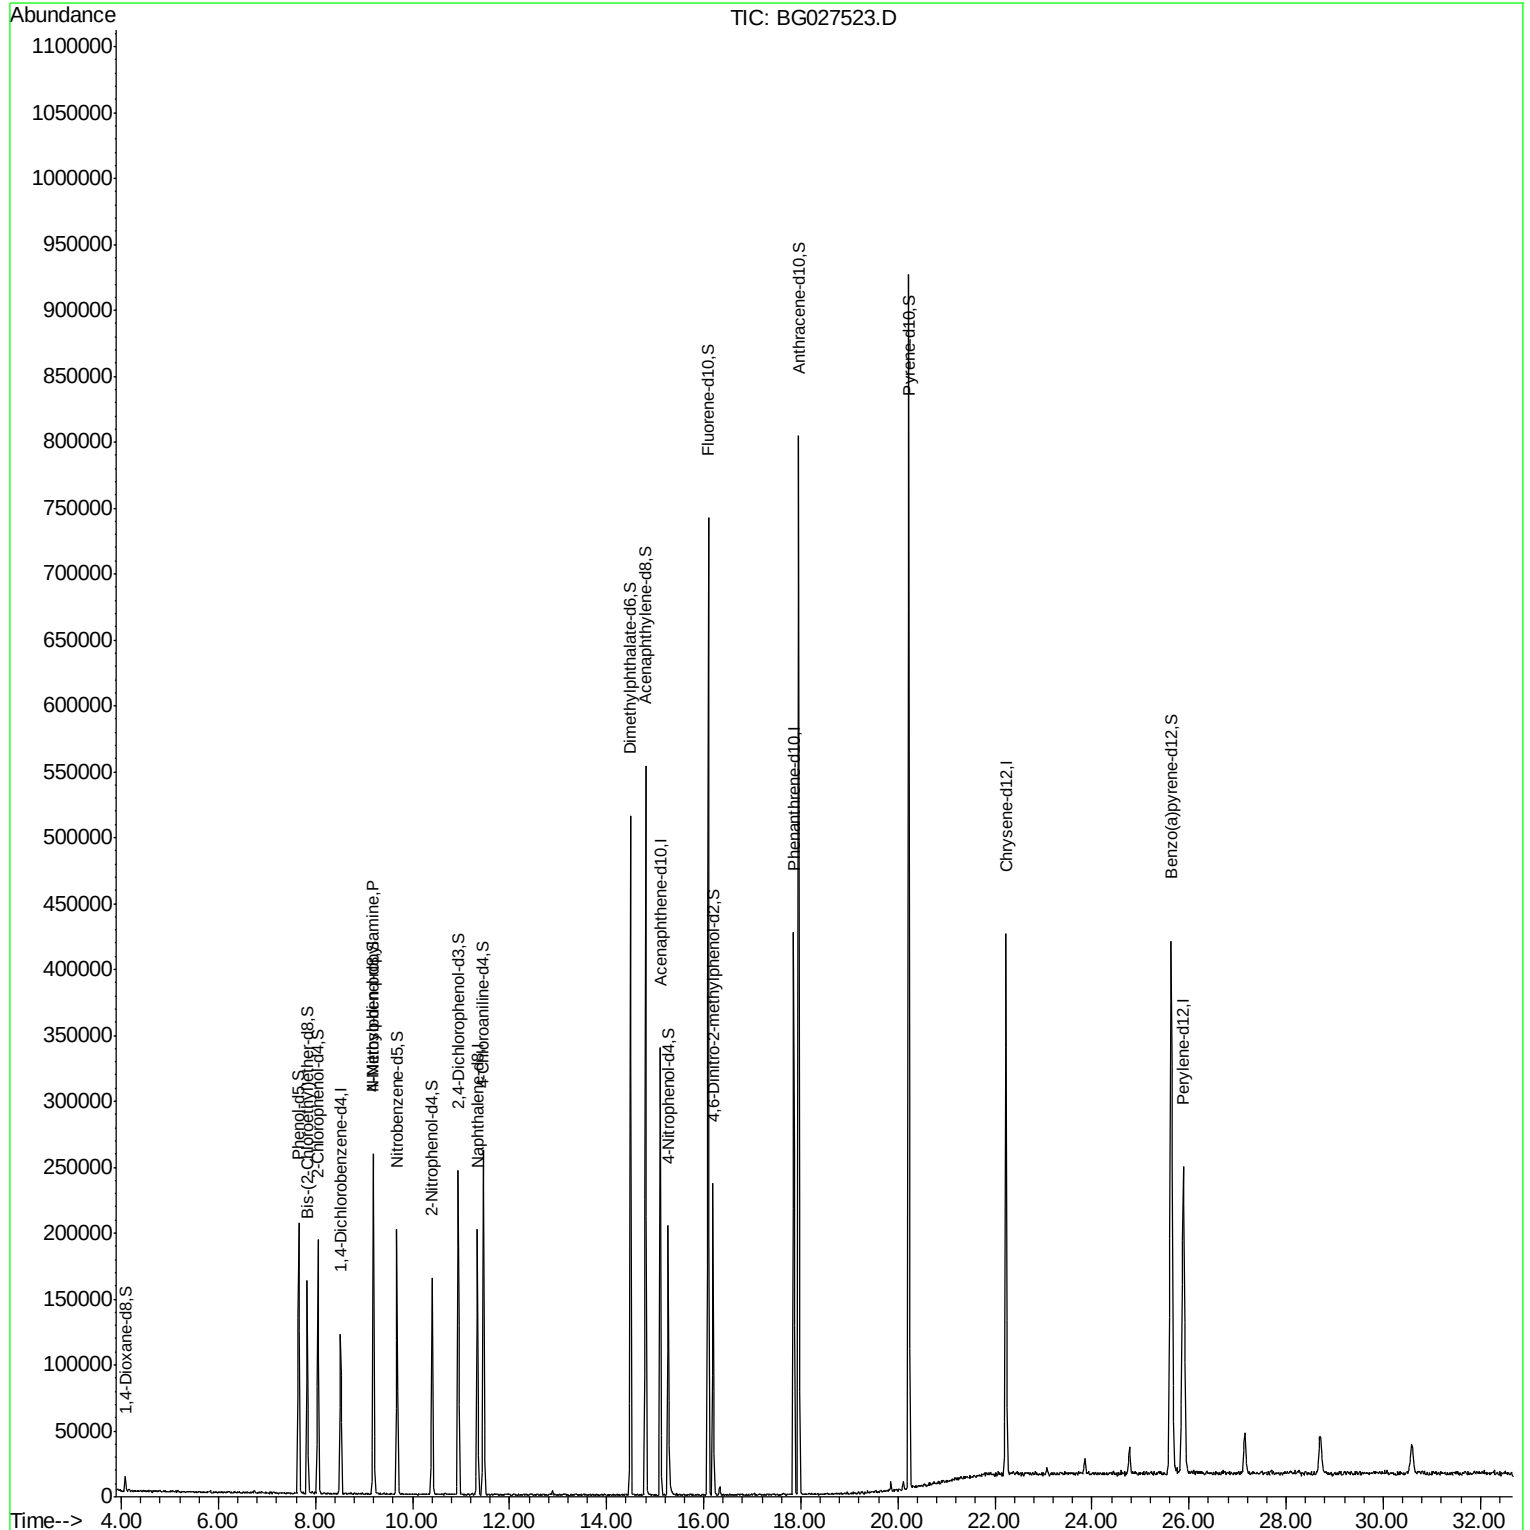

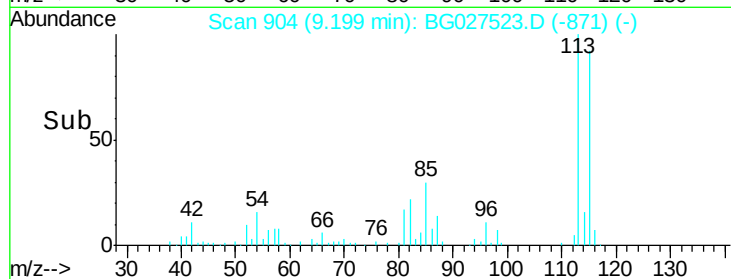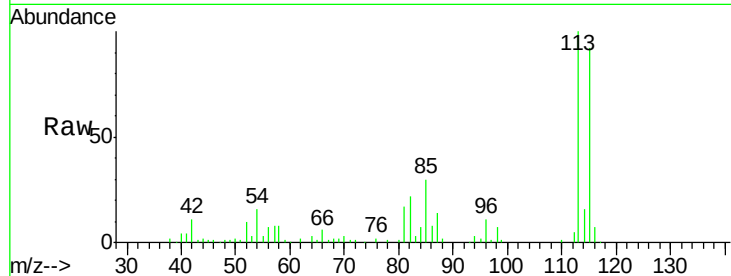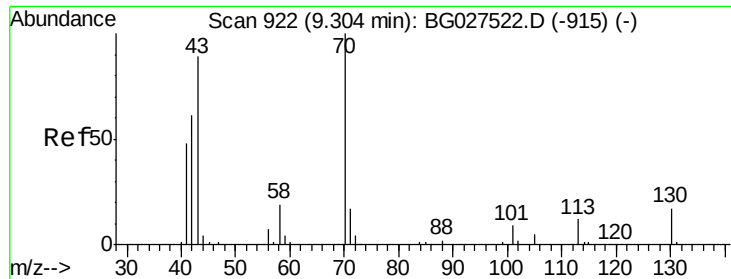

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.22 ng/ul
 RT: 9.20 min Scan# 904
 Delta R.T. -0.11 min
 Lab File: BG027523.D
 Acq: 19 Jun 2017 11:01

Instrument :
 BNA_G
 ClientSampleId :
 SBLK76

Tgt Ion:	70	Resp:	2962
Ion	Ratio	Lower	Upper
70	100		
42	328.8	59.0	88.6#
101	0.0	6.6	9.8#
130	0.0	15.6	23.4#

