

Data File : BG027524.D
Acq On : 19 Jun 2017 11:41
Operator : SJ/MA
Sample : PB99875BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK75

Quant Time: Jun 20 01:01:29 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 20 01:01:03 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.52	152	32092	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	161953	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	107410	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.85	188	253146	20.00	ng/ul	0.00
75) Chrysene-d12	22.23	240	268075	20.00	ng/ul	0.00
83) Perylene-d12	25.89	264	249977	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	4.08	96	6401	7.98	ng/uL	0.00
5) Phenol-d5	7.65	99	134253	38.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.83	67	101503	42.79	ng/ul	0.00
9) 2-Chlorophenol-d4	8.05	132	97054	42.21	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	110995	40.79	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	50208	42.68	ng/ul	0.00
22) 2-Nitrophenol-d4	10.40	143	57243	45.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	98170	41.58	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	155644	52.07	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	376008	41.81	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	445060	42.97	ng/ul	0.00
51) 4-Nitrophenol-d4	15.27	143	56030	31.85	ng/ul	0.00
57) Fluorene-d10	16.09	176	336192	39.85	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.20	200	55873	35.54	ng/ul	0.00
70) Anthracene-d10	17.95	188	524142	44.41	ng/ul	0.00
76) Pyrene-d10	20.22	212	564048	43.09	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.63	264	509862	45.30	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	9.19	70	3124	1.31 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG027524.D
Acq On : 19 Jun 2017 11:41
Operator : SJ/MA
Sample : PB99875BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK75

Quant Time: Jun 20 01:01:29 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 20 01:01:03 2017
Response via : Initial Calibration

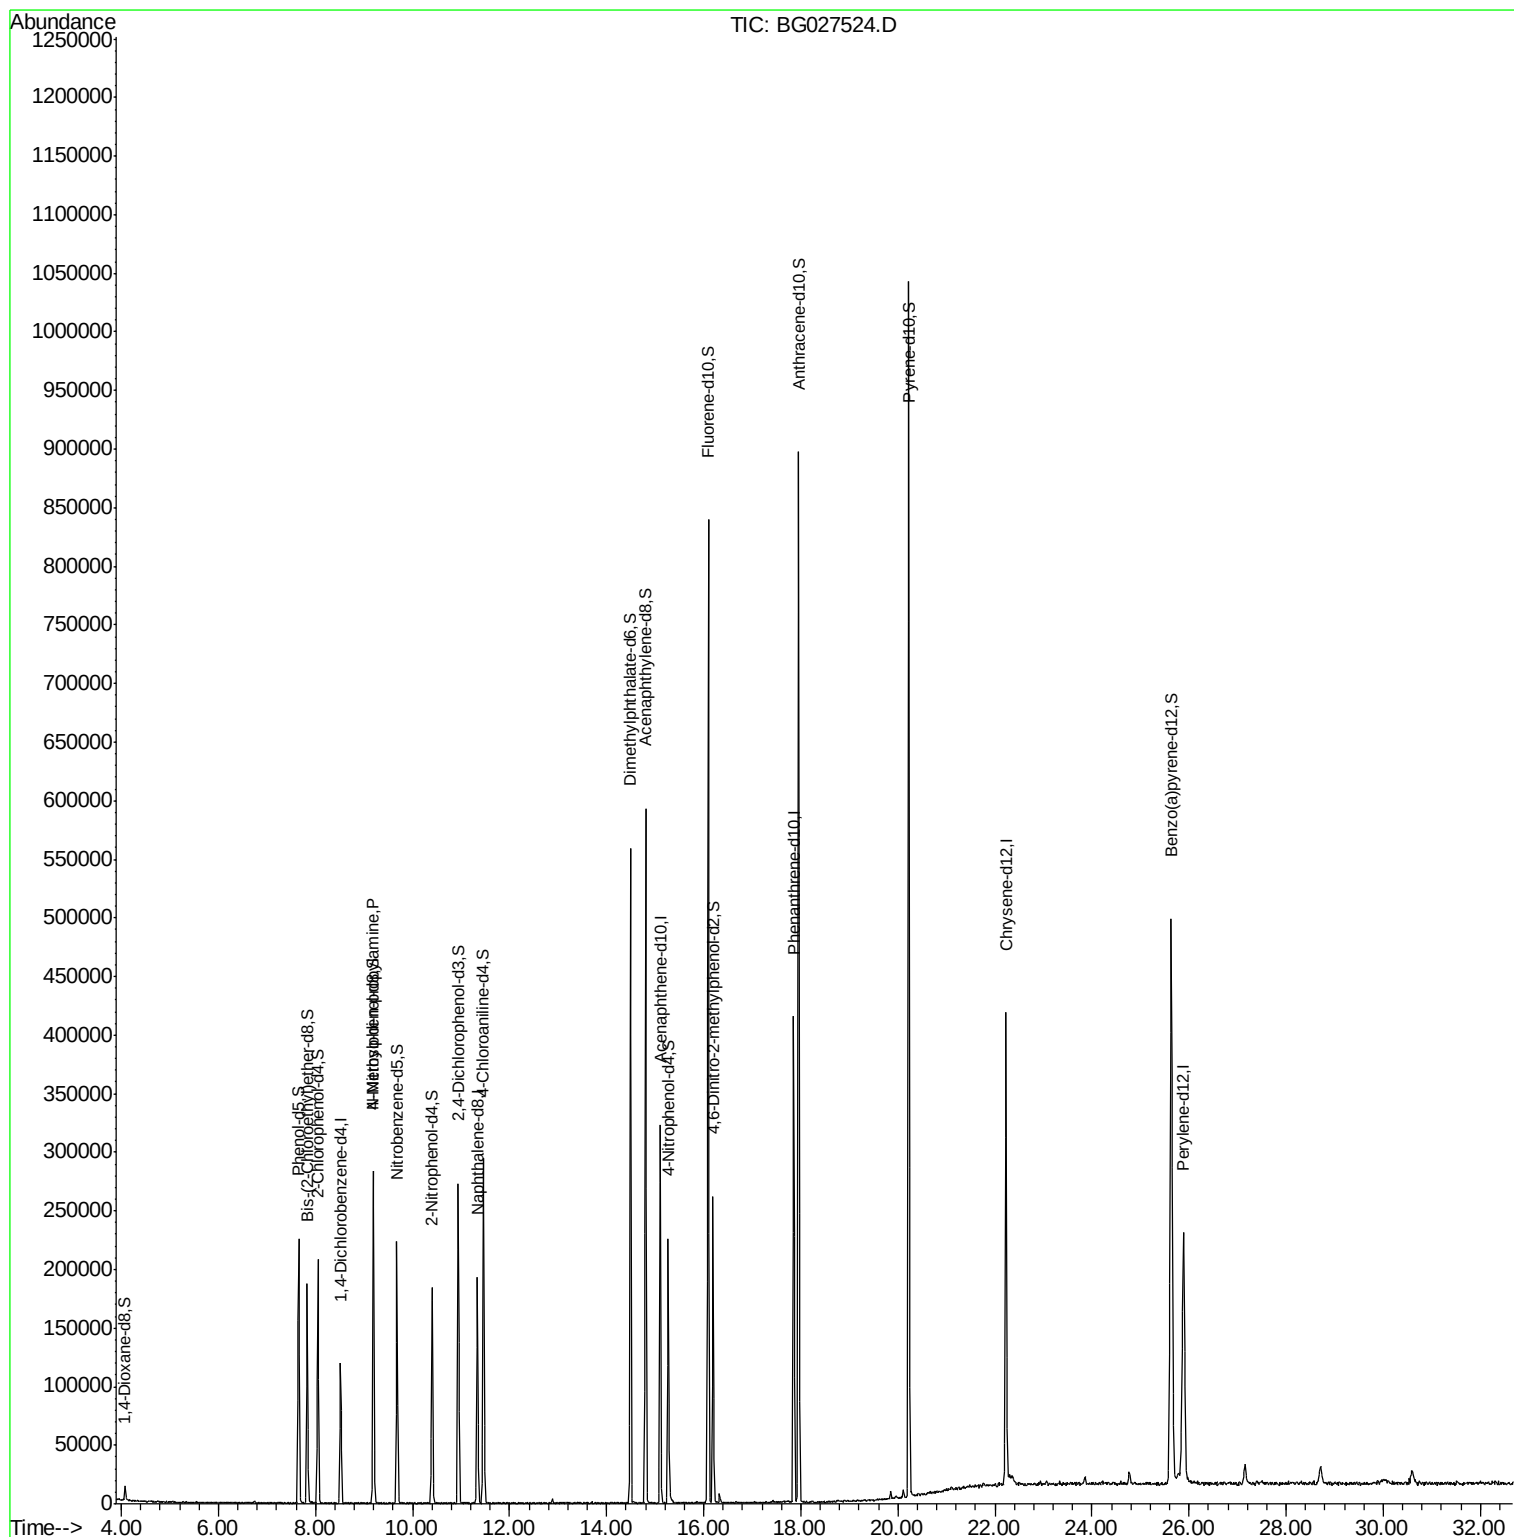

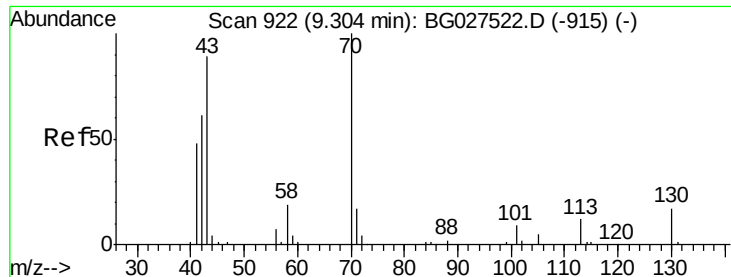

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.31 ng/ul
 RT: 9.19 min Scan# 903
 Delta R.T. -0.11 min
 Lab File: BG027524.D
 Acq: 19 Jun 2017 11:41

Instrument :
 BNA_G
 ClientSampleId :
 SBLK75

Tgt Ion:	70	Resp:	3124
Ion	Ratio	Lower	Upper
70	100		
42	380.0	59.0	88.6#
101	0.0	6.6	9.8#
130	0.0	15.6	23.4#

