

Data File : BG027538.D
Acq On : 19 Jun 2017 20:57
Operator : SJ/MA
Sample : PB99753BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK53

Quant Time: Jun 20 01:52:03 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 20 01:50:01 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.52	152	30682	20.00	ng/ul	0.00
18) Naphthalene-d8	11.33	136	157629	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	105983	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.85	188	250957	20.00	ng/ul	0.00
75) Chrysene-d12	22.23	240	278906	20.00	ng/ul	0.00
83) Perylene-d12	25.88	264	262827	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	4.08	96	4540	5.92	ng/uL	0.00
5) Phenol-d5	7.66	99	101544	30.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.83	67	74922	33.04	ng/ul	0.00
9) 2-Chlorophenol-d4	8.05	132	71649	32.59	ng/ul	0.00
13) 4-Methylphenol-d8	9.20	113	83242	32.00	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	37141	32.44	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	42305	34.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	75231	32.73	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	117205	40.29	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	286423	32.28	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	330792	32.37	ng/ul	0.00
51) 4-Nitrophenol-d4	15.27	143	36067	20.78	ng/ul	0.00
57) Fluorene-d10	16.09	176	256037	30.76	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.19	200	29211	18.74	ng/ul	0.00
70) Anthracene-d10	17.95	188	397985	34.01	ng/ul	0.00
76) Pyrene-d10	20.22	212	446438	32.78	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.63	264	406193	34.32	ng/ul	0.00

Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	9.19	70	2289	1.01 ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG027538.D

Acq On : 19 Jun 2017 20:57

Operator : SJ/MA

Sample : PB99753BL

Misc :

ALS Vial : 17 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

SBLK53


Quant Time: Jun 20 01:52:03 2017




Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Jun 20 01:50:01 2017

Response via : Initial Calibration

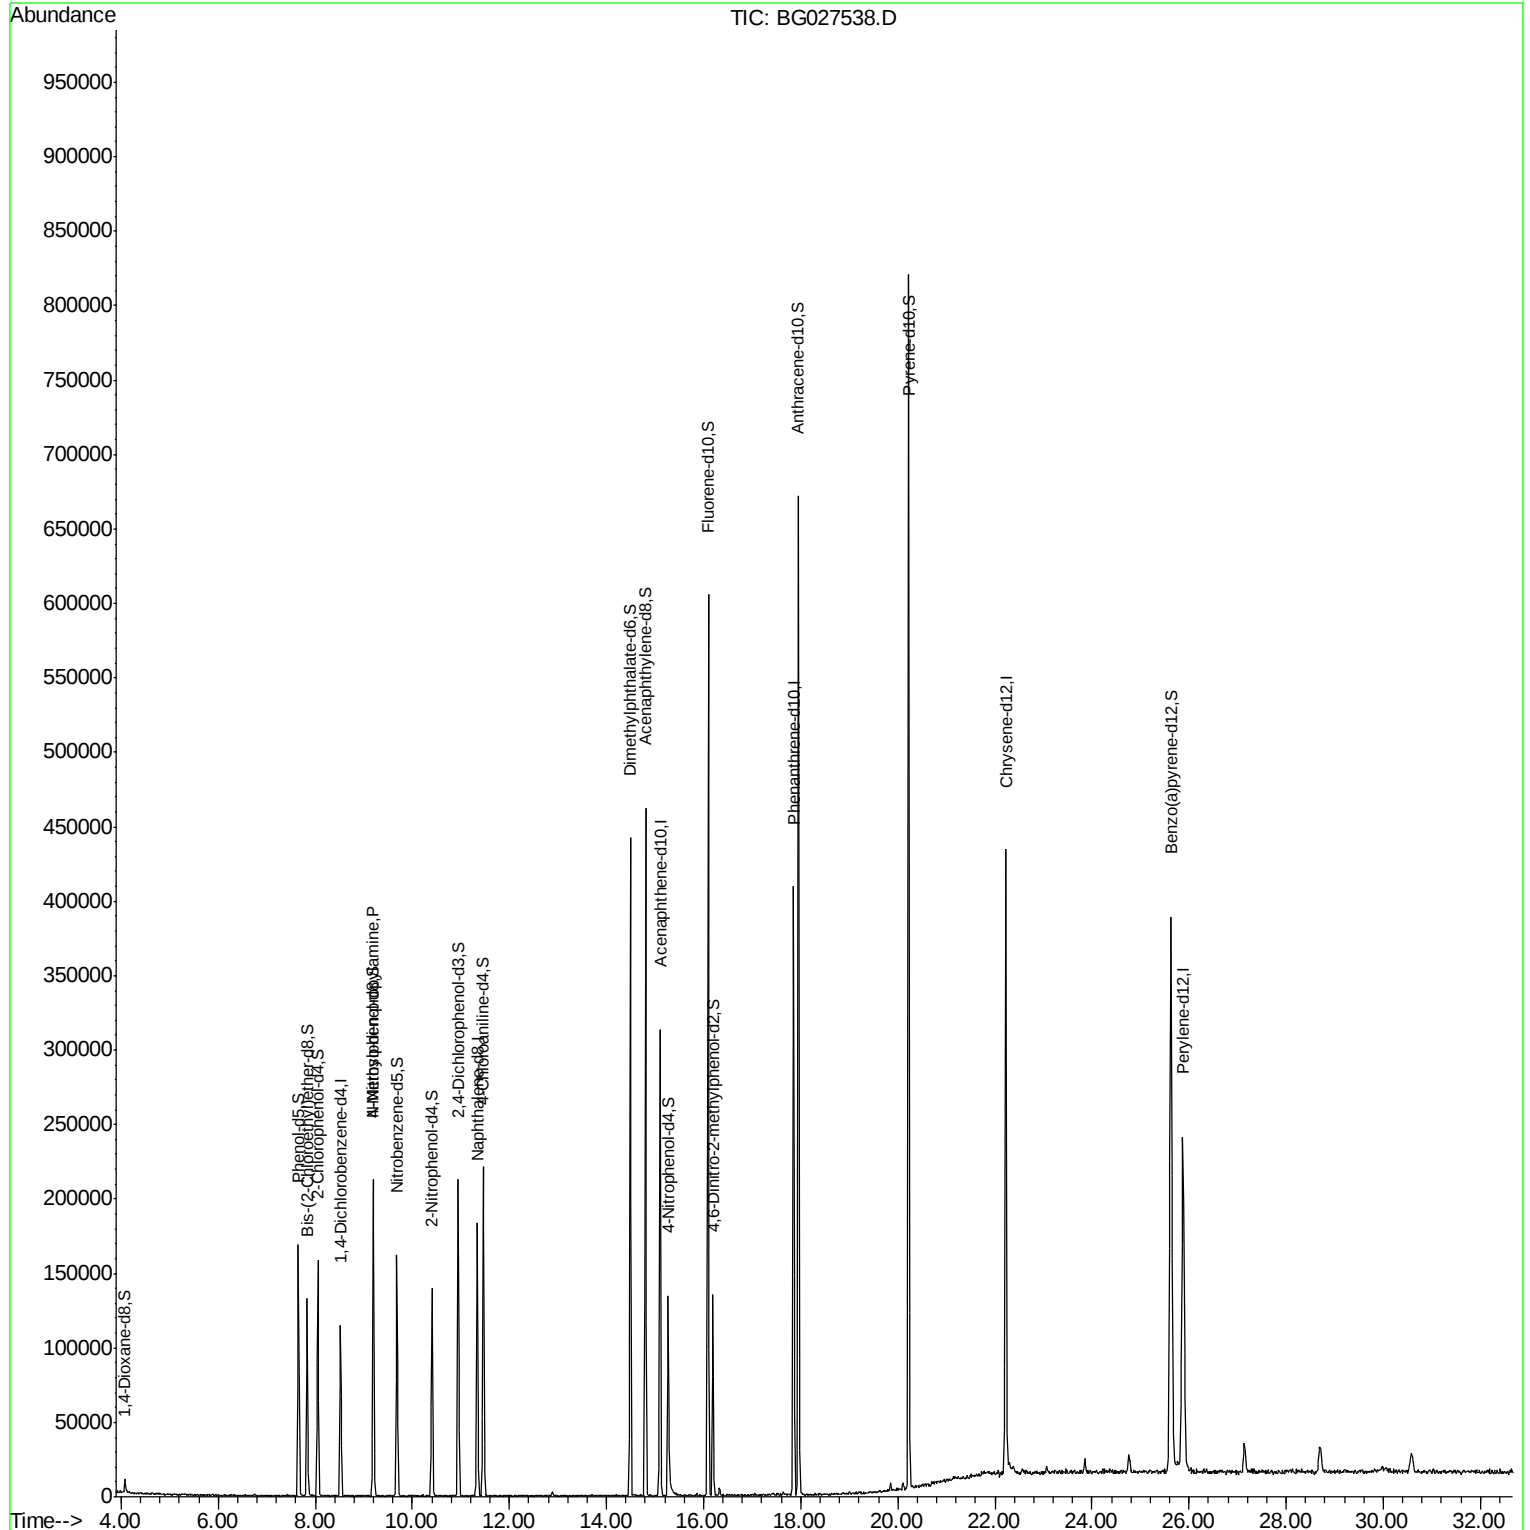

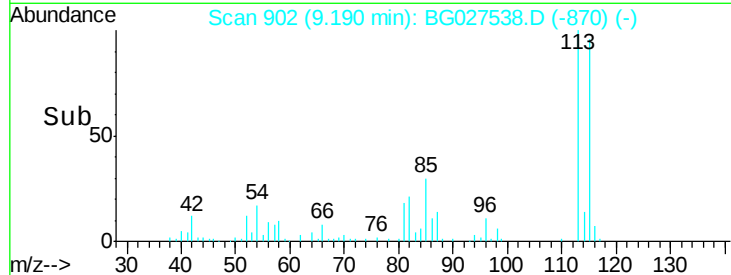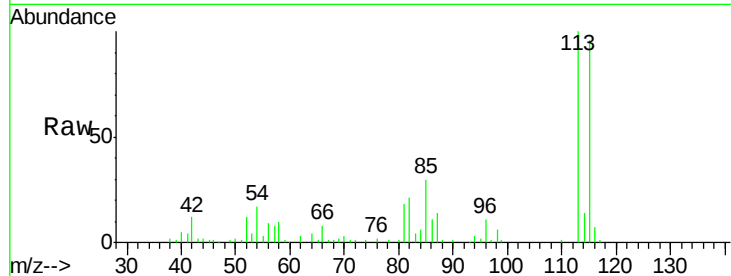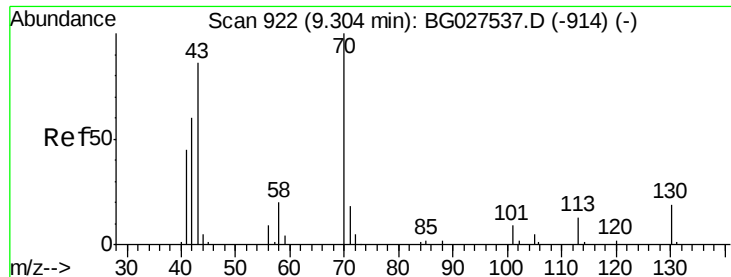

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.01 ng/ul
 RT: 9.19 min Scan# 902
 Delta R.T. -0.11 min
 Lab File: BG027538.D
 Acq: 19 Jun 2017 20:57

Instrument :
 BNA_G
 ClientSampleId :
 SBLK53

Tgt Ion:	70	Resp:	2289
Ion	Ratio	Lower	Upper
70	100		
42	341.1	59.0	88.6#
101	0.0	6.6	9.8#
130	0.0	15.6	23.4#

