

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
 Data File : BG027524.D
 Acq On : 19 Jun 2017 11:41
 Operator : SJ/MA
 Sample : PB99875BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.935	6	8	18	rVB5	923	1795	0.11%	0.011%
2	4.076	26	32	41	rVB3	12403	21040	1.34%	0.133%
3	4.170	46	48	55	rVB4	1262	1905	0.12%	0.012%
4	4.628	120	126	130	rVB3	738	1771	0.11%	0.011%
5	5.268	233	235	240	rBV3	1122	1806	0.11%	0.011%
6	6.731	480	484	492	rVB5	1491	3669	0.23%	0.023%
7	7.654	633	641	656	rVB	225739	413222	26.28%	2.615%
8	7.830	661	671	683	rBV	187580	322773	20.53%	2.042%
9	7.930	683	688	690	rVB4	1404	2440	0.16%	0.015%
10	8.047	700	708	719	rVB	207746	390118	24.81%	2.469%
11	8.518	779	788	798	rBV	119692	211589	13.46%	1.339%
12	9.193	895	903	918	rBV2	283639	515212	32.77%	3.260%
13	9.681	976	986	997	rBV	223074	417161	26.53%	2.640%
14	10.404	1101	1109	1120	rBV	183747	352954	22.45%	2.233%
15	10.938	1192	1200	1211	rBV	273150	521980	33.20%	3.303%
16	11.250	1247	1253	1255	rBV3	817	1775	0.11%	0.011%
17	11.338	1258	1268	1281	rVB	193887	368927	23.47%	2.335%
18	11.461	1281	1289	1305	rBV	295057	575691	36.62%	3.643%
19	12.883	1527	1531	1538	rVV4	4034	7094	0.45%	0.045%
20	13.706	1661	1671	1676	rVB3	1361	2165	0.14%	0.014%
21	14.493	1797	1805	1813	rBV	558983	871299	55.42%	5.513%
22	14.798	1848	1857	1868	rBV	592685	1011610	64.35%	6.401%
23	15.104	1894	1909	1921	rBV2	322608	547532	34.83%	3.465%
24	15.268	1930	1937	1955	rBV	225975	416973	26.52%	2.639%
25	15.462	1968	1970	1976	rVB2	937	1669	0.11%	0.011%
26	15.856	2035	2037	2049	rVB4	1366	2696	0.17%	0.017%
27	16.091	2069	2077	2087	rBV	839242	1326608	84.38%	8.395%
28	16.191	2087	2094	2105	rVV	261705	416216	26.47%	2.634%
29	16.261	2105	2106	2113	rVB2	1380	1798	0.11%	0.011%
30	16.326	2113	2117	2123	rBV3	8190	12290	0.78%	0.078%
31	17.431	2295	2305	2307	rBV3	1514	2483	0.16%	0.016%
32	17.854	2368	2377	2385	rBV2	415306	670815	42.67%	4.245%
33	17.954	2385	2394	2408	rVB	896031	1440557	91.63%	9.116%
34	18.218	2438	2439	2446	rVB5	1038	1782	0.11%	0.011%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
 Data File : BG027524.D
 Acq On : 19 Jun 2017 11:41
 Operator : SJ/MA
 Sample : PB99875BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

35	18.688	2514	2519	2521	rBV3	1040	1752	0.11%	0.011%
36	18.753	2525	2530	2531	rBV	1319	1656	0.11%	0.010%
37	18.900	2550	2555	2559	rBV4	1324	2025	0.13%	0.013%
38	19.088	2581	2587	2589	rVB5	930	1609	0.10%	0.010%
39	19.158	2596	2599	2604	rVB3	1138	2123	0.14%	0.013%
40	19.317	2619	2626	2631	rVV5	1002	2539	0.16%	0.016%
41	19.481	2648	2654	2660	rVB6	1058	3019	0.19%	0.019%
42	19.851	2712	2717	2722	rVB	7475	11936	0.76%	0.076%
43	19.957	2730	2735	2740	rBV6	1408	3311	0.21%	0.021%
44	20.110	2754	2761	2768	rVB3	6898	11879	0.76%	0.075%
45	20.221	2772	2780	2793	rBV	1037524	1572161	100.00%	9.948%
46	20.386	2806	2808	2811	rVB3	1817	2048	0.13%	0.013%
47	20.409	2811	2812	2814	rBV2	2137	1644	0.10%	0.010%
48	20.498	2821	2827	2830	rBV4	1810	3315	0.21%	0.021%
49	20.609	2844	2846	2848	rBV3	1627	1650	0.10%	0.010%
50	20.762	2869	2872	2874	rBV3	1963	2036	0.13%	0.013%
51	20.791	2874	2877	2878	rBV3	2107	2056	0.13%	0.013%
52	21.009	2909	2914	2917	rBV6	2398	3845	0.24%	0.024%
53	21.197	2944	2946	2949	rBV4	2131	2233	0.14%	0.014%
54	21.326	2965	2968	2972	rBV4	2224	3236	0.21%	0.020%
55	21.355	2972	2973	2977	rVV4	1894	1730	0.11%	0.011%
56	21.473	2991	2993	2999	rBV5	1846	2270	0.14%	0.014%
57	21.684	3027	3029	3035	rBV7	2950	5058	0.32%	0.032%
58	21.778	3043	3045	3048	rBV4	2299	2169	0.14%	0.014%
59	22.231	3113	3122	3133	rBV	403061	764313	48.62%	4.836%
60	22.495	3165	3167	3171	rBV5	3080	3977	0.25%	0.025%
61	22.901	3233	3236	3238	rBV4	3386	3832	0.24%	0.024%
62	23.053	3259	3262	3263	rBV3	2934	2949	0.19%	0.019%
63	23.259	3295	3297	3299	rBV2	2652	2089	0.13%	0.013%
64	23.488	3333	3336	3338	rBV4	2744	3229	0.21%	0.020%
65	23.682	3367	3369	3373	rBV5	2345	3862	0.25%	0.024%
66	23.858	3394	3399	3405	rVB8	7020	14081	0.90%	0.089%
67	24.540	3513	3515	3518	rBV4	1905	2251	0.14%	0.014%
68	24.593	3522	3524	3529	rBV4	3318	4140	0.26%	0.026%
69	24.763	3547	3553	3565	rVB4	11290	29732	1.89%	0.188%
70	25.633	3688	3701	3718	rBV2	481669	1531459	97.41%	9.691%
71	25.885	3730	3744	3757	rVB2	210711	750485	47.74%	4.749%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
Data File : BG027524.D
Acq On : 19 Jun 2017 11:41
Operator : SJ/MA
Sample : PB99875BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Title : SVOA CALIBRATION

72	26.326	3817	3819	3822	rVB3	3261	3638	0.23%	0.023%
73	27.155	3953	3960	3970	rVB5	16404	45322	2.88%	0.287%
74	27.390	3998	4000	4004	rBV5	2427	2475	0.16%	0.016%
75	27.860	4079	4080	4084	rBV4	3590	3769	0.24%	0.024%
76	28.717	4216	4226	4237	rVB8	14695	53344	3.39%	0.338%
77	30.222	4479	4482	4485	rBV4	2871	3338	0.21%	0.021%
78	30.586	4533	4544	4555	rBV7	12044	53356	3.39%	0.338%
79	30.744	4567	4571	4577	rVB7	3514	4886	0.31%	0.031%
80	30.856	4587	4590	4591	rBV2	3486	3516	0.22%	0.022%
81	31.138	4636	4638	4641	rBV3	2529	2649	0.17%	0.017%
82	31.514	4700	4702	4705	rBV4	1895	1718	0.11%	0.011%
83	32.378	4846	4849	4850	rVB3	3234	2087	0.13%	0.013%


Sum of corrected areas: 15803212

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
Data File : BG027524.D
Acq On : 19 Jun 2017 11:41
Operator : SJ/MA
Sample : PB99875BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK75

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

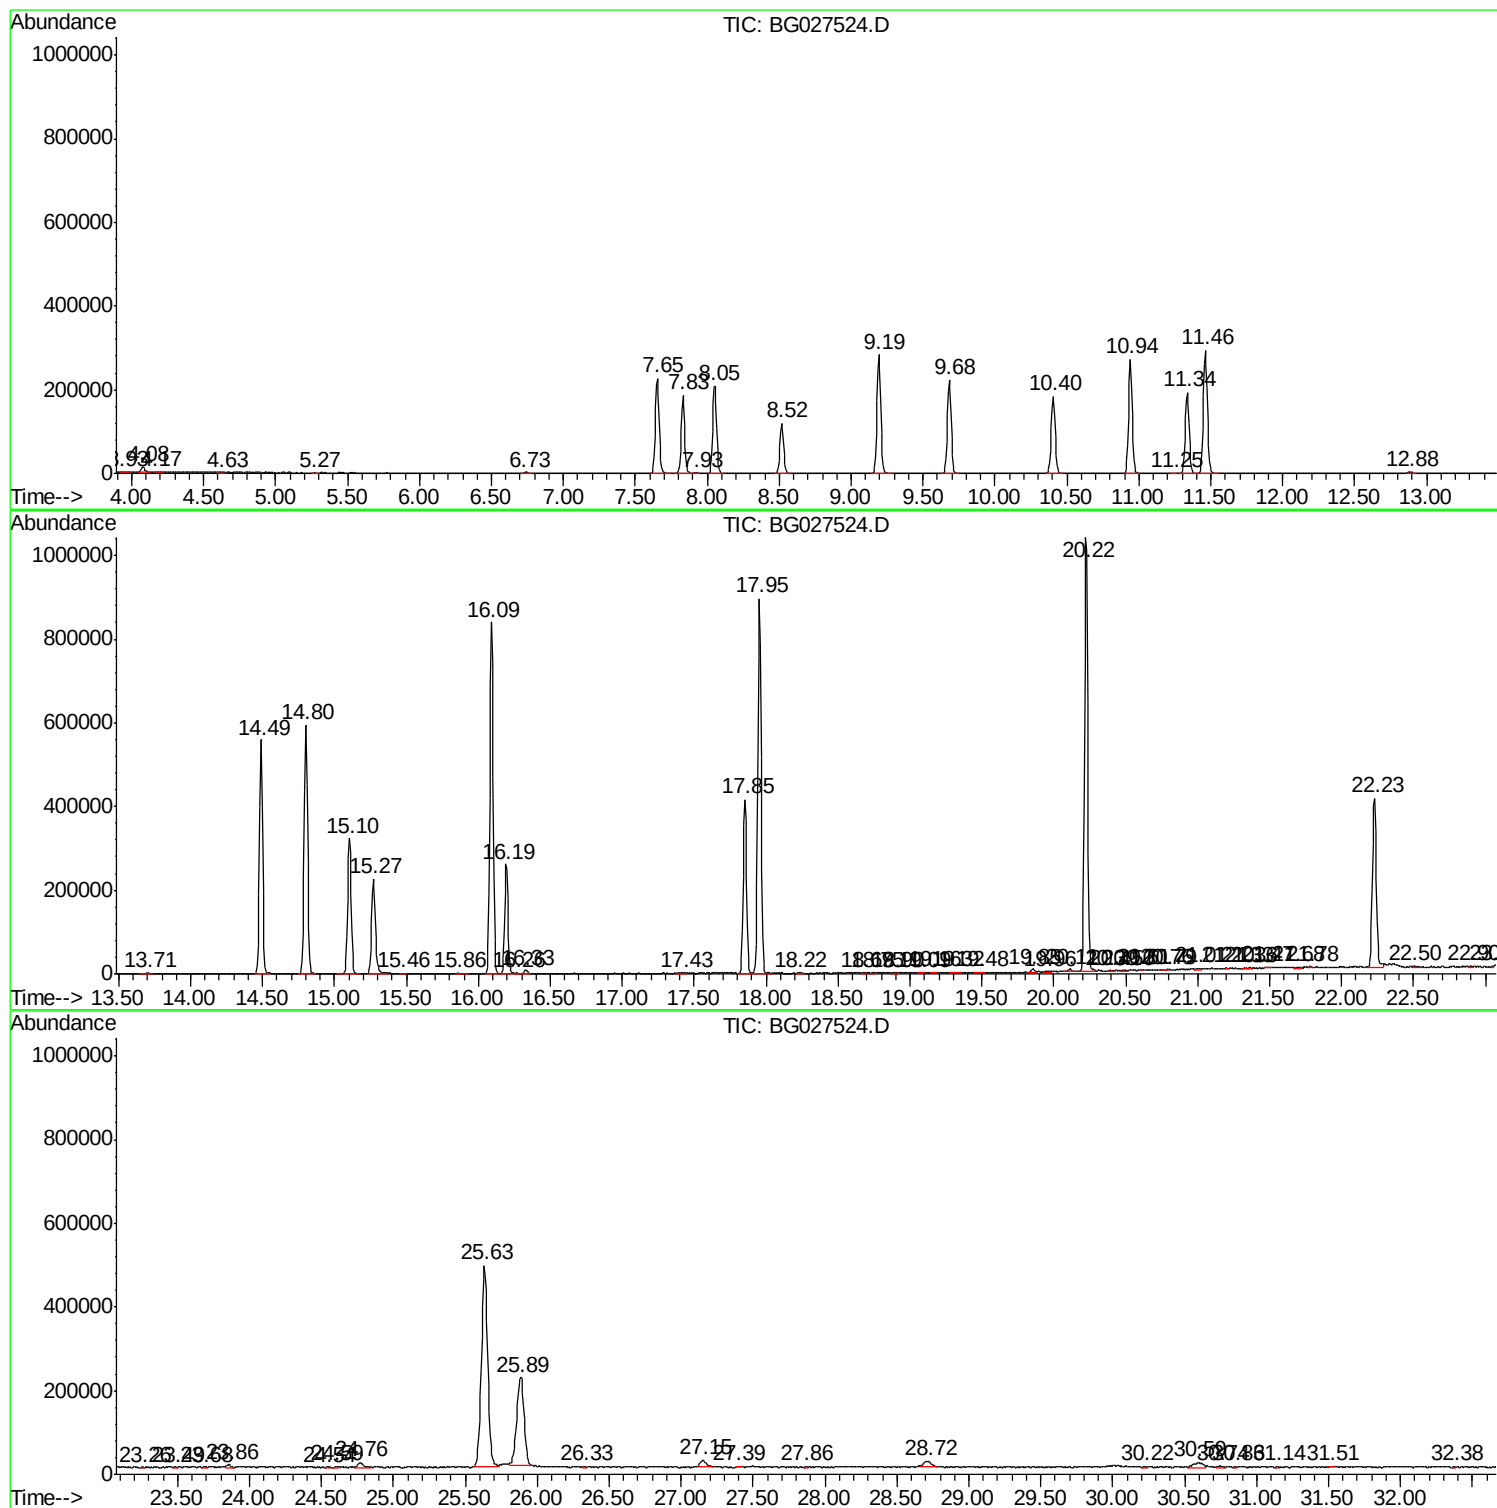

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061917\
Data File : BG027524.D
Acq On : 19 Jun 2017 11:41
Operator : SJ/MA
Sample : PB99875BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK75

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061917\
Data File : BG027524.D
Acq On : 19 Jun 2017 11:41
Operator : SJ/MA
Sample : PB99875BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK75

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc