

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
 Data File : BG027531.D
 Acq On : 19 Jun 2017 16:18
 Operator : SJ/MA
 Sample : I3658-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.076	23	32	34	rVV4	12641	30947	2.14%	0.228%
2	4.112	34	38	56	rVB	66484	114375	7.93%	0.843%
3	4.353	75	79	82	rVB4	1032	1446	0.10%	0.011%
4	5.510	272	276	280	rBV3	1382	2571	0.18%	0.019%
5	5.974	351	355	361	rBV5	1817	3854	0.27%	0.028%
6	7.655	634	641	652	rBV	41641	75561	5.24%	0.557%
7	7.831	663	671	683	rVB	138111	245185	16.99%	1.808%
8	8.048	700	708	717	rBV	135870	249433	17.29%	1.839%
9	8.160	722	727	732	rVB3	884	1707	0.12%	0.013%
10	8.518	780	788	800	rVB	126254	230205	15.96%	1.697%
11	9.194	894	903	915	rVV	123548	221755	15.37%	1.635%
12	9.682	976	986	1001	rVB	181146	338561	23.47%	2.496%
13	10.404	1098	1109	1120	rVB	150762	283229	19.63%	2.088%
14	10.945	1189	1201	1213	rBV	216665	415249	28.78%	3.062%
15	11.339	1260	1268	1277	rVB	212920	397956	27.58%	2.934%
16	11.462	1282	1289	1300	rBV3	11253	22565	1.56%	0.166%
17	12.884	1524	1531	1537	rBV4	3667	5667	0.39%	0.042%
18	13.454	1625	1628	1633	rBV5	1589	2645	0.18%	0.020%
19	13.724	1662	1674	1679	rBV7	2424	5977	0.41%	0.044%
20	14.488	1796	1804	1817	rBV	510801	753783	52.25%	5.557%
21	14.799	1848	1857	1868	rBV	512672	846571	58.68%	6.242%
22	15.105	1898	1909	1922	rBV2	365702	611963	42.42%	4.512%
23	15.275	1931	1938	1949	rBV2	39464	77765	5.39%	0.573%
24	15.481	1969	1973	1977	rBV2	1001	1783	0.12%	0.013%
25	15.863	2034	2038	2046	rBV4	1314	3071	0.21%	0.023%
26	16.039	2061	2068	2069	rBV3	2091	2451	0.17%	0.018%
27	16.092	2069	2077	2085	rVB	728550	1140177	79.03%	8.406%
28	16.192	2087	2094	2103	rVB	254424	394154	27.32%	2.906%
29	16.327	2111	2117	2123	rVB4	6551	9733	0.67%	0.072%
30	16.885	2206	2212	2219	rBV5	1127	2375	0.16%	0.018%
31	17.296	2277	2282	2284	rVB4	1173	1741	0.12%	0.013%
32	17.484	2308	2314	2315	rVB5	1227	1895	0.13%	0.014%
33	17.508	2315	2318	2323	rBV6	1132	1855	0.13%	0.014%
34	17.637	2337	2340	2346	rBV4	1808	2642	0.18%	0.019%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
 Data File : BG027531.D
 Acq On : 19 Jun 2017 16:18
 Operator : SJ/MA
 Sample : I3658-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

35	17.731	2350	2356	2359	rVB5	1567	3324	0.23%	0.025%
36	17.854	2368	2377	2386	rBV2	470670	753672	52.24%	5.557%
37	17.954	2386	2394	2407	rVB	797751	1272775	88.22%	9.384%
38	18.295	2449	2452	2457	rBV3	917	1447	0.10%	0.011%
39	18.389	2466	2468	2472	rVB2	1410	1758	0.12%	0.013%
40	18.424	2472	2474	2479	rBV4	1482	2044	0.14%	0.015%
41	18.471	2479	2482	2491	rVB5	1176	2608	0.18%	0.019%
42	18.695	2514	2520	2529	rBV6	7782	15791	1.09%	0.116%
43	18.771	2529	2533	2540	rVB4	2169	4623	0.32%	0.034%
44	18.853	2544	2547	2550	rBV4	1382	1628	0.11%	0.012%
45	19.071	2581	2584	2588	rVV5	1446	1987	0.14%	0.015%
46	19.182	2597	2603	2606	rBV4	1351	1988	0.14%	0.015%
47	19.223	2606	2610	2616	rVB4	1311	2364	0.16%	0.017%
48	19.470	2649	2652	2654	rBV4	2105	2194	0.15%	0.016%
49	19.505	2657	2658	2664	rBV3	1382	2573	0.18%	0.019%
50	19.823	2704	2712	2713	rBV6	2439	4148	0.29%	0.031%
51	19.858	2713	2718	2727	rVB3	7691	13514	0.94%	0.100%
52	19.946	2727	2733	2743	rBV4	13703	27189	1.88%	0.200%
53	20.087	2752	2757	2758	rBV3	5788	6926	0.48%	0.051%
54	20.111	2758	2761	2768	rVB3	7147	10298	0.71%	0.076%
55	20.169	2768	2771	2772	rBV2	1924	1635	0.11%	0.012%
56	20.222	2772	2780	2791	rVV	970598	1442769	100.00%	10.637%
57	20.328	2796	2798	2805	rVB8	1558	2385	0.17%	0.018%
58	20.422	2812	2814	2815	rBV2	2427	1708	0.12%	0.013%
59	20.498	2826	2827	2834	rVB7	1642	2580	0.18%	0.019%
60	20.763	2870	2872	2875	rBV4	1737	1837	0.13%	0.014%
61	20.798	2875	2878	2881	rBV5	2291	2927	0.20%	0.022%
62	21.309	2963	2965	2967	rVB3	2408	2088	0.14%	0.015%
63	21.691	3028	3030	3032	rVB3	3734	2595	0.18%	0.019%
64	21.785	3044	3046	3053	rBV8	3266	5537	0.38%	0.041%
65	22.226	3112	3121	3130	rBV	464533	876374	60.74%	6.461%
66	23.072	3262	3265	3268	rVB5	5707	5935	0.41%	0.044%
67	23.219	3288	3290	3294	rBV5	2956	3269	0.23%	0.024%
68	23.319	3306	3307	3309	rBV2	2997	2616	0.18%	0.019%
69	23.507	3336	3339	3342	rBV4	3302	4406	0.31%	0.032%
70	23.654	3361	3364	3365	rBV3	3286	2772	0.19%	0.020%
71	23.753	3380	3381	3383	rBV2	2619	2307	0.16%	0.017%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
 Data File : BG027531.D
 Acq On : 19 Jun 2017 16:18
 Operator : SJ/MA
 Sample : I3658-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

72	23.853	3391	3398	3405	rBV6	9379	20219	1.40%	0.149%
73	24.582	3520	3522	3525	rBV4	2219	3408	0.24%	0.025%
74	24.770	3547	3554	3560	rBV6	11935	31103	2.16%	0.229%
75	25.628	3686	3700	3715	rBV2	413718	1414234	98.02%	10.427%
76	25.880	3729	3743	3766	rVB4	252107	919210	63.71%	6.777%
77	27.149	3949	3959	3971	rBV6	16439	55961	3.88%	0.413%
78	27.467	4011	4013	4018	rVB6	2781	4468	0.31%	0.033%
79	28.007	4103	4105	4107	rBV3	2371	2367	0.16%	0.017%
80	28.054	4112	4113	4117	rVB4	1940	1835	0.13%	0.014%
81	28.706	4215	4224	4234	rBV5	13429	45735	3.17%	0.337%
82	29.793	4406	4409	4410	rBV3	2359	2138	0.15%	0.016%
83	29.981	4438	4441	4444	rBV5	1926	2488	0.17%	0.018%
84	30.234	4482	4484	4488	rVB4	1853	1865	0.13%	0.014%
85	30.581	4537	4543	4558	rVB10	12904	46817	3.24%	0.345%
86	31.744	4739	4741	4746	rBV6	1884	3959	0.27%	0.029%
87	31.791	4747	4749	4754	rVB6	3832	5496	0.38%	0.041%
88	31.832	4754	4756	4758	rBV3	2710	2859	0.20%	0.021%
89	32.443	4859	4860	4863	rVB3	2204	1924	0.13%	0.014%


Sum of corrected areas: 13563524

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
Data File : BG027531.D
Acq On : 19 Jun 2017 16:18
Operator : SJ/MA
Sample : I3658-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC83

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

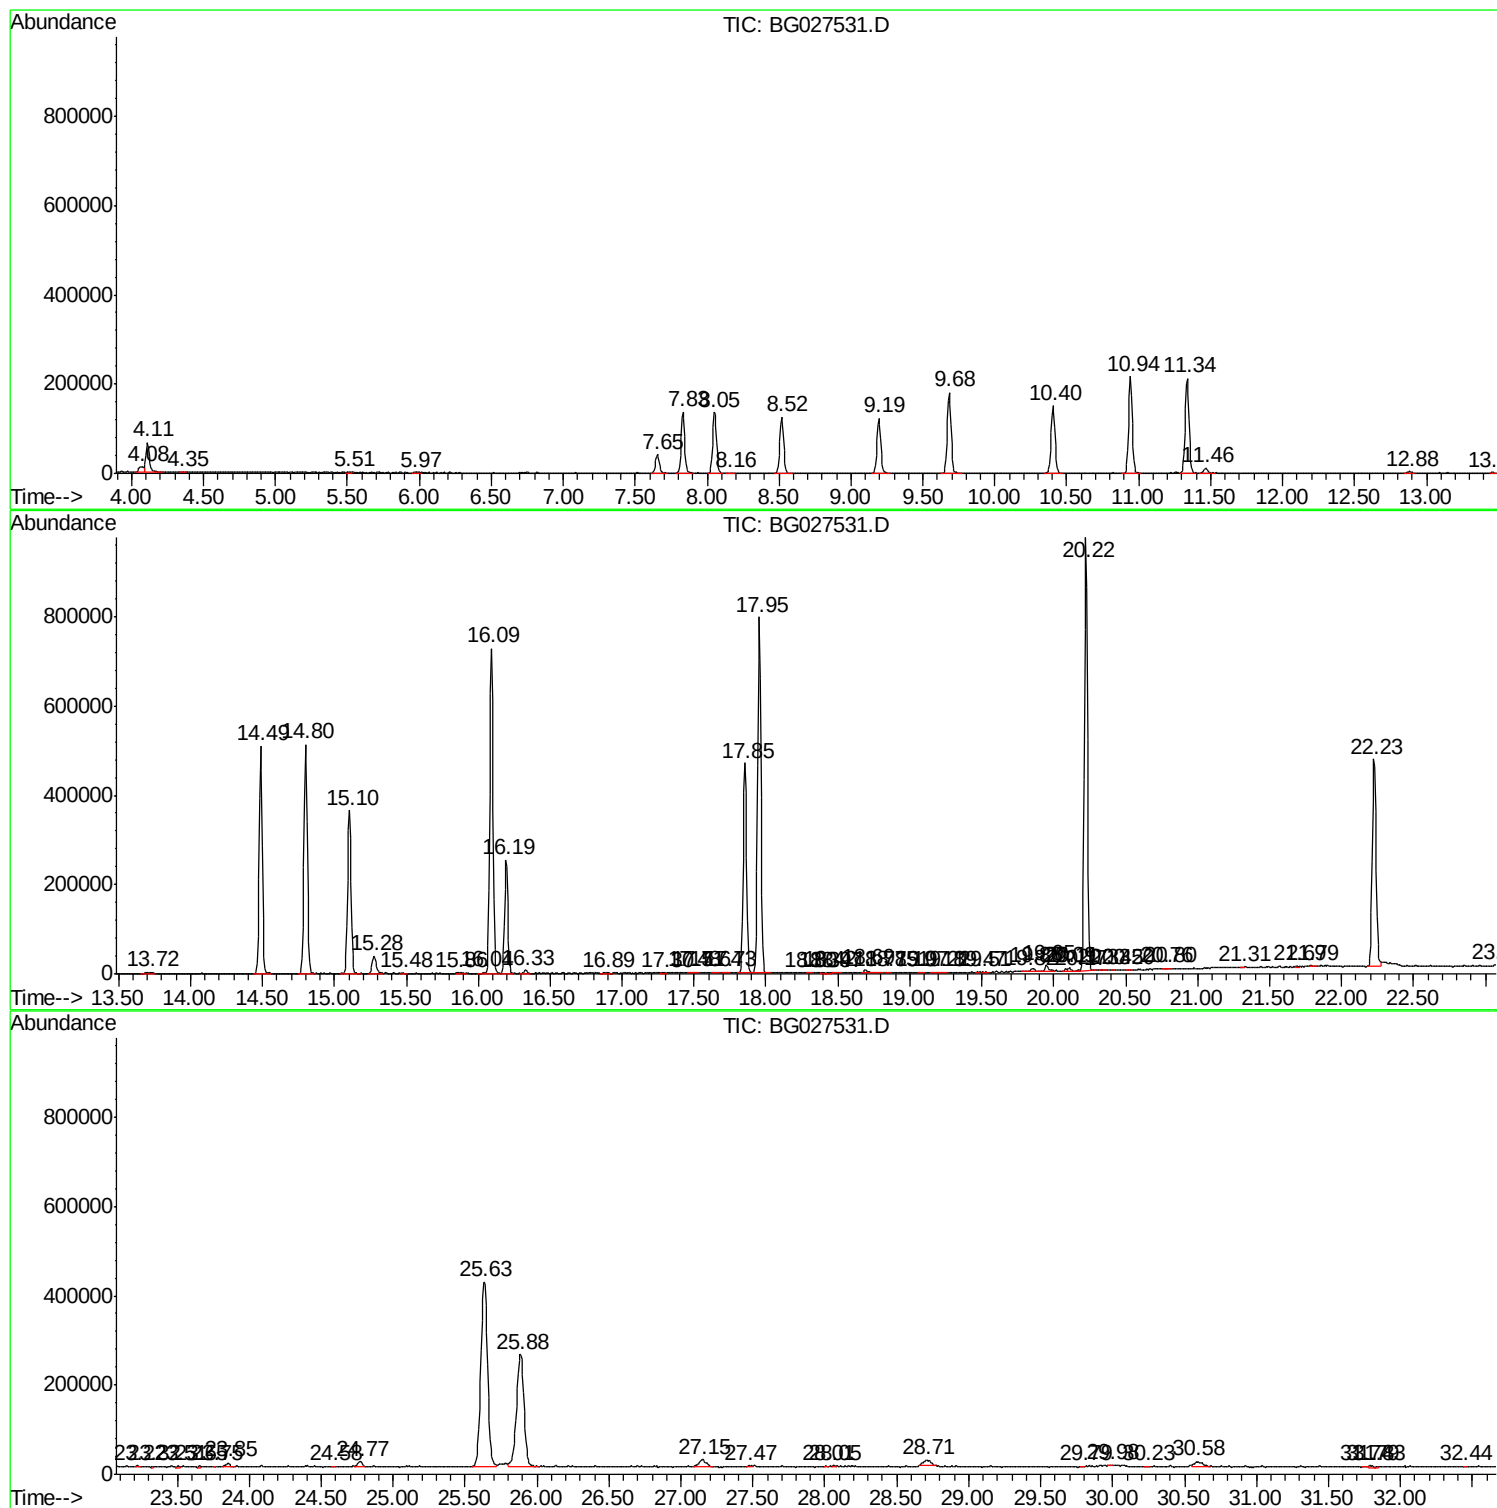

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061917\
Data File : BG027531.D
Acq On : 19 Jun 2017 16:18
Operator : SJ/MA
Sample : I3658-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC83

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061917\
Data File : BG027531.D
Acq On : 19 Jun 2017 16:18
Operator : SJ/MA
Sample : I3658-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC83

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc