

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
 Data File : BG027533.D
 Acq On : 19 Jun 2017 17:37
 Operator : SJ/MA
 Sample : I3658-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC84

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.076	24	32	45	rVB6	10146	25153	1.60%	0.174%
2	5.662	299	302	311	rVB4	1486	3041	0.19%	0.021%
3	6.362	420	421	429	rBV4	1026	2383	0.15%	0.016%
4	6.738	478	485	490	rBV3	1570	2532	0.16%	0.017%
5	7.654	633	641	651	rVB	50173	90764	5.77%	0.626%
6	7.831	664	671	685	rBV	163190	278308	17.70%	1.920%
7	8.048	699	708	723	rVB	156617	293688	18.67%	2.026%
8	8.518	778	788	799	rVB	130745	236383	15.03%	1.631%
9	9.194	894	903	914	rVB2	145470	256502	16.31%	1.769%
10	9.681	976	986	999	rBV	200192	381430	24.25%	2.631%
11	10.404	1100	1109	1121	rVB	169772	322968	20.54%	2.228%
12	10.945	1190	1201	1211	rBV	252208	473868	30.13%	3.269%
13	11.338	1258	1268	1279	rVB	214664	406616	25.85%	2.805%
14	11.467	1282	1290	1300	rBV2	12866	26298	1.67%	0.181%
15	11.685	1318	1327	1328	rBV3	984	1833	0.12%	0.013%
16	12.883	1523	1531	1537	rBV2	4048	7256	0.46%	0.050%
17	13.465	1623	1630	1635	rVB3	1602	2437	0.15%	0.017%
18	13.547	1637	1644	1647	rBV3	848	1757	0.11%	0.012%
19	13.700	1664	1670	1671	rBV3	1980	2524	0.16%	0.017%
20	13.730	1671	1675	1679	rVB3	2814	4485	0.29%	0.031%
21	14.252	1754	1764	1765	rVB3	825	2035	0.13%	0.014%
22	14.335	1769	1778	1779	rBV2	744	1930	0.12%	0.013%
23	14.487	1792	1804	1812	rBV	532373	832987	52.97%	5.746%
24	14.546	1812	1814	1820	rVB2	1161	1727	0.11%	0.012%
25	14.799	1845	1857	1867	rBV	555014	936450	59.54%	6.460%
26	14.987	1886	1889	1894	rVB2	1093	1649	0.10%	0.011%
27	15.104	1900	1909	1921	rBV2	370218	621125	39.49%	4.285%
28	15.275	1929	1938	1948	rBV	44065	84696	5.39%	0.584%
29	15.856	2034	2037	2041	rBV3	1091	1649	0.10%	0.011%
30	16.091	2067	2077	2088	rBV	800845	1256611	79.90%	8.668%
31	16.191	2088	2094	2107	rVB	219823	335056	21.30%	2.311%
32	16.332	2109	2118	2123	rBV2	7484	11899	0.76%	0.082%
33	16.450	2131	2138	2140	rBV3	1089	1749	0.11%	0.012%
34	17.043	2235	2239	2244	rVB4	889	1749	0.11%	0.012%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
 Data File : BG027533.D
 Acq On : 19 Jun 2017 17:37
 Operator : SJ/MA
 Sample : I3658-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC84

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

35	17.214	2263	2268	2270	rBV3	1517	2640	0.17%	0.018%
36	17.349	2289	2291	2296	rBV3	1359	1866	0.12%	0.013%
37	17.408	2296	2301	2303	rBV4	1586	2567	0.16%	0.018%
38	17.560	2324	2327	2332	rBV4	1042	2053	0.13%	0.014%
39	17.643	2335	2341	2347	rVB3	1734	2484	0.16%	0.017%
40	17.713	2347	2353	2361	rVB6	1701	4416	0.28%	0.030%
41	17.854	2369	2377	2385	rBV	485960	753790	47.93%	5.200%
42	17.954	2385	2394	2409	rVB	845718	1362935	86.66%	9.401%
43	18.230	2436	2441	2446	rVB5	1113	1759	0.11%	0.012%
44	18.688	2513	2519	2530	rBV6	4798	12259	0.78%	0.085%
45	18.782	2530	2535	2540	rVB8	1656	3697	0.24%	0.026%
46	19.035	2573	2578	2581	rBV5	995	1785	0.11%	0.012%
47	19.170	2595	2601	2606	rBV6	1997	4959	0.32%	0.034%
48	19.211	2606	2608	2614	rVB6	2207	3198	0.20%	0.022%
49	19.264	2614	2617	2621	rBV4	936	1725	0.11%	0.012%
50	19.323	2621	2627	2629	rBV5	1820	2109	0.13%	0.015%
51	19.611	2671	2676	2683	rBV6	1501	3809	0.24%	0.026%
52	19.852	2711	2717	2729	rVB	9169	16837	1.07%	0.116%
53	19.946	2729	2733	2744	rBV10	7949	19684	1.25%	0.136%
54	20.110	2752	2761	2768	rBV3	7388	17538	1.12%	0.121%
55	20.222	2770	2780	2790	rBV	1041987	1572690	100.00%	10.848%
56	20.363	2803	2804	2806	rBV2	2317	1874	0.12%	0.013%
57	20.381	2806	2807	2810	rVV3	2053	1841	0.12%	0.013%
58	20.428	2812	2815	2818	rVB4	2268	2741	0.17%	0.019%
59	20.663	2854	2855	2865	rBV8	2884	4725	0.30%	0.033%
60	20.798	2877	2878	2882	rBV4	1856	1681	0.11%	0.012%
61	20.950	2903	2904	2909	rBV5	2290	3842	0.24%	0.027%
62	21.250	2954	2955	2958	rVB3	3021	2429	0.15%	0.017%
63	21.421	2983	2984	2991	rBV7	2605	5112	0.33%	0.035%
64	21.714	3033	3034	3037	rVB3	2713	2332	0.15%	0.016%
65	22.061	3090	3093	3099	rVB6	3008	4496	0.29%	0.031%
66	22.225	3112	3121	3131	rBV	469315	891008	56.66%	6.146%
67	22.842	3224	3226	3229	rBV4	1588	1842	0.12%	0.013%
68	23.060	3261	3263	3271	rVB8	5031	7993	0.51%	0.055%
69	23.301	3303	3304	3307	rBV3	2739	2610	0.17%	0.018%
70	23.477	3332	3334	3336	rBV2	2901	2227	0.14%	0.015%
71	23.788	3386	3387	3391	rBV2	2884	3237	0.21%	0.022%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
 Data File : BG027533.D
 Acq On : 19 Jun 2017 17:37
 Operator : SJ/MA
 Sample : I3658-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC84

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

72	23.847	3391	3397	3406	rVV5	11804	27882	1.77%	0.192%
73	24.029	3426	3428	3429	rBV2	2418	1940	0.12%	0.013%
74	24.170	3449	3452	3453	rBV3	2433	1939	0.12%	0.013%
75	24.546	3515	3516	3521	rBV5	2423	3825	0.24%	0.026%
76	24.699	3540	3542	3544	rVB3	3474	2618	0.17%	0.018%
77	24.770	3547	3554	3562	rBV4	15629	36057	2.29%	0.249%
78	25.633	3686	3701	3718	rBV3	474664	1553922	98.81%	10.719%
79	25.886	3730	3744	3767	rVV2	252844	926065	58.88%	6.388%
80	26.033	3767	3769	3773	rVB5	3996	5679	0.36%	0.039%
81	26.174	3791	3793	3802	rVB8	2974	4970	0.32%	0.034%
82	26.374	3824	3827	3832	rBV6	2280	2549	0.16%	0.018%
83	27.020	3935	3937	3940	rBV4	2074	1952	0.12%	0.013%
84	27.143	3950	3958	3968	rVB5	23281	71205	4.53%	0.491%
85	27.484	4011	4016	4019	rBV5	2287	4385	0.28%	0.030%
86	27.948	4092	4095	4099	rBV6	2857	3447	0.22%	0.024%
87	28.324	4158	4159	4162	rBV3	1902	1648	0.10%	0.011%
88	28.406	4172	4173	4178	rBV4	3201	4769	0.30%	0.033%
89	28.706	4213	4224	4238	rVB4	23443	86933	5.53%	0.600%
90	29.194	4306	4307	4310	rVB3	3890	2845	0.18%	0.020%
91	29.217	4310	4311	4315	rBV3	3160	3300	0.21%	0.023%
92	29.423	4344	4346	4349	rVB3	2634	2770	0.18%	0.019%
93	29.711	4391	4395	4400	rBV6	3721	7282	0.46%	0.050%
94	29.846	4416	4418	4421	rVB5	3681	3881	0.25%	0.027%
95	30.234	4480	4484	4488	rBV5	2318	3779	0.24%	0.026%
96	30.580	4532	4543	4559	rVB7	16613	73126	4.65%	0.504%
97	31.238	4653	4655	4657	rVB3	3066	1722	0.11%	0.012%
98	31.885	4763	4765	4767	rBV3	3157	2996	0.19%	0.021%
99	32.243	4824	4826	4832	rBV6	3522	4951	0.31%	0.034%
100	32.549	4876	4878	4880	rBV3	3142	2234	0.14%	0.015%


Sum of corrected areas: 14496999

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061917\
Data File : BG027533.D
Acq On : 19 Jun 2017 17:37
Operator : SJ/MA
Sample : I3658-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC84

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

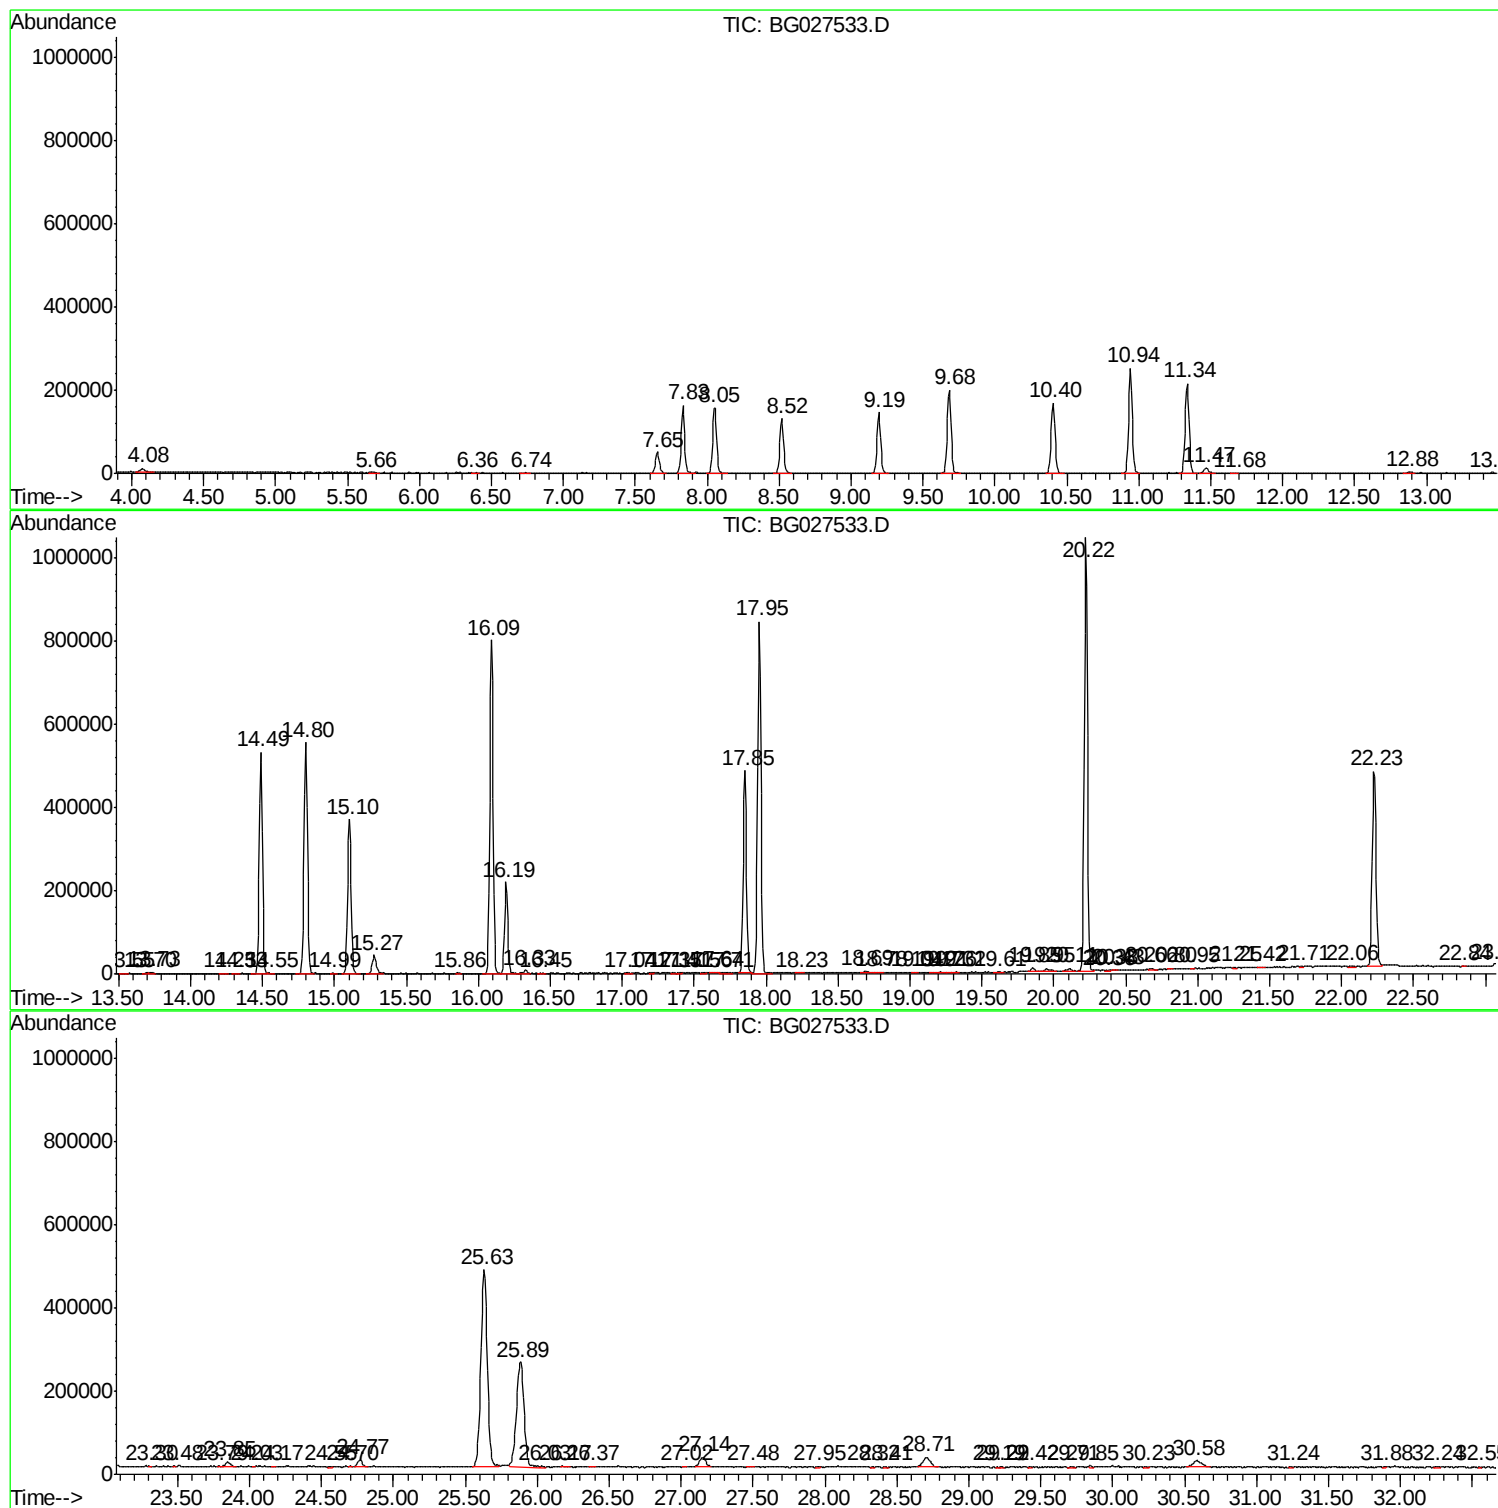

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061917\
Data File : BG027533.D
Acq On : 19 Jun 2017 17:37
Operator : SJ/MA
Sample : I3658-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC84

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061917\
Data File : BG027533.D
Acq On : 19 Jun 2017 17:37
Operator : SJ/MA
Sample : I3658-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC84

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc