
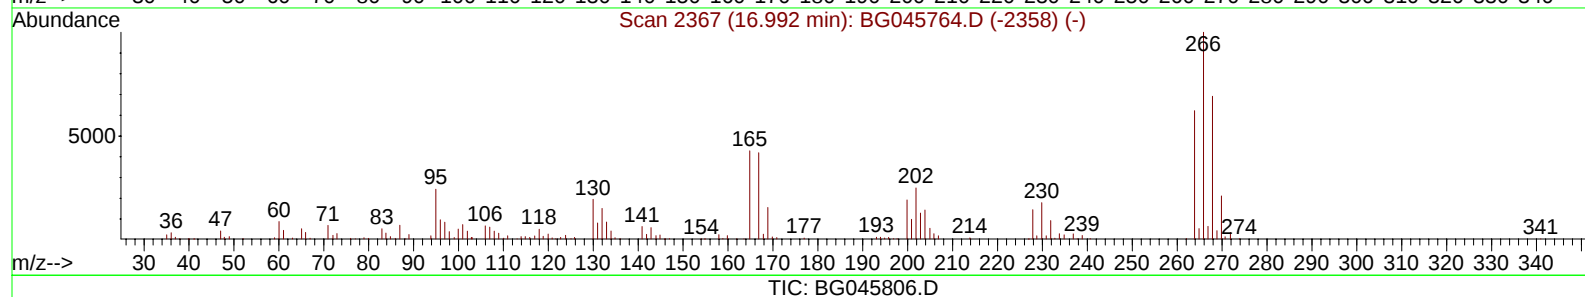
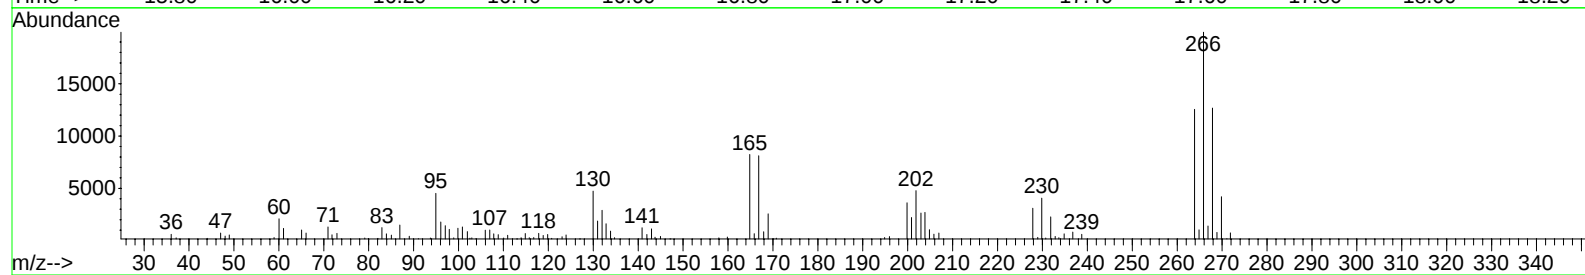


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061920\
Data File : BG045806.D
Acq On : 19 Jun 2020 8:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 18:27:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 18:34:19 2020
Response via : Initial Calibration

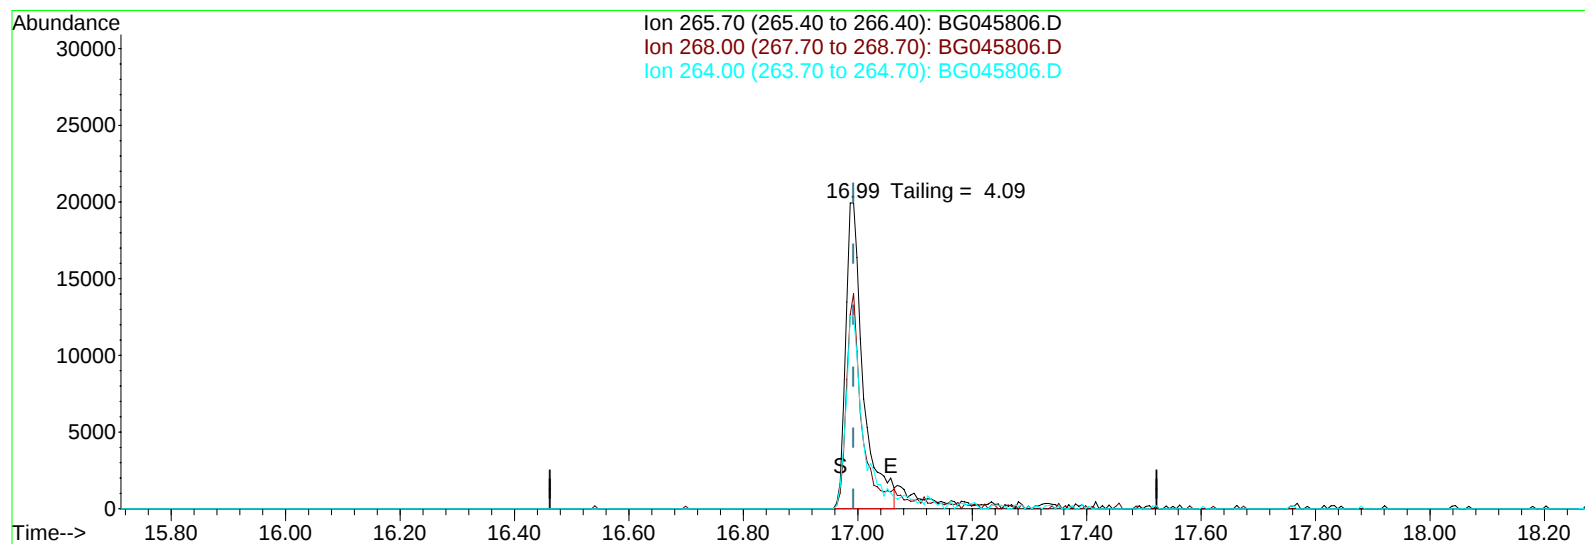

(70) Pentachlorophenol (C)




16.987min (-0.005) 64497.63ng

response 45478

Ion	Exp%	Act%
265.70	100	100
268.00	69.20	63.58
264.00	62.20	63.01
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061920\
 Data File : BG045806.D
 Acq On : 19 Jun 2020 8:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 18:27:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 18:34:19 2020
 Response via : Initial Calibration

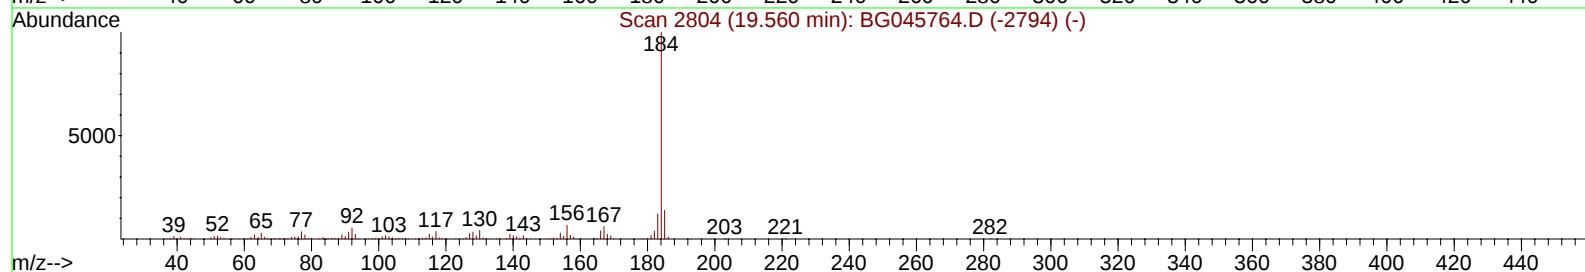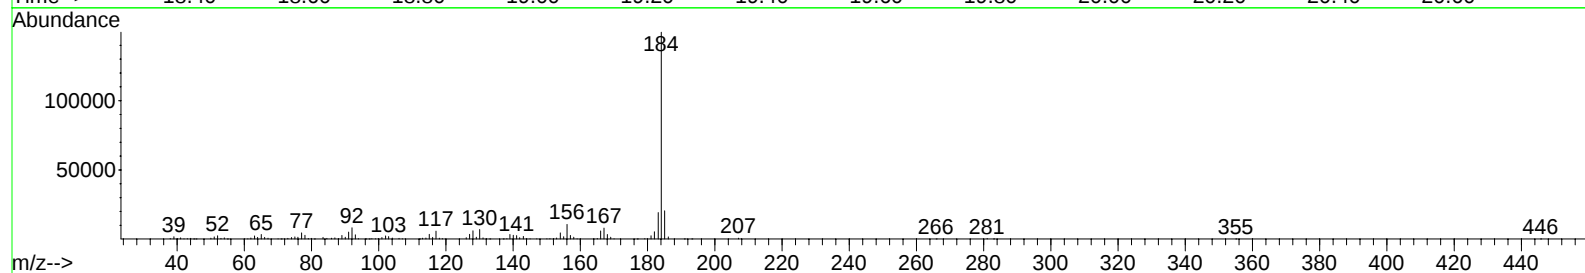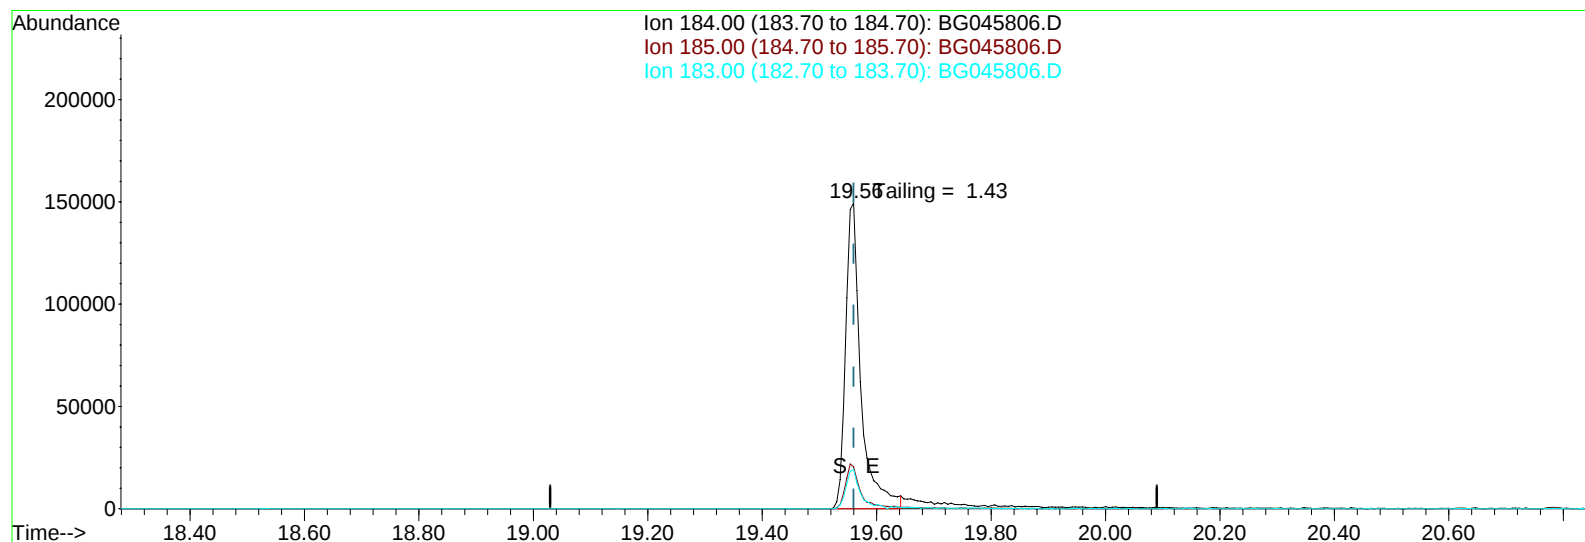

TIC: BG045806.D

(77) Benzidine

19.560min (+0.000) 193861.80ng

response 292310

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.69
183.00	12.10	12.86
0.00	0.00	0.00