


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061920\
 Data File : BG045806.D
 Acq On : 19 Jun 2020 8:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 15 18:34:19 2020

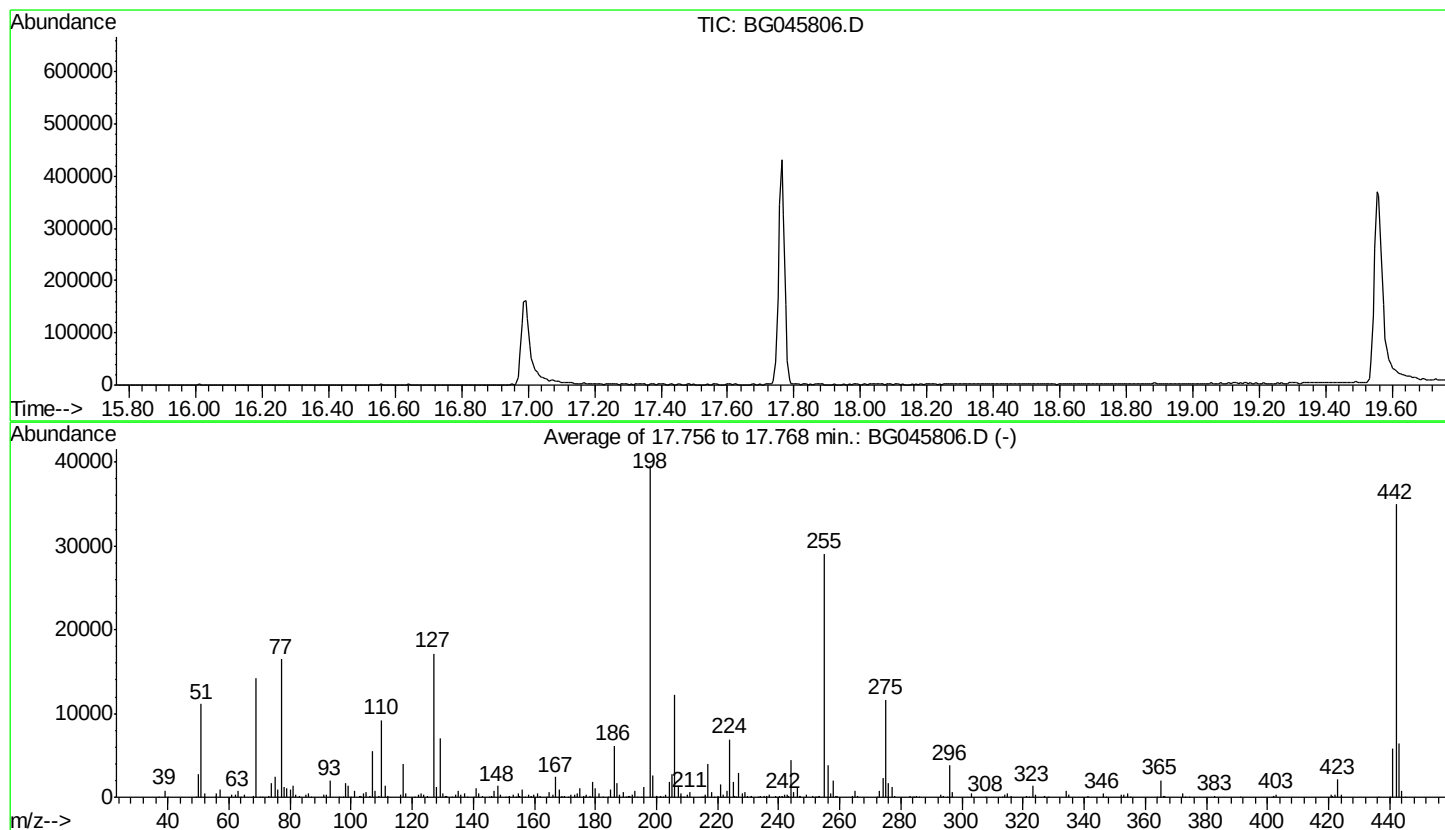

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	11105	PASS
68	69	0.00	2	1.4	195	PASS
69	198	0.00	100	35.8	14163	PASS
70	69	0.00	2	0.5	73	PASS
127	198	10	80	43.4	17165	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39589	PASS
199	198	5	9	6.4	2549	PASS
275	198	10	60	29.4	11648	PASS
365	198	1	100	5.2	2045	PASS
441	198	0.01	100	14.8	5846	PASS
442	198	50	100	88.2	34933	PASS
443	442	15	24	18.6	6491	PASS