

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062016\
 Data File : BG022463.D
 Acq On : 21 Jun 2016 5:41
 Operator : UM/SJ
 Sample : H3602-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P8-B5(0-16)G

Quant Time: Jun 21 06:54:01 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 21 03:17:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	25306	20.00	ng	0.00
21) Naphthalene-d8	10.81	136	123441	20.00	ng	0.00
38) Acenaphthene-d10	14.63	164	78348	20.00	ng	0.00
63) Phenanthrene-d10	17.38	188	171454	20.00	ng	0.00
75) Chrysene-d12	21.64	240	135748	20.00	ng	0.00
86) Perylene-d12	24.84	264	119637	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	98196	75.02	ng	0.00
7) Phenol-d6	7.18	99	91542	44.48	ng	0.00
23) Nitrobenzene-d5	9.16	82	168773	95.32	ng	0.00
41) 2,4,6-Tribromophenol	16.13	330	94833	107.12	ng	0.00
44) 2-Fluorobiphenyl	13.25	172	474332	92.26	ng	0.00
78) Terphenyl-d14	19.98	244	545472	95.40	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062016\
Data File : BG022463.D
Acq On : 21 Jun 2016 5:41
Operator : UM/SJ
Sample : H3602-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P8-B5(0-16)G

Quant Time: Jun 21 06:54:01 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 21 03:17:27 2016
Response via : Initial Calibration

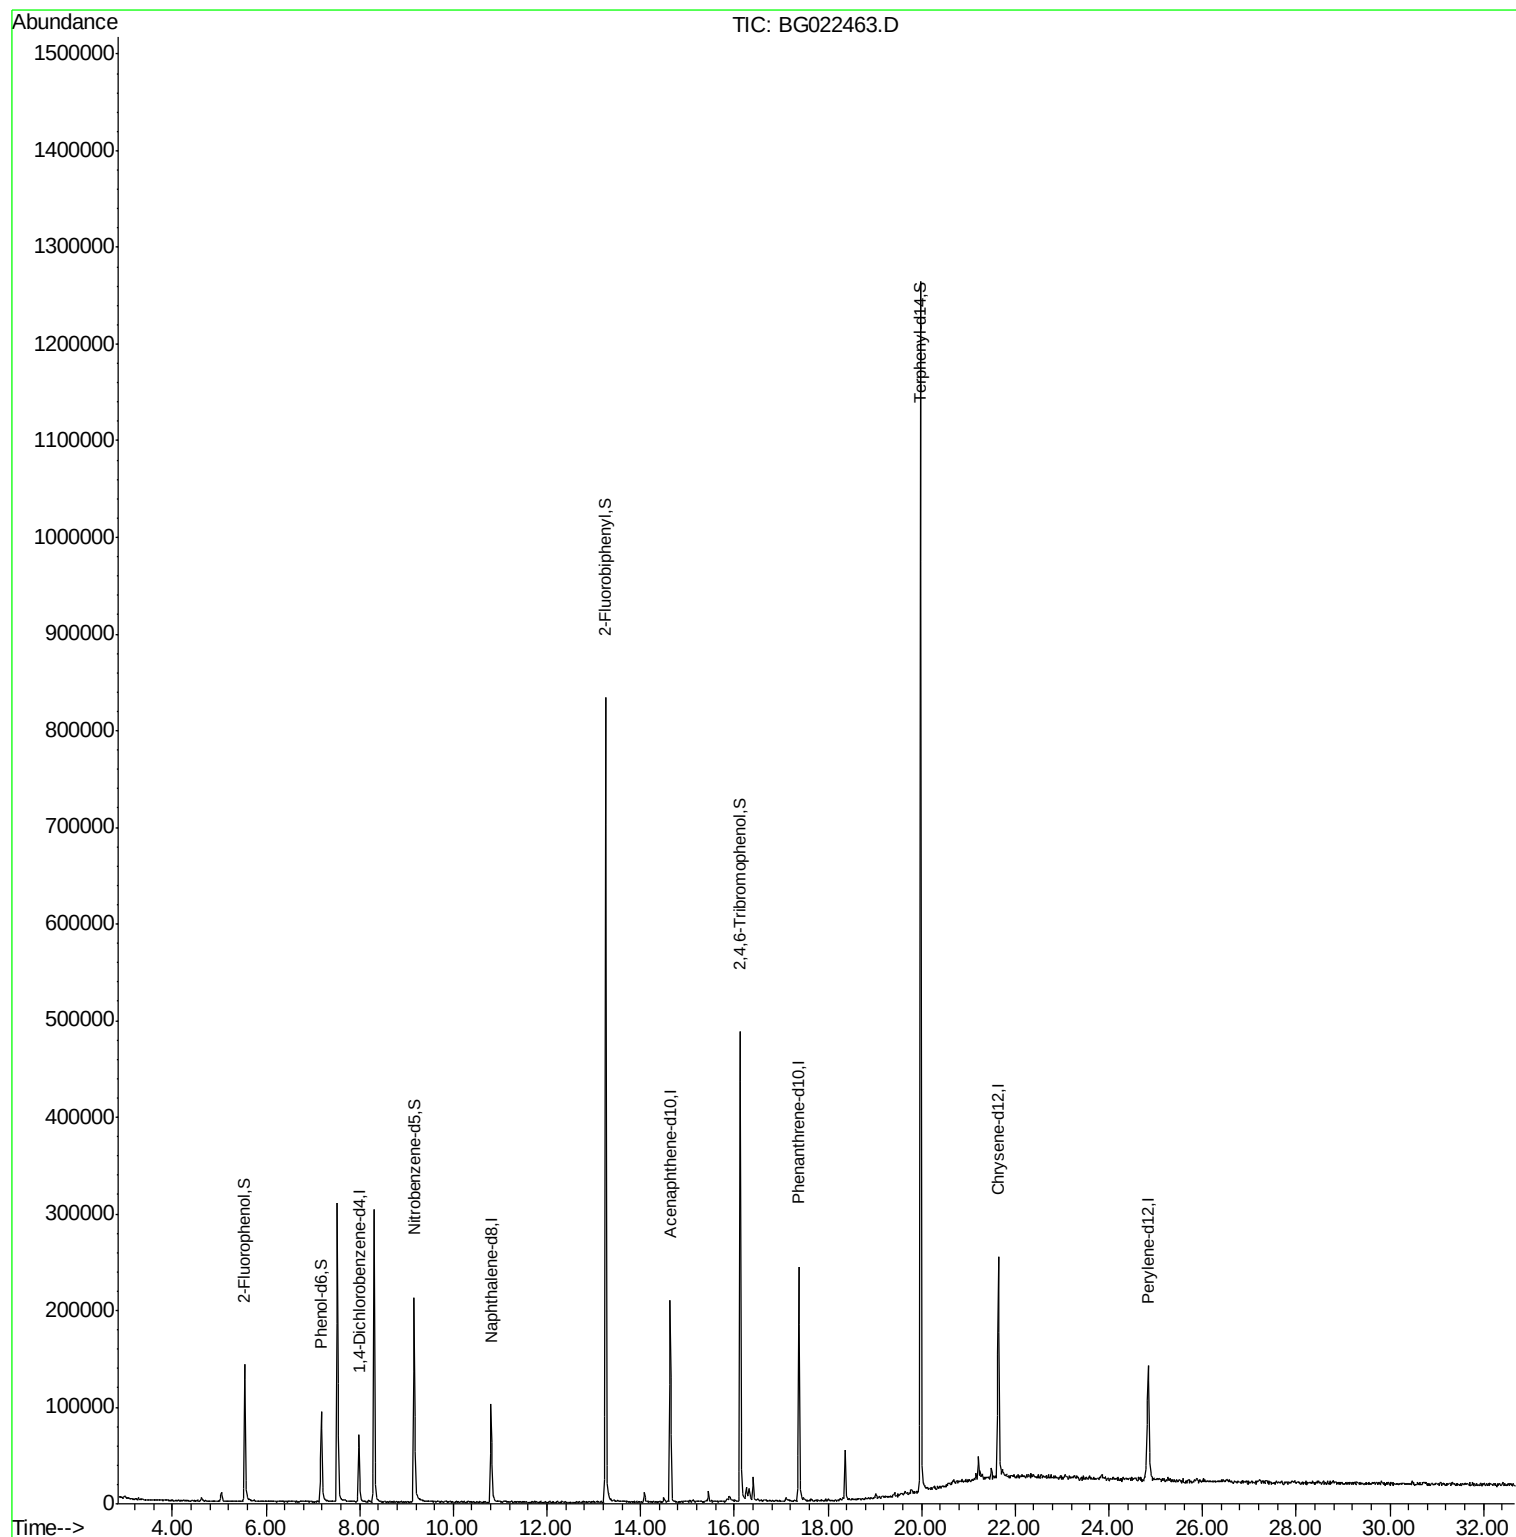

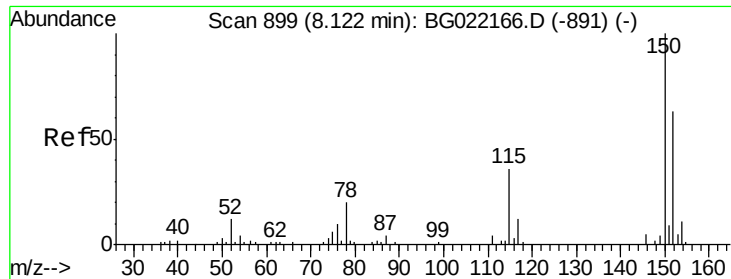


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.99 min Scan# 877
 Delta R.T. 0.00 min
 Lab File: BG022463.D
 Acq: 21 Jun 2016 5:41

Instrument :
 BNA_G
 ClientSampleId :
 P8-B5(0-16)G

Tgt Ion:152 Resp: 25306
 Ion Ratio Lower Upper
 152 100
 150 136.2 130.1 195.1
 115 55.9 62.2 93.2#

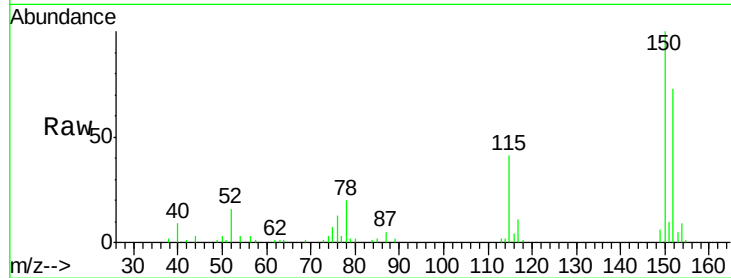


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

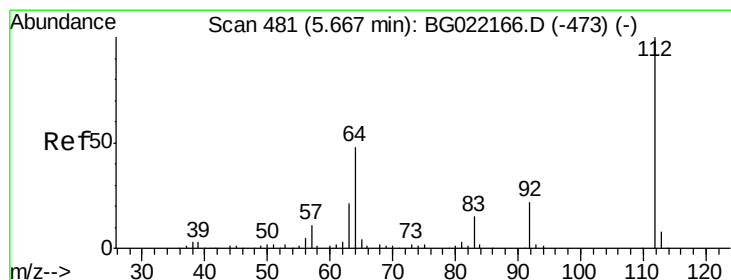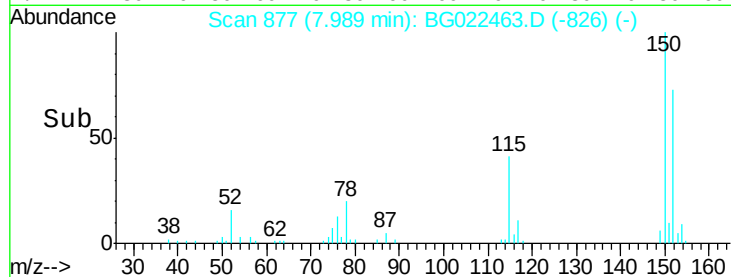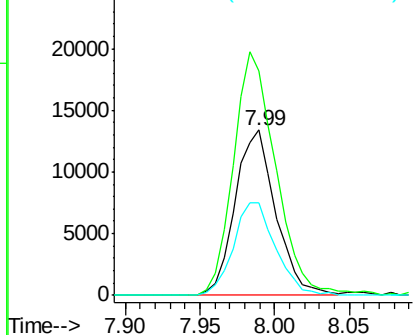



#5


2-Fluorophenol
 Concen: 75.02 ng
 RT: 5.55 min Scan# 461
 Delta R.T. 0.00 min
 Lab File: BG022463.D
 Acq: 21 Jun 2016 5:41

Tgt Ion:112 Resp: 98196
 Ion Ratio Lower Upper
 112 100
 64 48.8 51.1 76.7#
 63 22.9 24.6 37.0#

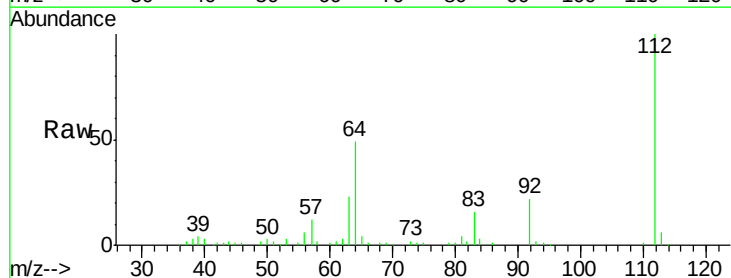

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

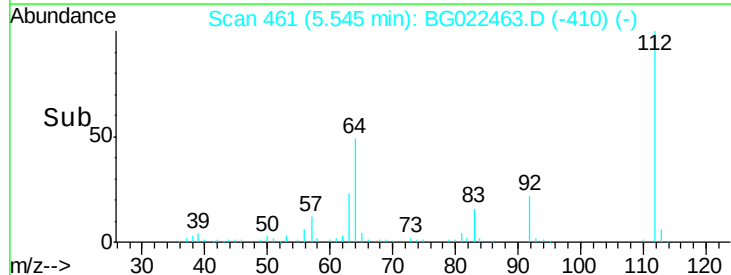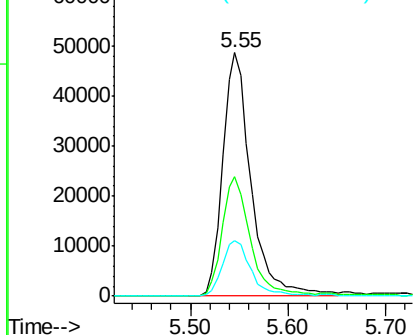

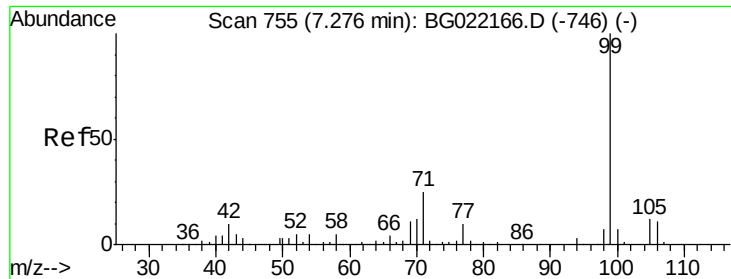

#7

Phenol-d6

Concen: 44.48 ng

RT: 7.18 min Scan# 739

Delta R.T. 0.00 min

Lab File: BG022463.D

Acq: 21 Jun 2016 5:41

Instrument :

BNA_G

ClientSampleId :

P8-B5(0-16)G


Tgt Ion: 99 Resp: 91542

Ion Ratio Lower Upper




99 100

42 10.8 16.4 24.6#

71 26.3 25.0 37.4

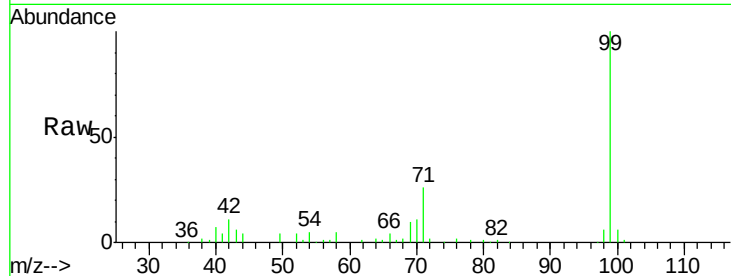

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

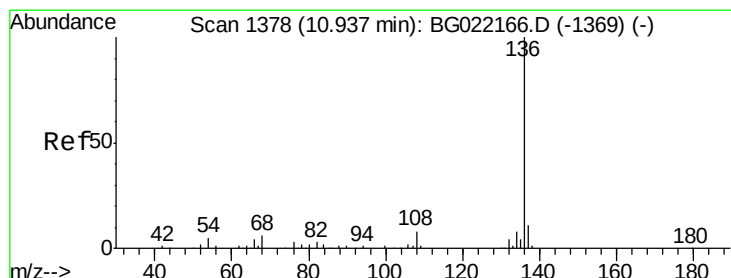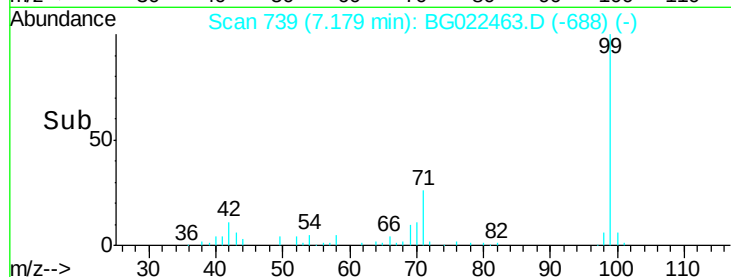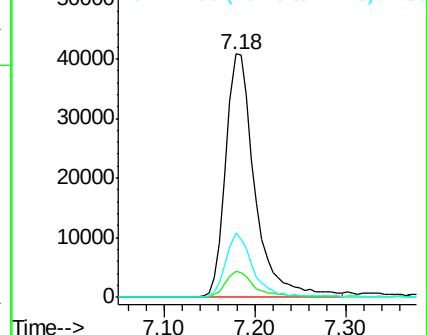

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.81 min Scan# 1357

Delta R.T. 0.00 min

Lab File: BG022463.D

Acq: 21 Jun 2016 5:41

Tgt Ion: 136 Resp: 123441


Ion Ratio Lower Upper

136 100



137 9.4 9.0 13.4


54 6.5 9.6 14.4#

68 5.2 6.4 9.6#

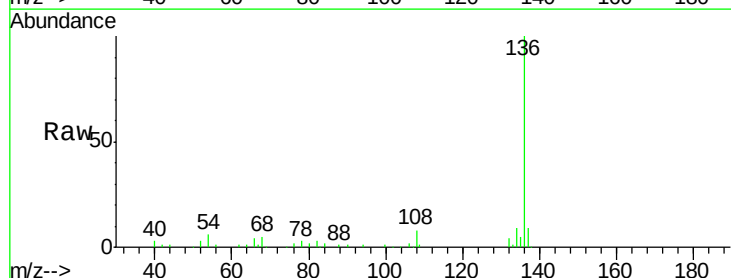

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



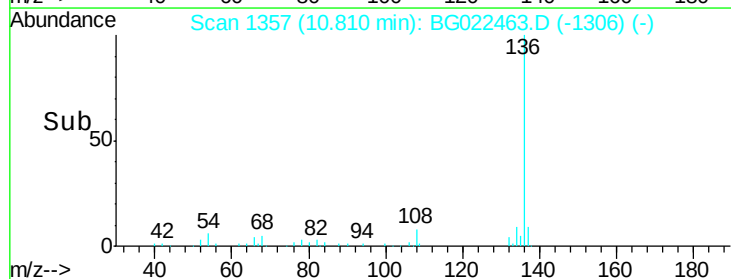
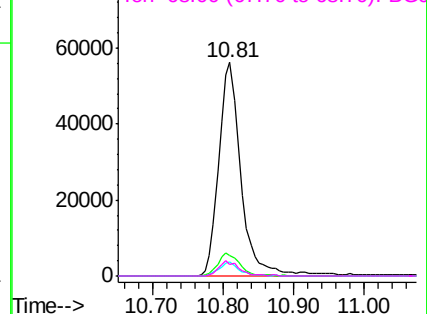


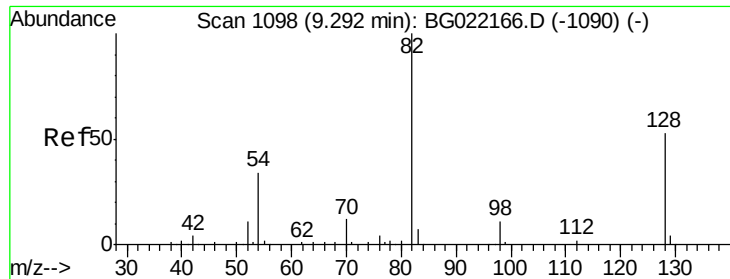

#23
 Nitrobenzene-d5
 Concen: 95.32 ng
 RT: 9.16 min Scan# 1077
 Delta R.T. -0.00 min
 Lab File: BG022463.D
 Acq: 21 Jun 2016 5:41




Instrument :
 BNA_G
 ClientSampleId :
 P8-B5(0-16)G


Tgt Ion: 82 Resp: 168773
 Ion Ratio Lower Upper
 82 100
 128 51.2 33.4 50.0#
 54 35.6 46.1 69.1#

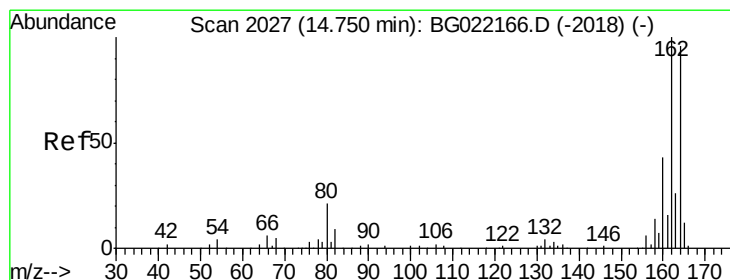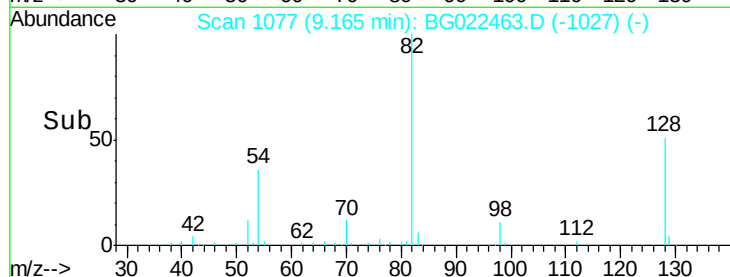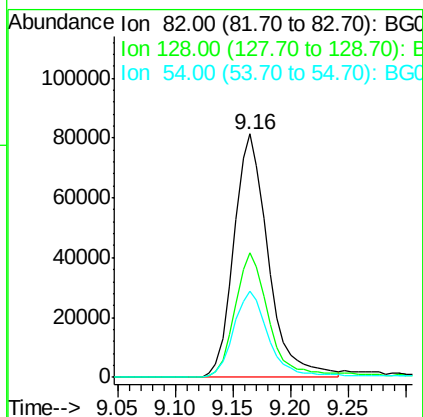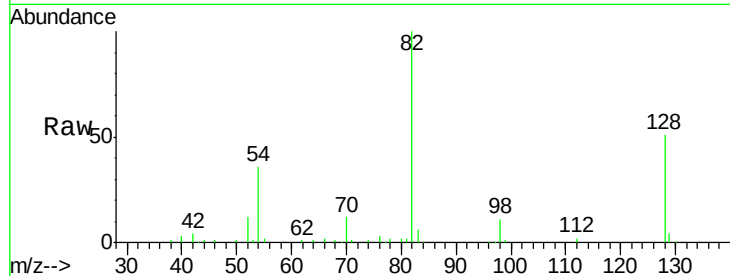

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.63 min Scan# 2008
 Delta R.T. -0.00 min
 Lab File: BG022463.D
 Acq: 21 Jun 2016 5:41

Tgt Ion: 164 Resp: 78348
 Ion Ratio Lower Upper
 164 100
 162 113.7 78.0 117.0
 160 49.7 32.9 49.3#

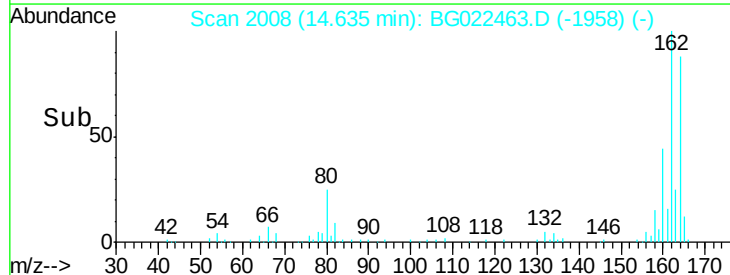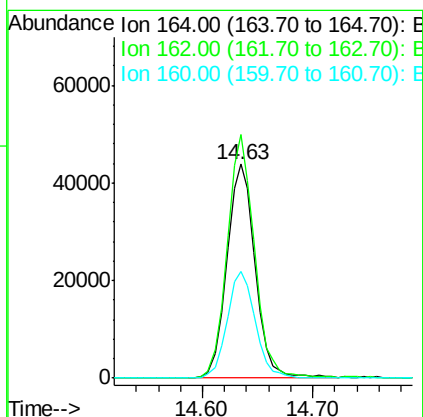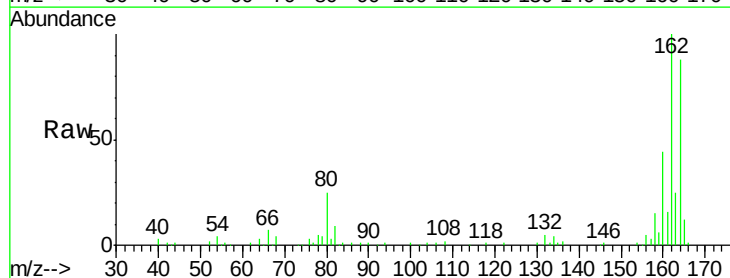


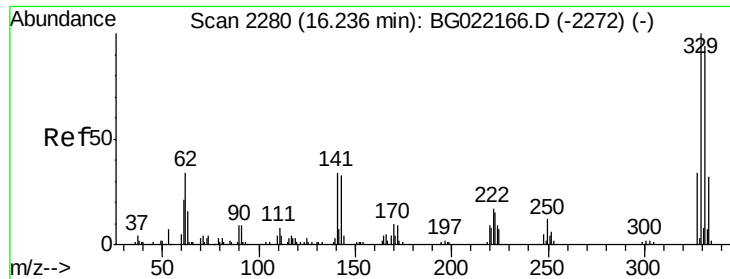




#41
 2,4,6-Tribromophenol
 Concen: 107.12 ng
 RT: 16.13 min Scan# 2262
 Delta R.T. -0.00 min
 Lab File: BG022463.D
 Acq: 21 Jun 2016 5:41

Instrument :
 BNA_G
 ClientSampleId :
 P8-B5(0-16)G

Tgt Ion:330 Resp: 94833
 Ion Ratio Lower Upper
 330 100
 332 96.2 78.0 117.0
 141 48.1 33.8 50.8

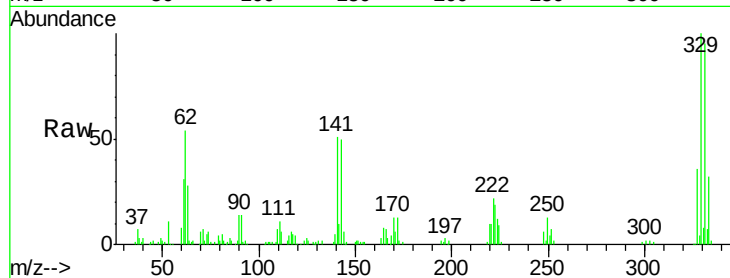


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

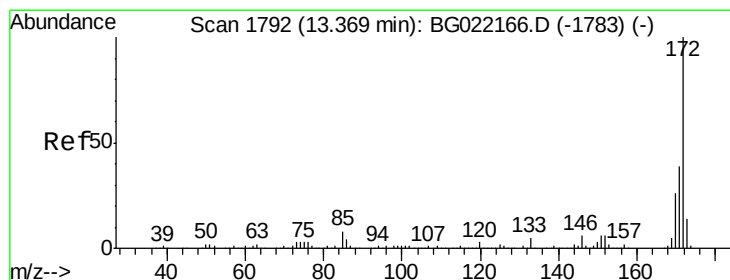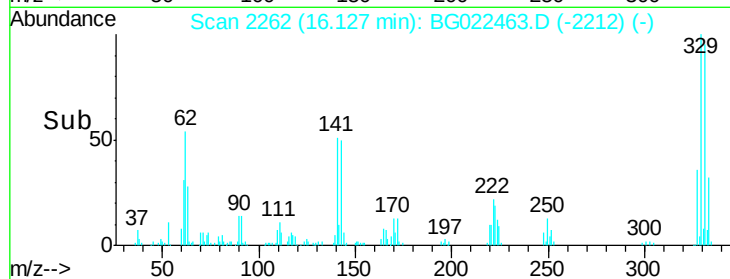
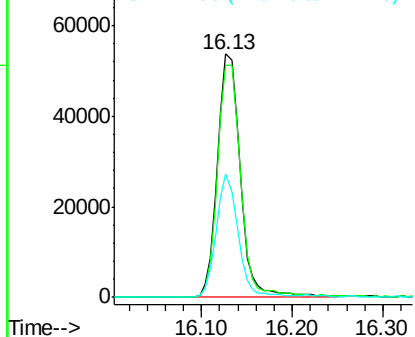



#44
 2-Fluorobiphenyl
 Concen: 92.26 ng
 RT: 13.25 min Scan# 1773
 Delta R.T. 0.00 min
 Lab File: BG022463.D
 Acq: 21 Jun 2016 5:41

Tgt Ion:172 Resp: 474332
 Ion Ratio Lower Upper
 172 100
 171 39.4 27.8 41.6
 170 26.2 19.6 29.4

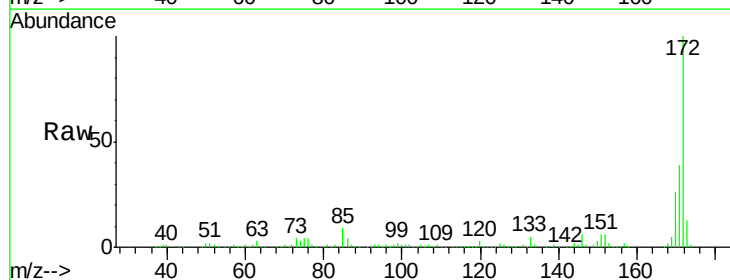

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

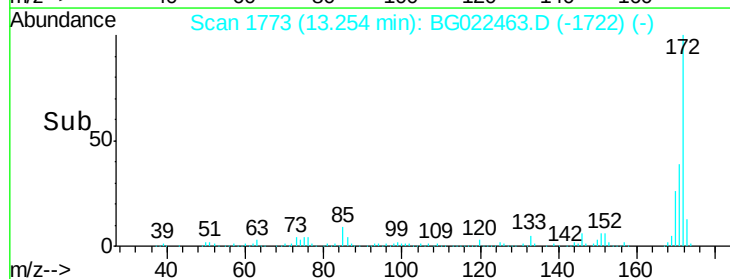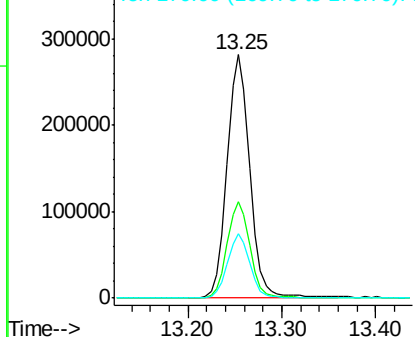

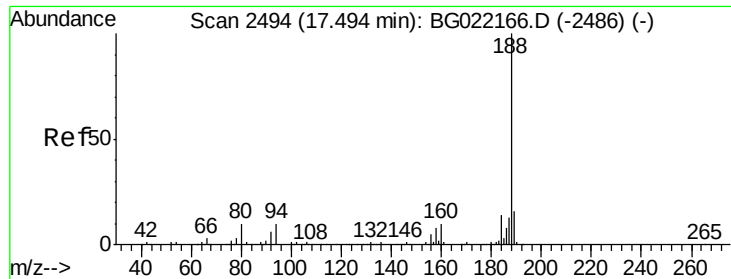

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.38 min Scan# 2475

Delta R.T. -0.00 min

Lab File: BG022463.D

Acq: 21 Jun 2016 5:41

Instrument :

BNA_G

ClientSampleId :

P8-B5(0-16)G


Tgt Ion:188 Resp: 171454

Ion Ratio Lower Upper

188 100

94 11.8 7.5 11.3#




80 12.8 8.6 13.0

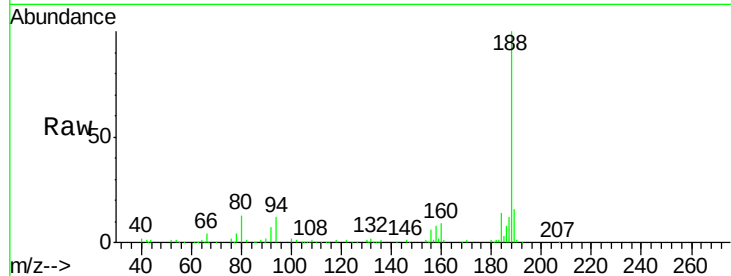

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

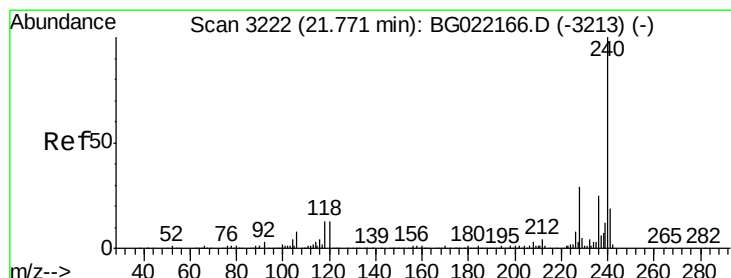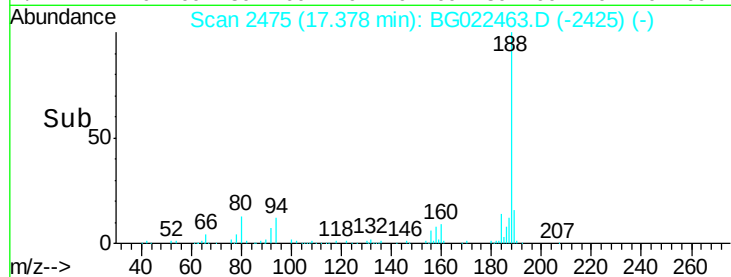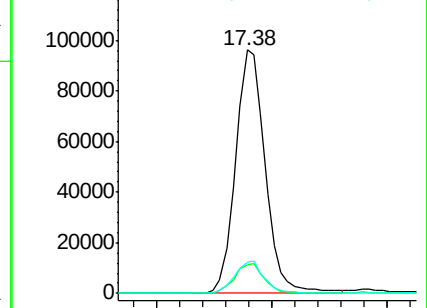

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.64 min Scan# 3200

Delta R.T. -0.00 min

Lab File: BG022463.D

Acq: 21 Jun 2016 5:41


Tgt Ion:240 Resp: 135748

Ion Ratio Lower Upper

240 100

120 16.4 8.4 12.6#



236 26.9 19.6 29.4

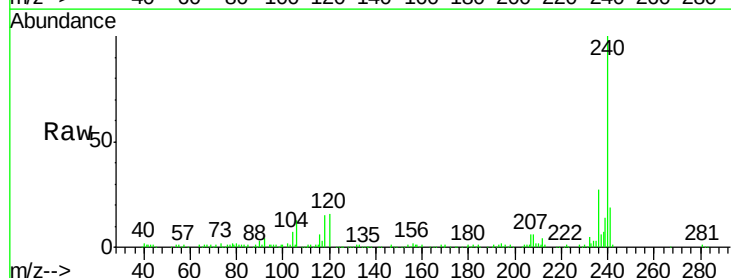


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

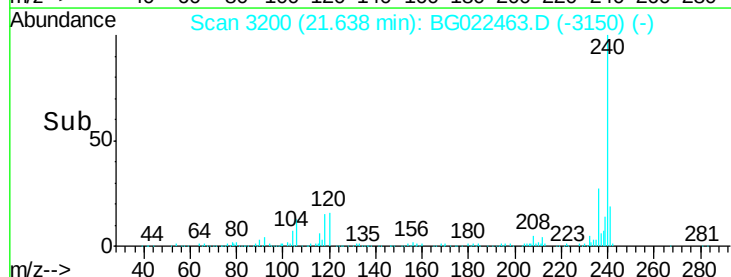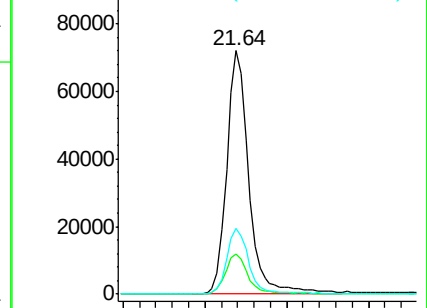

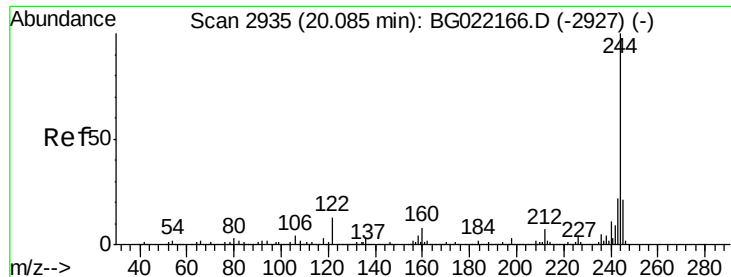

#78

Terphenyl-d14

Concen: 95.40 ng

RT: 19.98 min Scan# 2918

Delta R.T. -0.00 min

Lab File: BG022463.D

Acq: 21 Jun 2016 5:41

Instrument :

BNA_G

ClientSampleId :

P8-B5(0-16)G


Tgt Ion:244 Resp: 545472

Ion Ratio Lower Upper

244 100

212 7.6 6.5 9.7




122 15.7 8.6 12.8#

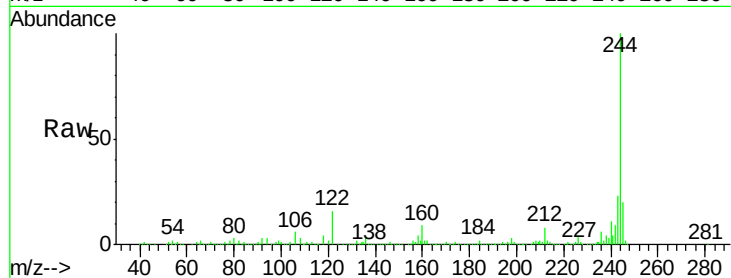

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

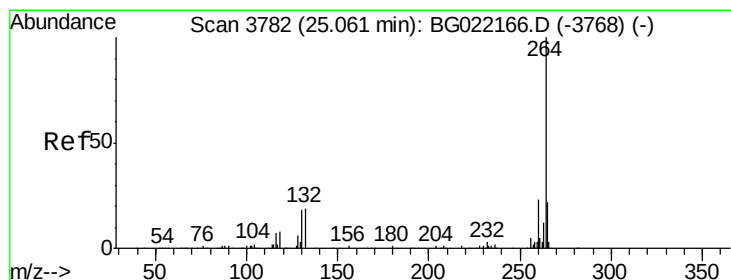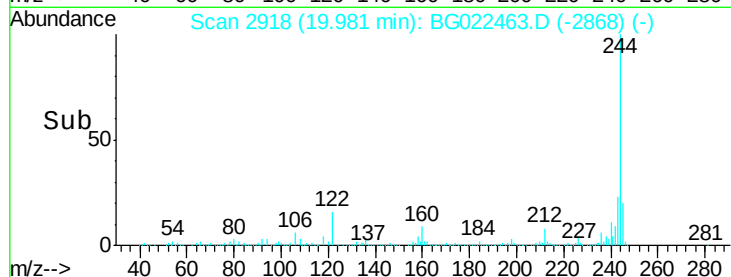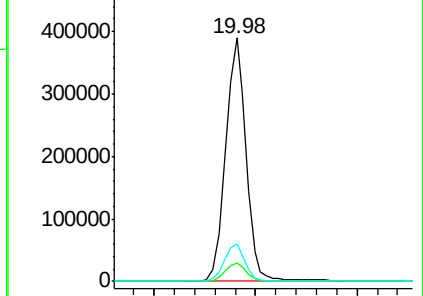

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.84 min Scan# 3745

Delta R.T. -0.00 min

Lab File: BG022463.D

Acq: 21 Jun 2016 5:41


Tgt Ion:264 Resp: 119637

Ion Ratio Lower Upper

264 100

260 24.1 20.2 30.4

265 21.0 17.8 26.8

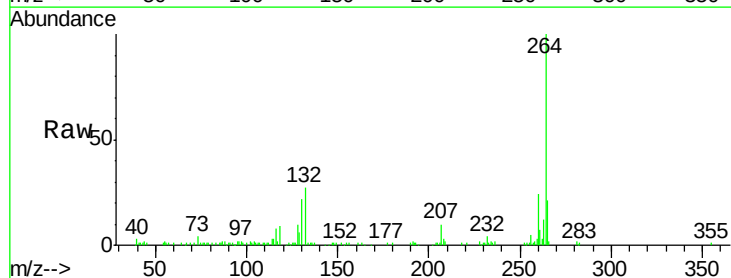

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

