


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062016\
 Data File : BG022448.D
 Acq On : 20 Jun 2016 17:15
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 17:40:23 2016

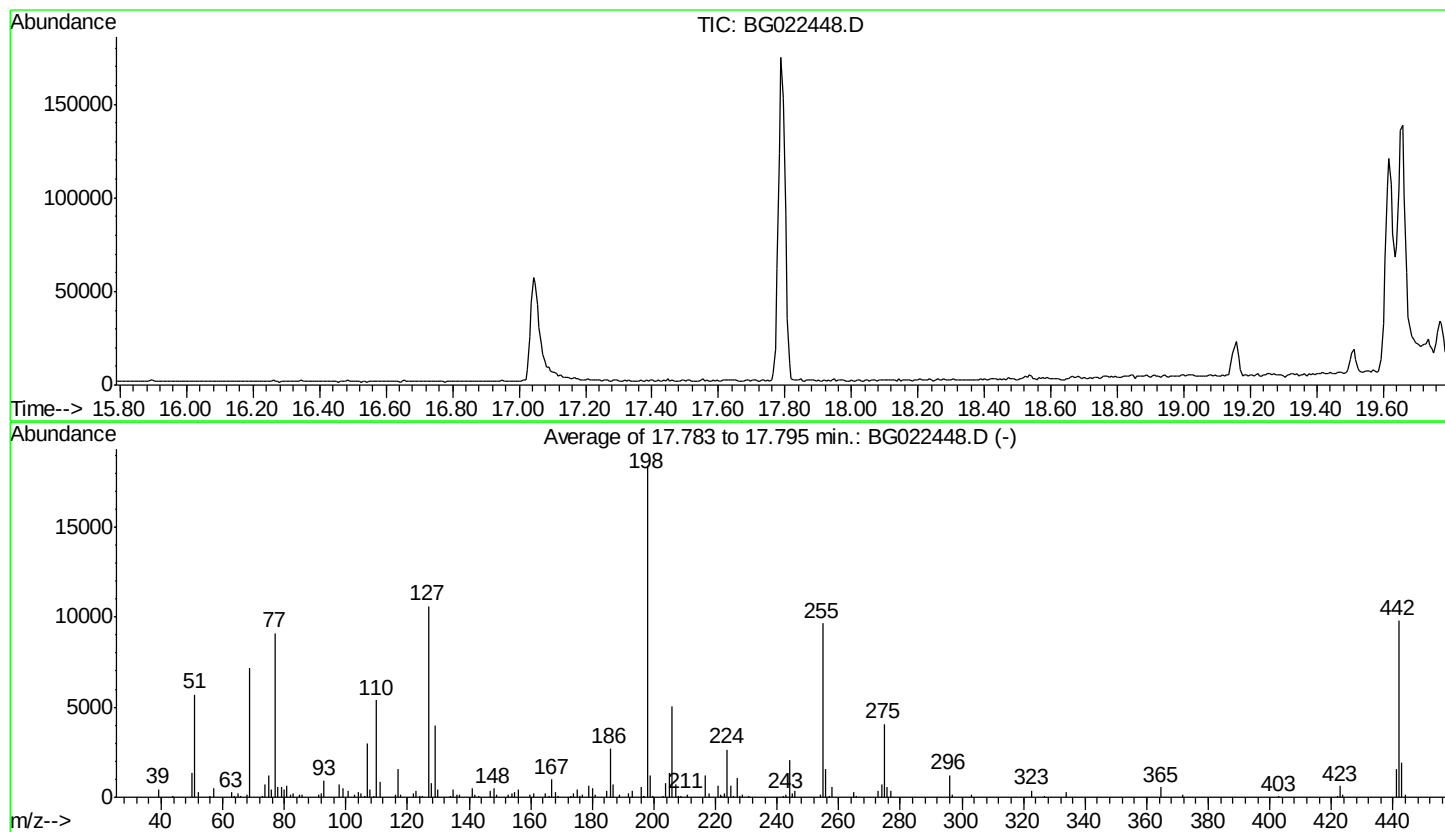

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2537

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	5692	PASS
68	69	0.00	2	1.6	116	PASS
69	198	0.00	100	39.2	7209	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.7	10617	PASS
197	198	0.00	2	0.3	50	PASS
198	198	100	100	100.0	18398	PASS
199	198	5	9	6.7	1228	PASS
275	198	10	60	22.2	4083	PASS
365	198	1	100	3.0	559	PASS
441	442	0.01	24	16.2	1587	PASS
442	198	50	100	53.2	9780	PASS
443	442	15	24	19.7	1928	PASS