


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062016\
 Data File : BG022464.D
 Acq On : 21 Jun 2016 6:21
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 17:40:23 2016

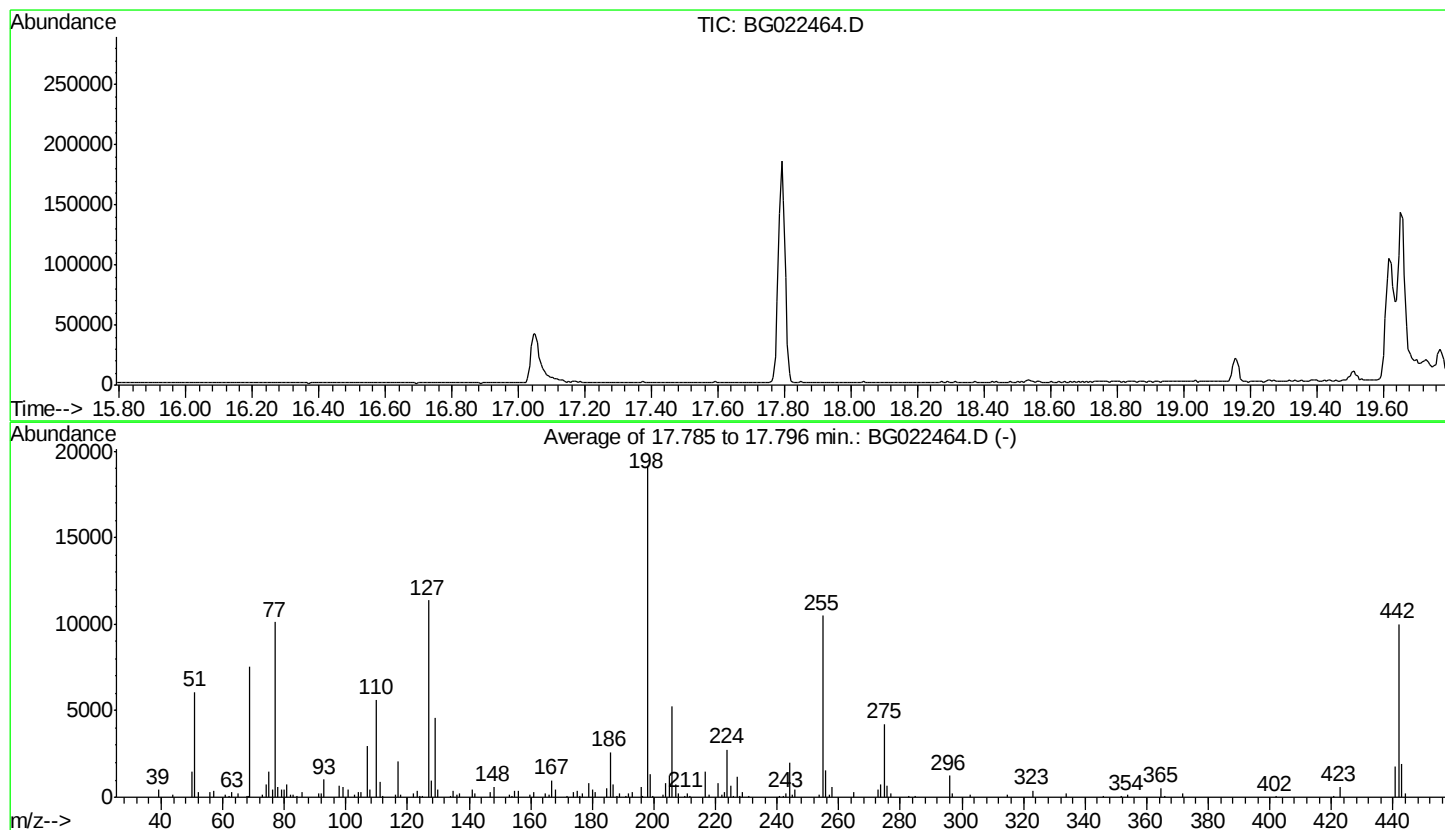

AutoFind: Scans 2544, 2545, 2546; Background Corrected with Scan 2538

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	6104	PASS
68	69	0.00	2	0.9	69	PASS
69	198	0.00	100	39.3	7536	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.3	11372	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19170	PASS
199	198	5	9	7.0	1345	PASS
275	198	10	60	22.0	4221	PASS
365	198	1	100	2.8	538	PASS
441	442	0.01	24	17.4	1742	PASS
442	198	50	100	52.2	10011	PASS
443	442	15	24	19.3	1928	PASS