

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062017\
 Data File : BG027556.D
 Acq On : 20 Jun 2017 18:18
 Operator : SJ/MA
 Sample : I3658-05DL 2X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC83DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.059	24	29	32	rBV5	4401	10141	1.27%	0.154%
2	4.100	33	36	47	rVB	25184	43986	5.49%	0.666%
3	4.517	106	107	111	rVB3	1019	1014	0.13%	0.015%
4	4.917	172	175	179	rVB3	1033	1001	0.12%	0.015%
5	5.281	235	237	240	rVB3	1143	883	0.11%	0.013%
6	5.310	240	242	245	rBV4	1059	1189	0.15%	0.018%
7	5.475	266	270	272	rBV3	1171	1139	0.14%	0.017%
8	5.504	272	275	279	rVV2	760	1224	0.15%	0.019%
9	5.698	306	308	313	rVB2	1026	1669	0.21%	0.025%
10	5.863	327	336	337	rBV2	791	1587	0.20%	0.024%
11	5.980	350	356	365	rVB4	1443	3736	0.47%	0.057%
12	6.186	389	391	396	rVB3	982	1473	0.18%	0.022%
13	6.233	396	399	401	rBV	666	936	0.12%	0.014%
14	6.339	413	417	419	rVB2	653	819	0.10%	0.012%
15	6.656	468	471	472	rBV	921	895	0.11%	0.014%
16	6.944	514	520	522	rBV3	469	832	0.10%	0.013%
17	7.032	528	535	536	rBV2	648	1226	0.15%	0.019%
18	7.202	563	564	568	rBV	880	835	0.10%	0.013%
19	7.261	573	574	583	rBV2	757	1916	0.24%	0.029%
20	7.649	630	640	650	rBV2	13605	26796	3.34%	0.406%
21	7.825	662	670	681	rVB	45934	82140	10.25%	1.244%
22	8.048	700	708	716	rBV	48823	91983	11.48%	1.393%
23	8.248	739	742	747	rVB2	874	1237	0.15%	0.019%
24	8.336	754	757	762	rVB2	678	982	0.12%	0.015%
25	8.383	762	765	769	rVV2	634	876	0.11%	0.013%
26	8.424	769	772	776	rVB2	731	1074	0.13%	0.016%
27	8.513	778	787	798	rBV2	102157	185196	23.10%	2.805%
28	8.654	804	811	813	rBV2	1028	1656	0.21%	0.025%
29	8.712	818	821	827	rVB2	609	1222	0.15%	0.019%
30	8.783	829	833	837	rVB2	911	1440	0.18%	0.022%
31	8.836	840	842	848	rBV3	689	1151	0.14%	0.017%
32	8.912	852	855	860	rBV2	676	1124	0.14%	0.017%
33	9.188	894	902	913	rBV2	36100	67958	8.48%	1.029%
34	9.329	924	926	929	rVB2	856	947	0.12%	0.014%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062017\
 Data File : BG027556.D
 Acq On : 20 Jun 2017 18:18
 Operator : SJ/MA
 Sample : I3658-05DL 2X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC83DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

35	9.359	929	931	934	rBV2	962	1069	0.13%	0.016%
36	9.570	963	967	971	rVB3	842	1128	0.14%	0.017%
37	9.676	971	985	994	rBV	55160	109672	13.68%	1.661%
38	10.399	1100	1108	1119	rBV3	53284	109947	13.72%	1.665%
39	10.739	1159	1166	1168	rVB3	701	902	0.11%	0.014%
40	10.933	1192	1199	1211	rBV	72713	143869	17.95%	2.179%
41	11.021	1211	1214	1220	rBV	485	989	0.12%	0.015%
42	11.327	1257	1266	1276	rVB	146424	276340	34.47%	4.185%
43	11.468	1283	1290	1301	rVB4	2058	5121	0.64%	0.078%
44	11.750	1335	1338	1342	rVB	566	957	0.12%	0.014%
45	12.179	1406	1411	1418	rBV2	602	1135	0.14%	0.017%
46	12.426	1450	1453	1459	rBV	652	867	0.11%	0.013%
47	12.872	1526	1529	1536	rBV3	1103	1621	0.20%	0.025%
48	13.695	1665	1669	1671	rBV	654	884	0.11%	0.013%
49	13.712	1671	1672	1677	rVB	977	960	0.12%	0.015%
50	13.994	1717	1720	1725	rBV2	578	850	0.11%	0.013%
51	14.323	1774	1776	1783	rVB2	739	1007	0.13%	0.015%
52	14.482	1793	1803	1812	rBV	165490	259471	32.37%	3.929%
53	14.741	1842	1847	1849	rBV3	839	1042	0.13%	0.016%
54	14.793	1849	1856	1863	rVB	163550	268500	33.50%	4.066%
55	14.940	1878	1881	1885	rBV2	1042	1011	0.13%	0.015%
56	15.093	1900	1907	1920	rVB2	248517	412638	51.48%	6.249%
57	15.275	1932	1938	1950	rBV6	8152	22063	2.75%	0.334%
58	15.446	1963	1967	1972	rBV3	751	1101	0.14%	0.017%
59	15.516	1978	1979	1983	rVB3	985	860	0.11%	0.013%
60	15.628	1996	1998	2003	rVB2	774	1299	0.16%	0.020%
61	15.681	2003	2007	2009	rBV2	1277	1269	0.16%	0.019%
62	15.851	2033	2036	2042	rVB4	1345	1657	0.21%	0.025%
63	15.892	2042	2043	2046	rVB3	1132	899	0.11%	0.014%
64	15.945	2046	2052	2057	rBV6	1700	3804	0.47%	0.058%
65	16.027	2060	2066	2069	rBV3	1711	3365	0.42%	0.051%
66	16.080	2069	2075	2087	rVB	241067	385520	48.10%	5.838%
67	16.198	2087	2095	2098	rBV5	2436	4533	0.57%	0.069%
68	16.321	2112	2116	2121	rBV5	2682	4071	0.51%	0.062%
69	16.392	2125	2128	2132	rBV2	1050	1922	0.24%	0.029%
70	16.591	2160	2162	2166	rBV	911	1098	0.14%	0.017%
71	16.691	2178	2179	2184	rBV3	1051	1324	0.17%	0.020%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062017\
 Data File : BG027556.D
 Acq On : 20 Jun 2017 18:18
 Operator : SJ/MA
 Sample : I3658-05DL 2X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC83DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP


If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

72	16.744	2186	2188	2190	rVB3	1344	877	0.11%	0.013%
73	16.820	2196	2201	2206	rBV4	1566	2380	0.30%	0.036%
74	16.950	2217	2223	2225	rVB4	1206	2084	0.26%	0.032%
75	17.214	2266	2268	2270	rBV2	1727	1268	0.16%	0.019%
76	17.290	2279	2281	2283	rVB2	1532	1222	0.15%	0.019%
77	17.384	2294	2297	2301	rBV4	1691	2097	0.26%	0.032%
78	17.531	2320	2322	2324	rBV3	1345	991	0.12%	0.015%
79	17.625	2334	2338	2345	rVB4	2327	4300	0.54%	0.065%
80	17.725	2354	2355	2360	rBV4	1208	1223	0.15%	0.019%
81	17.761	2360	2361	2363	rBV2	1050	918	0.11%	0.014%
82	17.843	2368	2375	2384	rBV2	356391	574794	71.71%	8.705%
83	17.943	2384	2392	2402	rVB	298235	474346	59.18%	7.184%
84	18.160	2424	2429	2431	rBV5	1299	1919	0.24%	0.029%
85	18.231	2440	2441	2443	rBV2	1546	941	0.12%	0.014%
86	18.342	2458	2460	2465	rBV5	1474	1301	0.16%	0.020%
87	18.383	2465	2467	2471	rBV5	1189	1757	0.22%	0.027%
88	18.483	2482	2484	2486	rVB2	1721	1127	0.14%	0.017%
89	18.589	2499	2502	2504	rBV4	3086	3881	0.48%	0.059%
90	18.724	2519	2525	2529	rBV7	1844	4949	0.62%	0.075%
91	19.323	2624	2627	2628	rBV3	1913	1648	0.21%	0.025%
92	19.870	2712	2720	2729	rBV3	5867	18538	2.31%	0.281%
93	20.211	2771	2778	2788	rBV	369607	570000	71.11%	8.632%
94	20.375	2789	2806	2808	rBV10	22800	79886	9.97%	1.210%
95	22.214	3112	3119	3138	rVB	383049	801570	100.00%	12.139%
96	23.830	3390	3394	3402	rVB6	12665	25784	3.22%	0.390%
97	24.746	3544	3550	3559	rVB5	16294	39871	4.97%	0.604%
98	25.598	3685	3695	3709	rBV2	173875	584618	72.93%	8.854%
99	25.857	3726	3739	3759	rVB2	212965	754247	94.10%	11.423%
100	27.114	3946	3953	3963	rVB6	21158	67583	8.43%	1.023%

Sum of corrected areas: 6603168

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

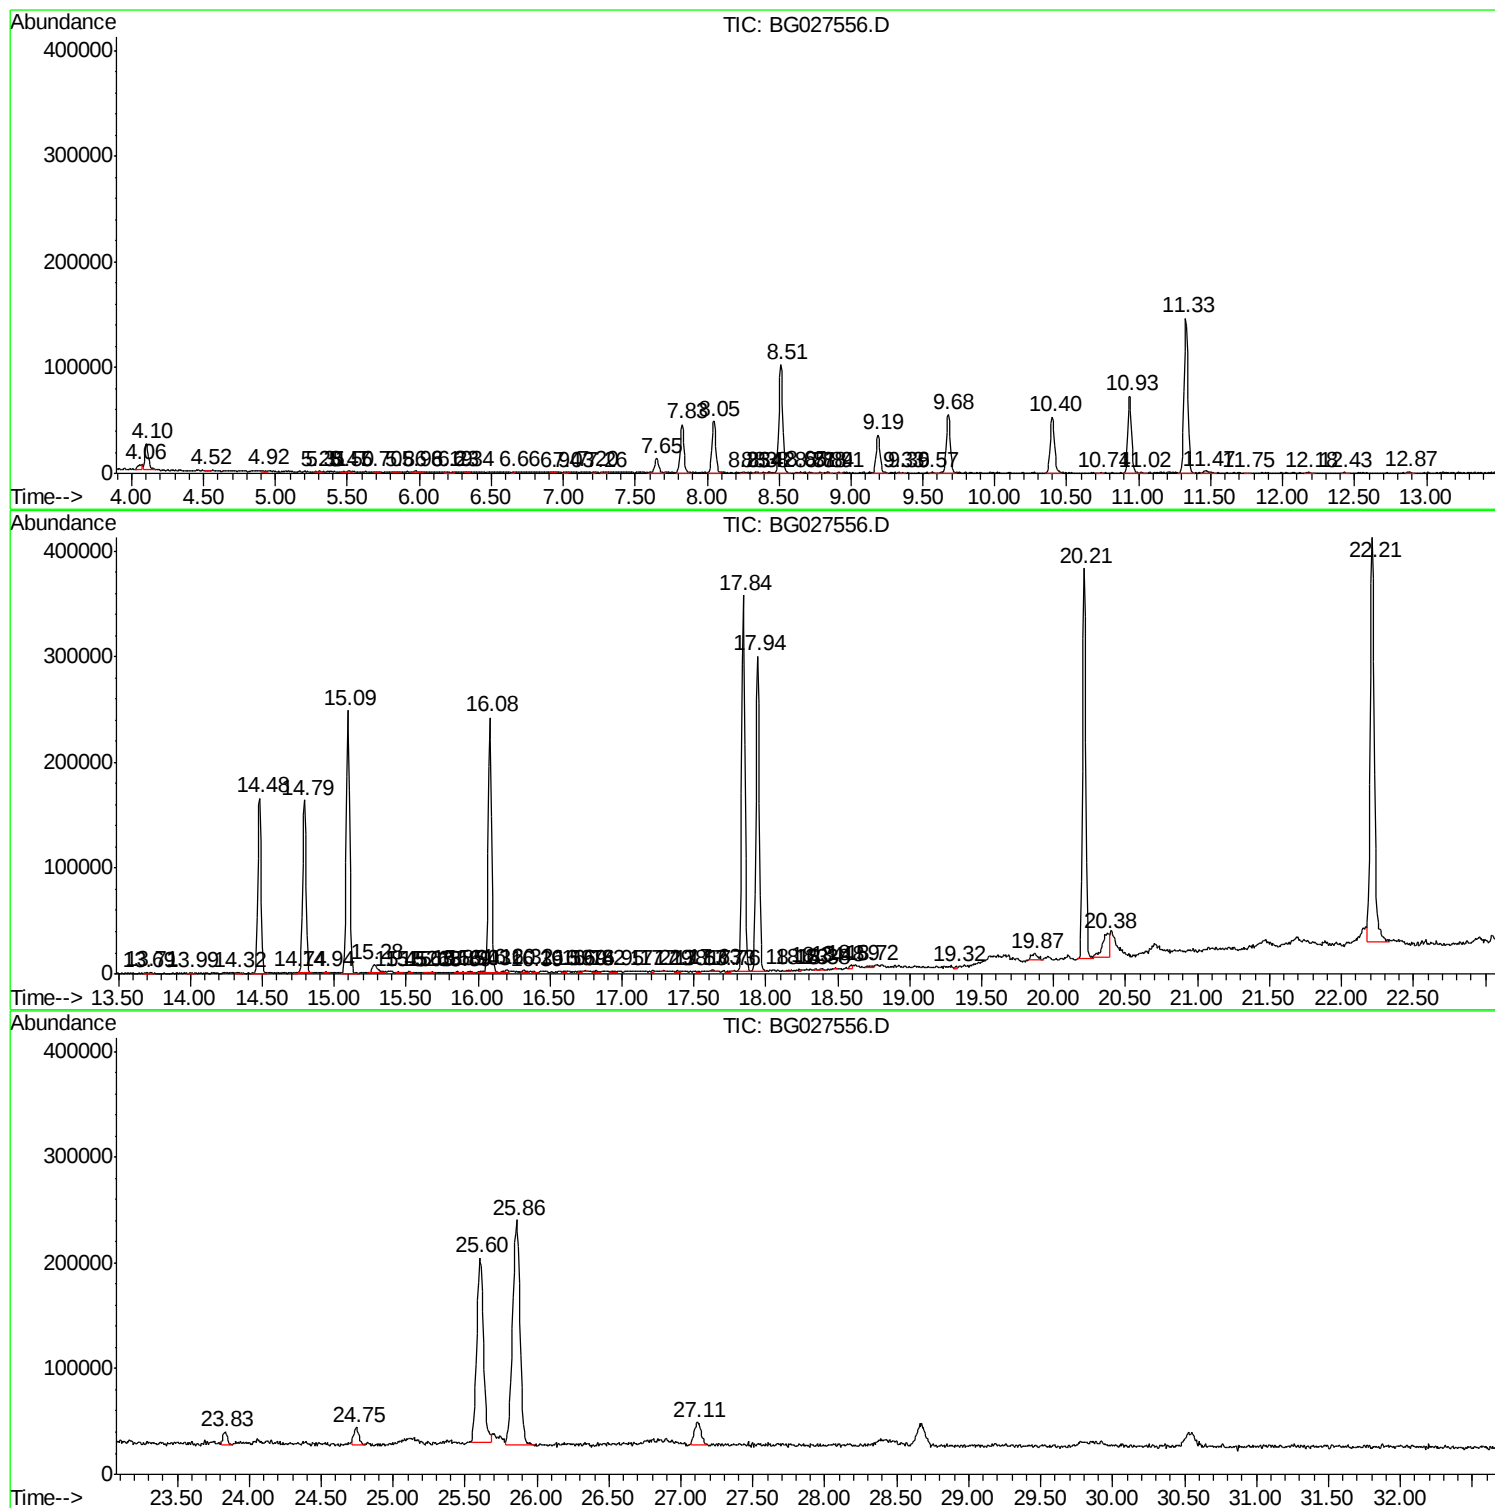

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG062017\
Data_File : BG027556.D
Acq_On : 20 Jun 2017 18:188
Operator : SJ/MAA
Sample : I3658-05DL_2XX
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
BDC83DL

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
