

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
 Data File : BG053943.D
 Acq On : 20 Jun 2022 11:30
 Operator : CG/JU
 Sample : SSTD00528
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD005428

Quant Time: Jun 20 14:08:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 14:06:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.077	152	18974	20.000	ng/u1	0.00
20) Naphthalene-d8	10.891	136	74990	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.704	164	58638	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.448	188	155084	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.726	240	185686	20.000	ng/u1	# 0.00
88) Perylene-d12	24.981	264	192473	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.506	96	789	1.573	ng/uL	0.00
4) Pyridine-d5	3.923	84	4237	3.831	ng/u1	0.00
7) Phenol-d5	7.231	99	6295	4.363	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.401	67	3815	4.090	ng/u1	0.00
11) 2-Chlorophenol-d4	7.613	132	5107	4.451	ng/u1	0.00
15) 4-Methylphenol-d8	8.776	113	5051	4.226	ng/u1	0.00
21) Nitrobenzene-d5	9.234	128	2658	5.929	ng/u1	0.00
24) 2-Nitrophenol-d4	9.963	143	2664	5.988	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.503	165	5729	4.741	ng/u1	0.00
31) 4-Chloroaniline-d4	11.015	131	7455	4.497	ng/u1	0.00
46) Dimethylphthalate-d6	14.105	166	21429	4.756	ng/u1	0.00
49) Acenaphthylene-d8	14.399	160	24199	4.806	ng/u1	0.00
54) 4-Nitrophenol-d4	14.881	143	2087	3.369	ng/u1	0.00
60) Fluorene-d10	15.691	176	20119	5.098	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.797	200	2883	4.650	ng/u1	0.00
73) Anthracene-d10	17.542	188	35105	5.012	ng/u1	0.00
81) Pyrene-d10	19.828	212	44799	4.533	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.757	264	45230	4.699	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.535	88	402	0.762	ng/uL#	82
5) Pyridine	3.940	79	5084	4.347	ng/u1	85
6) Benzaldehyde	7.213	77	3973	5.228	ng/u1#	84
8) Phenol	7.254	94	6448	4.175	ng/u1	93
10) Bis(2-Chloroethyl)ether	7.495	93	5375	4.544	ng/u1#	78
12) 2-Chlorophenol	7.636	128	5174	4.407	ng/u1	97
13) 2-Methylphenol	8.512	108	4921	4.148	ng/u1	86
14) 2,2'-oxybis(1-Chloropr...	8.606	45	7896	3.972	ng/u1	96
16) Acetophenone	8.899	105	8669	4.644	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.876	70	4381	4.204	ng/u1	98
18) 4-Methylphenol	8.841	108	5485	4.373	ng/u1	100
19) Hexachloroethane	9.164	117	2270	4.561	ng/u1	89
22) Nitrobenzene	9.281	77	6269	5.362	ng/u1	98
23) Isophorone	9.804	82	11962	4.339	ng/u1#	97
25) 2-Nitrophenol	9.992	139	2675	5.650	ng/u1#	84
26) 2,4-Dimethylphenol	10.051	107	6232	4.360	ng/u1	90
27) Bis(2-Chloroethoxy)met...	10.280	93	6887	4.344	ng/u1#	90
29) 2,4-Dichlorophenol	10.533	162	6085	5.078	ng/u1#	80
30) Naphthalene	10.938	128	18362	4.838	ng/u1	98
32) 4-Chloroaniline	11.038	127	7627	4.670	ng/u1	96
33) Hexachlorobutadiene	11.226	225	6197	6.231	ng/u1#	86
34) Caprolactam	11.778	113	707	2.108	ng/u1	77
35) 4-Chloro-3-methylphenol	12.154	107	6053	4.787	ng/u1	97
36) 2-Methylnaphthalene	12.542	142	13599	5.073	ng/u1	89

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
 Data File : BG053943.D
 Acq On : 20 Jun 2022 11:30
 Operator : CG/JU
 Sample : SST00528
 Misc :
 ALS Vial : 2 Sample Multiplier: 1


Instrument :
 BNA_G
 ClientSampleId :
 SST005428


Quant Time: Jun 20 14:08:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 14:06:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.754	142	13498	5.061	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.906	216	11589	5.650	ng/ul	91
40) Hexachlorocyclopentadiene	12.889	237	4311	3.092	ng/ul#	96
41) 2,4,6-Trichlorophenol	13.141	196	5503	4.709	ng/ul	94
42) 2,4,5-Trichlorophenol	13.212	196	6232	4.957	ng/ul	85
43) 1,1'-Biphenyl	13.541	154	19831	4.675	ng/ul	98
44) 2-Chloronaphthalene	13.582	162	16914	5.119	ng/ul	99
45) 2-Nitroaniline	13.782	65	3480	4.954	ng/ul	97
47) Dimethylphthalate	14.152	163	21061	4.881	ng/ul	98
48) 2,6-Dinitrotoluene	14.264	165	3731	5.926	ng/ul	87
50) Acenaphthylene	14.428	152	25120	4.654	ng/ul	96
51) 3-Nitroaniline	14.599	138	3355	5.565	ng/ul#	91
52) Acenaphthene	14.763	153	16563	4.623	ng/ul	98
53) 2,4-Dinitrophenol	14.810	184	731	2.201	ng/ul#	58
55) 4-Nitrophenol	14.892	109	1851	3.166	ng/ul#	79
56) Dibenzofuran	15.098	168	25488	4.919	ng/ul	99
57) 2,4-Dinitrotoluene	15.051	165	5524	6.281	ng/ul#	95
58) 2,3,4,6-Tetrachlorophenol	15.327	232	5051	4.535	ng/ul#	89
59) Diethylphthalate	15.509	149	20360	4.561	ng/ul	98
61) Fluorene	15.744	166	20802	4.899	ng/ul	96
62) 4-Chlorophenyl-phenyle...	15.738	204	13403	5.626	ng/ul	94
63) 4-Nitroaniline	15.756	138	2571	4.418	ng/ul	93
66) 4,6-Dinitro-2-methylph...	15.815	198	2591	4.493	ng/ul#	93
67) N-Nitrosodiphenylamine	15.950	169	18329	4.328	ng/ul	93
68) 4-Bromophenyl-phenylether	16.631	248	9126	5.307	ng/ul	95
69) Hexachlorobenzene	16.755	284	11066	5.960	ng/ul	91
70) Atrazine	16.890	200	8614	4.611	ng/ul	96
71) Pentachlorophenol	17.107	266	2514	2.278	ng/ul#	83
72) Phenanthrene	17.489	178	37510	4.688	ng/ul	99
74) Anthracene	17.577	178	38623	4.731	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.506	216	14627	5.964	ng/ul	91
76) Pentachlorobenzene	15.022	250	11505	5.223	ng/ul#	91
77) Carbazole	17.842	167	30318	4.260	ng/ul	96
78) Di-n-butylphthalate	18.406	149	33342	3.747	ng/ul	99
80) Fluoranthene	19.499	202	50504	4.396	ng/ul#	93
82) Pyrene	19.857	202	51500	4.523	ng/ul#	94
83) Butylbenzylphthalate	20.738	149	14064	3.394	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.614	252	18039	4.366	ng/ul#	99
85) Benzo(a)anthracene	21.702	228	55496	4.727	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.608	149	22140	3.638	ng/ul	98
87) Chrysene	21.767	228	54294	4.838	ng/ul	97
89) Di-n-octyl phthalate	22.836	149	37208	3.553	ng/ul	100
90) Benzo(b)fluoranthene	23.941	252	55823	4.623	ng/ul#	97
91) Benzo(k)fluoranthene	24.011	252	55048	4.786	ng/ul#	98
93) Benzo(a)pyrene	24.822	252	54963	4.713	ng/ul#	98
94) Indeno(1,2,3-cd)pyrene	28.700	276	63624	4.756	ng/ul#	94
95) Dibenzo(a,h)anthracene	28.770	278	52584	4.578	ng/ul#	91
96) Benzo(g,h,i)perylene	29.863	276	54169	4.801	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 20 14:08:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 14:06:57 2022
Response via : Initial Calibration









#2
 1,4-Dioxane
 Concen: 0.762 ng/uL
 RT: 3.535 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BG053943.D
 Acq: 20 Jun 2022 11:30

Instrument :
 BNA_G
 ClientSampleId :
 SSTD005428

Tgt Ion: 88 Resp: 402




Ion	Ratio	Lower	Upper
88	100		
43	32.4	48.1	72.1#
58	77.8	59.8	89.6

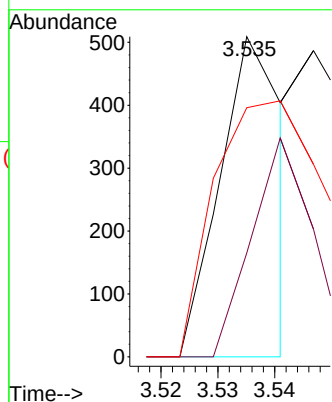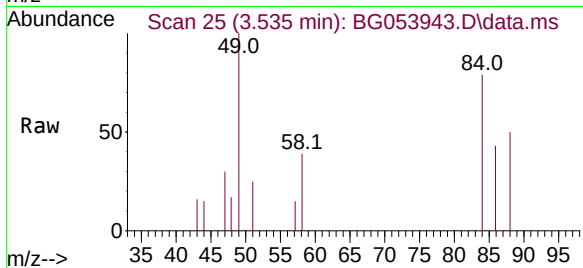


#5
 Pyridine
 Concen: 4.347 ng/uL
 RT: 3.940 min Scan# 94
 Delta R.T. 0.006 min
 Lab File: BG053943.D
 Acq: 20 Jun 2022 11:30

Tgt Ion: 79 Resp: 5084

Ion	Ratio	Lower	Upper
79	100		
52	77.4	75.4	113.2
51	50.5	35.2	52.8




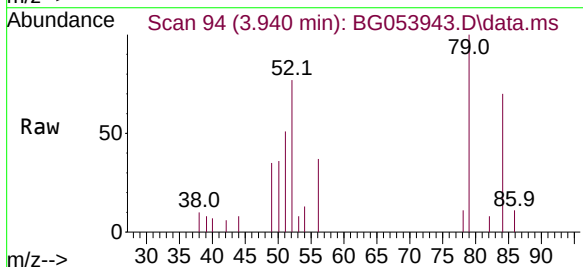




#6
Benzaldehyde
Concen: 5.228 ng/ul
RT: 7.213 min Scan# 61
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion: 77 Resp: 3973
Ion Ratio Lower Upper
77 100
105 79.2 79.7 119.5#
106 78.4 71.0 106.4



#8
Phenol
Concen: 4.175 ng/ul
RT: 7.254 min Scan# 658
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion: 94 Resp: 6448
Ion Ratio Lower Upper
94 100
65 32.5 24.1 36.1
66 46.3 32.5 48.7









#10
Bis(2-Chloroethyl)ether
Concen: 4.544 ng/ul
RT: 7.495 min Scan# 699
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion: 93 Resp: 5375
Ion Ratio Lower Upper
93 100
63 67.1 72.3 108.5#
95 27.1 29.4 44.0#

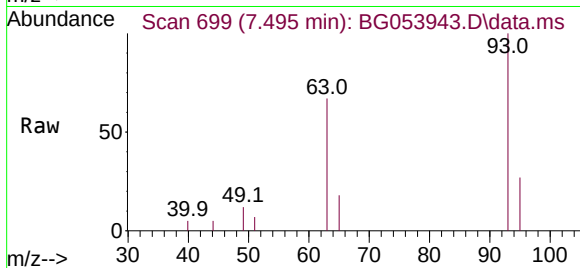

#12
2-Chlorophenol
Concen: 4.407 ng/ul
RT: 7.636 min Scan# 723
Delta R.T. -0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:128 Resp: 5174
Ion Ratio Lower Upper
128 100
64 54.3 41.4 62.2
130 34.8 27.0 40.6

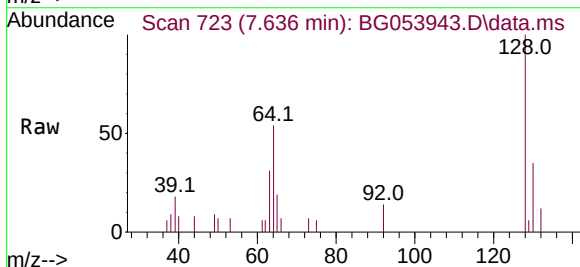



#13

2-Methylphenol

Concen: 4.148 ng/ul

RT: 8.512 min Scan# 81

Delta R.T. -0.000 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30

Instrument :

BNA_G

ClientSampleId :





SSTD005428

Tgt Ion:108 Resp: 4921

Ion Ratio Lower Upper

108 100

107 81.7 75.8 113.8

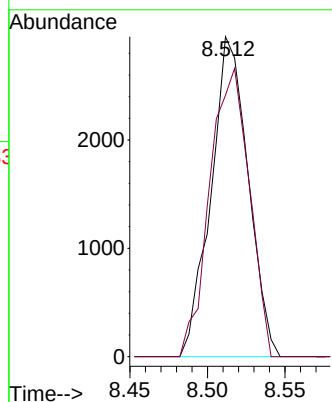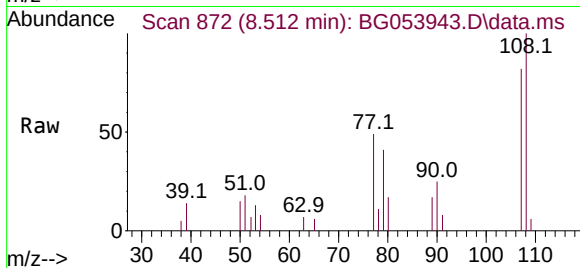

#14

2,2'-oxybis(1-Chloropropane)

Concen: 3.972 ng/ul

RT: 8.606 min Scan# 888

Delta R.T. -0.000 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30




Tgt Ion: 45 Resp: 7896


Ion Ratio Lower Upper

45 100

77 15.1 10.2 15.4

79 10.7 8.1 12.1




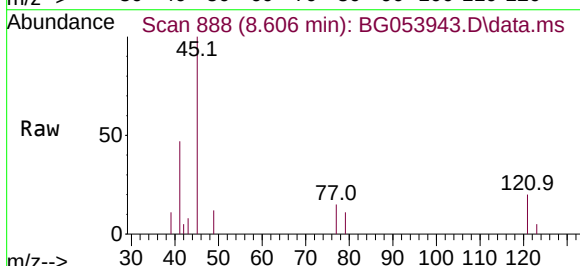




#16
Acetophenone
Concen: 4.644 ng/ul
RT: 8.899 min Scan# 91
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:105 Resp: 8669
Ion Ratio Lower Upper
105 100
77 74.8 61.0 91.6
51 30.2 22.8 34.2



#17
N-Nitroso-di-n-propylamine
Concen: 4.204 ng/ul
RT: 8.876 min Scan# 934
Delta R.T. -0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion: 70 Resp: 4381
Ion Ratio Lower Upper
70 100
42 64.1 50.2 75.4
101 10.4 7.1 10.7
130 19.1 15.5 23.3


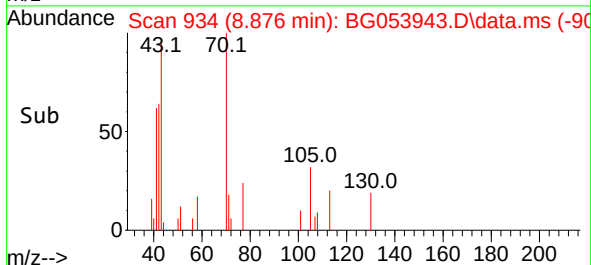
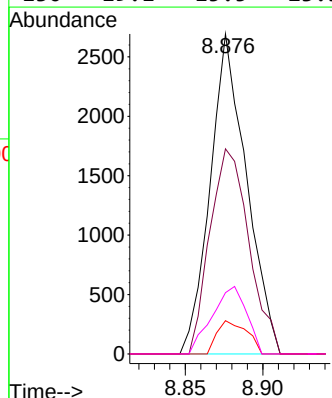





#18
4-Methylphenol
Concen: 4.373 ng/ul
RT: 8.841 min Scan# 91
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:108 Resp: 5485
Ion Ratio Lower Upper
108 100
107 113.0 90.7 136.1

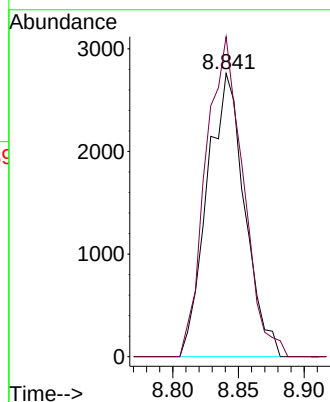

#19
Hexachloroethane
Concen: 4.561 ng/ul
RT: 9.164 min Scan# 983
Delta R.T. -0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:117 Resp: 2270
Ion Ratio Lower Upper
117 100
201 125.1 117.4 176.0
199 79.6 64.0 96.0


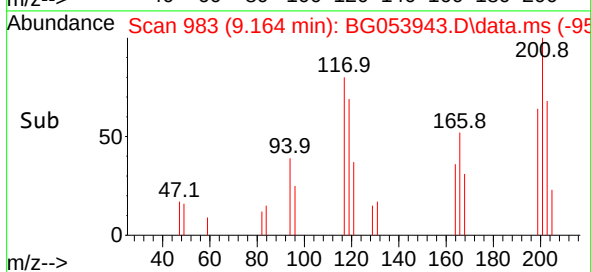
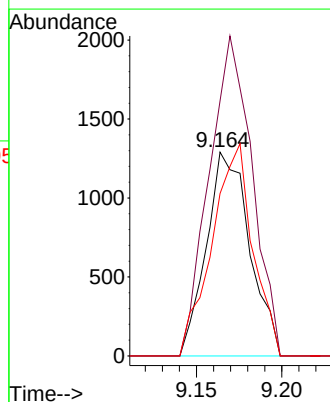





#22
Nitrobenzene
Concen: 5.362 ng/ul
RT: 9.281 min Scan# 1003
Delta R.T. 0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion: 77 Resp: 6269
Ion Ratio Lower Upper
77 100
123 40.1 31.2 46.8
65 14.7 10.5 15.7



#23
Isophorone
Concen: 4.339 ng/ul
RT: 9.804 min Scan# 1092
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion: 82 Resp: 11962
Ion Ratio Lower Upper
82 100
95 9.5 6.1 9.1#
138 18.1 13.6 20.4









#25
2-Nitrophenol
Concen: 5.650 ng/ul
RT: 9.992 min Scan# 1125
Delta R.T. -0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:139 Resp: 2675
Ion Ratio Lower Upper
139 100
65 44.6 47.7 71.5#
109 39.0 27.1 40.7



#26
2,4-Dimethylphenol
Concen: 4.360 ng/ul
RT: 10.051 min Scan# 1134
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:107 Resp: 6232
Ion Ratio Lower Upper
107 100
121 40.8 39.9 59.9
122 75.8 66.7 100.1

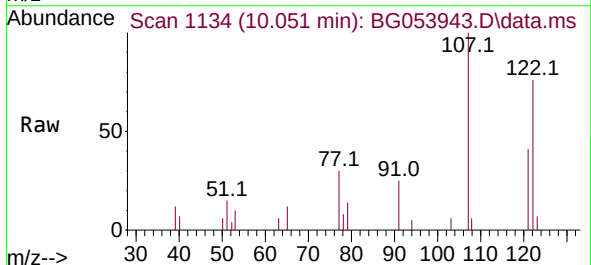



#27

Bis(2-Chloroethoxy)methane

Concen: 4.344 ng/ul

RT: 10.280 min Scan# 1173

Delta R.T. -0.006 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30

Instrument :

BNA_G

ClientSampleId :

SSTD005428





Tgt Ion: 93 Resp: 6887

Ion Ratio Lower Upper

93 100

95 25.8 26.5 39.7#

123 12.1 8.8 13.2

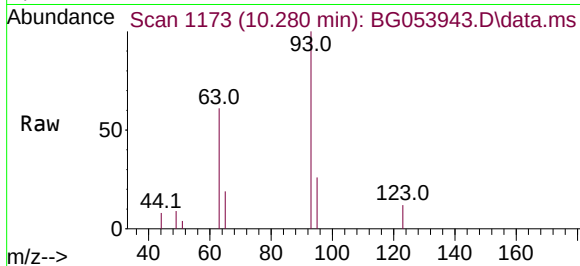

#29

2,4-Dichlorophenol

Concen: 5.078 ng/ul

RT: 10.533 min Scan# 1216

Delta R.T. -0.000 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30




Tgt Ion:162 Resp: 6085


Ion Ratio Lower Upper

162 100

164 48.1 50.9 76.3#

98 23.8 28.5 42.7#




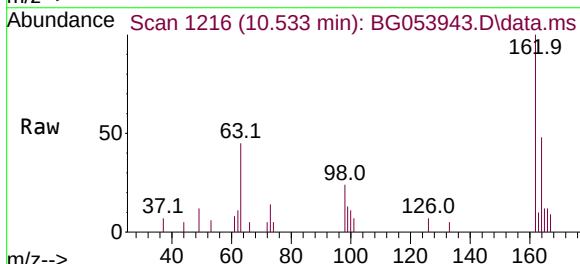




#30
Naphthalene
Concen: 4.838 ng/ul
RT: 10.938 min Scan# 1285
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:128 Resp: 18362
Ion Ratio Lower Upper
128 100
129 12.6 9.0 13.6
127 14.6 11.1 16.7



#32
4-Chloroaniline
Concen: 4.670 ng/ul
RT: 11.038 min Scan# 1302
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:127 Resp: 7627
Ion Ratio Lower Upper
127 100
129 29.7 25.4 38.2




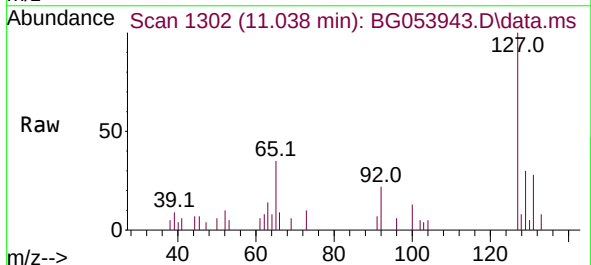




#33
Hexachlorobutadiene
Concen: 6.231 ng/ul
RT: 11.226 min Scan# 11
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:225 Resp: 6197
Ion Ratio Lower Upper
225 100
223 48.7 50.2 75.2#
227 57.3 51.8 77.6

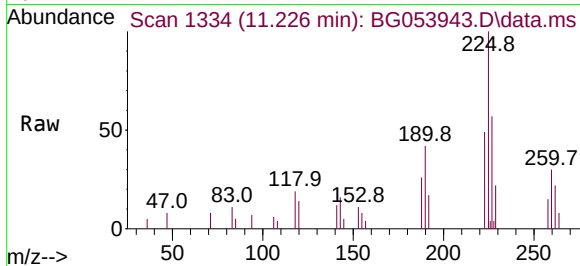

#34
Caprolactam
Concen: 2.108 ng/ul
RT: 11.778 min Scan# 1428
Delta R.T. -0.012 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:113 Resp: 707
Ion Ratio Lower Upper
113 100
55 171.3 167.8 251.6
56 130.6 127.6 191.4




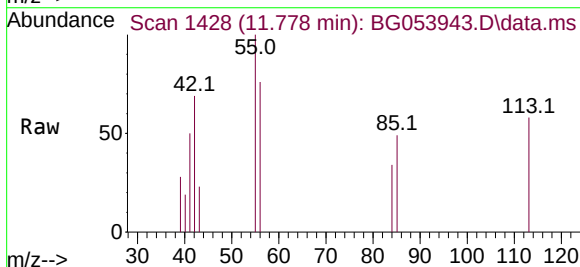




#35
 4-Chloro-3-methylphenol
 Concen: 4.787 ng/ul
 RT: 12.154 min Scan# 1492
 Delta R.T. -0.000 min
 Lab File: BG053943.D
 Acq: 20 Jun 2022 11:30




Instrument :
 BNA_G
 ClientSampleId :
 SSTD005428


Tgt Ion:	107	Resp:	6053
Ion	Ratio	Lower	Upper
107	100		
144	25.7	21.3	31.9
142	77.6	65.0	97.4

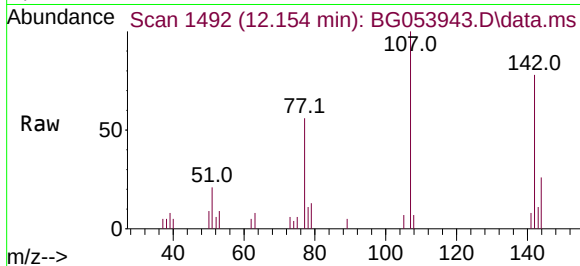

#36
 2-Methylnaphthalene
 Concen: 5.073 ng/ul
 RT: 12.542 min Scan# 1558
 Delta R.T. 0.006 min
 Lab File: BG053943.D
 Acq: 20 Jun 2022 11:30

Tgt Ion:	142	Resp:	13599
Ion	Ratio	Lower	Upper
142	100		
141	84.6	76.3	114.5

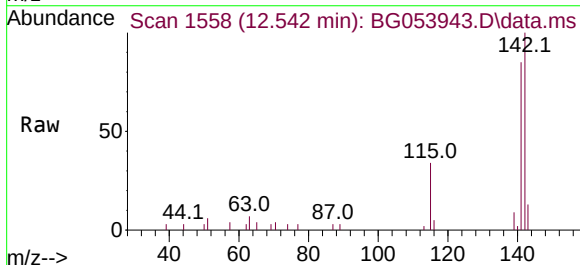



#37

1-Methylnaphthalene

Concen: 5.061 ng/ul

RT: 12.754 min Scan# 1

Delta R.T. -0.000 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30

Instrument :

BNA_G

ClientSampleId :

SSTD005428





Tgt Ion:142 Resp: 13498

Ion Ratio Lower Upper

142 100

141 91.6 73.4 110.2

116 4.4 3.2 4.8

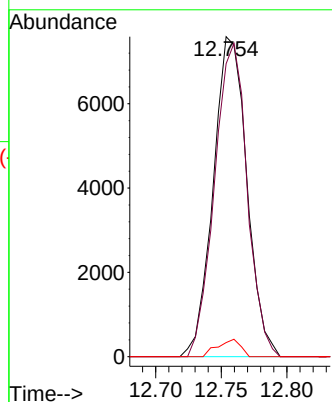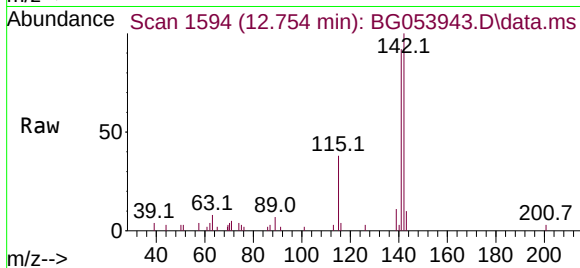

#39

1,2,4,5-Tetrachlorobenzene

Concen: 5.650 ng/ul

RT: 12.906 min Scan# 1620

Delta R.T. -0.000 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30

Tgt Ion:216 Resp: 11589




Ion Ratio Lower Upper


216 100

214 81.5 58.1 87.1

179 15.3 14.8 22.2


108 12.0 10.4 15.6

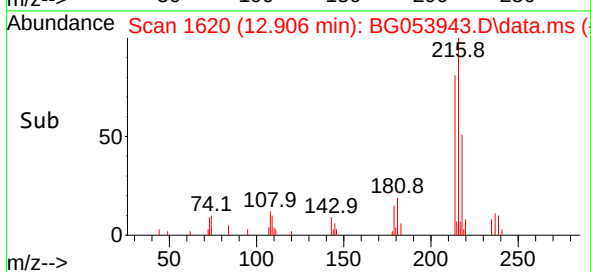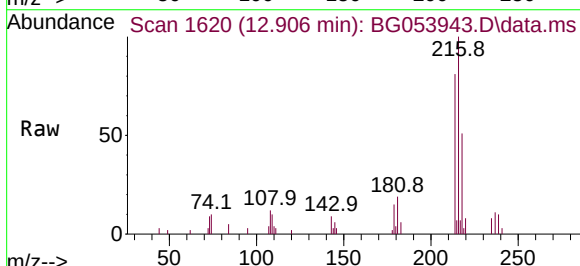






#40
Hexachlorocyclopentadiene
Concen: 3.092 ng/ul
RT: 12.889 min Scan# 1617
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Instrument :
BNA_G
ClientSampleId :
SSTD005428







Tgt Ion:237 Resp: 4311
Ion Ratio Lower Upper
237 100
235 56.8 47.0 70.6
272 15.0 8.6 12.8#



#41
2,4,6-Trichlorophenol
Concen: 4.709 ng/ul
RT: 13.141 min Scan# 1660
Delta R.T. 0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:196 Resp: 5503
Ion Ratio Lower Upper
196 100
198 95.7 81.9 122.9
200 29.3 25.7 38.5


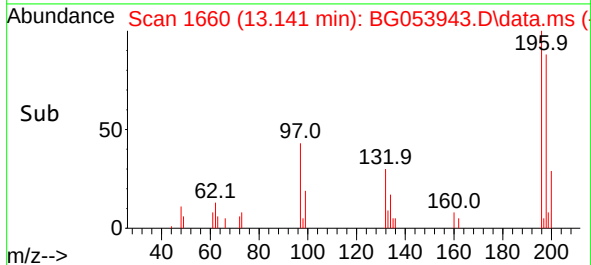






#42
2,4,5-Trichlorophenol
Concen: 4.957 ng/ul
RT: 13.212 min Scan# 1
Delta R.T. 0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:196 Resp: 6232
Ion Ratio Lower Upper
196 100
198 78.4 76.3 114.5
200 27.3 25.5 38.3



#43
1,1'-Biphenyl
Concen: 4.675 ng/ul
RT: 13.541 min Scan# 1728
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:154 Resp: 19831
Ion Ratio Lower Upper
154 100
153 42.3 32.7 49.1
76 10.4 9.0 13.6









#44
2-Chloronaphthalene
Concen: 5.119 ng/ul
RT: 13.582 min Scan# 1735
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:	162	Resp:	16914
Ion	Ratio	Lower	Upper
162	100		
164	32.0	25.7	38.5
127	34.5	28.3	42.5

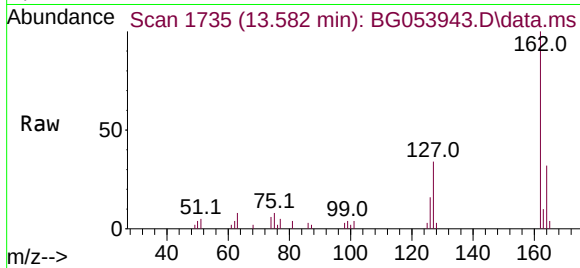

#45
2-Nitroaniline
Concen: 4.954 ng/ul
RT: 13.782 min Scan# 1769
Delta R.T. 0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:	65	Resp:	3480
Ion	Ratio	Lower	Upper
65	100		
92	61.4	52.2	78.4
138	100.6	79.0	118.4

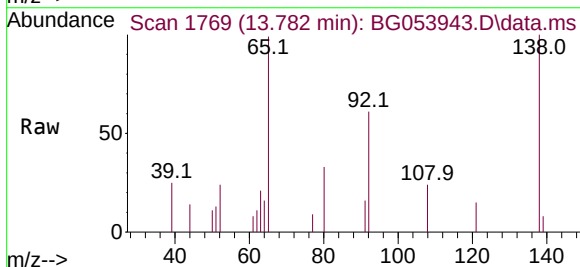



#47

Dimethylphthalate

Concen: 4.881 ng/ul

RT: 14.152 min Scan# 1832

Delta R.T. 0.006 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30

Instrument :

BNA_G

ClientSampleId :

SSTD005428





Tgt Ion:163 Resp: 21061

Ion Ratio Lower Upper

163 100

194 3.9 3.7 5.5

164 9.0 7.9 11.9

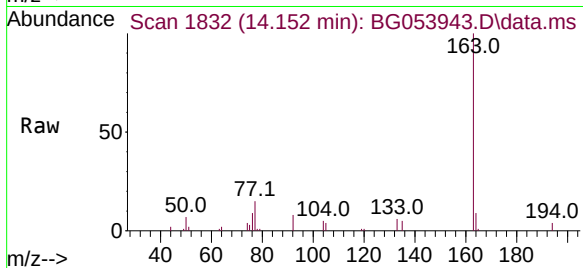

#48

2,6-Dinitrotoluene

Concen: 5.926 ng/ul

RT: 14.264 min Scan# 1851

Delta R.T. -0.000 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30




Tgt Ion:165 Resp: 3731


Ion Ratio Lower Upper

165 100

89 45.2 44.7 67.1

121 24.8 16.9 25.3




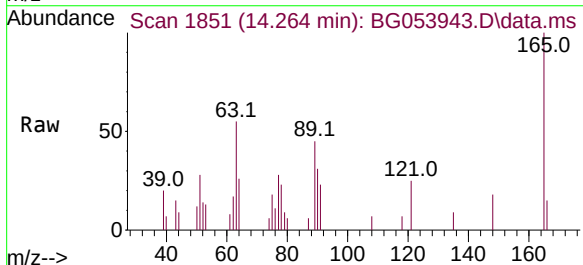




#50
Acenaphthylene
Concen: 4.654 ng/ul
RT: 14.428 min Scan# 1878
Delta R.T. 0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:152 Resp: 25120
Ion Ratio Lower Upper
152 100
151 17.2 16.2 24.2
153 13.2 10.5 15.7



#51
3-Nitroaniline
Concen: 5.565 ng/ul
RT: 14.599 min Scan# 1908
Delta R.T. 0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:138 Resp: 3355
Ion Ratio Lower Upper
138 100
108 12.3 17.8 26.6#
92 125.2 94.2 141.4


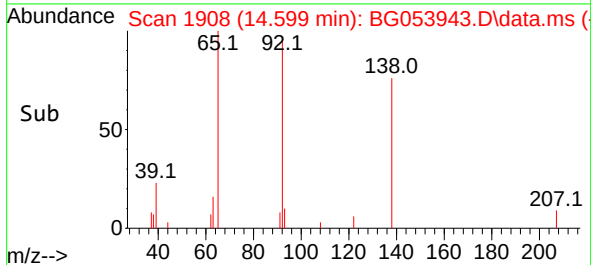






#52
Acenaphthene
Concen: 4.623 ng/ul
RT: 14.763 min Scan# 1936
Delta R.T. -0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:153 Resp: 16563
Ion Ratio Lower Upper
153 100
152 46.4 37.5 56.3
154 88.8 68.8 103.2

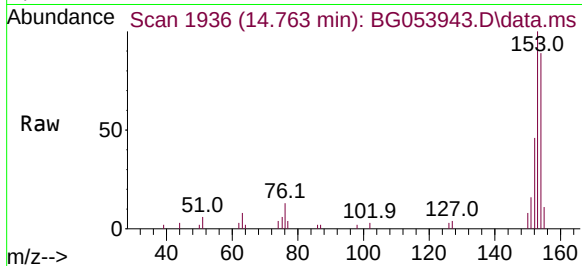

#53
2,4-Dinitrophenol
Concen: 2.201 ng/ul
RT: 14.810 min Scan# 1944
Delta R.T. 0.012 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:184 Resp: 731
Ion Ratio Lower Upper
184 100
63 51.0 34.7 52.1
154 52.1 87.3 130.9#




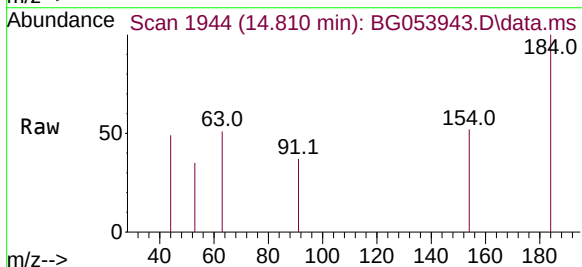




#55
4-Nitrophenol
Concen: 3.166 ng/ul
RT: 14.892 min Scan# 1958
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:109 Resp: 1851
Ion Ratio Lower Upper
109 100
139 86.4 92.9 139.3#
65 104.2 97.8 146.6



#56
Dibenzofuran
Concen: 4.919 ng/ul
RT: 15.098 min Scan# 1993
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:168 Resp: 25488
Ion Ratio Lower Upper
168 100
139 34.7 28.2 42.2









#57
2,4-Dinitrotoluene
Concen: 6.281 ng/ul
RT: 15.051 min Scan# 1985
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:165 Resp: 5524
Ion Ratio Lower Upper
165 100
63 38.7 33.0 49.4
182 0.0 2.8 4.2#



#58
2,3,4,6-Tetrachlorophenol
Concen: 4.535 ng/ul
RT: 15.327 min Scan# 2032
Delta R.T. 0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:232 Resp: 5051
Ion Ratio Lower Upper
232 100
131 29.7 27.5 41.3
130 0.0 1.8 2.8#
166 18.0 20.7 31.1#









#59
Diethylphthalate
Concen: 4.561 ng/ul
RT: 15.509 min Scan# 2063
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:149 Resp: 20360
Ion Ratio Lower Upper
149 100
177 22.2 18.9 28.3
150 13.4 10.6 15.8

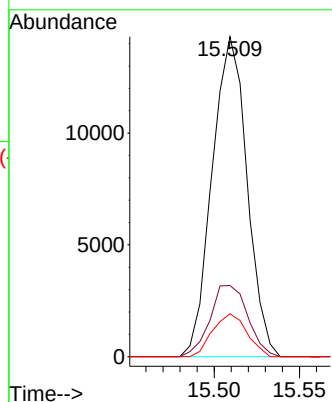

#61
Fluorene
Concen: 4.899 ng/ul
RT: 15.744 min Scan# 2103
Delta R.T. -0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:166 Resp: 20802
Ion Ratio Lower Upper
166 100
165 97.6 81.7 122.5
167 13.9 11.0 16.4



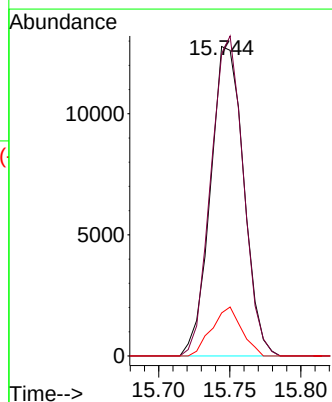





#62
4-Chlorophenyl-phenylether
Concen: 5.626 ng/ul
RT: 15.738 min Scan# 2102
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:204 Resp: 13403
Ion Ratio Lower Upper
204 100
206 30.3 27.1 40.7
141 46.4 40.7 61.1



#63
4-Nitroaniline
Concen: 4.418 ng/ul
RT: 15.756 min Scan# 2105
Delta R.T. 0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:138 Resp: 2571
Ion Ratio Lower Upper
138 100
92 45.7 42.0 63.0
108 93.5 79.0 118.6









#66
 4,6-Dinitro-2-methylphenol
 Concen: 4.493 ng/ul
 RT: 15.815 min Scan# 2115
 Delta R.T. -0.006 min
 Lab File: BG053943.D
 Acq: 20 Jun 2022 11:30




Instrument :
 BNA_G
 ClientSampleId :
 SSTD005428


Tgt Ion:198 Resp: 2591
 Ion Ratio Lower Upper
 198 100
 182 9.4 3.4 5.0#
 77 20.8 14.7 22.1



#67
 N-Nitrosodiphenylamine
 Concen: 4.328 ng/ul
 RT: 15.950 min Scan# 2138
 Delta R.T. -0.000 min
 Lab File: BG053943.D
 Acq: 20 Jun 2022 11:30

Tgt Ion:169 Resp: 18329
 Ion Ratio Lower Upper
 169 100
 168 71.1 51.0 76.4
 167 37.8 28.7 43.1









#68
4-Bromophenyl-phenylether
Concen: 5.307 ng/ul
RT: 16.631 min Scan# 21
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:248 Resp: 9126
Ion Ratio Lower Upper
248 100
250 94.0 78.2 117.2
141 52.7 46.7 70.1

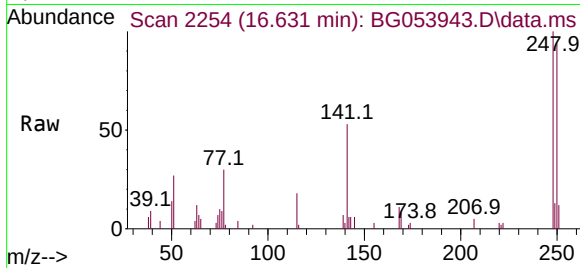

#69
Hexachlorobenzene
Concen: 5.960 ng/ul
RT: 16.755 min Scan# 2275
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:284 Resp: 11066
Ion Ratio Lower Upper
284 100
142 21.0 20.8 31.2
249 29.7 27.4 41.0




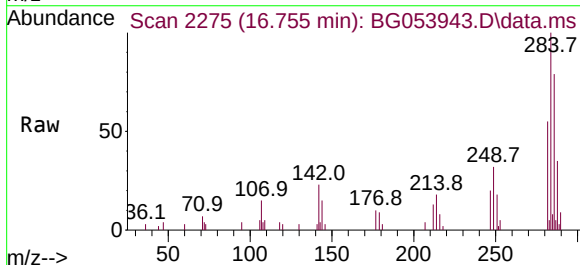




#70
 Atrazine
 Concen: 4.611 ng/ul
 RT: 16.890 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BG053943.D
 Acq: 20 Jun 2022 11:30




Instrument :
 BNA_G
 ClientSampleId :
 SST005428


Tgt Ion:200 Resp: 8614
 Ion Ratio Lower Upper
 200 100
 173 20.7 19.8 29.6
 215 46.9 38.8 58.2

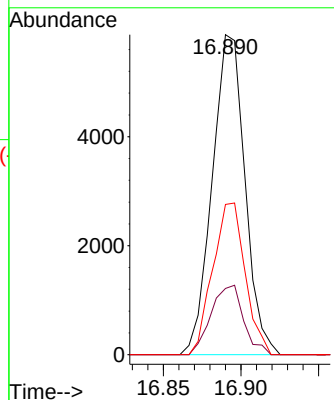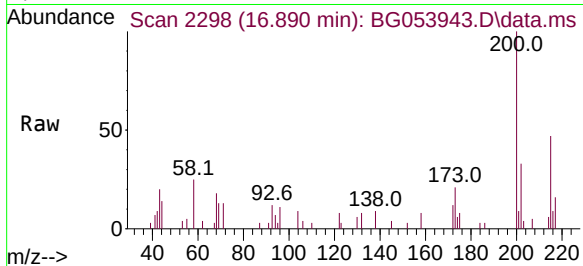

#71
 Pentachlorophenol
 Concen: 2.278 ng/ul
 RT: 17.107 min Scan# 2335
 Delta R.T. 0.012 min
 Lab File: BG053943.D
 Acq: 20 Jun 2022 11:30

Tgt Ion:266 Resp: 2514
 Ion Ratio Lower Upper
 266 100
 264 52.7 56.8 85.2#
 268 51.0 48.0 72.0



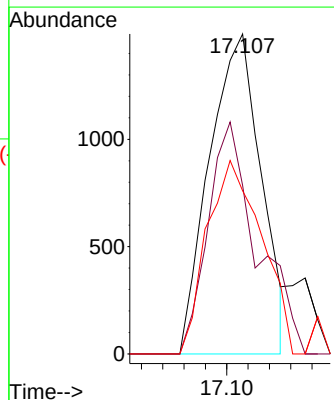
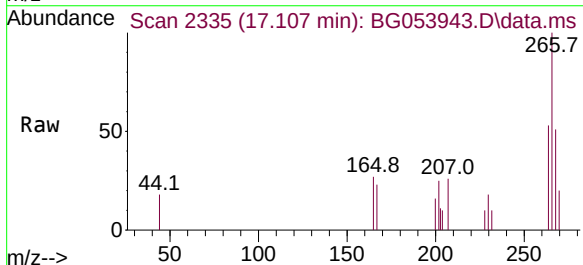




#72
Phenanthrene
Concen: 4.688 ng/ul
RT: 17.489 min Scan# 2400
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:178 Resp: 37510
Ion Ratio Lower Upper
178 100
179 16.2 12.6 19.0
176 19.3 15.7 23.5



#74
Anthracene
Concen: 4.731 ng/ul
RT: 17.577 min Scan# 2415
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:178 Resp: 38623
Ion Ratio Lower Upper
178 100
179 14.2 12.4 18.6
176 18.7 14.6 22.0




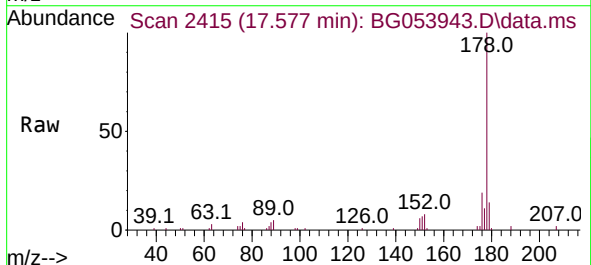




#75
1,2,3,4-Tetrachlorobenzene
Concen: 5.964 ng/uL
RT: 13.506 min Scan# 1722
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:216 Resp: 14627
Ion Ratio Lower Upper
216 100
214 70.4 64.2 96.4
218 45.1 39.0 58.4



#76
Pentachlorobenzene
Concen: 5.223 ng/uL
RT: 15.022 min Scan# 1980
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:250 Resp: 11505
Ion Ratio Lower Upper
250 100
248 72.8 47.7 71.5#
252 63.6 50.0 75.0


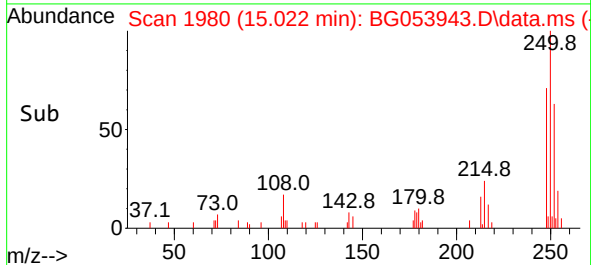






#77
 Carbazole
 Concen: 4.260 ng/ul
 RT: 17.842 min Scan# 2460
 Delta R.T. -0.000 min
 Lab File: BG053943.D
 Acq: 20 Jun 2022 11:30




Instrument :
 BNA_G
 ClientSampleId :
 SSTD005428


Tgt Ion:167	Resp:	30318
Ion	Ratio	Lower Upper
167	100	
166	20.3	18.2 27.2
139	12.0	9.0 13.6

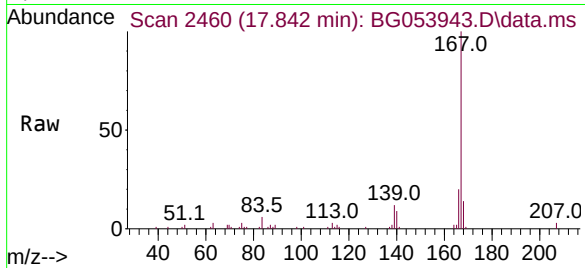

#78
 Di-n-butylphthalate
 Concen: 3.747 ng/ul
 RT: 18.406 min Scan# 2556
 Delta R.T. -0.000 min
 Lab File: BG053943.D
 Acq: 20 Jun 2022 11:30

Tgt Ion:149	Resp:	33342
Ion	Ratio	Lower Upper
149	100	
150	8.6	7.1 10.7
104	5.2	4.2 6.2




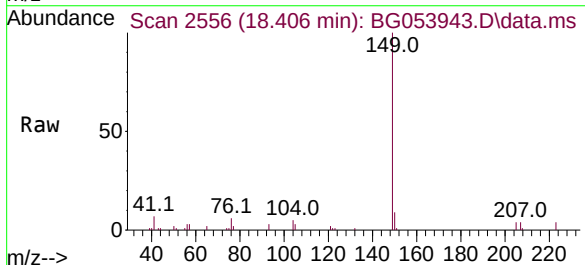




#80
Fluoranthene
Concen: 4.396 ng/ul
RT: 19.499 min Scan# 21
Delta R.T. 0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:202 Resp: 50504
Ion Ratio Lower Upper
202 100
101 5.5 6.6 9.8#
100 5.2 5.8 8.8#



#82
Pyrene
Concen: 4.523 ng/ul
RT: 19.857 min Scan# 2803
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:202 Resp: 51500
Ion Ratio Lower Upper
202 100
101 6.8 7.3 10.9#
100 6.1 6.2 9.4#









#83
Butylbenzylphthalate
Concen: 3.394 ng/ul
RT: 20.738 min Scan# 2953
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:	149	Resp:	14064
Ion Ratio	Lower	Upper	
149	100		
91	63.6	54.0	81.0
206	25.0	19.5	29.3



#84
3,3'-Dichlorobenzidine
Concen: 4.366 ng/ul
RT: 21.614 min Scan# 3102
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:	252	Resp:	18039
Ion Ratio	Lower	Upper	
252	100		
254	62.4	49.6	74.4
126	4.2	6.0	9.0

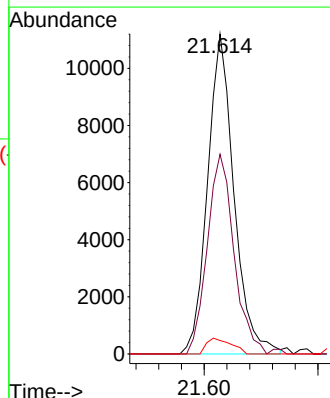



#85

Benzo(a)anthracene

Concen: 4.727 ng/ul

RT: 21.702 min Scan# 3117

Delta R.T. -0.000 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30

Instrument :

BNA_G

ClientSampleId :

SSTD005428





Tgt Ion:228 Resp: 55496

Ion Ratio Lower Upper

228 100

229 19.9 16.5 24.7

226 25.9 22.1 33.1

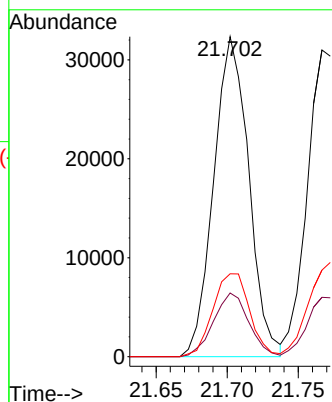

#86

Bis(2-ethylhexyl)phthalate

Concen: 3.638 ng/ul

RT: 21.608 min Scan# 3101

Delta R.T. -0.000 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30




Tgt Ion:149 Resp: 22140


Ion Ratio Lower Upper

149 100

167 27.8 21.7 32.5

279 5.9 3.9 5.9





#87

Chrysene

Concen: 4.838 ng/ul

RT: 21.767 min Scan# 3128

Delta R.T. -0.000 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30

Instrument :

BNA_G

ClientSampleId :

SSTD005428





Tgt Ion:228 Resp: 54294

Ion Ratio Lower Upper

228 100

226 28.2 24.2 36.4

229 19.4 16.3 24.5

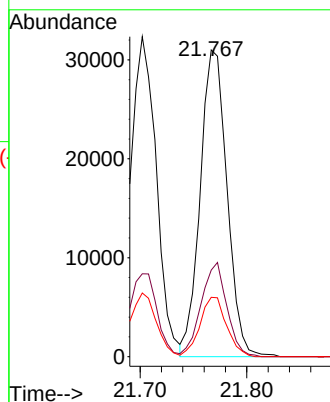

#89

Di-n-octyl phthalate

Concen: 3.553 ng/ul




RT: 22.836 min Scan# 3310


Delta R.T. -0.000 min

Lab File: BG053943.D

Acq: 20 Jun 2022 11:30

Tgt Ion:149 Resp: 37208









#90
Benzo(b)fluoranthene
Concen: 4.623 ng/ul
RT: 23.941 min Scan# 3498
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:252 Resp: 55823
Ion Ratio Lower Upper
252 100
253 23.5 18.2 27.4
125 4.9 6.1 9.1#



#91
Benzo(k)fluoranthene
Concen: 4.786 ng/ul
RT: 24.011 min Scan# 3510
Delta R.T. -0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:252 Resp: 55048
Ion Ratio Lower Upper
252 100
253 21.2 17.4 26.2
125 5.1 5.4 8.0#









#93
Benzo(a)pyrene
Concen: 4.713 ng/ul
RT: 24.822 min Scan# 3648
Delta R.T. -0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30




Instrument :
BNA_G
ClientSampleId :
SSTD005428


Tgt Ion:252 Resp: 54963
Ion Ratio Lower Upper
252 100
253 22.5 17.6 26.4
125 6.4 6.8 10.2#



#94
Indeno(1,2,3-cd)pyrene
Concen: 4.756 ng/ul
RT: 28.700 min Scan# 4308
Delta R.T. -0.000 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:276 Resp: 63624
Ion Ratio Lower Upper
276 100
138 9.8 10.1 15.1#
277 22.0 19.9 29.9









#95
Dibenzo(a,h)anthracene
Concen: 4.578 ng/ul
RT: 28.770 min Scan# 41
Delta R.T. 0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Instrument :
BNA_G
ClientSampleId :
SSTD005428

Tgt Ion:278 Resp: 52584
Ion Ratio Lower Upper
278 100
139 6.6 8.6 13.0#
279 20.4 19.4 29.0

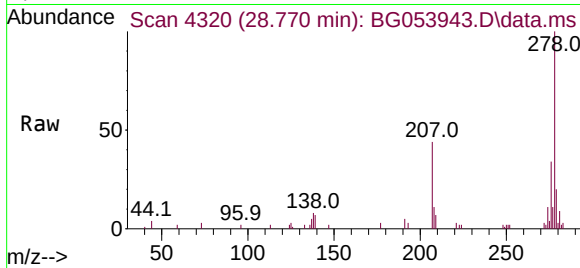

#96
Benzo(g,h,i)perylene
Concen: 4.801 ng/ul
RT: 29.863 min Scan# 4506
Delta R.T. 0.006 min
Lab File: BG053943.D
Acq: 20 Jun 2022 11:30

Tgt Ion:276 Resp: 54169
Ion Ratio Lower Upper
276 100
138 9.6 11.3 16.9#
277 22.0 18.6 27.8

