

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
 Data File : BG053961.D
 Acq On : 20 Jun 2022 23:11
 Operator : CG/JU
 Sample : N3358-19
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4T2

Quant Time: Jun 20 23:59:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.079	152	19986	20.000	ng/ul	0.00
20) Naphthalene-d8	10.887	136	78871	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.700	164	59834	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.444	188	164928	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.716	240	190256	20.000	ng/ul	# 0.00
88) Perylene-d12	24.977	264	193727	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.502	96	1986	4.728	ng/uL	0.00
4) Pyridine-d5	3.919	84	14026	12.277	ng/ul	0.00
7) Phenol-d5	7.239	99	186	0.130	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.397	67	27415	31.741	ng/ul	0.00
11) 2-Chlorophenol-d4	0.000	132	0	0.000	ng/ul	
15) 4-Methylphenol-d8	8.784	113	1926	1.578	ng/ul	0.00
21) Nitrobenzene-d5	9.236	128	19245	32.874	ng/ul	0.00
24) 2-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0	0.000	ng/ul	
31) 4-Chloroaniline-d4	11.011	131	51340	29.530	ng/ul	0.00
46) Dimethylphthalate-d6	14.101	166	171567	36.449	ng/ul	0.00
49) Acenaphthylene-d8	14.395	160	177816	34.740	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
60) Fluorene-d10	15.693	176	156561	37.029	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	17.544	188	293161	39.359	ng/ul	0.00
81) Pyrene-d10	19.830	212	396387	39.959	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.759	264	403546	41.267	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.215	107	4380	3.309	ng/ul#	Qvalue 18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
Data File : BG053961.D
Acq On : 20 Jun 2022 23:11
Operator : CG/JU
Sample : N3358-19
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4T2


Quant Time: Jun 20 23:59:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

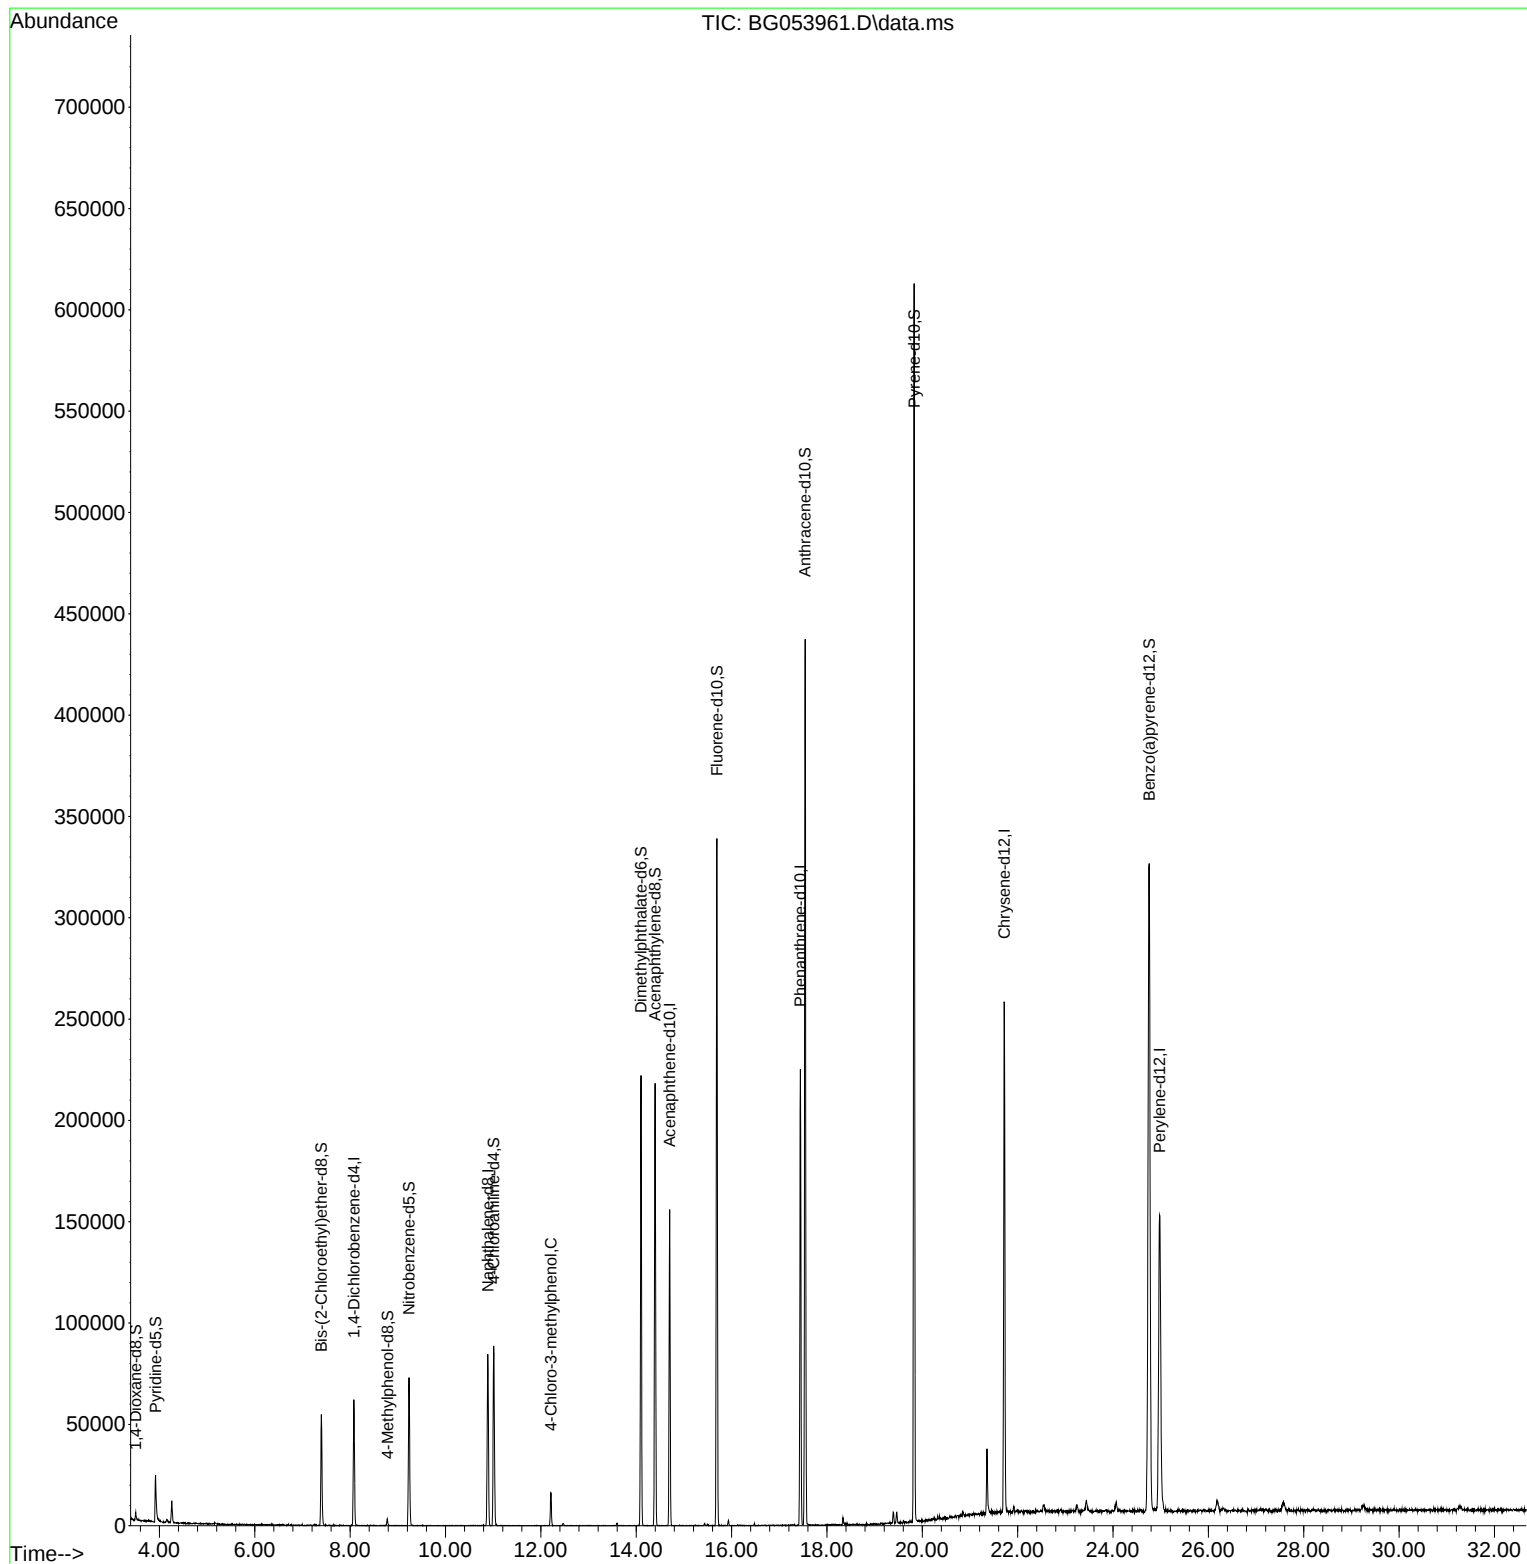

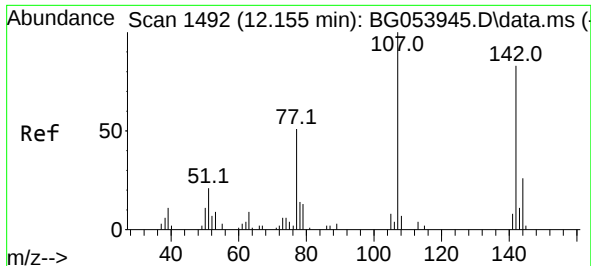

#35
 4-Chloro-3-methylphenol
 Concen: 3.309 ng/ul
 RT: 12.215 min Scan# 11
 Delta R.T. 0.061 min
 Lab File: BG053961.D
 Acq: 20 Jun 2022 23:11

Instrument :
 BNA_G
 ClientSampleId :
 EW4T2

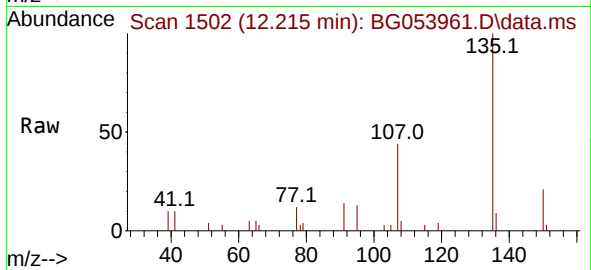

Tgt Ion:	107	Resp:	4380
Ion	Ratio	Lower	Upper
107	100		
144	0.0	21.3	31.9#
142	0.0	65.0	97.4#

