




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
Data File : BG053963.D
Acq On : 21 Jun 2022 00:29
Operator : CG/JU
Sample : N3358-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4S5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 02:39:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

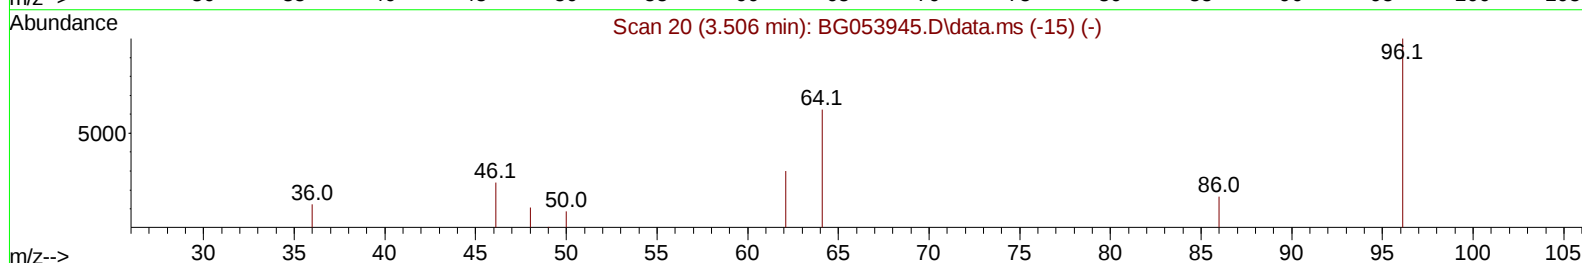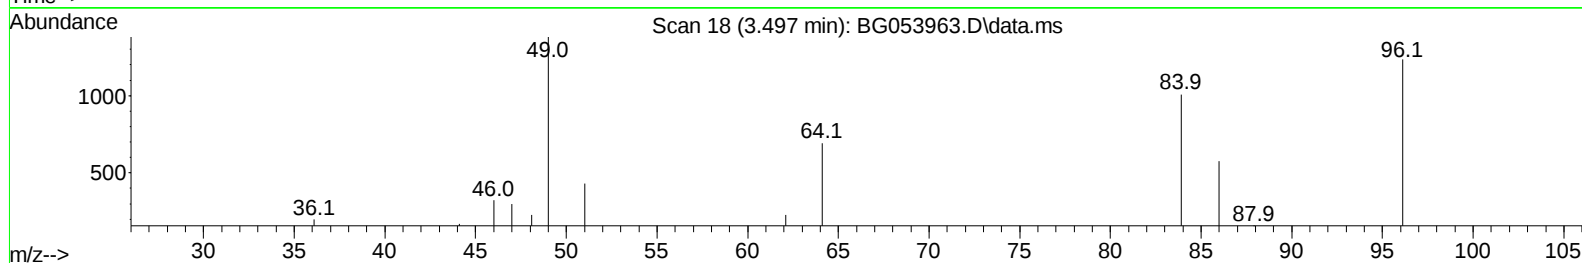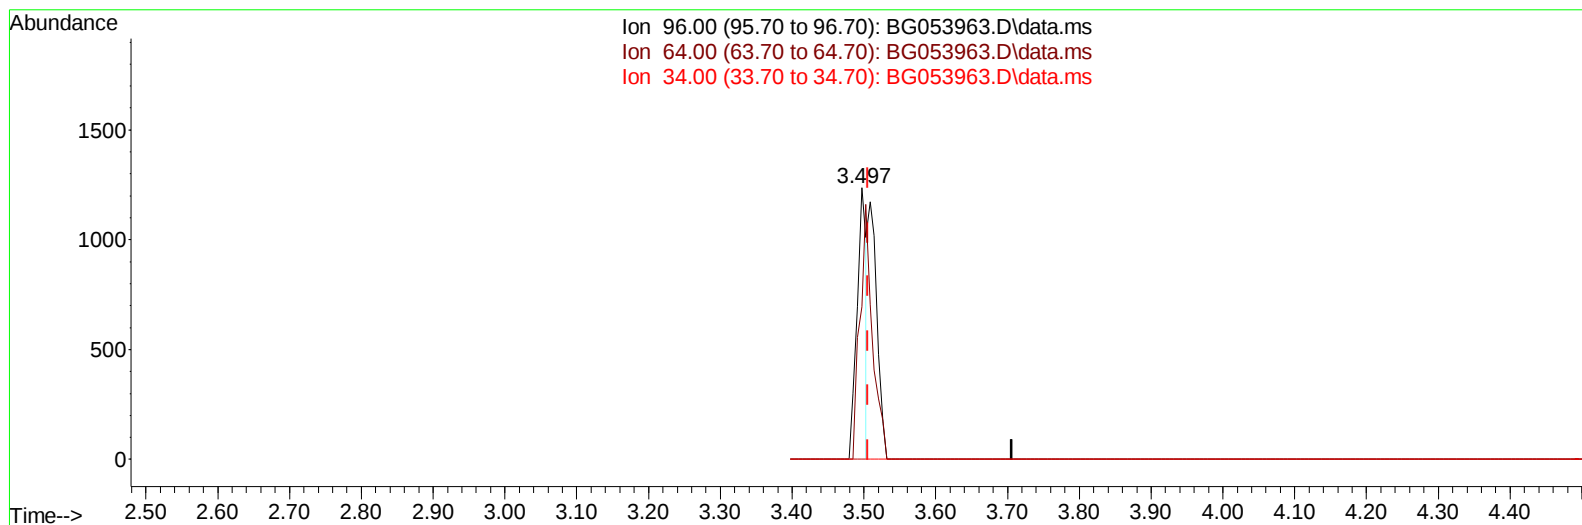

TIC: BG053963.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.497min (-0.009) 2.62 ng/uL

response 1142

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	73.20	56.15#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
 Data File : BG053963.D
 Acq On : 21 Jun 2022 00:29
 Operator : CG/JU
 Sample : N3358-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4S5

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:39:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

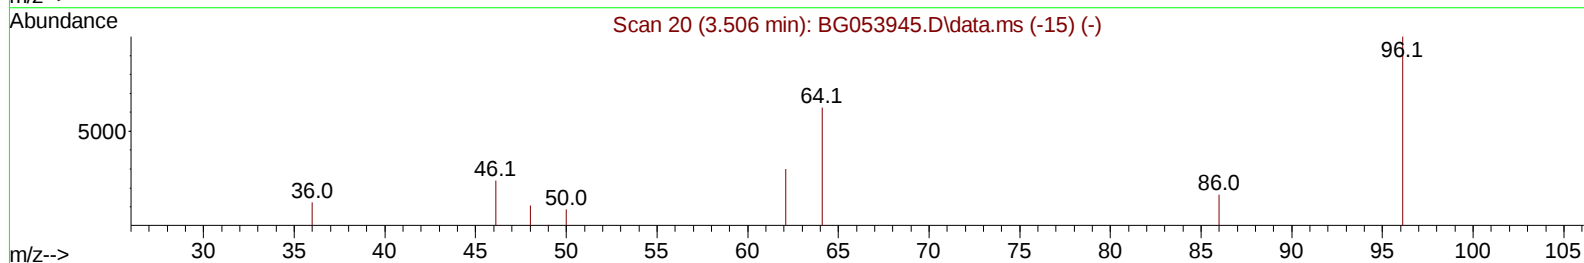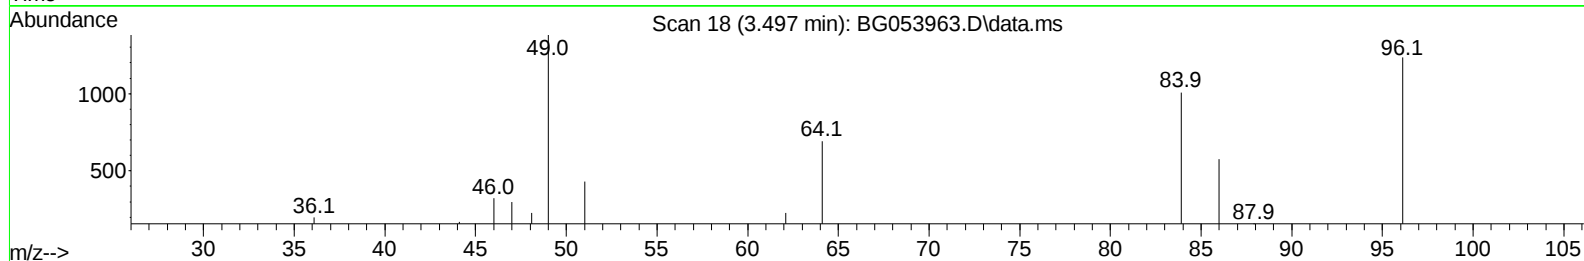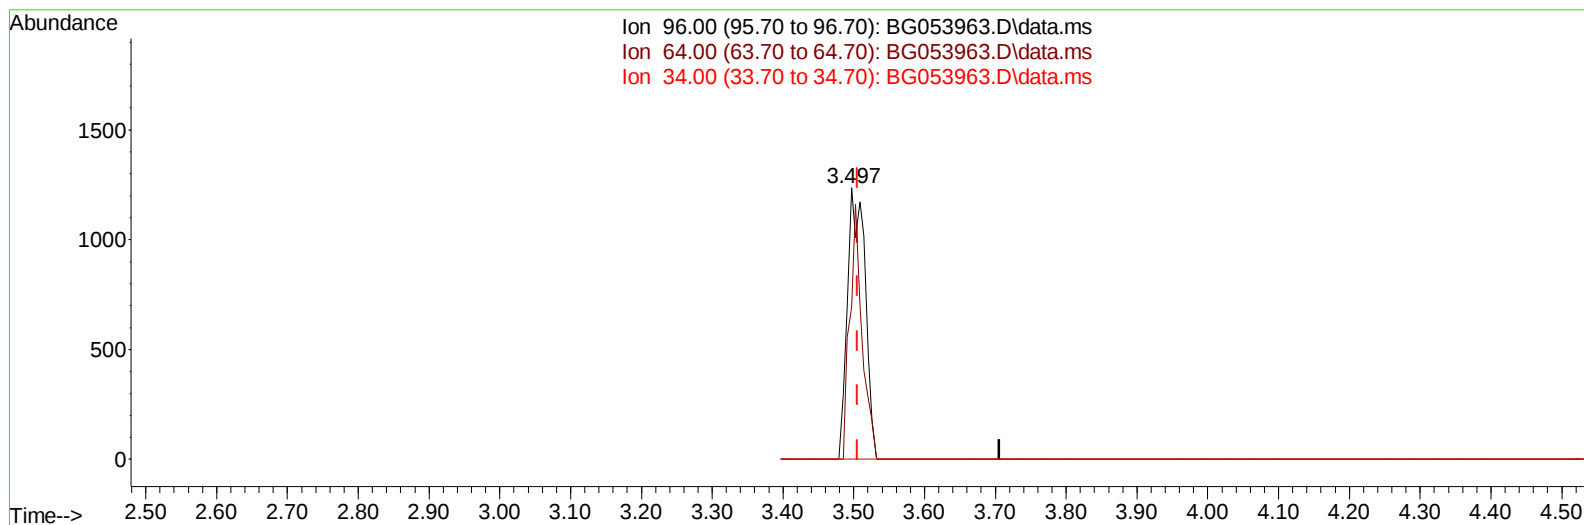

TIC: BG053963.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.497min (-0.009) 4.91 ng/uL m

response 2142

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	73.20	56.15#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
 Data File : BG053963.D
 Acq On : 21 Jun 2022 00:29
 Operator : CG/JU
 Sample : N3358-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4S5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 02:39:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.080	152	20766	20.000	ng/ul	0.00
20) Naphthalene-d8	10.888	136	83990	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.701	164	64185	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	172419	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.717	240	197873	20.000	ng/ul	# 0.00
88) Perylene-d12	24.978	264	200554	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.497	96	2142m	4.908	ng/uL	0.00
4) Pyridine-d5	3.920	84	9387	7.908	ng/ul	0.00
7) Phenol-d5	7.234	99	12092	8.128	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.398	67	28828	32.123	ng/ul	0.00
11) 2-Chlorophenol-d4	7.610	132	31196	26.296	ng/ul	0.00
15) 4-Methylphenol-d8	8.773	113	23352	18.409	ng/ul	0.00
21) Nitrobenzene-d5	9.237	128	19802	31.763	ng/ul	0.00
24) 2-Nitrophenol-d4	9.960	143	21062	31.797	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.500	165	45229	30.862	ng/ul	0.00
31) 4-Chloroaniline-d4	11.012	131	37283	20.137	ng/ul	0.00
46) Dimethylphthalate-d6	14.102	166	182062	36.056	ng/ul	0.00
49) Acenaphthylene-d8	14.396	160	183048	33.338	ng/ul	0.00
54) 4-Nitrophenol-d4	14.883	143	5572	8.059	ng/ul	0.00
60) Fluorene-d10	15.694	176	158647	34.978	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.800	200	32099	34.127	ng/ul	0.00
73) Anthracene-d10	17.545	188	303159	38.933	ng/ul	0.00
81) Pyrene-d10	19.825	212	410797	39.818	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.754	264	406409	40.145	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
Data File : BG053963.D
Acq On : 21 Jun 2022 00:29
Operator : CG/JU
Sample : N3358-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4S5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
Supervised By :mohammad ahmed 06/27/2022

Quant Time: Jun 21 02:39:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

