

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
 Data File : BG053961.D
 Acq On : 20 Jun 2022 23:11
 Operator : CG/JU
 Sample : N3358-19
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4T2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.502	16	19	28	rVB4	4019	5814	0.62%	0.093%
2	3.919	86	90	104	rBV	23062	41535	4.42%	0.665%
3	4.154	126	130	136	rVB3	1581	2911	0.31%	0.047%
4	4.260	142	148	156	rVB	11009	17529	1.87%	0.281%
5	5.135	293	297	300	rVB3	609	962	0.10%	0.015%
6	6.551	534	538	542	rBV	614	1298	0.14%	0.021%
7	7.256	656	658	663	rVB	805	1117	0.12%	0.018%
8	7.397	674	682	692	rBB	54869	94791	10.09%	1.518%
9	8.079	791	798	806	rBB	62208	108153	11.51%	1.732%
10	8.778	912	917	924	rBB3	3434	5369	0.57%	0.086%
11	9.236	988	995	1006	rBV	73144	135114	14.38%	2.163%
12	10.887	1268	1276	1285	rBB	84688	156204	16.63%	2.501%
13	11.011	1291	1297	1305	rBV	88792	167611	17.84%	2.683%
14	12.209	1495	1501	1507	rBB2	16401	26567	2.83%	0.425%
15	12.468	1541	1545	1549	rBB2	1137	2016	0.21%	0.032%
16	13.590	1733	1736	1741	rBB	1185	1867	0.20%	0.030%
17	14.101	1817	1823	1834	rBB	222176	333783	35.53%	5.344%
18	14.395	1866	1873	1882	rBB	218314	366841	39.05%	5.873%
19	14.700	1918	1925	1932	rBB	156016	245465	26.13%	3.930%
20	15.435	2046	2050	2054	rBB2	1205	1588	0.17%	0.025%
21	15.494	2055	2060	2063	rBB	863	1058	0.11%	0.017%
22	15.693	2087	2094	2103	rBB	339104	541926	57.69%	8.676%
23	15.934	2130	2135	2140	rBB3	2724	3830	0.41%	0.061%
24	16.481	2223	2228	2230	rBB	1252	1256	0.13%	0.020%
25	17.444	2383	2392	2401	rBV	225161	353792	37.66%	5.664%
26	17.544	2402	2409	2417	rVV	436924	681967	72.60%	10.918%
27	18.337	2540	2544	2549	rBV3	3695	5444	0.58%	0.087%
28	19.131	2677	2679	2684	rBV2	846	998	0.11%	0.016%
29	19.389	2720	2723	2728	rVV2	5674	8778	0.93%	0.141%
30	19.465	2728	2736	2742	rVV	5683	9869	1.05%	0.158%
31	19.642	2764	2766	2770	rBV3	939	1402	0.15%	0.022%
32	19.742	2780	2783	2787	rVB3	1229	1363	0.15%	0.022%
33	19.830	2791	2798	2809	rBV	611388	908198	96.68%	14.540%
34	19.947	2816	2818	2823	rVB2	883	1148	0.12%	0.018%
35	20.141	2847	2851	2854	rBV2	1015	1165	0.12%	0.019%
36	20.259	2867	2871	2872	rVB3	1405	1621	0.17%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
 Data File : BG053961.D
 Acq On : 20 Jun 2022 23:11
 Operator : CG/JU
 Sample : N3358-19
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4T2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.276	2872	2874	2878	rBV3	831	1046	0.11%	0.017%
38	20.323	2880	2882	2885	rVV3	1817	1652	0.18%	0.026%
39	20.359	2886	2888	2890	rVB2	1837	1305	0.14%	0.021%
40	20.735	2949	2952	2953	rBV2	953	1215	0.13%	0.019%
41	20.782	2957	2960	2962	rBV2	1548	2162	0.23%	0.035%
42	20.852	2970	2972	2977	rVB4	2070	2472	0.26%	0.040%
43	20.911	2980	2982	2985	rBV3	1228	1182	0.13%	0.019%
44	21.281	3042	3045	3046	rBV3	1851	1841	0.20%	0.029%
45	21.310	3049	3050	3052	rVV2	1278	948	0.10%	0.015%
46	21.357	3052	3058	3071	rVV2	32506	55007	5.86%	0.881%
47	21.669	3107	3111	3112	rBV3	1596	1705	0.18%	0.027%
48	21.716	3112	3119	3128	rVV2	252263	445212	47.39%	7.128%
49	21.892	3148	3149	3151	rBV2	1308	1288	0.14%	0.021%
50	21.921	3151	3154	3157	rVB4	3327	4495	0.48%	0.072%
51	22.386	3232	3233	3235	rBV2	1506	1080	0.11%	0.017%
52	22.532	3255	3258	3260	rBV3	3126	4225	0.45%	0.068%
53	23.226	3375	3376	3377	rBV	1858	1164	0.12%	0.019%
54	23.243	3377	3379	3384	rVB6	3560	4714	0.50%	0.075%
55	23.343	3393	3396	3397	rBV3	1721	1810	0.19%	0.029%
56	23.443	3408	3413	3417	rBV5	4908	9468	1.01%	0.152%
57	23.702	3454	3457	3459	rBV2	1165	1460	0.16%	0.023%
58	24.066	3514	3519	3525	rVB6	4940	10669	1.14%	0.171%
59	24.113	3525	3527	3529	rBV3	1217	976	0.10%	0.016%
60	24.560	3601	3603	3606	rBV3	1691	2144	0.23%	0.034%
61	24.759	3625	3637	3651	rVB2	319138	939397	100.00%	15.040%
62	24.977	3665	3674	3691	rVV3	145659	453641	48.29%	7.263%
63	25.106	3694	3696	3699	rBV5	1489	996	0.11%	0.016%
64	25.529	3767	3768	3770	rBV2	1383	1075	0.11%	0.017%
65	25.552	3770	3772	3773	rBV2	1257	1025	0.11%	0.016%
66	25.782	3809	3811	3814	rBV4	1280	1237	0.13%	0.020%
67	26.187	3873	3880	3889	rVB9	5742	18757	2.00%	0.300%
68	26.827	3987	3989	3995	rBV5	2199	4012	0.43%	0.064%
69	26.986	4014	4016	4018	rVB3	1346	1194	0.13%	0.019%
70	27.356	4077	4079	4082	rBV2	1290	1267	0.13%	0.020%
71	27.462	4095	4097	4099	rBV2	1332	1161	0.12%	0.019%
72	27.527	4106	4108	4109	rBV2	1579	1308	0.14%	0.021%
73	27.562	4111	4114	4115	rBV2	2255	2576	0.27%	0.041%
74	28.085	4201	4203	4205	rBV3	1222	1092	0.12%	0.017%
75	28.461	4265	4267	4270	rVB3	1557	1542	0.16%	0.025%
76	28.884	4337	4339	4341	rBV3	1280	1414	0.15%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
 Data File : BG053961.D
 Acq On : 20 Jun 2022 23:11
 Operator : CG/JU
 Sample : N3358-19
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4T2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	29.477	4438	4440	4442	rBV2	1987	1619	0.17%	0.026%
78	30.106	4546	4547	4550	rVB3	1265	959	0.10%	0.015%
79	30.723	4650	4652	4654	rBV3	1447	952	0.10%	0.015%
80	30.870	4675	4677	4679	rBV3	1303	1009	0.11%	0.016%
81	31.005	4698	4700	4703	rBV4	1205	943	0.10%	0.015%
82	31.234	4733	4739	4741	rBV5	1968	4562	0.49%	0.073%
83	31.258	4741	4743	4746	rVV3	1873	2147	0.23%	0.034%
84	31.775	4829	4831	4832	rBV	1650	1239	0.13%	0.020%
85	32.151	4894	4895	4898	rVB3	2031	1385	0.15%	0.022%



Sum of corrected areas: 6246099

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
Data File : BG053961.D
Acq On : 20 Jun 2022 23:11
Operator : CG/JU
Sample : N3358-19
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4T2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

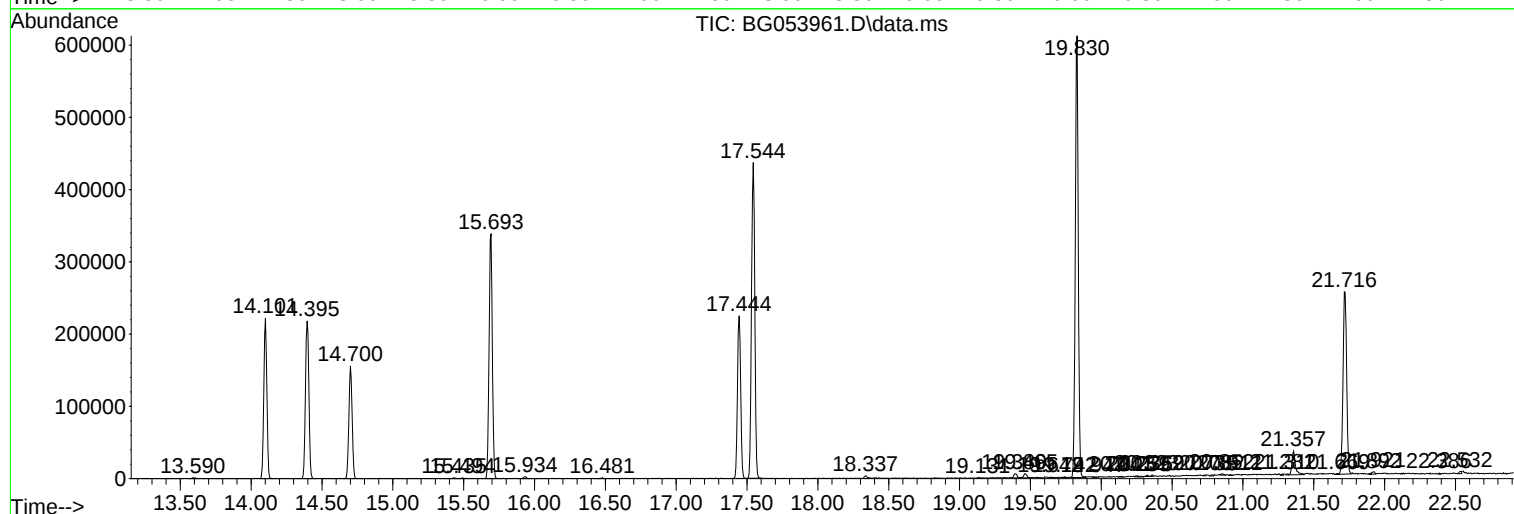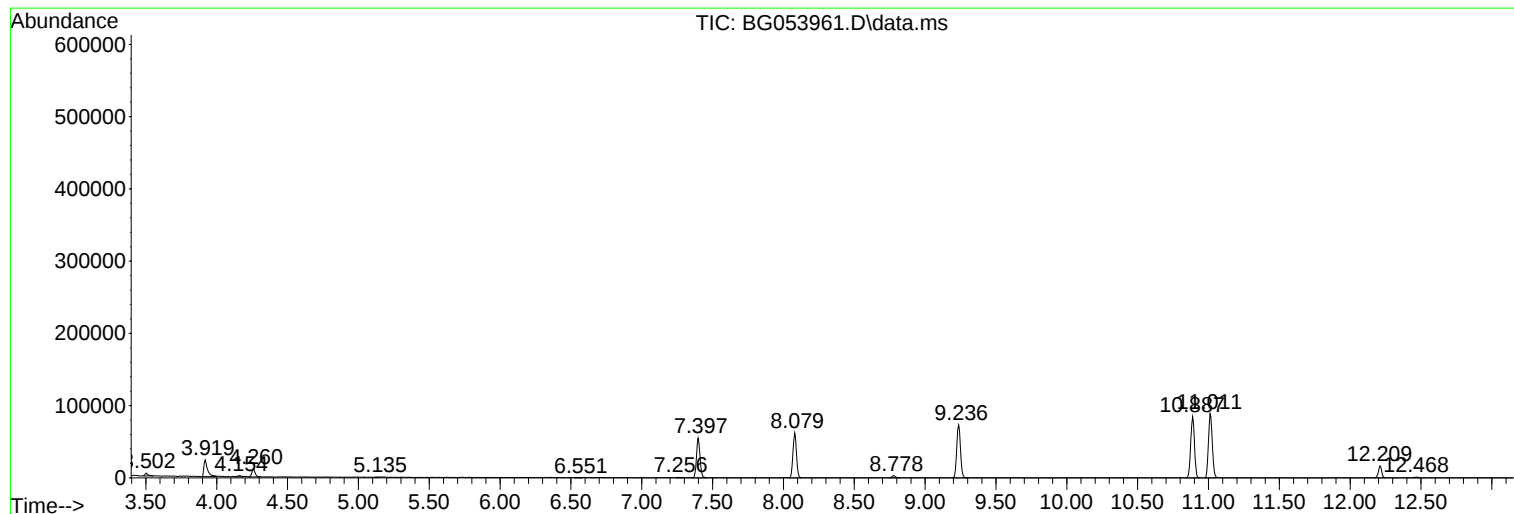

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
Data File : BG053961.D
Acq On : 20 Jun 2022 23:11
Operator : CG/JU
Sample : N3358-19
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4T2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
Data File : BG053961.D
Acq On : 20 Jun 2022 23:11
Operator : CG/JU
Sample : N3358-19
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4T2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------