


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062022\
 Data File : BG053942.D
 Acq On : 20 Jun 2022 10:42
 Operator : CG/JU
 Sample : DFTPP478
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP478

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION
 Last Update : Mon Jun 20 15:29:13 2022

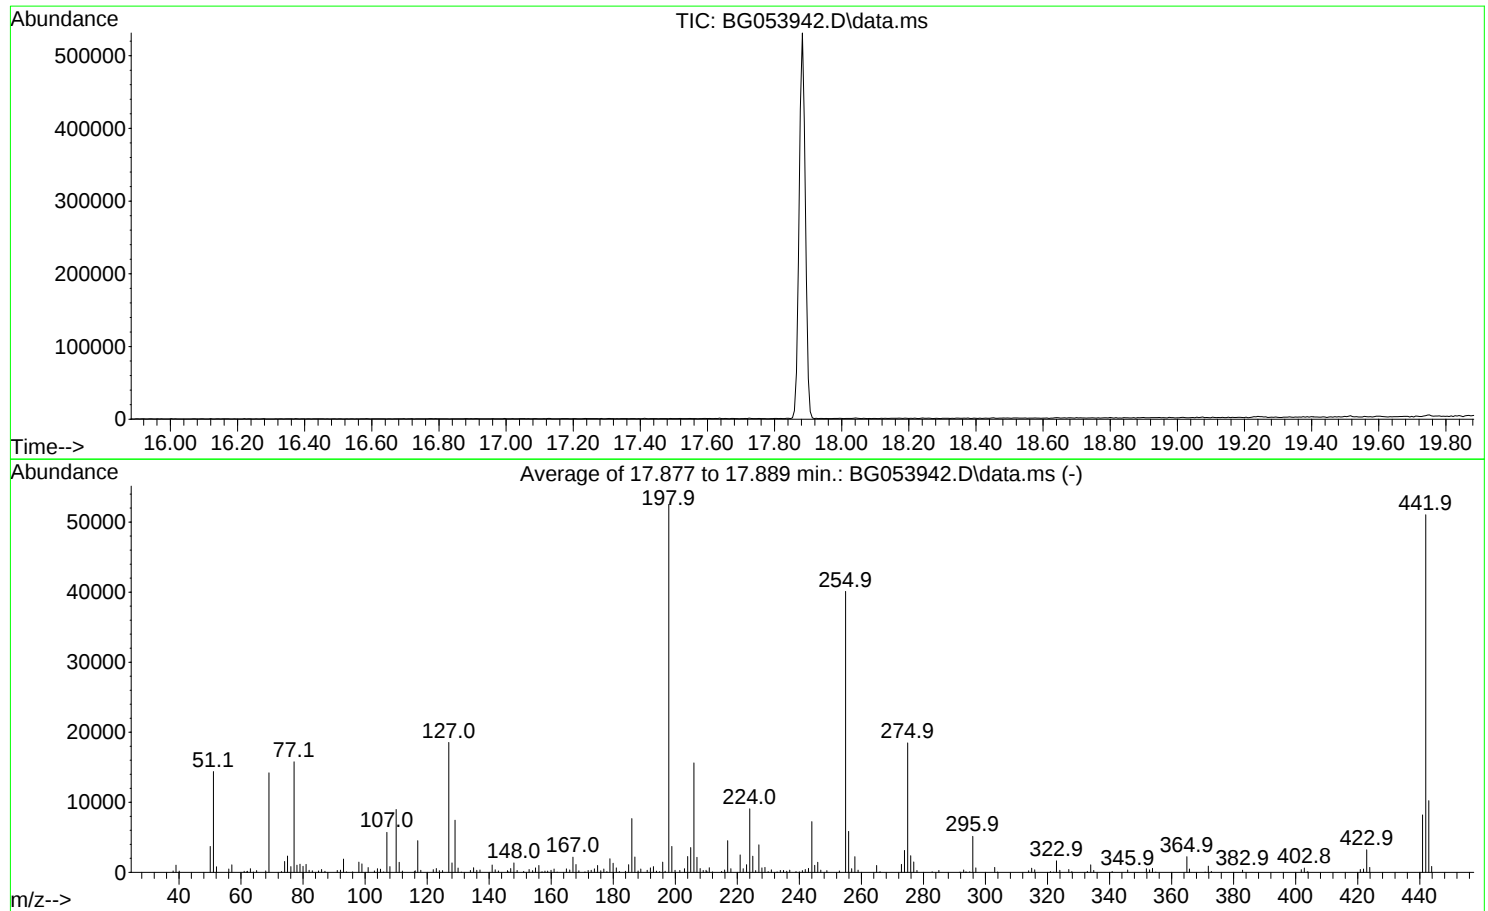

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	14391	PASS
68	69	0.00	2	1.5	217	PASS
69	198	0.00	100	27.0	14198	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.3	18539	PASS
197	198	0.00	2	0.3	153	PASS
198	198	100	100	100.0	52509	PASS
199	198	5	9	7.0	3695	PASS
275	198	10	60	35.2	18469	PASS
365	198	1	100	4.2	2230	PASS
441	198	0.01	100	15.6	8192	PASS
442	198	50	100	97.2	51053	PASS
443	442	15	24	20.0	10226	PASS

Scan 2460 (17.842 min): BG053942.D\data.ms
DFTPP478

m/z	Abundance
44.10	359.0
207.00	603.0
208.00	206.0
208.90	153.0

Instrument :
BNA_G
ClientSampleId :
DFTPP478

m/z	Abundance
38.10	260.0
39.10	1089.0
40.00	212.0
44.10	279.0
50.10	4200.0
51.10	15319.0
52.10	892.0
56.10	524.0
57.00	1294.0
61.90	272.0
63.10	615.0
65.10	362.0
69.00	14820.0
73.10	171.0
74.00	1558.0
75.00	2278.0
76.10	822.0
77.10	16536.0
78.00	1113.0
79.00	1321.0
80.00	896.0
81.00	1352.0
81.90	351.0
83.00	296.0
85.10	228.0
86.00	438.0
87.00	249.0
91.00	243.0
92.10	301.0
93.10	1692.0
98.00	1595.0
99.00	1325.0
101.00	645.0
103.10	201.0
104.00	423.0
105.00	479.0
107.00	5853.0
108.00	926.0
110.00	9111.0
111.00	1380.0
112.00	237.0
116.20	284.0
117.00	4779.0
117.90	265.0
122.00	355.0
123.00	530.0
124.00	217.0
125.00	251.0
127.00	18464.0
128.00	1232.0
129.00	7376.0
130.00	553.0
133.90	253.0
135.00	580.0
136.00	330.0
137.00	421.0
140.90	1027.0
142.00	309.0
143.00	219.0
146.00	289.0
147.00	581.0
148.00	1294.0
149.00	335.0
151.20	227.0
152.90	490.0
154.00	219.0
155.00	600.0
156.00	943.0
158.00	266.0
158.90	186.0
159.90	339.0
160.90	451.0
164.90	565.0
166.00	352.0
167.00	2378.0
168.00	1311.0
168.90	256.0
171.90	235.0
172.90	380.0
173.80	450.0
174.90	1021.0
176.00	237.0
177.00	472.0
177.90	201.0
178.90	1966.0
180.00	1156.0
181.00	594.0
182.00	153.0
184.00	189.0
185.00	1191.0
186.00	7711.0
187.00	2168.0

Instrument :

BNA_G

ClientSampleId :

DFTPP478

188.00	198.0
188.90	561.0
191.00	342.0
191.90	635.0
192.90	746.0
194.00	171.0
195.00	187.0
195.90	1465.0
197.90	50864.0
198.90	3487.0
199.90	220.0
201.50	195.0
203.00	498.0
204.00	2205.0
204.90	3367.0
206.00	15218.0
207.00	2597.0
208.00	664.0
208.80	259.0
210.00	326.0
210.90	595.0
212.00	174.0
214.90	235.0
216.00	286.0
216.90	3970.0
217.90	500.0
220.90	2490.0
221.80	483.0
223.00	1038.0
224.00	8802.0
225.00	2196.0
225.90	218.0
227.00	3366.0
227.90	691.0
228.90	635.0
229.90	154.0
230.90	370.0
233.90	280.0
234.80	327.0
235.90	187.0
236.90	298.0
241.00	273.0
241.90	350.0
242.90	550.0
244.00	7162.0
245.00	1106.0
245.90	1241.0
246.90	332.0
248.90	225.0
253.00	236.0
254.90	36368.0
255.90	5117.0
256.80	522.0
257.90	1969.0
258.90	296.0
264.90	888.0
266.10	176.0
272.90	1134.0
273.90	2916.0
274.90	16496.0
275.90	2349.0
276.90	1280.0
277.90	317.0
285.00	188.0
292.90	351.0
295.90	4410.0
296.90	634.0
303.00	784.0
313.90	233.0
314.90	498.0
315.90	299.0
320.90	172.0
322.00	169.0
322.90	1245.0
323.90	229.0
326.80	285.0
332.90	238.0
333.90	901.0
335.00	247.0
345.80	191.0
351.90	488.0
352.90	221.0
353.90	412.0
354.90	151.0
364.90	1794.0
365.80	380.0
371.80	740.0
382.80	246.0
401.80	344.0
402.80	537.0
420.90	355.0
421.80	344.0
422.90	2674.0
423.80	616.0
440.90	6211.0
441.90	39096.0

Instrument :
BNA_G
ClientSampleId :
DFTPP478

442.908367.0

443.90851.0

Instrument :
BNA_G
ClientSampleId :
DFTPP478

m/z	Abundance
38.20	188.0
39.00	1233.0
40.10	152.0
44.10	400.0
50.10	4038.0
51.10	17152.0
52.10	996.0
56.00	549.0
57.10	1198.0
61.00	252.0
62.10	298.0
63.10	564.0
64.00	155.0
65.00	425.0
68.00	320.0
69.00	16350.0
73.00	186.0
74.10	1836.0
75.00	2786.0
76.10	1060.0
77.10	18088.0
78.10	1137.0
79.00	1241.0
80.00	1072.0
81.00	1317.0
82.00	358.0
83.00	249.0
85.00	192.0
86.00	518.0
87.10	218.0
91.10	364.0
92.00	352.0
93.00	2434.0
94.00	221.0
98.00	1723.0
99.00	1460.0
101.00	822.0
103.00	222.0
104.00	636.0
104.90	487.0
106.00	217.0
107.00	6800.0
108.00	846.0
110.00	10718.0
111.00	1784.0
112.00	324.0
116.10	412.0
117.00	5312.0
118.00	384.0
122.00	444.0
122.90	627.0
124.00	313.0
124.90	253.0
127.00	21944.0
128.00	1660.0
129.00	8747.0
130.00	821.0
131.00	165.0
134.00	271.0
135.00	861.0
136.00	280.0
137.10	356.0
141.00	1205.0
141.90	441.0
142.90	263.0
145.80	193.0
146.30	192.0
147.00	645.0
148.00	1610.0
148.90	300.0
151.00	159.0
152.90	485.0
154.00	328.0
155.00	789.0
156.00	1264.0
156.80	157.0
157.10	188.0
158.00	270.0
158.90	156.0
159.90	316.0
160.90	625.0
161.90	163.0
164.90	625.0
166.00	369.0
167.00	2319.0
168.00	1304.0
168.90	286.0
170.90	197.0
171.90	405.0
172.90	280.0
173.90	605.0
175.00	1221.0

Instrument :
BNA_G
ClientSampleId :
DFTPP478

176.00	245.0
176.90	540.0
178.00	176.0
178.90	2257.0
180.00	1676.0
181.00	684.0
181.90	160.0
183.90	269.0
184.90	1176.0
186.00	8759.0
186.90	2692.0
188.00	152.0
189.00	535.0
190.90	261.0
192.00	820.0
193.00	874.0
193.90	219.0
194.90	169.0
195.90	1628.0
197.90	60104.0
198.90	4270.0
199.90	374.0
201.40	358.0
202.90	651.0
204.00	2580.0
205.00	4360.0
206.00	18080.0
207.00	3075.0
208.00	921.0
209.00	469.0
209.80	313.0
210.20	395.0
211.00	897.0
215.00	213.0
215.90	491.0
216.90	5324.0
217.90	627.0
220.90	2777.0
221.90	660.0
222.90	1435.0
224.00	10464.0
225.00	2660.0
225.90	307.0
226.90	4803.0
227.90	630.0
228.90	914.0
230.00	193.0
231.00	434.0
232.80	203.0
233.80	264.0
234.90	243.0
235.90	301.0
236.90	375.0
238.90	189.0
240.00	224.0
240.90	314.0
241.90	535.0
243.00	667.0
244.00	7920.0
244.90	1056.0
245.90	1699.0
246.90	409.0
248.90	338.0
252.90	224.0
254.90	46520.0
255.90	7101.0
256.90	533.0
257.90	2452.0
258.90	419.0
264.90	976.0
265.80	153.0
272.90	1275.0
273.90	3465.0
274.90	21456.0
275.90	2743.0
276.90	1668.0
277.90	301.0
282.80	270.0
284.90	395.0
291.80	158.0
293.00	377.0
293.60	156.0
294.90	271.0
295.90	6007.0
296.90	843.0
303.00	763.0
313.90	262.0
314.90	592.0
315.90	413.0
322.90	2048.0
323.90	315.0
326.90	528.0
327.90	155.0
333.90	1101.0
334.80	309.0
340.80	169.0

Instrument :
BNA_G
ClientSampleId :
DFTPP478

345.80	436.0
351.80	543.0
352.90	406.0
353.90	733.0
364.90	2837.0
365.70	516.0
370.80	166.0
371.90	1246.0
372.80	215.0
382.90	443.0
401.90	391.0
402.80	718.0
403.70	197.0
420.80	456.0
421.90	558.0
422.90	3649.0
423.90	854.0
440.90	9521.0
441.90	59504.0
442.90	11632.0
443.80	798.0

Instrument :
BNA_G
ClientSampleId :
DFTPP478

m/z	Abundance
38.00	166.0
39.10	791.0
40.00	208.0
44.00	332.0
50.10	2881.0
51.10	10703.0
52.10	520.0
56.00	366.0
57.00	762.0
61.00	205.0
62.00	200.0
63.00	403.0
68.00	332.0
69.00	11424.0
74.10	1240.0
75.00	1946.0
76.00	602.0
77.10	12737.0
78.00	846.0
79.00	946.0
79.90	623.0
81.00	743.0
82.00	207.0
83.00	163.0
84.90	198.0
86.00	290.0
91.00	192.0
92.00	305.0
93.00	1561.0
96.00	191.0
98.00	1101.0
99.00	878.0
101.00	611.0
102.90	182.0
104.00	503.0
105.00	402.0
107.00	4479.0
108.00	677.0
110.00	7121.0
111.00	1149.0
115.90	348.0
117.00	3495.0
118.00	214.0
122.00	350.0
123.00	472.0
123.90	205.0
125.00	224.0
127.00	15210.0
128.00	1168.0
129.00	6201.0
130.00	449.0
134.00	270.0
135.00	581.0
136.00	262.0
137.10	289.0
141.00	935.0
142.00	318.0
143.00	161.0
145.90	283.0
146.90	437.0
148.00	1128.0
149.10	214.0
153.00	249.0
154.00	219.0
154.90	564.0
156.00	748.0
158.80	194.0
160.00	236.0
160.90	361.0
165.00	338.0
166.00	334.0
167.00	1844.0
167.90	717.0
169.00	159.0
171.90	201.0
172.90	251.0
174.00	463.0
175.00	680.0
176.00	241.0
176.90	436.0
178.90	1631.0
179.90	1064.0
181.00	623.0
185.00	926.0
186.00	6570.0
187.00	1731.0
188.00	280.0
188.80	363.0
190.90	295.0
192.00	469.0
193.00	833.0
194.00	168.0

Instrument :
BNA_G
ClientSampleId :
DFTPP478

196.00	1306.0
196.70	459.0
197.90	46560.0
198.90	3327.0
199.90	286.0
201.40	276.0
202.90	449.0
204.00	2029.0
205.00	2915.0
206.00	13555.0
207.00	2615.0
208.00	647.0
209.00	331.0
209.90	236.0
210.90	479.0
215.80	249.0
216.90	4246.0
217.90	476.0
220.90	2214.0
222.00	427.0
222.90	806.0
224.00	7919.0
225.00	2084.0
225.90	232.0
226.90	3643.0
227.90	613.0
228.90	593.0
230.90	300.0
233.90	289.0
235.00	261.0
236.90	262.0
238.90	192.0
240.90	187.0
241.90	364.0
243.00	497.0
244.00	6618.0
244.90	870.0
245.90	1376.0
246.90	236.0
248.70	168.0
252.80	168.0
254.90	37416.0
255.90	5340.0
256.90	512.0
257.90	2275.0
258.90	232.0
264.90	1119.0
272.90	1044.0
273.90	3008.0
274.90	17456.0
275.90	2048.0
276.80	1504.0
277.90	217.0
285.00	267.0
292.90	273.0
293.90	168.0
295.90	5034.0
296.80	419.0
302.90	613.0
303.90	151.0
313.80	161.0
314.90	717.0
315.80	356.0
320.90	153.0
322.90	1631.0
324.00	352.0
326.80	450.0
327.80	196.0
332.80	193.0
333.90	1203.0
334.90	240.0
340.90	216.0
345.90	416.0
351.80	524.0
352.90	449.0
353.80	545.0
364.90	2059.0
365.80	548.0
371.90	700.0
372.80	176.0
382.80	258.0
401.70	453.0
402.80	630.0
403.90	275.0
420.80	441.0
421.90	571.0
422.90	3320.0
423.90	680.0
440.90	8845.0
441.90	54560.0
442.90	10679.0
443.80	876.0

Instrument :
BNA_G
ClientSampleId :
DFTPP478