
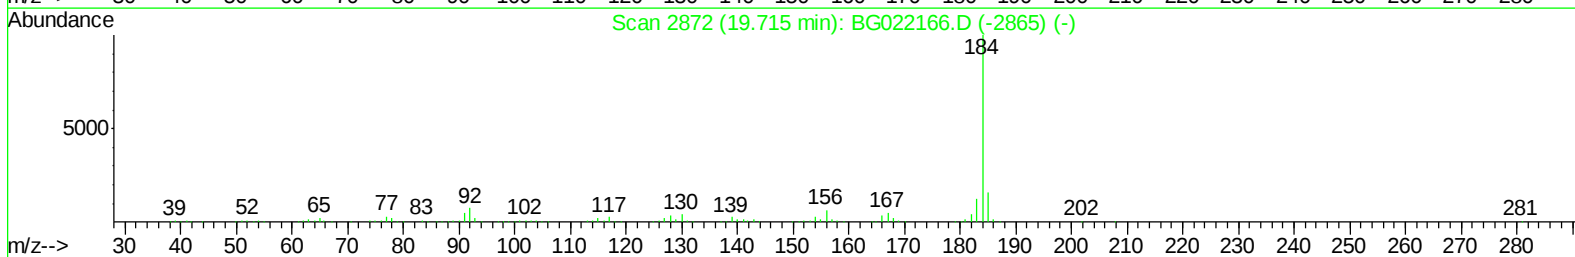
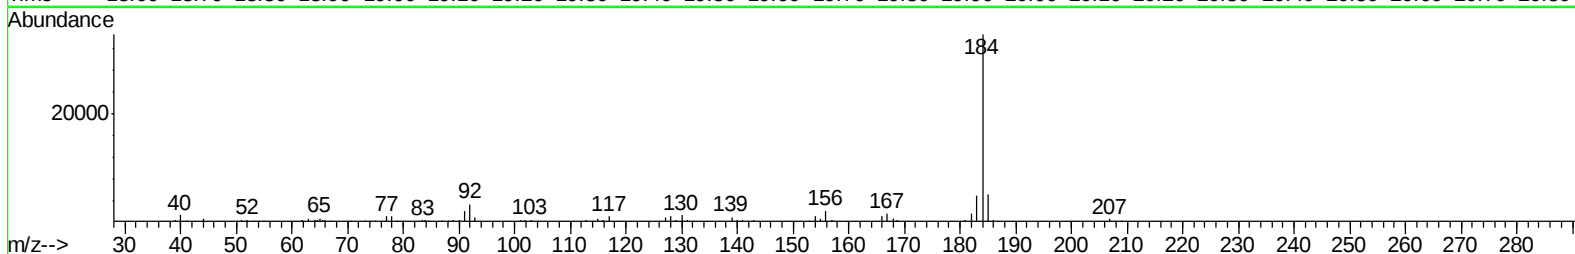


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062116\
Data File : BG022467.D
Acq On : 21 Jun 2016 15:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 07:24:21 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:27:56 2016
Response via : Initial Calibration

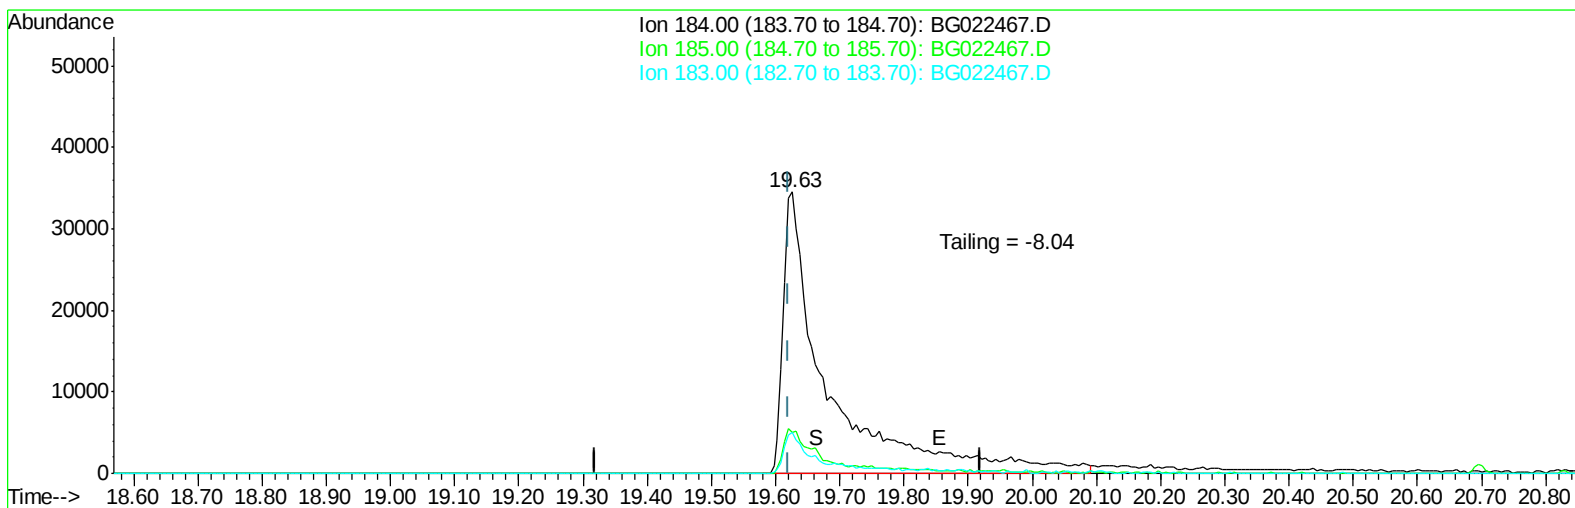

TIC: BG022467.D

(76) Benzidine




19.626min (+0.007) 0.00ng m

response 166665

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.69
183.00	12.80	14.41
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062116\
Data File : BG022467.D
Acq On : 21 Jun 2016 15:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 07:24:21 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:27:56 2016
Response via : Initial Calibration

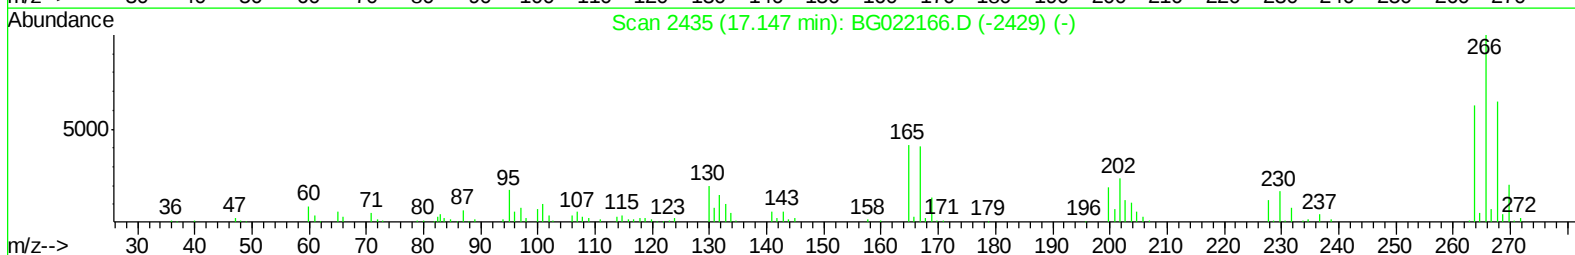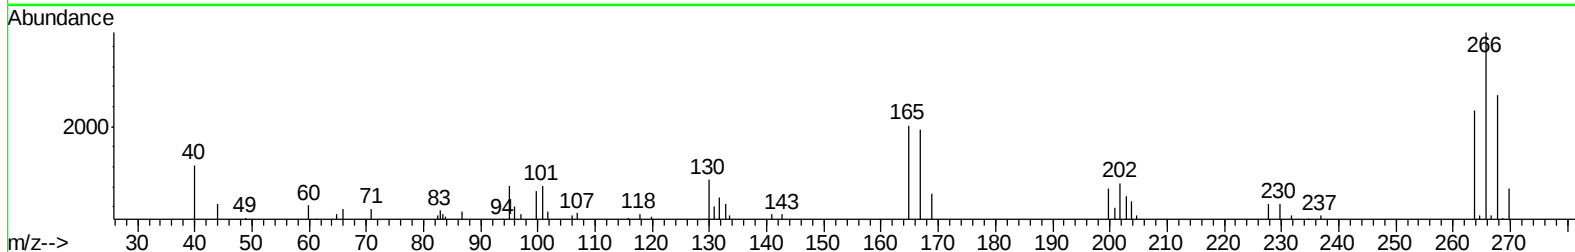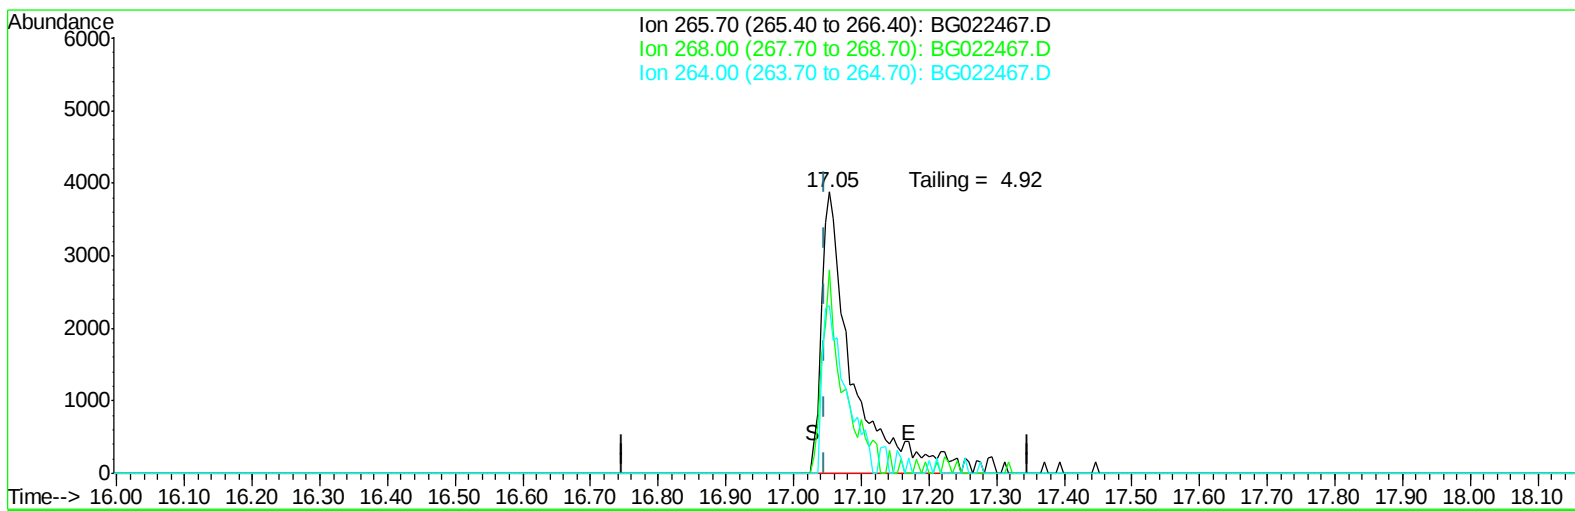

TIC: BG022467.D

(69) Pentachlorophenol (C)

17.053min (+0.007) 0.00ng

response 11045

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	72.24
264.00	67.20	65.44
0.00	0.00	0.00