

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062116\
 Data File : BG022473.D
 Acq On : 21 Jun 2016 19:34
 Operator : UM/SJ
 Sample : H3631-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PL-DA-6-COMP

Quant Time: Jun 22 02:22:00 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 22 02:15:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	20468	20.00	ng	0.00
21) Naphthalene-d8	10.81	136	95429	20.00	ng	0.00
38) Acenaphthene-d10	14.63	164	61238	20.00	ng	0.00
63) Phenanthrene-d10	17.38	188	140725	20.00	ng	0.00
75) Chrysene-d12	21.64	240	117585	20.00	ng	0.00
86) Perylene-d12	24.85	264	72144	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.54	112	174329	164.68	ng	0.00
7) Phenol-d6	7.17	99	237770	142.85	ng	0.00
23) Nitrobenzene-d5	9.16	82	135993	99.35	ng	0.00
41) 2,4,6-Tribromophenol	16.13	330	83994	121.39	ng	0.00
44) 2-Fluorobiphenyl	13.25	172	388712	96.73	ng	0.00
78) Terphenyl-d14	19.98	244	551077	111.27	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062116\
Data File : BG022473.D
Acq On : 21 Jun 2016 19:34
Operator : UM/SJ
Sample : H3631-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-DA-6-COMP

Quant Time: Jun 22 02:22:00 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 02:15:22 2016
Response via : Initial Calibration

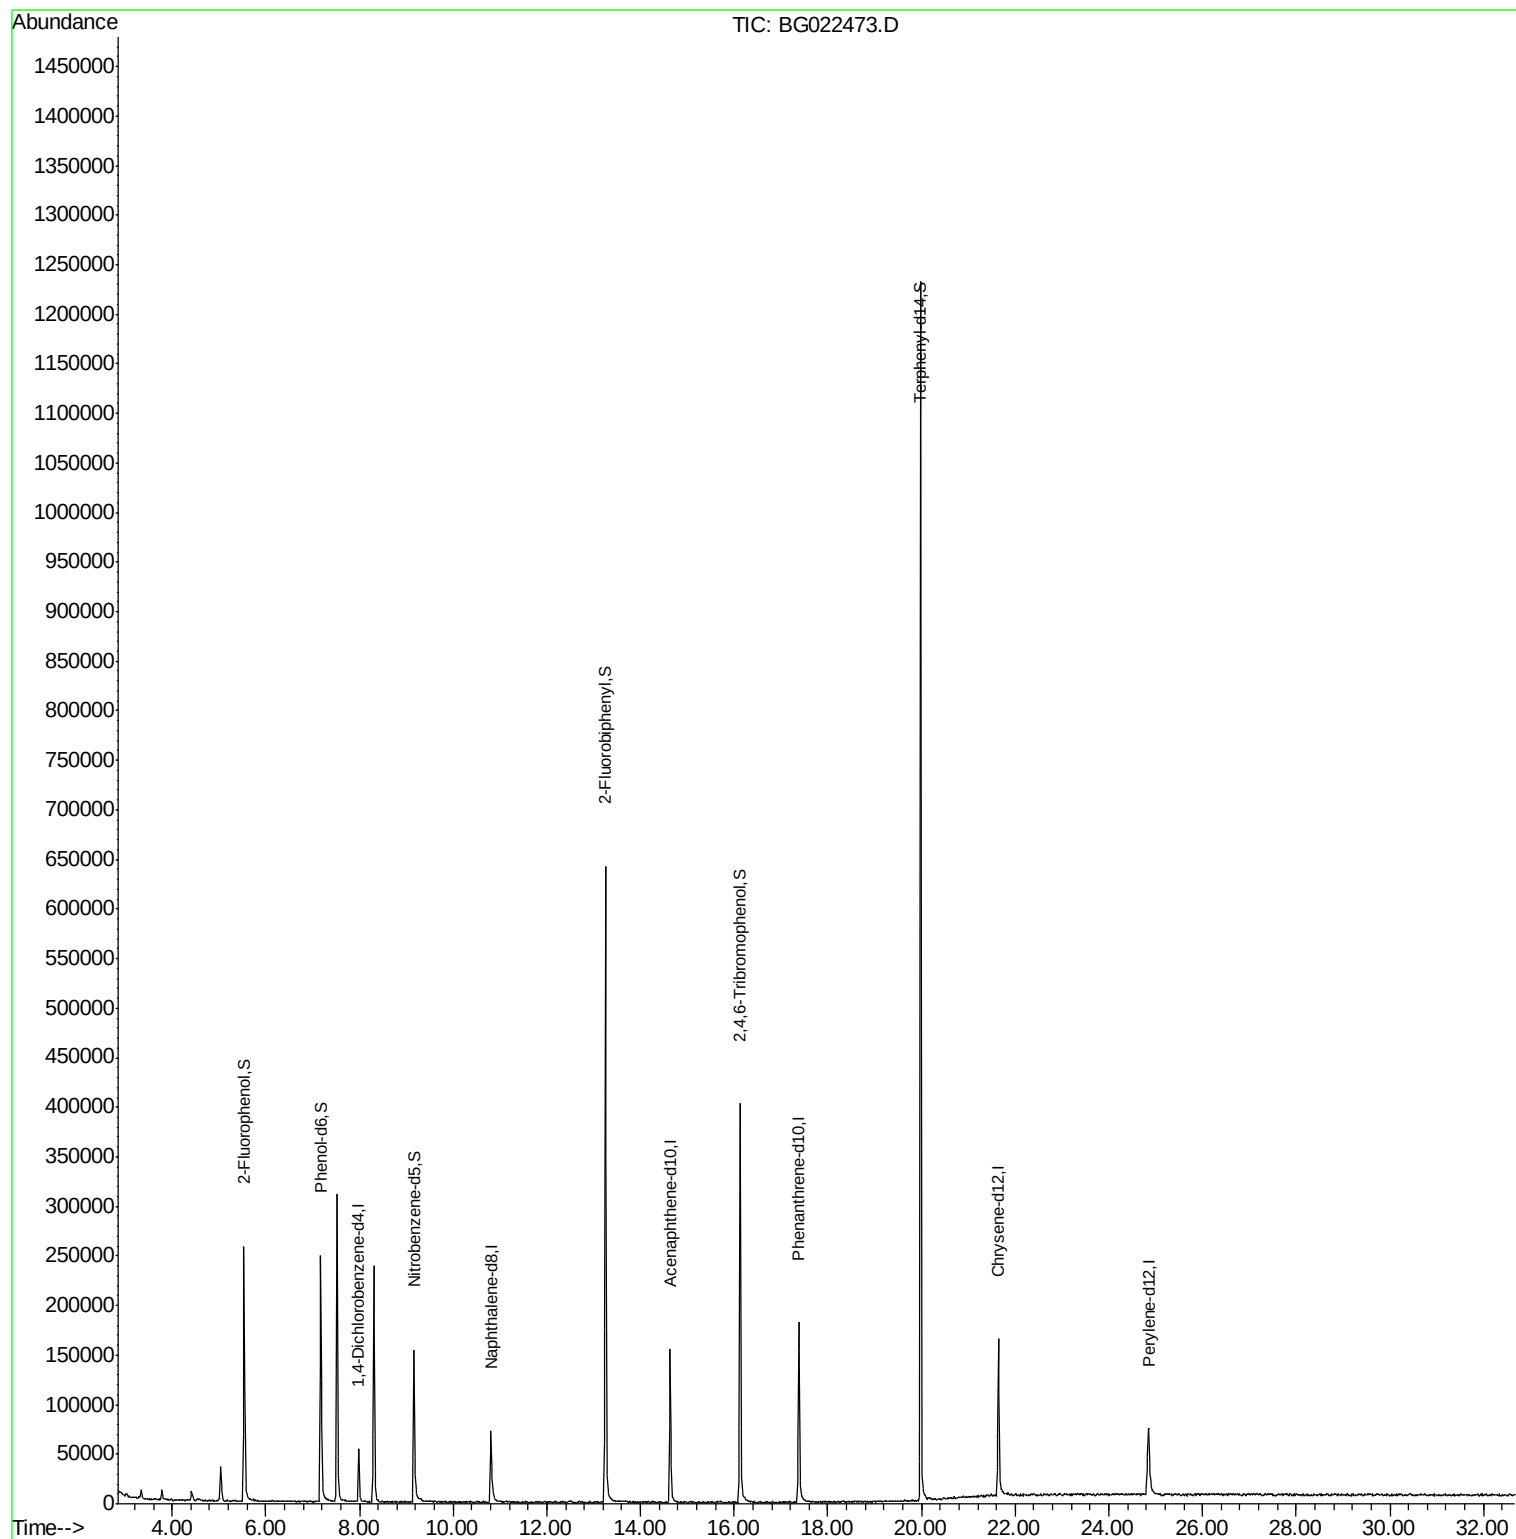

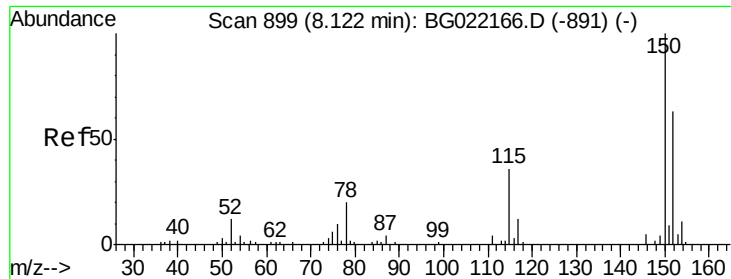


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.98 min Scan# 875
Delta R.T. -0.00 min
Lab File: BG022473.D
Acq: 21 Jun 2016 19:34

Instrument :
BNA_G
ClientSampleId :
PL-DA-6-COMP

Tot Ion:152 Resp: 20468
Ion Ratio Lower Upper
152 100
150 158.5 130.1 195.1
115 56.8 62.2 93.2#

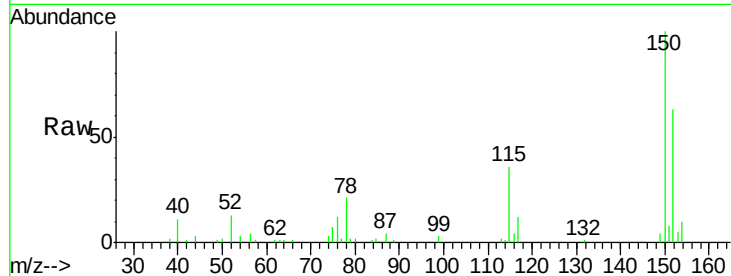


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

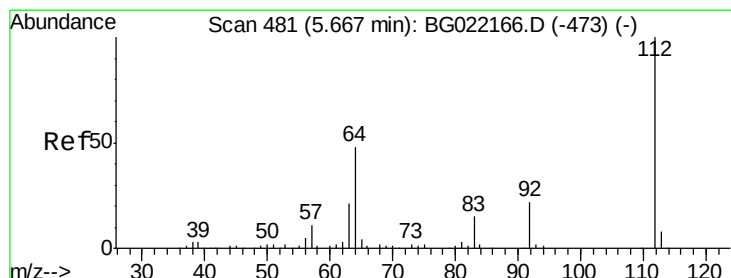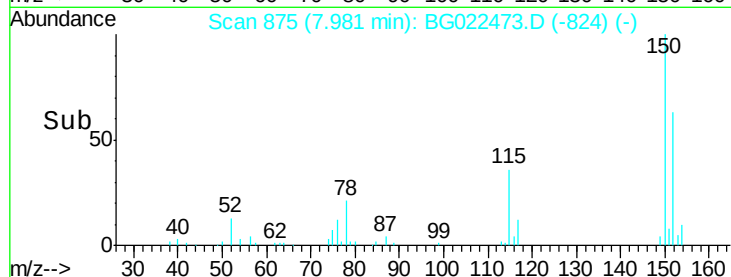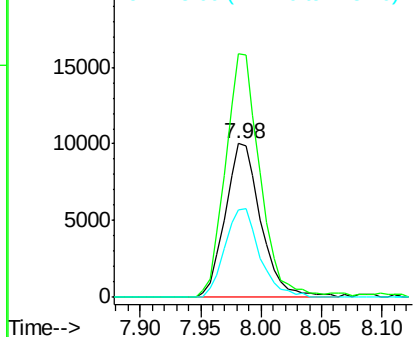



#5


2-Fluorophenol
Concen: 164.68 ng
RT: 5.54 min Scan# 459
Delta R.T. -0.00 min
Lab File: BG022473.D
Acq: 21 Jun 2016 19:34

Tgt Ion:112 Resp: 174329
Ion Ratio Lower Upper
112 100
64 48.0 51.1 76.7#
63 22.7 24.6 37.0#

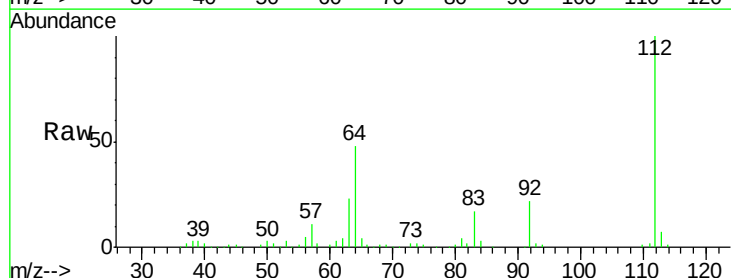

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

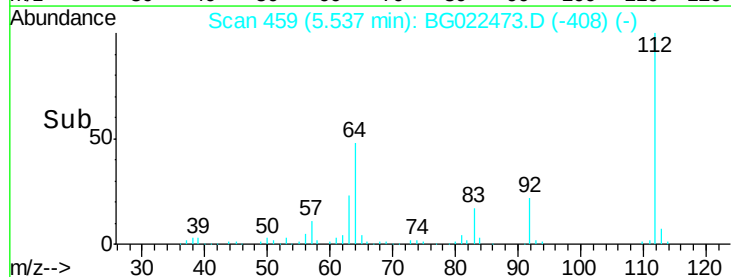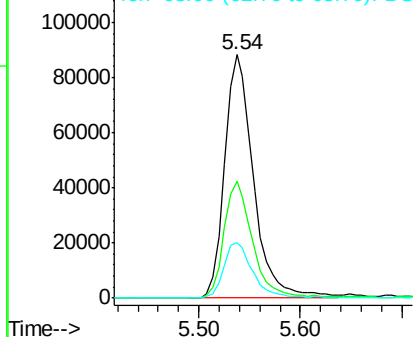

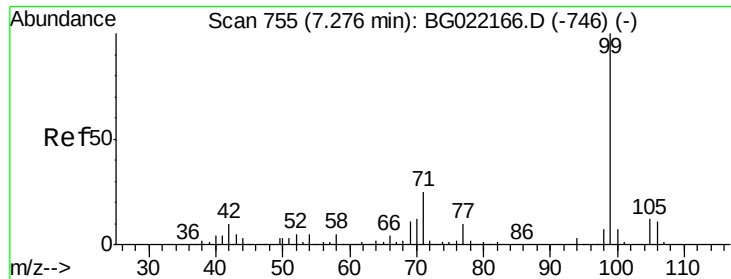

#7

Phenol-d6

Concen: 142.85 ng

RT: 7.17 min Scan# 737

Delta R.T. -0.00 min

Lab File: BG022473.D

Acq: 21 Jun 2016 19:34

Instrument :

BNA_G

ClientSampleId :

PL-DA-6-COMP


Tot Ion: 99 Resp: 237770

Ion Ratio Lower Upper




99 100

42 9.9 16.4 24.6#

71 24.3 25.0 37.4#

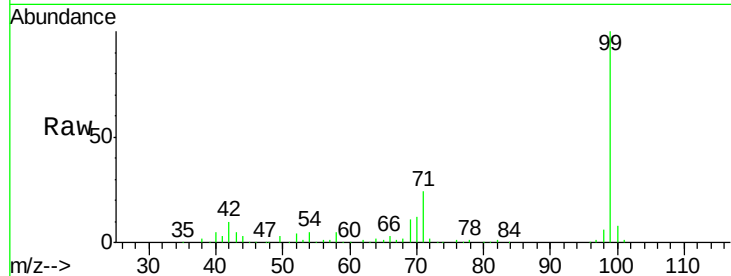

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

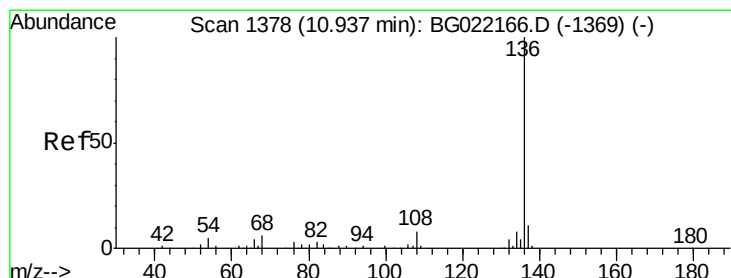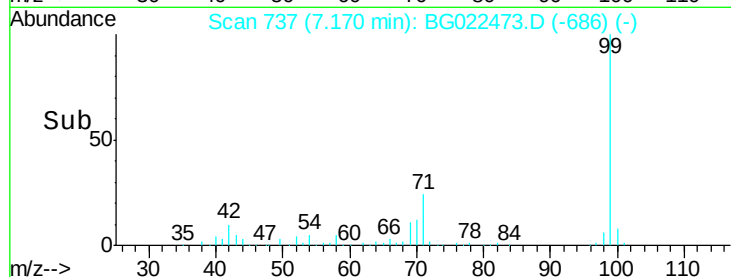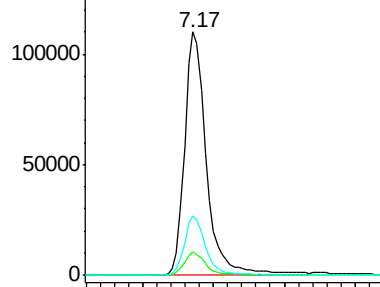

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.81 min Scan# 1356

Delta R.T. 0.00 min

Lab File: BG022473.D

Acq: 21 Jun 2016 19:34

Tgt Ion: 136 Resp: 95429


Ion Ratio Lower Upper

136 100



137 10.9 9.0 13.4


54 6.6 9.6 14.4#

68 5.9 6.4 9.6#

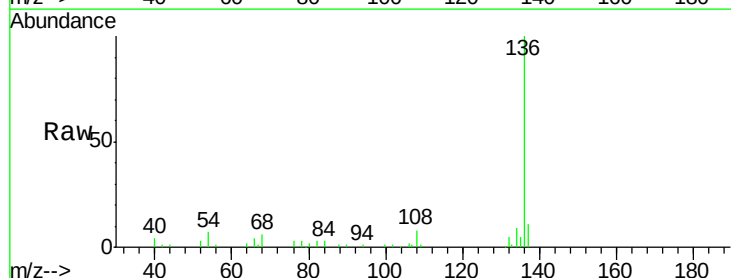

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



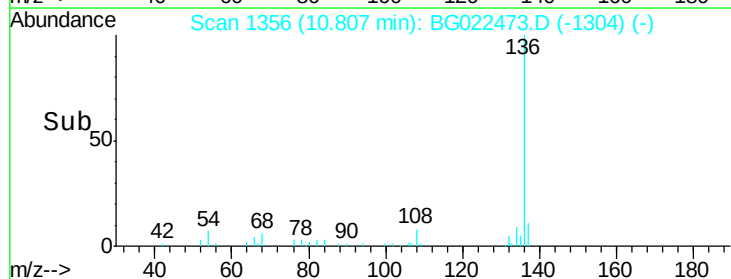
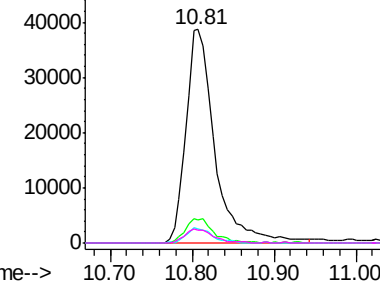


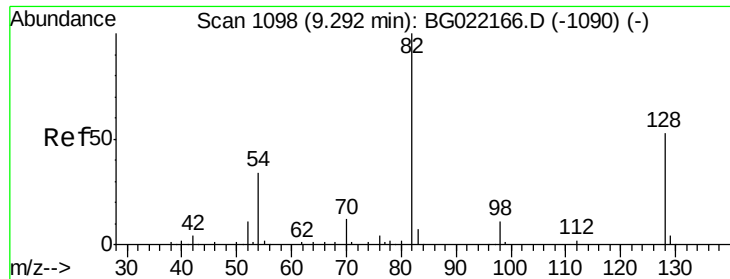

#23
Nitrobenzene-d5
Concen: 99.35 ng
RT: 9.16 min Scan# 1076
Delta R.T. -0.00 min
Lab File: BG022473.D
Acq: 21 Jun 2016 19:34




Instrument :
BNA_G
ClientSampleId :
PL-DA-6-COMP


Tot Ion: 82 Resp: 135993
Ion Ratio Lower Upper
82 100
128 49.7 33.4 50.0
54 35.7 46.1 69.1#

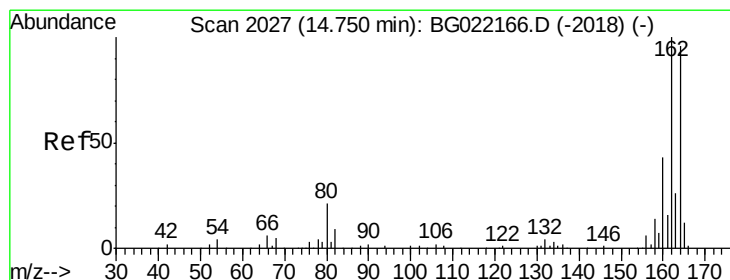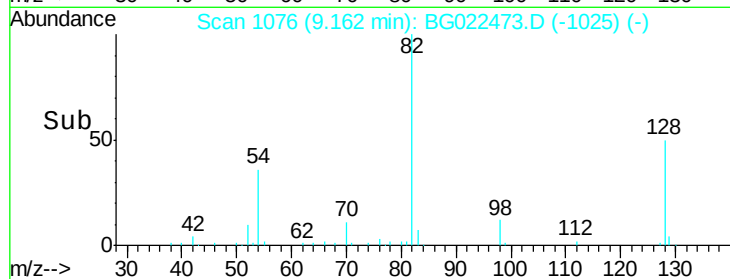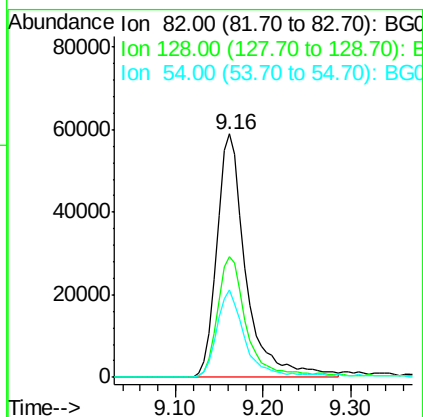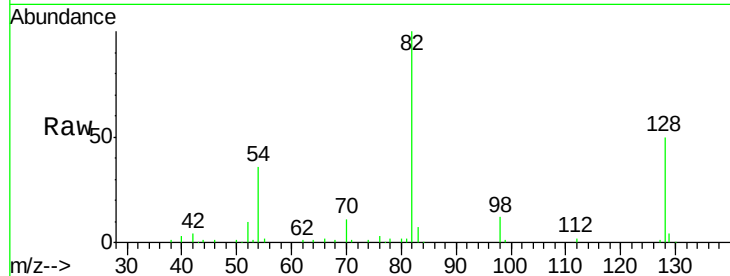

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.63 min Scan# 2007
Delta R.T. -0.00 min
Lab File: BG022473.D
Acq: 21 Jun 2016 19:34

Tgt Ion:164 Resp: 61238
Ion Ratio Lower Upper
164 100
162 110.8 78.0 117.0
160 47.9 32.9 49.3

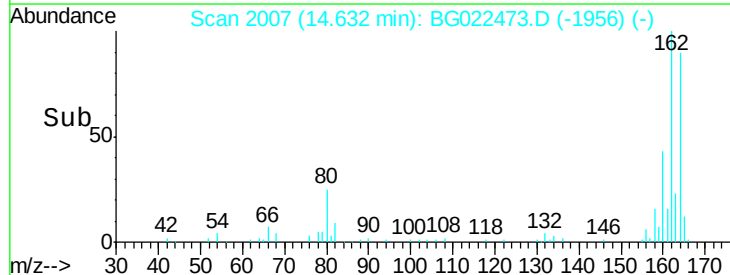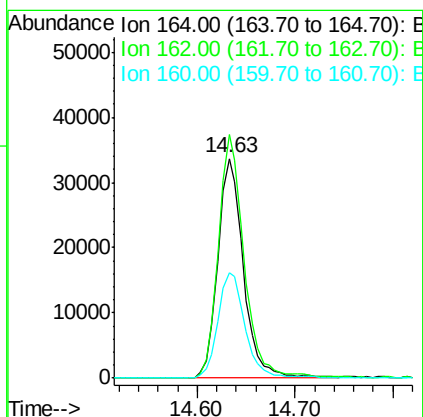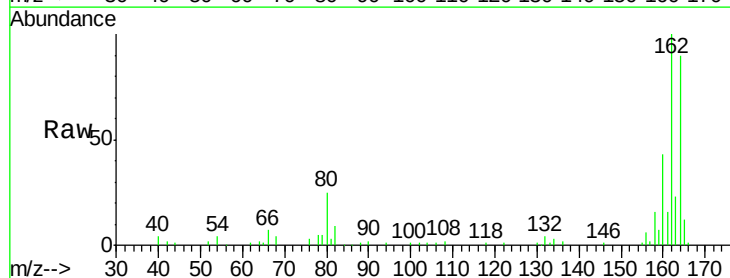

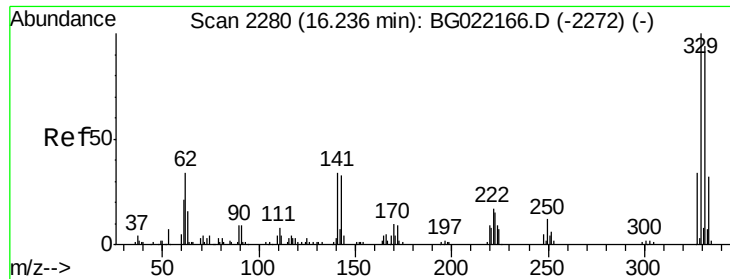

#41

2,4,6-Tribromophenol

Concen: 121.39 ng

RT: 16.13 min Scan# 2262

Delta R.T. 0.00 min

Lab File: BG022473.D

Acq: 21 Jun 2016 19:34

Instrument :

BNA_G

ClientSampleId :

PL-DA-6-COMP


Tot Ion:330 Resp: 83994

Ion Ratio Lower Upper




330 100

332 94.1 78.0 117.0

141 49.1 33.8 50.8

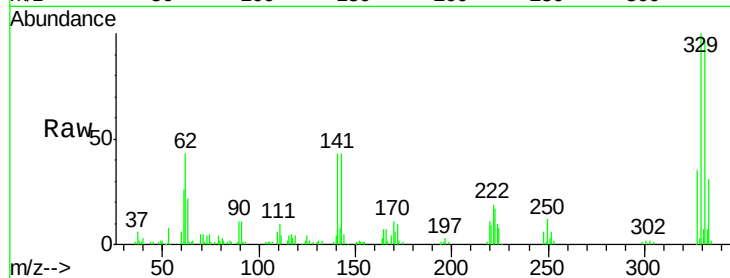

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

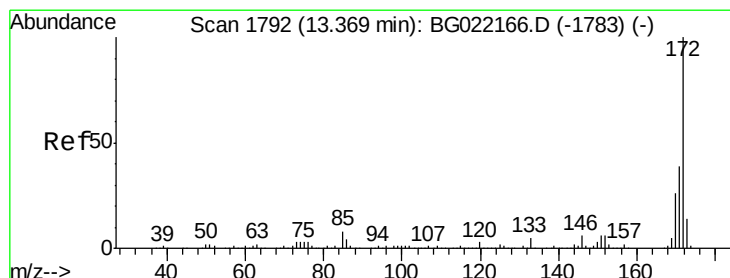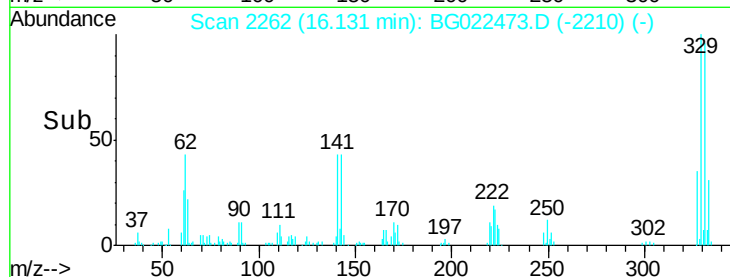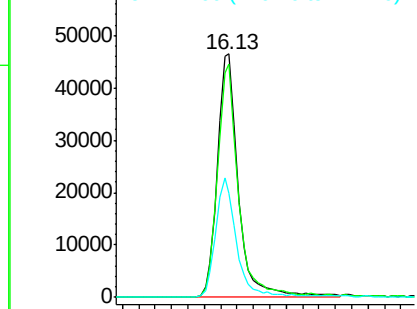

#44

2-Fluorobiphenyl

Concen: 96.73 ng

RT: 13.25 min Scan# 1772

Delta R.T. -0.00 min

Lab File: BG022473.D

Acq: 21 Jun 2016 19:34


Tgt Ion:172 Resp: 388712

Ion Ratio Lower Upper



172 100


171 41.0 27.8 41.6

170 26.4 19.6 29.4

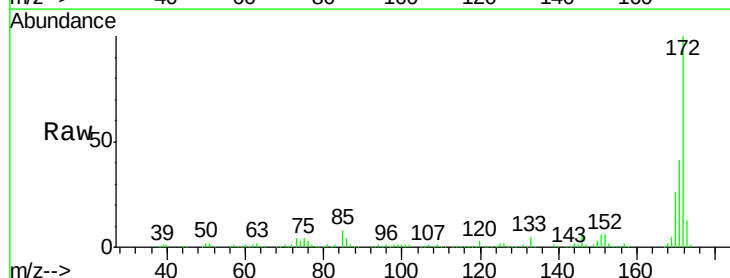

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E



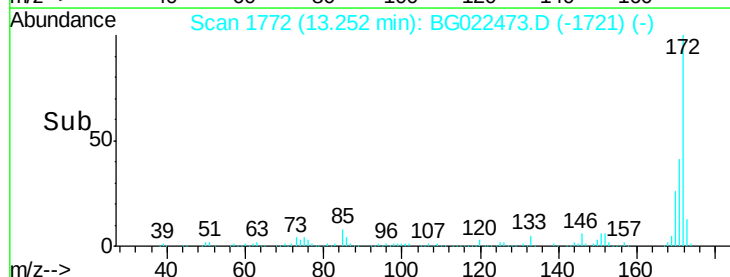
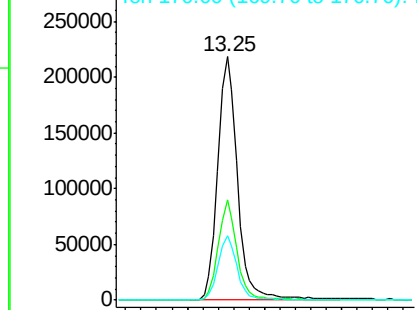


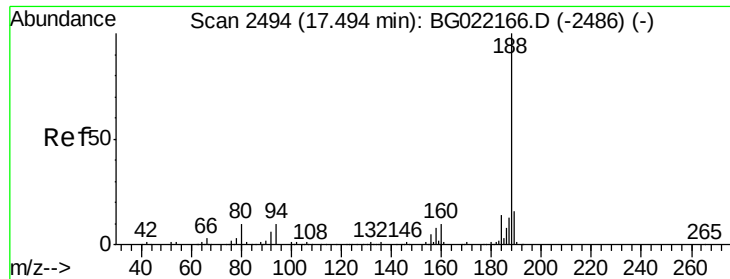

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.38 min Scan# 2475
Delta R.T. 0.00 min
Lab File: BG022473.D
Acq: 21 Jun 2016 19:34




Instrument :
BNA_G
ClientSampleId :
PL-DA-6-COMP


Tot Ion:188 Resp: 140725
Ion Ratio Lower Upper
188 100
94 11.7 7.5 11.3#
80 13.0 8.6 13.0#

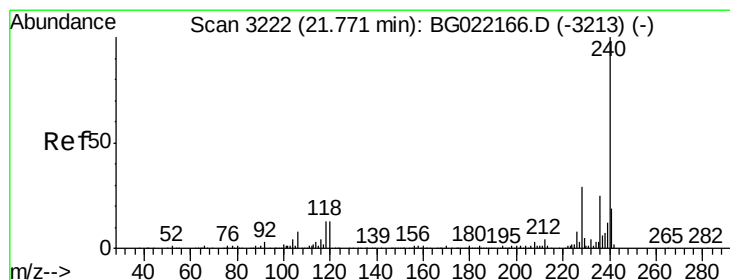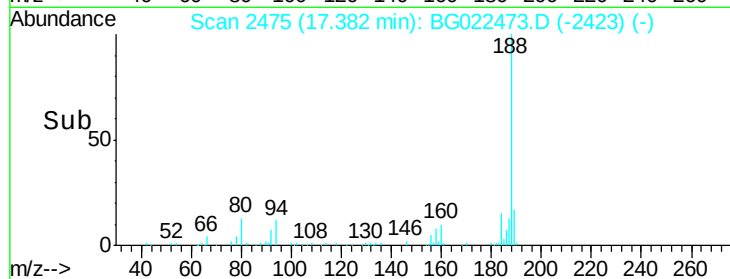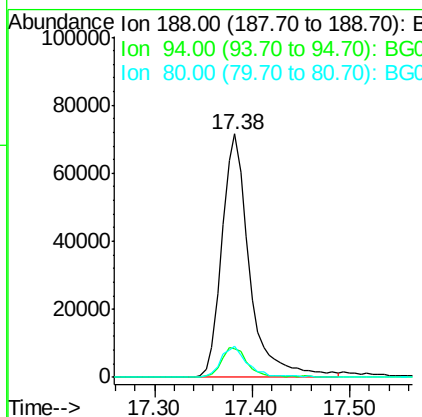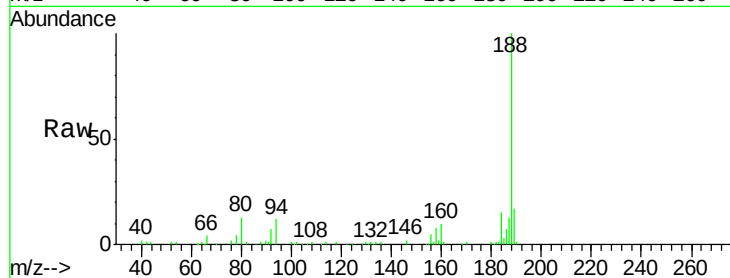

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.64 min Scan# 3200
Delta R.T. 0.00 min
Lab File: BG022473.D
Acq: 21 Jun 2016 19:34

Tgt Ion:240 Resp: 117585
Ion Ratio Lower Upper
240 100
120 18.0 8.4 12.6#
236 28.1 19.6 29.4

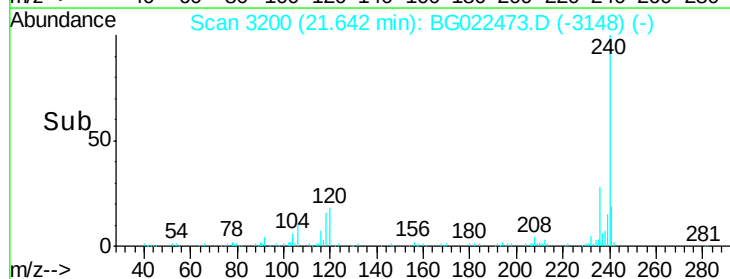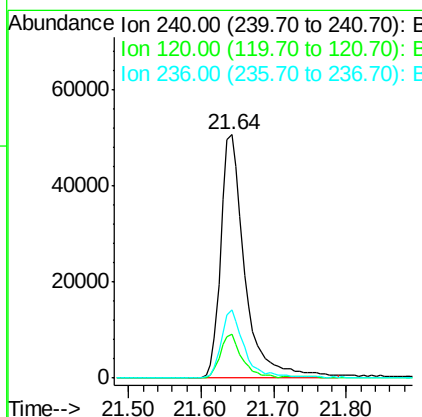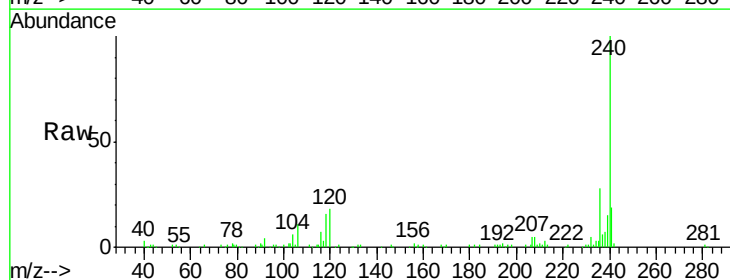

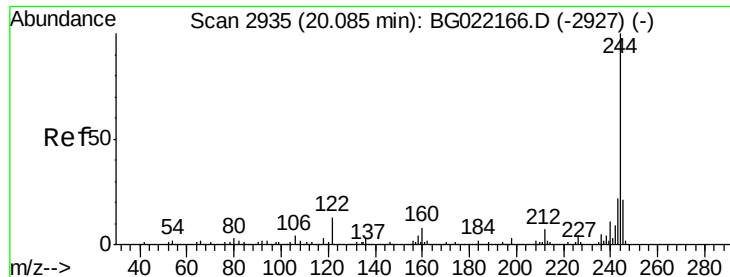

#78

Terphenyl-d14

Concen: 111.27 ng

RT: 19.98 min Scan# 2917

Delta R.T. -0.00 min

Lab File: BG022473.D

Acq: 21 Jun 2016 19:34

Instrument :

BNA_G

ClientSampleId :

PL-DA-6-COMP


Tot Ion:244 Resp: 551077

Ion Ratio Lower Upper

244 100

212 7.4 6.5 9.7




122 15.8 8.6 12.8#

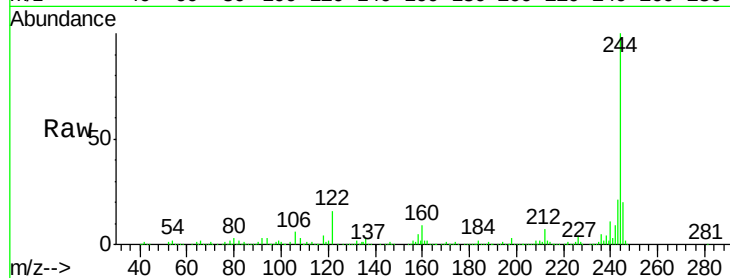

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

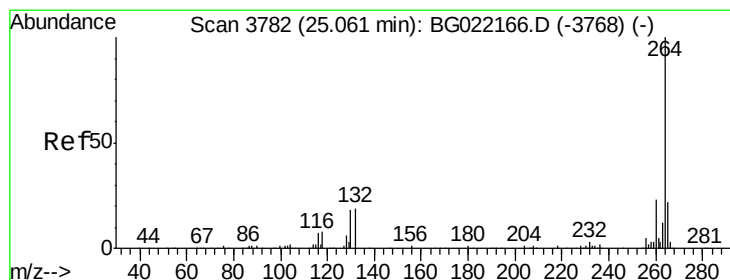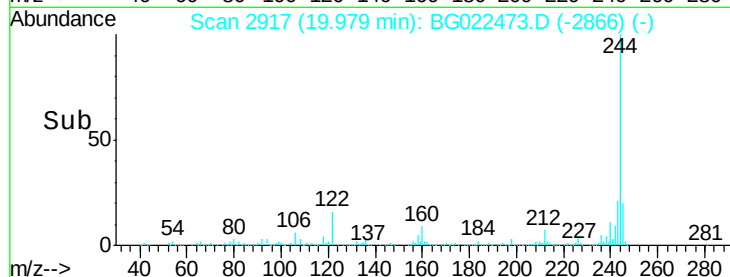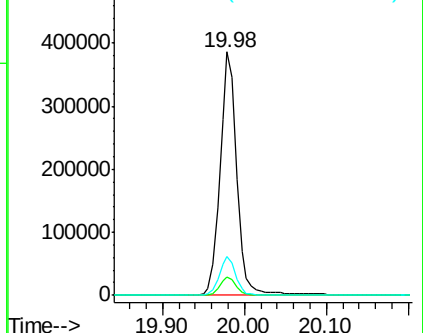

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.85 min Scan# 3746

Delta R.T. 0.01 min

Lab File: BG022473.D

Acq: 21 Jun 2016 19:34


Tgt Ion:264 Resp: 72144

Ion Ratio Lower Upper

264 100

260 26.9 20.2 30.4

265 21.7 17.8 26.8

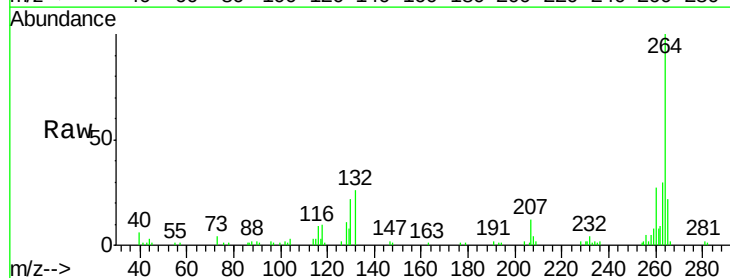

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

