


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062116\
 Data File : BG022484.D
 Acq On : 22 Jun 2016 3:34
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 22 01:27:56 2016

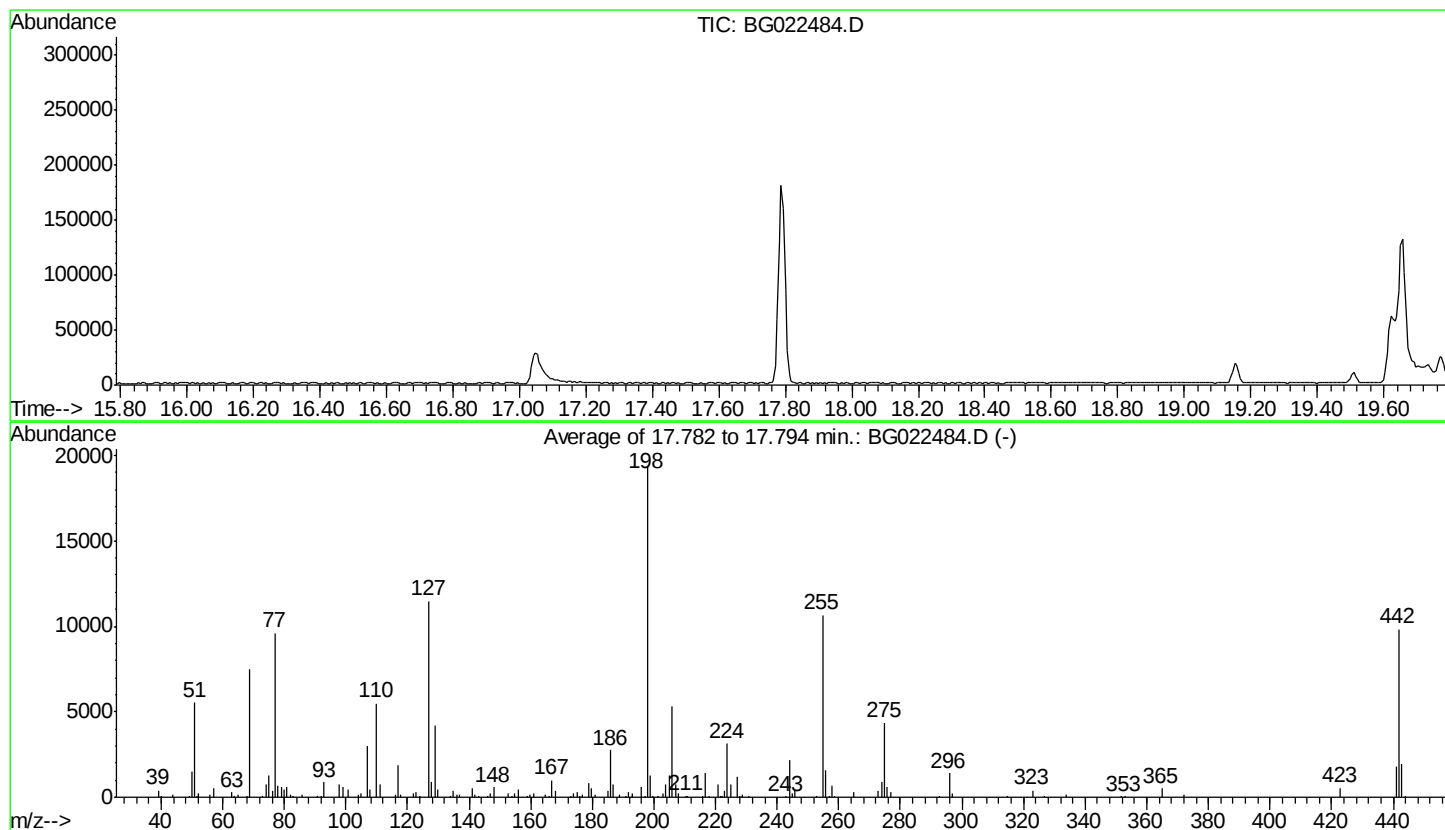

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2537

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	5518	PASS
68	69	0.00	2	1.5	111	PASS
69	198	0.00	100	38.6	7485	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.1	11470	PASS
197	198	0.00	2	0.5	90	PASS
198	198	100	100	100.0	19404	PASS
199	198	5	9	6.5	1267	PASS
275	198	10	60	22.4	4355	PASS
365	198	1	100	2.6	511	PASS
441	442	0.01	24	18.0	1771	PASS
442	198	50	100	50.8	9848	PASS
443	442	15	24	19.6	1928	PASS