


Data Path : Z:\HPCHEM1\BNA_G\Data\BG062117\
Data File : BG027558.D
Acq On : 21 Jun 2017 13:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 21 18:52:15 2017

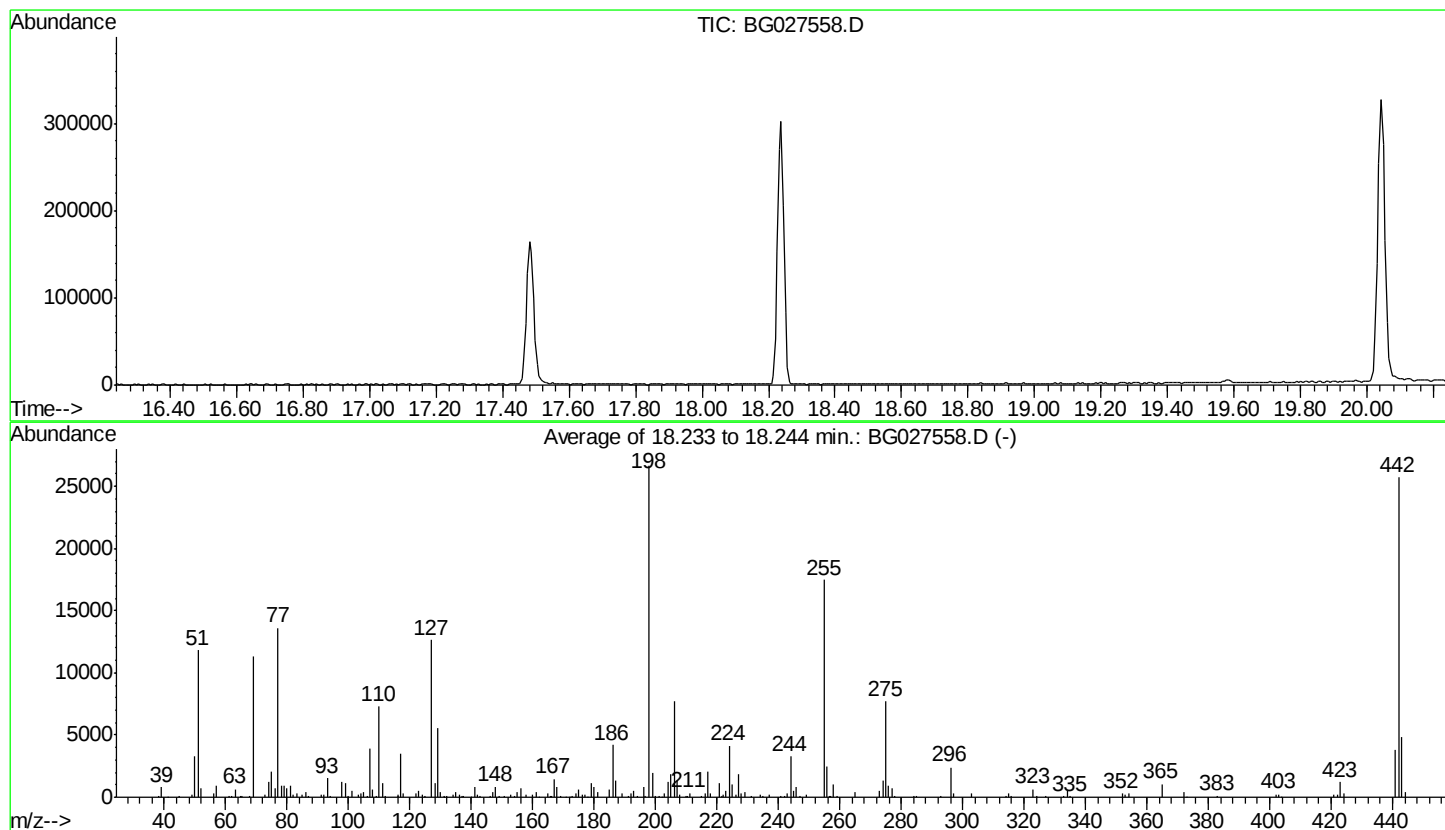

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	11805	PASS
68	69	0.00	2	1.4	155	PASS
69	198	0.00	100	42.4	11295	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	12614	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26664	PASS
199	198	5	9	7.3	1942	PASS
275	198	10	60	28.8	7679	PASS
365	198	1	100	4.0	1071	PASS
441	442	0.01	24	14.8	3798	PASS
442	198	50	100	96.4	25696	PASS
443	442	15	24	19.0	4874	PASS