
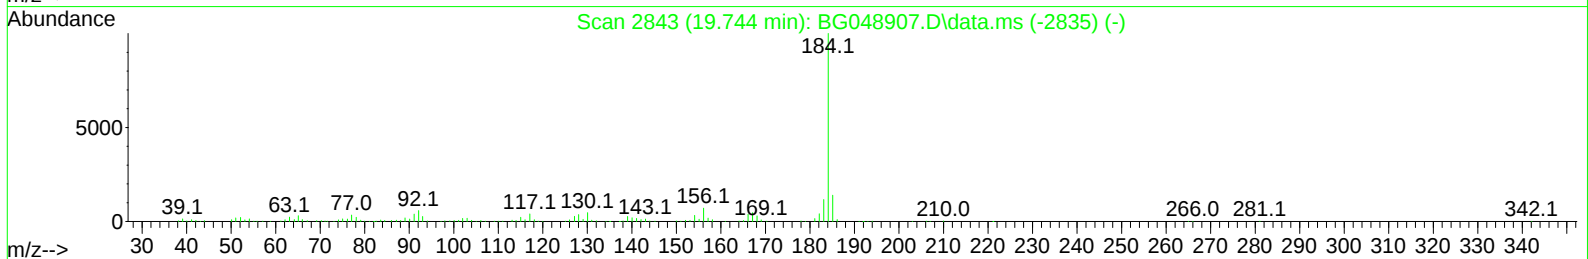
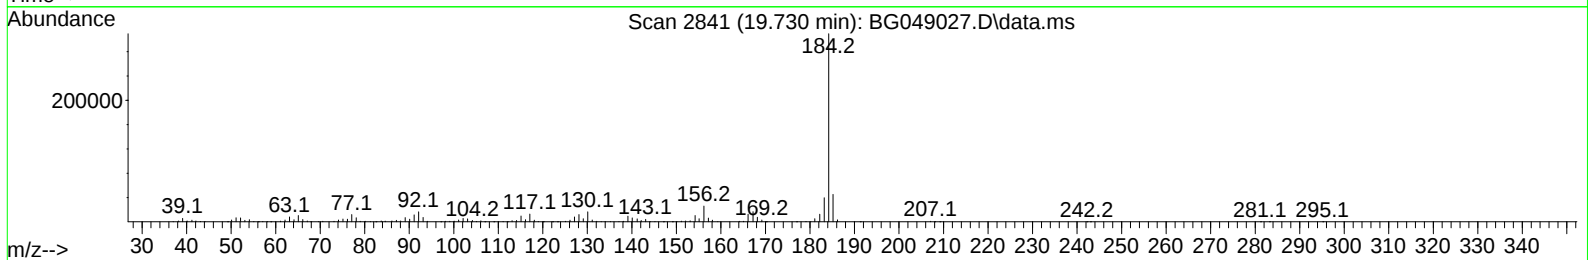


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
 Data File : BG049027.D
 Acq On : 21 Jun 2021 10:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 13:15:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 12:04:50 2021
 Response via : Initial Calibration

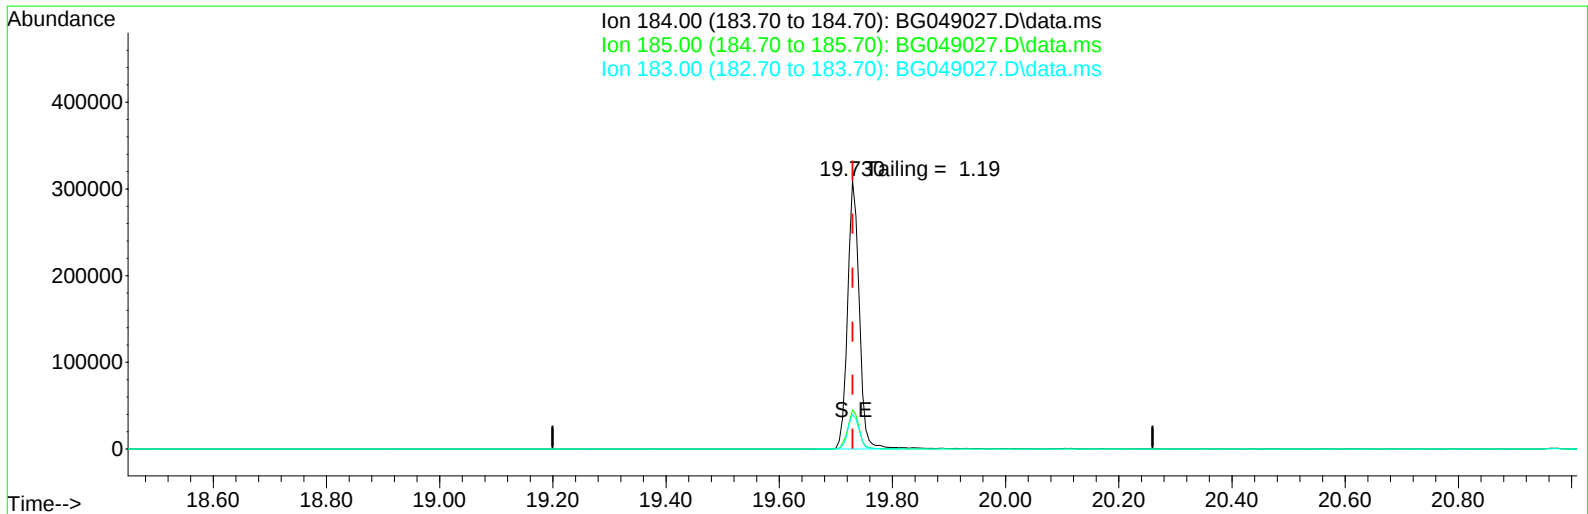

TIC: BG049027.D\data.ms

(77) Benzidine




19.730min (+ 0.000) 291214.73 ng m

response 439988

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.62
183.00	11.70	12.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
Data File : BG049027.D
Acq On : 21 Jun 2021 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 13:15:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

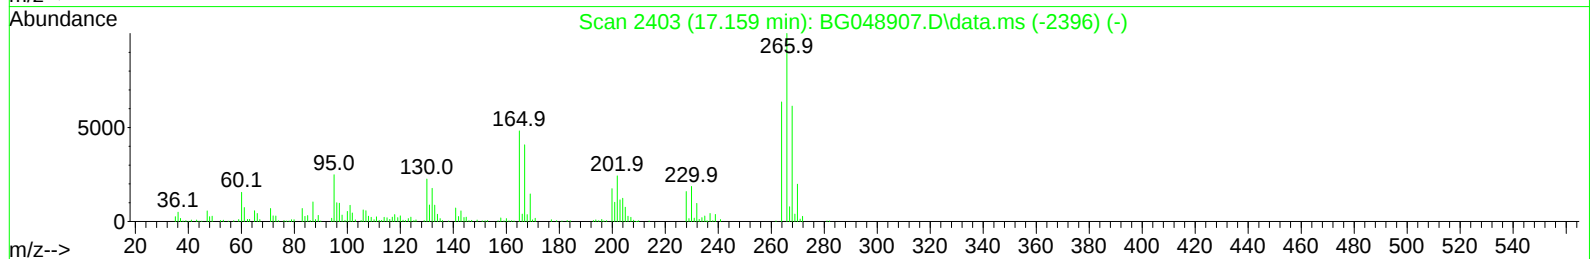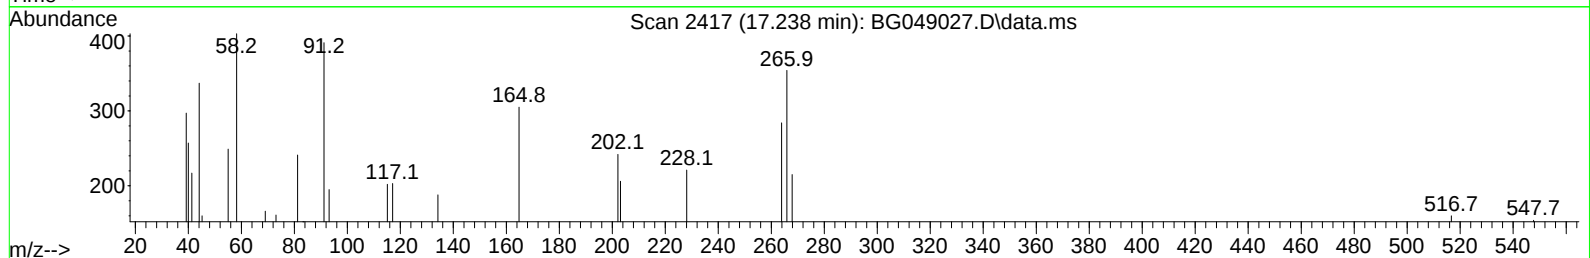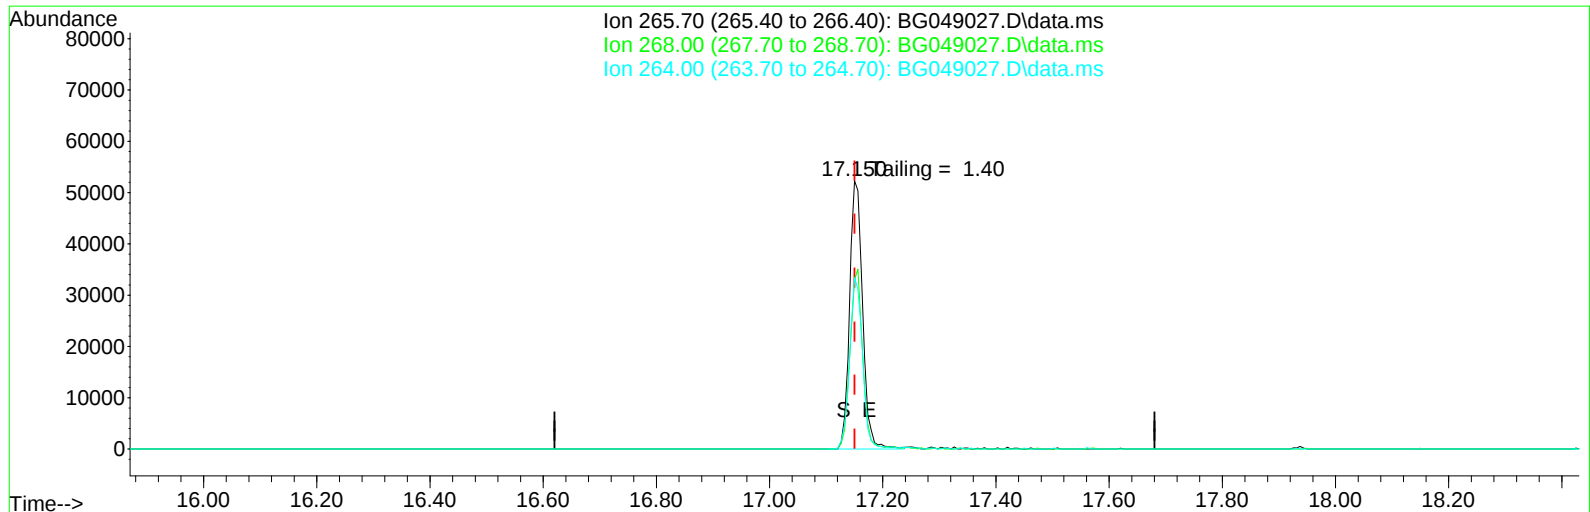

TIC: BG049027.D\data.ms

(70) Pentachlorophenol (C)

17.150min (+ 0.000) 28263.73 ng

response 83214

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.08
264.00	61.30	63.99
0.00	0.00	0.00