

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
 Data File : BG049034.D
 Acq On : 21 Jun 2021 16:01
 Operator : CG/JU
 Sample : M2764-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PHC-250EM-001

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.155	15	20	31	rVV3	47894	131302	7.30%	1.190%
2	3.243	31	35	41	rVB4	16803	31080	1.73%	0.282%
3	5.200	363	368	374	rBV2	14224	25514	1.42%	0.231%
4	5.670	440	448	461	rBV	615973	1046059	58.13%	9.478%
5	7.268	713	720	731	rBV	635562	1131759	62.89%	10.254%
6	8.114	856	864	872	rBV	152672	265147	14.73%	2.402%
7	9.277	1054	1062	1071	rBV	382547	717111	39.85%	6.497%
8	10.699	1299	1304	1310	rBV3	22768	39598	2.20%	0.359%
9	10.934	1334	1344	1351	rBV	198963	365903	20.33%	3.315%
10	13.378	1752	1760	1769	rVB	884490	1425552	79.22%	12.916%
11	14.753	1985	1994	2002	rBV	308015	495520	27.54%	4.490%
12	16.240	2240	2247	2254	rBV	782326	1229337	68.31%	11.138%
13	17.503	2453	2462	2467	rBV	352804	566378	31.47%	5.132%
14	18.384	2606	2612	2617	rBV	153294	219712	12.21%	1.991%
15	18.678	2656	2662	2666	rBV9	11568	23651	1.31%	0.214%
16	18.872	2691	2695	2699	rBV3	39897	55965	3.11%	0.507%
17	19.283	2761	2765	2771	rBV6	34543	52793	2.93%	0.478%
18	19.647	2823	2827	2831	rBV2	80600	108252	6.02%	0.981%
19	19.912	2870	2872	2876	rVB5	14205	18087	1.01%	0.164%
20	20.106	2900	2905	2911	rVB	1346851	1799592	100.00%	16.305%
21	20.323	2940	2942	2946	rVB3	28018	28174	1.57%	0.255%
22	21.422	3125	3129	3135	rVB3	71764	109348	6.08%	0.991%
23	21.792	3186	3192	3201	rVB2	331684	591816	32.89%	5.362%
24	25.123	3750	3759	3772	rBV2	187529	559199	31.07%	5.067%




Sum of corrected areas: 11036849

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
Data File : BG049034.D
Acq On : 21 Jun 2021 16:01
Operator : CG/JU
Sample : M2764-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PHC-250EM-001

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

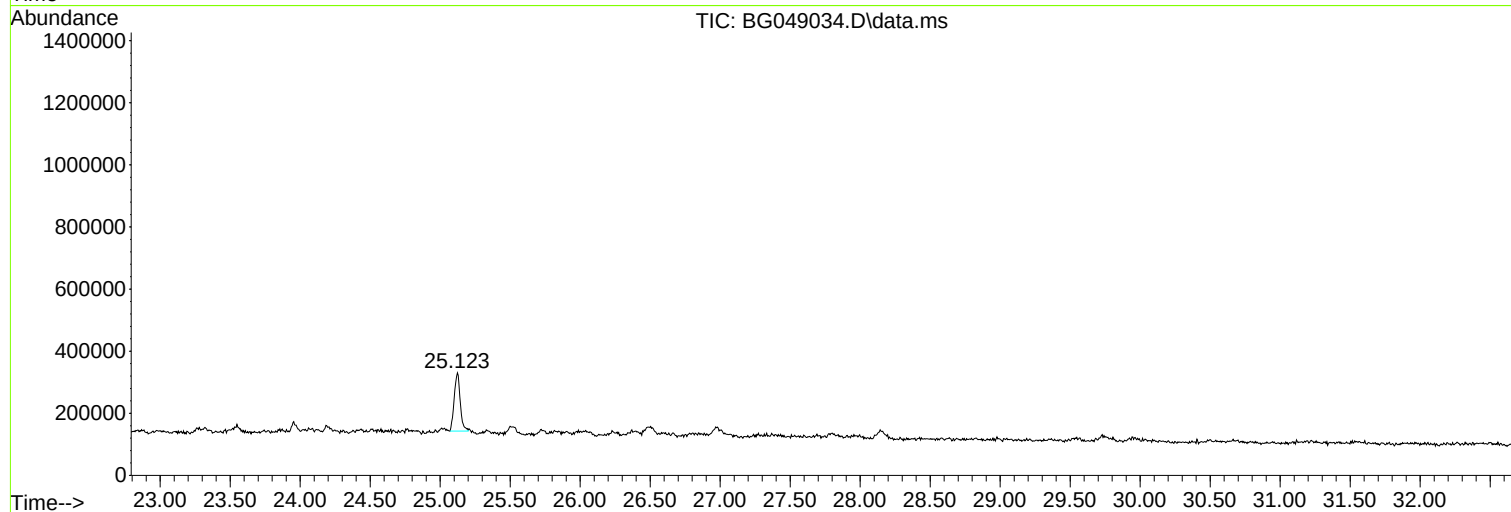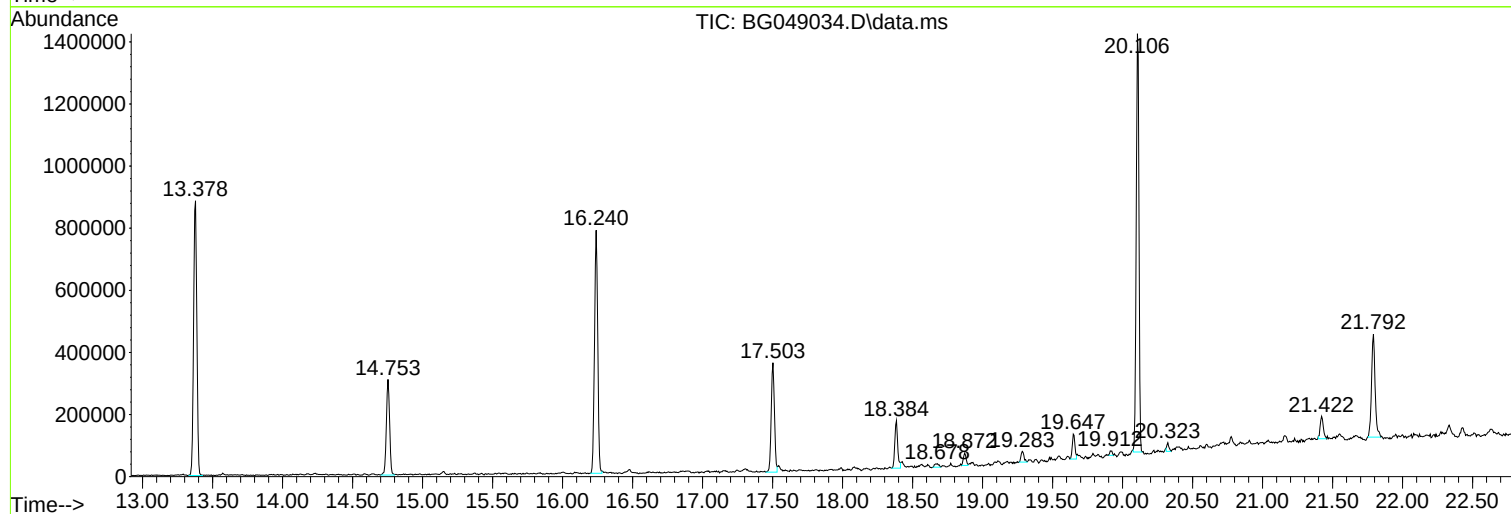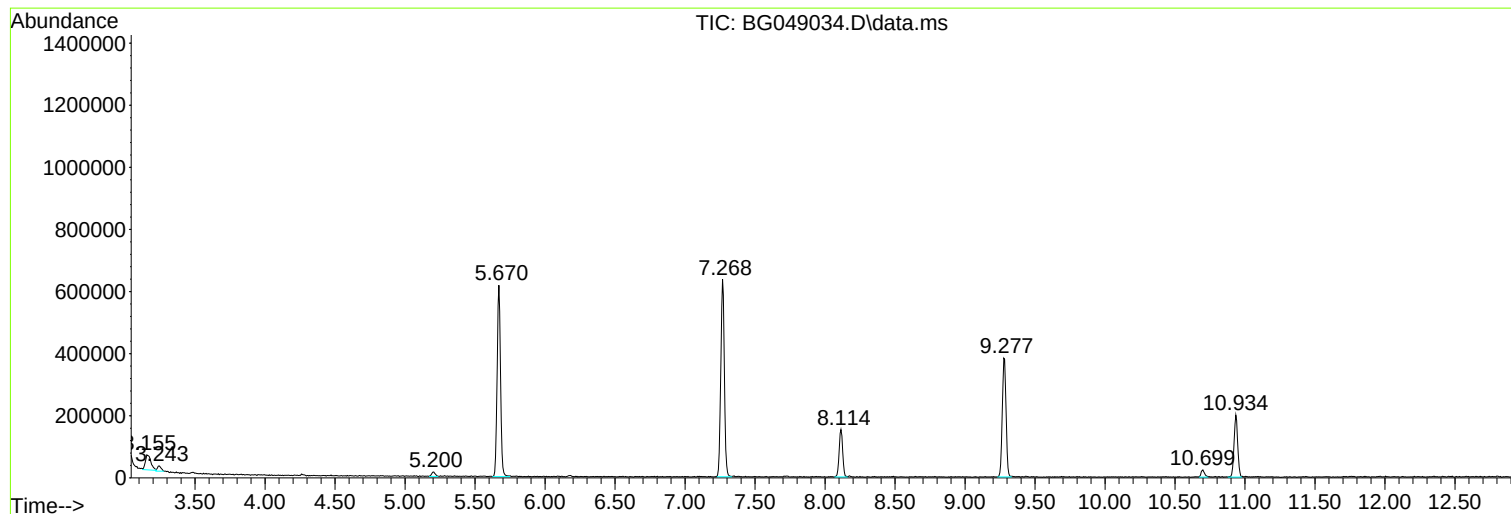

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
Data File : BG049034.D
Acq On : 21 Jun 2021 16:01
Operator : CG/JU
Sample : M2764-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PHC-250EM-001

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
Data File : BG049034.D
Acq On : 21 Jun 2021 16:01
Operator : CG/JU
Sample : M2764-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PHC-250EM-001

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------