

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
 Data File : BG049035.D
 Acq On : 21 Jun 2021 16:42
 Operator : CG/JU
 Sample : M2764-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PHC-250EM-002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.163	15	21	32	rBV2	41039	121730	6.11%	1.024%
2	3.251	32	36	42	rVB3	15840	32751	1.64%	0.276%
3	5.202	363	368	375	rVB3	15160	28035	1.41%	0.236%
4	5.672	438	448	457	rBV	628546	1066786	53.57%	8.978%
5	7.270	712	720	736	rBV	670338	1203417	60.43%	10.128%
6	8.116	857	864	871	rBV	158456	273296	13.72%	2.300%
7	9.279	1051	1062	1070	rBV	417961	772280	38.78%	6.500%
8	10.695	1298	1303	1311	rBV2	37710	66052	3.32%	0.556%
9	10.936	1336	1344	1351	rBV	208478	368756	18.52%	3.103%
10	13.380	1752	1760	1768	rVB	980066	1568756	78.77%	13.203%
11	14.755	1987	1994	2002	rVB	319310	505402	25.38%	4.253%
12	16.242	2239	2247	2258	rBV	886584	1377025	69.14%	11.589%
13	17.505	2456	2462	2473	rBV	388302	602497	30.25%	5.071%
14	18.169	2568	2575	2579	rBV9	10773	19953	1.00%	0.168%
15	18.386	2607	2612	2617	rBV	92161	132578	6.66%	1.116%
16	18.662	2655	2659	2666	rBV4	25137	48502	2.44%	0.408%
17	18.874	2691	2695	2700	rVB2	62440	91296	4.58%	0.768%
18	19.121	2730	2737	2743	rBV2	12369	29310	1.47%	0.247%
19	19.285	2761	2765	2770	rVB3	36308	49968	2.51%	0.421%
20	19.649	2823	2827	2830	rBV3	44064	59053	2.97%	0.497%
21	20.108	2900	2905	2912	rVB	1519180	1991562	100.00%	16.761%
22	20.325	2938	2942	2947	rBV2	32061	52563	2.64%	0.442%
23	21.418	3125	3128	3136	rVB3	73144	107694	5.41%	0.906%
24	21.794	3186	3192	3203	rVB	336217	594807	29.87%	5.006%
25	22.334	3280	3284	3289	rVB8	36300	63196	3.17%	0.532%
26	22.423	3297	3299	3305	rVB7	35360	51804	2.60%	0.436%
27	25.125	3750	3759	3774	rVB2	200854	603021	30.28%	5.075%




Sum of corrected areas: 11882090

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
Data File : BG049035.D
Acq On : 21 Jun 2021 16:42
Operator : CG/JU
Sample : M2764-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PHC-250EM-002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

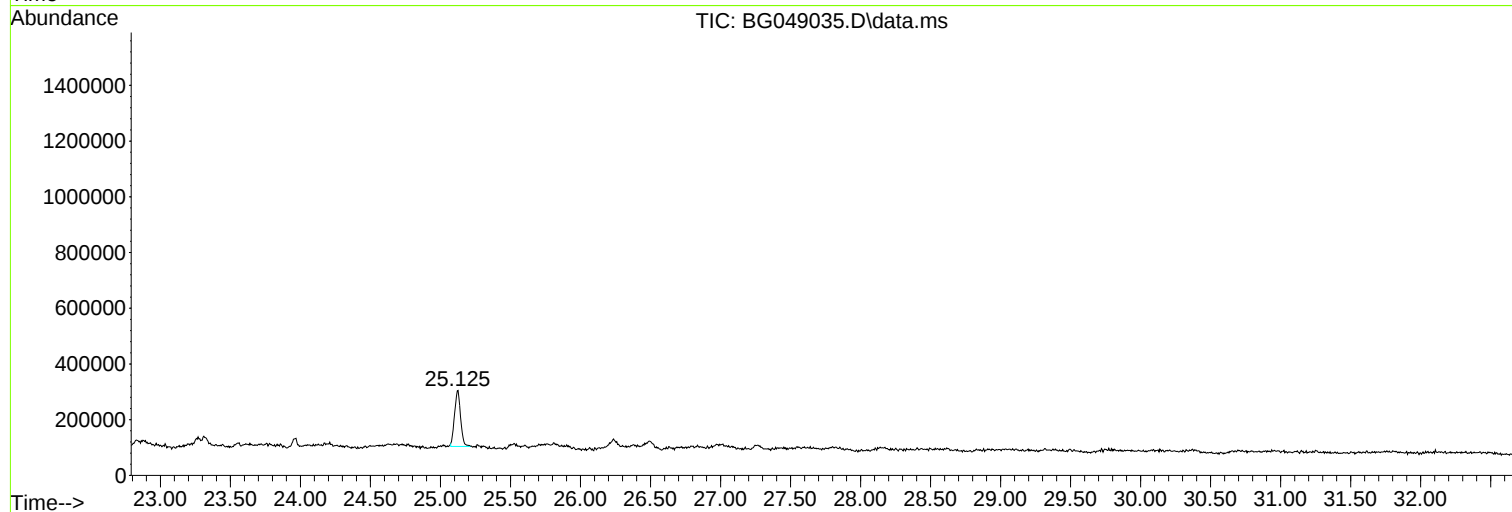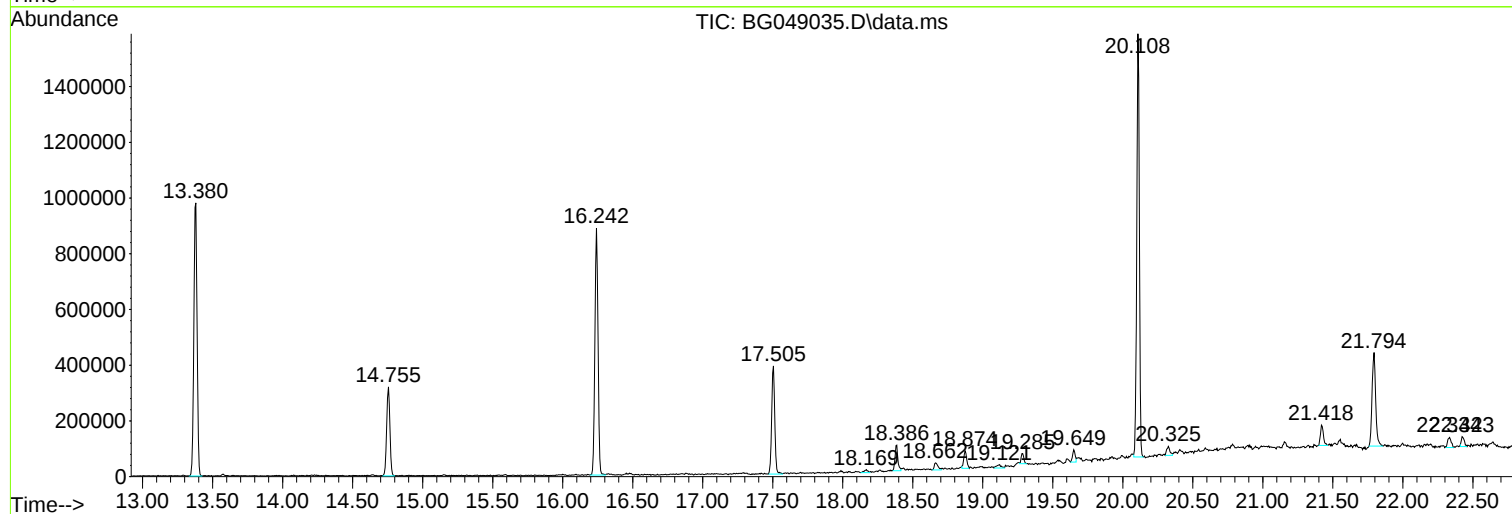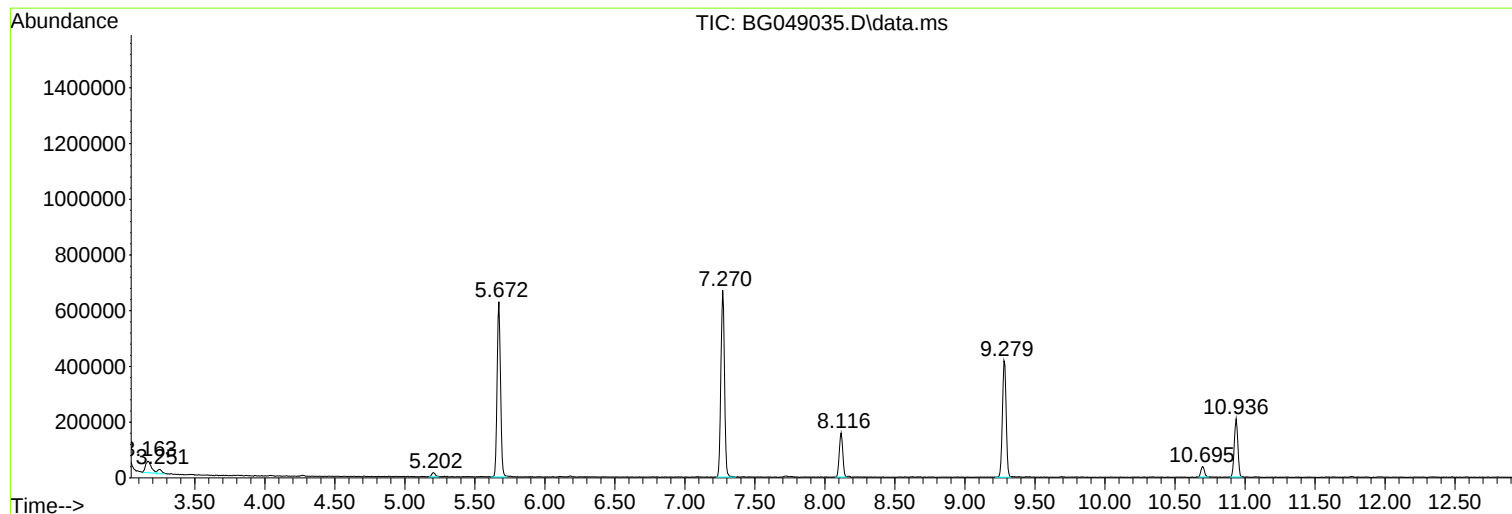

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
Data File : BG049035.D
Acq On : 21 Jun 2021 16:42
Operator : CG/JU
Sample : M2764-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PHC-250EM-002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
Data File : BG049035.D
Acq On : 21 Jun 2021 16:42
Operator : CG/JU
Sample : M2764-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PHC-250EM-002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------