


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
 Data File : BG049027.D
 Acq On : 21 Jun 2021 10:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 16 12:04:50 2021

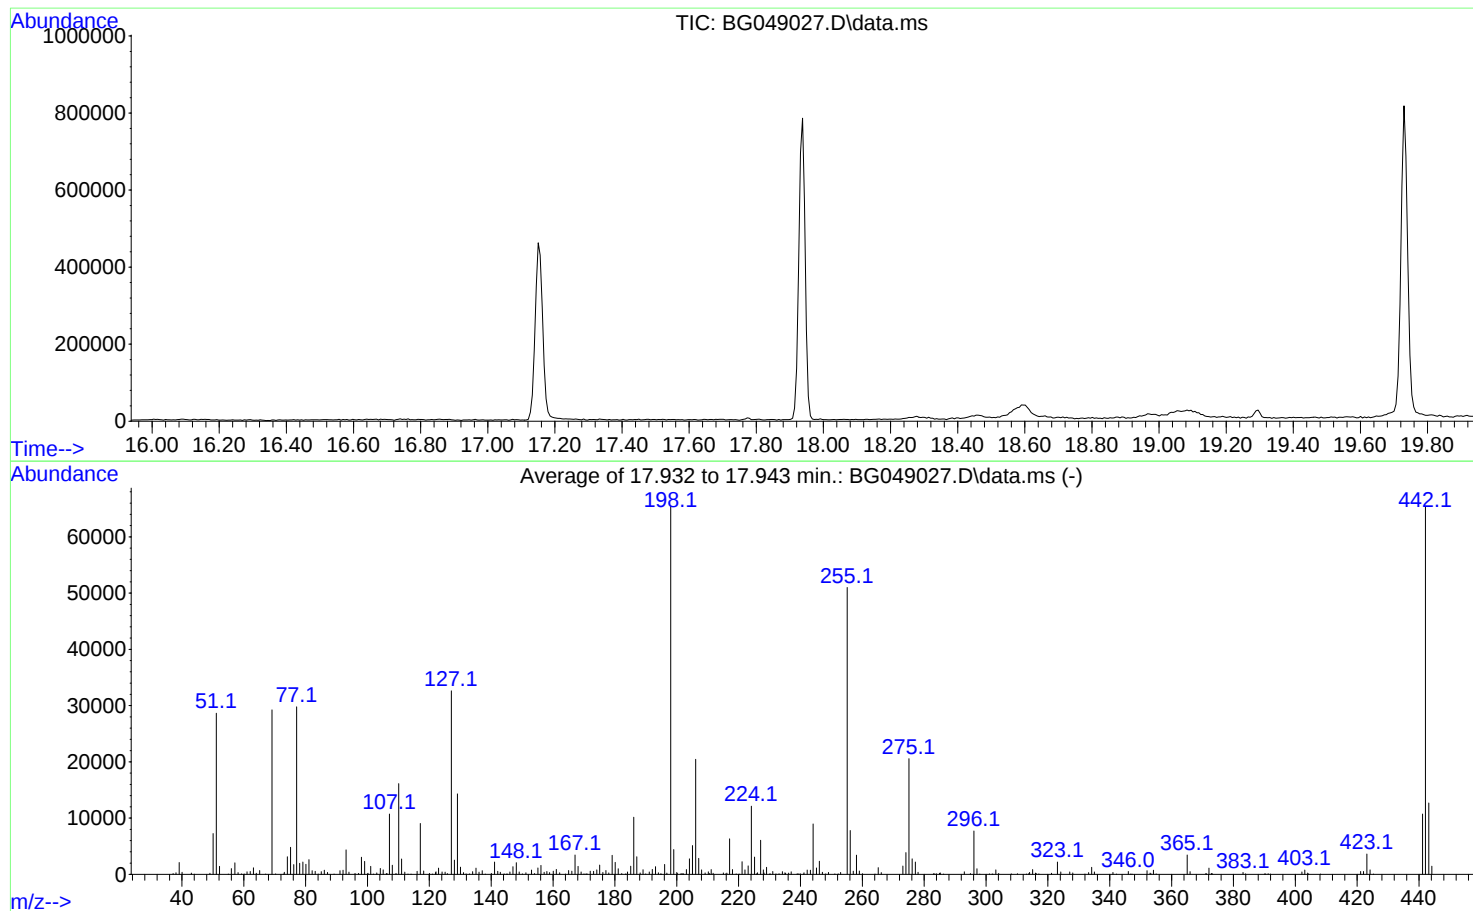




AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.8	28640	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.7	29232	PASS
70	69	0.00	2	0.3	100	PASS
127	198	10	80	49.9	32637	PASS
197	198	0.00	2	0.4	233	PASS
198	198	100	100	100.0	65395	PASS
199	198	5	9	6.8	4417	PASS
275	198	10	60	31.4	20563	PASS
365	198	1	100	5.3	3451	PASS
441	198	0.01	100	16.4	10733	PASS
442	442	100	100	100.0	65363	PASS
443	442	15	24	19.4	12687	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
 Data File : BG049027.D
 Acq On : 21 Jun 2021 10:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 21 13:15:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 12:04:50 2021
 Response via : Initial Calibration

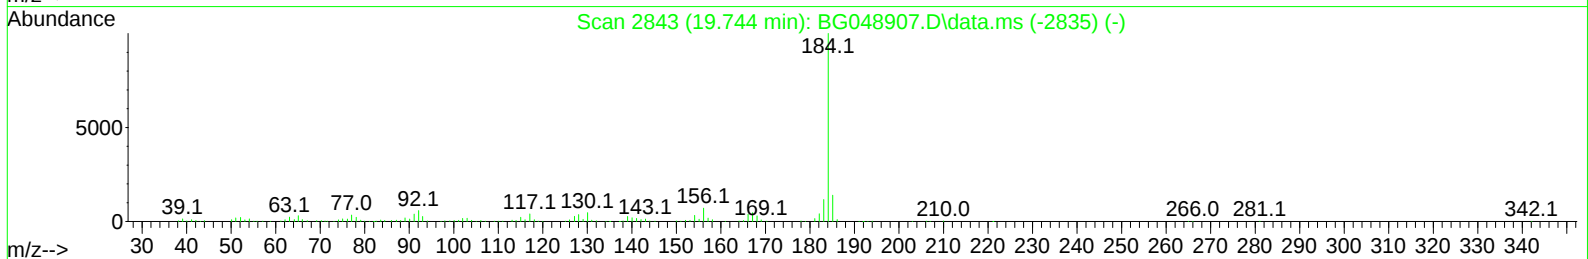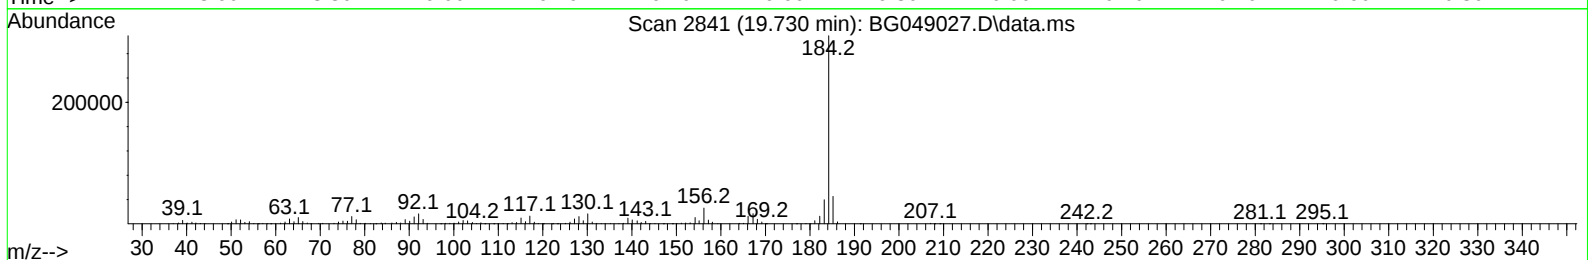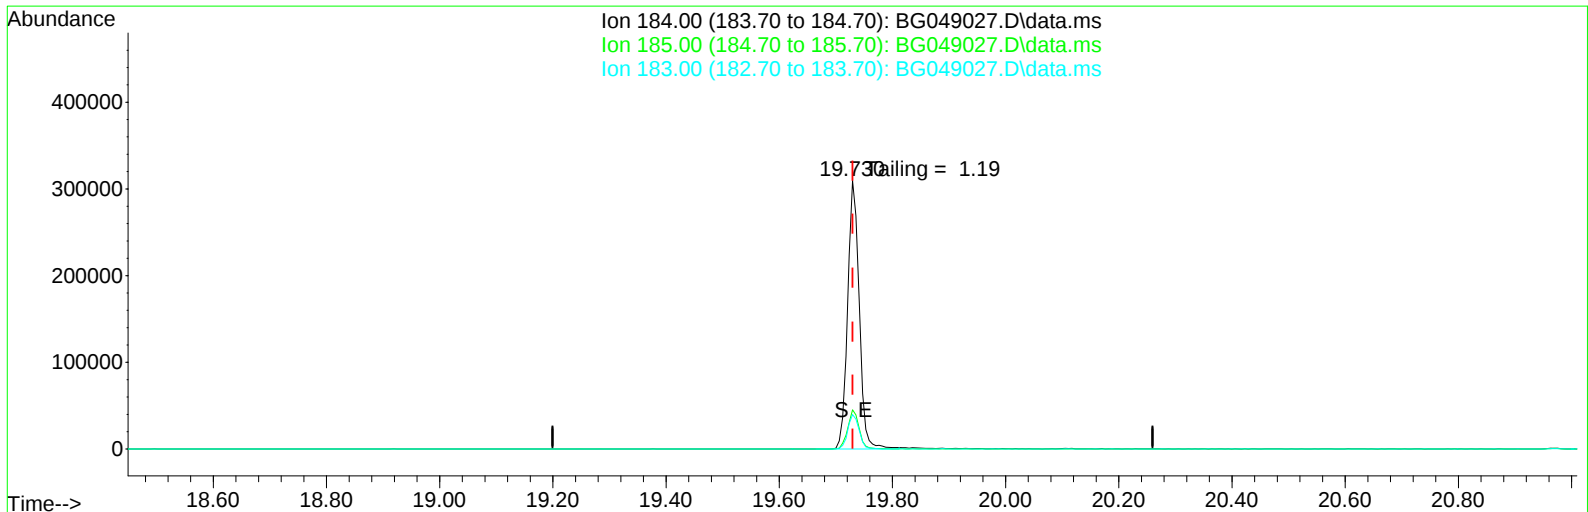

TIC: BG049027.D\data.ms

(77) Benzidine

19.730min (+ 0.000) 291214.73 ng m




response 439988

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.62
183.00	11.70	12.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062121\
 Data File : BG049027.D
 Acq On : 21 Jun 2021 10:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 21 13:15:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 12:04:50 2021
 Response via : Initial Calibration

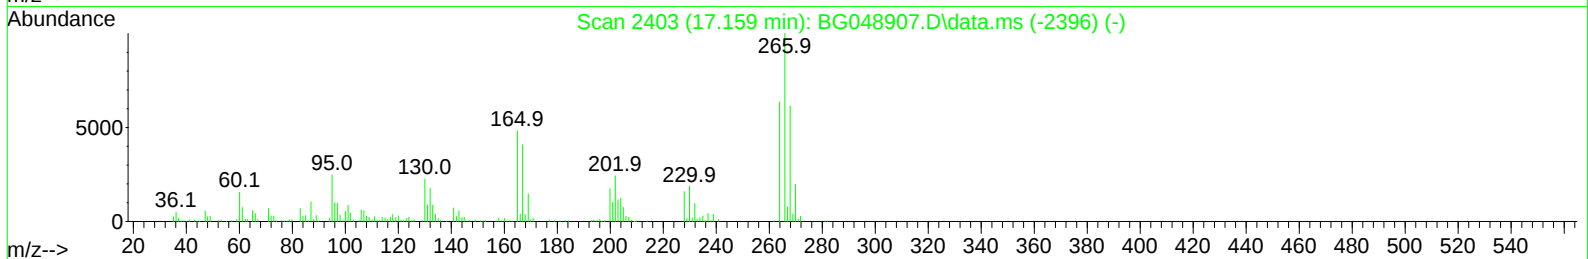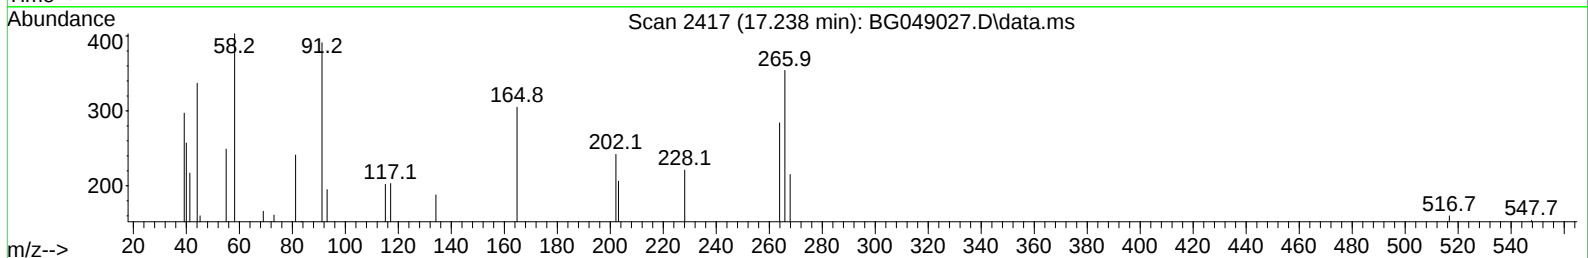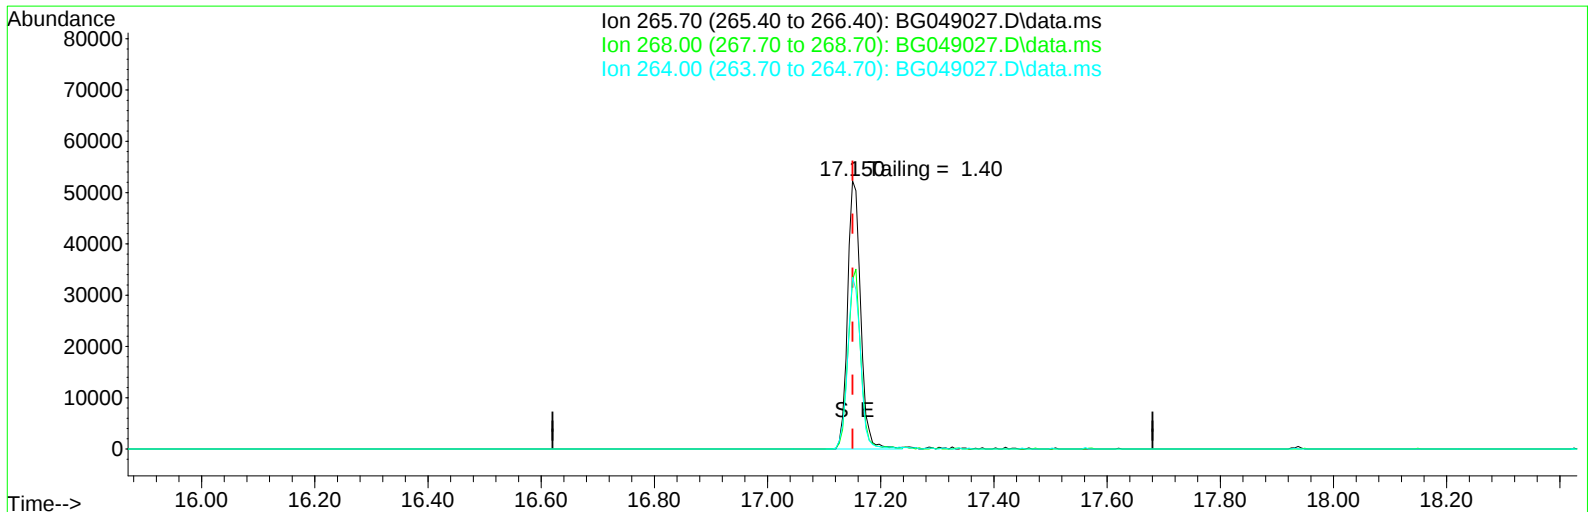

TIC: BG049027.D\data.ms

(70) Pentachlorophenol (C)

17.150min (+ 0.000) 28263.73 ng

response 83214

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.08
264.00	61.30	63.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/21/2021	BNA_G	BG049027.D
Compound Name	Response	Retention Time
DDT	233428	20.96
DDD	3240	20.96
DDE	454	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3694	237122	1.56

Instrument :
BNA_G
ClientSampleId :
DFTPP