

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
 Data File : BG061613.D
 Acq On : 21 Jun 2024 9:48
 Operator : MA/JU
 Sample : PB161409BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK409

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061613.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	27	31	36	rVV2	13663	19874	1.20%	0.131%
2	3.557	45	46	50	rBV4	2602	3311	0.20%	0.022%
3	3.880	99	101	116	rVV	179764	302103	18.22%	1.996%
4	3.986	116	119	123	rVV5	3665	6625	0.40%	0.044%
5	4.033	125	127	130	rVB4	3400	3355	0.20%	0.022%
6	4.062	130	132	134	rBV2	2566	2602	0.16%	0.017%
7	4.315	172	175	177	rBV3	2734	2589	0.16%	0.017%
8	4.403	188	190	195	rVB5	2504	3477	0.21%	0.023%
9	4.450	195	198	201	rBV2	2108	3253	0.20%	0.021%
10	4.674	235	236	240	rVB	2324	2581	0.16%	0.017%
11	4.709	240	242	245	rBV2	1988	2851	0.17%	0.019%
12	4.744	245	248	249	rVV	2970	3300	0.20%	0.022%
13	4.779	253	254	258	rVV2	3708	3375	0.20%	0.022%
14	4.832	261	263	266	rBV	2444	2500	0.15%	0.017%
15	5.220	327	329	333	rBV	1941	3124	0.19%	0.021%
16	5.572	388	389	396	rVB2	2782	4456	0.27%	0.029%
17	5.672	404	406	408	rVV	3343	3089	0.19%	0.020%
18	5.708	408	412	415	rVV2	2076	3766	0.23%	0.025%
19	5.749	417	419	421	rVB2	3754	2574	0.16%	0.017%
20	6.142	484	486	489	rBV3	2738	3213	0.19%	0.021%
21	6.765	587	592	593	rBV	3115	3425	0.21%	0.023%
22	6.789	593	596	598	rBV	2219	2491	0.15%	0.016%
23	6.847	602	606	608	rVB	3185	3517	0.21%	0.023%
24	6.877	608	611	616	rBV2	2505	4394	0.27%	0.029%
25	7.206	659	667	678	rBV	213346	356002	21.47%	2.352%
26	7.400	693	700	707	rVB	149345	251490	15.17%	1.662%
27	7.511	717	719	722	rVB	2959	2457	0.15%	0.016%
28	7.594	725	733	743	rVV	180336	323700	19.52%	2.139%
29	8.075	806	815	824	rVB	142452	251356	15.16%	1.661%
30	8.140	824	826	829	rBV2	1846	2522	0.15%	0.017%
31	8.540	893	894	899	rBV2	3237	3252	0.20%	0.021%
32	8.587	901	902	905	rBV2	2871	2682	0.16%	0.018%
33	8.763	925	932	939	rBV	247291	414525	25.00%	2.739%
34	8.921	958	959	962	rBV	2756	2881	0.17%	0.019%
35	8.980	965	969	973	rVB	2560	3990	0.24%	0.026%
36	9.233	1006	1012	1020	rVB	181694	321847	19.41%	2.126%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
 Data File : BG061613.D
 Acq On : 21 Jun 2024 9:48
 Operator : MA/JU
 Sample : PB161409BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK409

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	9.832	1111	1114	1117	rVB	3743	5242	0.32%	0.035%
38	9.961	1128	1136	1144	rVV	136952	242365	14.62%	1.601%
39	10.490	1217	1226	1234	rBV2	231930	403153	24.32%	2.664%
40	10.884	1284	1293	1301	rBV	213312	390065	23.53%	2.577%
41	11.013	1308	1315	1325	rVB	261050	471189	28.42%	3.113%
42	11.084	1325	1327	1330	rBV	3855	4268	0.26%	0.028%
43	11.119	1332	1333	1336	rVV	2354	2848	0.17%	0.019%
44	11.142	1336	1337	1342	rVB	3158	3366	0.20%	0.022%
45	11.260	1354	1357	1358	rBV	2698	2765	0.17%	0.018%
46	11.313	1365	1366	1370	rVB	3031	2480	0.15%	0.016%
47	11.354	1370	1373	1375	rBV	2578	3195	0.19%	0.021%
48	11.401	1378	1381	1383	rBV	2307	2438	0.15%	0.016%
49	11.706	1429	1433	1434	rBV	2185	2538	0.15%	0.017%
50	11.983	1477	1480	1483	rBV	2348	2600	0.16%	0.017%
51	12.094	1495	1499	1500	rBV	2071	2905	0.18%	0.019%
52	12.241	1522	1524	1528	rVB2	2800	3447	0.21%	0.023%
53	12.335	1537	1540	1542	rBV	2357	3122	0.19%	0.021%
54	12.470	1557	1563	1570	rVB3	6685	13229	0.80%	0.087%
55	12.658	1593	1595	1599	rBV	1883	2546	0.15%	0.017%
56	12.981	1648	1650	1653	rBV	3340	4601	0.28%	0.030%
57	13.011	1653	1655	1659	rVB2	2361	3019	0.18%	0.020%
58	13.075	1663	1666	1668	rBV	3608	2728	0.16%	0.018%
59	13.152	1677	1679	1682	rVB2	3547	3952	0.24%	0.026%
60	13.293	1702	1703	1706	rVB	2997	2453	0.15%	0.016%
61	13.739	1776	1779	1781	rBV2	2445	3435	0.21%	0.023%
62	14.039	1829	1830	1833	rBV	2646	2864	0.17%	0.019%
63	14.110	1836	1842	1848	rVV	491521	721404	43.51%	4.766%
64	14.397	1883	1891	1898	rBV	508226	781591	47.14%	5.164%
65	14.568	1918	1920	1922	rBV	2824	2834	0.17%	0.019%
66	14.703	1936	1943	1950	rVB	359582	567252	34.21%	3.748%
67	14.862	1964	1970	1979	rBV	261487	411778	24.84%	2.721%
68	15.402	2059	2062	2065	rBV2	3290	3190	0.19%	0.021%
69	15.496	2077	2078	2082	rBV2	2754	2808	0.17%	0.019%
70	15.690	2105	2111	2117	rVB	659794	1015617	61.25%	6.710%
71	15.790	2123	2128	2136	rBV	174165	265154	15.99%	1.752%
72	15.931	2150	2152	2156	rVB5	5588	5148	0.31%	0.034%
73	16.048	2170	2172	2175	rVB	5885	4314	0.26%	0.029%
74	16.078	2175	2177	2178	rBV	4057	2659	0.16%	0.018%
75	16.219	2198	2201	2205	rBV3	4319	6222	0.38%	0.041%
76	16.424	2234	2236	2237	rBV	3548	2624	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
 Data File : BG061613.D
 Acq On : 21 Jun 2024 9:48
 Operator : MA/JU
 Sample : PB161409BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK409

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

77	16.595	2263	2265	2268	rBV2	2280	2656	0.16%	0.018%
78	17.130	2353	2356	2359	rBV	2807	3928	0.24%	0.026%
79	17.447	2401	2410	2417	rBV	536277	827106	49.89%	5.465%
80	17.541	2420	2426	2436	rBV2	831803	1252533	75.54%	8.275%
81	17.776	2465	2466	2469	rBV2	2856	2596	0.16%	0.017%
82	17.829	2474	2475	2478	rBV	2919	2710	0.16%	0.018%
83	17.952	2495	2496	2498	rBV2	4315	3802	0.23%	0.025%
84	18.017	2506	2507	2511	rVB	6035	3796	0.23%	0.025%
85	18.052	2511	2513	2514	rBV2	4647	4304	0.26%	0.028%
86	18.087	2518	2519	2521	rBV	3973	2967	0.18%	0.020%
87	18.193	2535	2537	2540	rBV3	2893	2863	0.17%	0.019%
88	18.393	2570	2571	2573	rBV	3849	3297	0.20%	0.022%
89	18.487	2585	2587	2592	rVB3	5729	6516	0.39%	0.043%
90	18.522	2592	2593	2595	rBV2	4691	3306	0.20%	0.022%
91	18.898	2655	2657	2659	rBV2	3804	3182	0.19%	0.021%
92	19.392	2736	2741	2745	rVB3	15497	20979	1.27%	0.139%
93	19.462	2750	2753	2757	rVB3	14199	18068	1.09%	0.119%
94	19.715	2794	2796	2798	rBV2	5885	3720	0.22%	0.025%
95	19.820	2808	2814	2824	rBV	1068006	1558443	93.99%	10.296%
96	19.956	2835	2837	2839	rBV3	6869	7796	0.47%	0.052%
97	20.044	2850	2852	2853	rBV2	5236	3339	0.20%	0.022%
98	21.707	3129	3135	3144	rVB	584028	974923	58.80%	6.441%
99	24.715	3637	3647	3659	rVB2	604593	1658021	100.00%	10.954%
100	24.932	3675	3684	3696	rVB2	379338	1052955	63.51%	6.957%




Sum of corrected areas: 15135763

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
Data File : BG061613.D
Acq On : 21 Jun 2024 9:48
Operator : MA/JU
Sample : PB161409BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

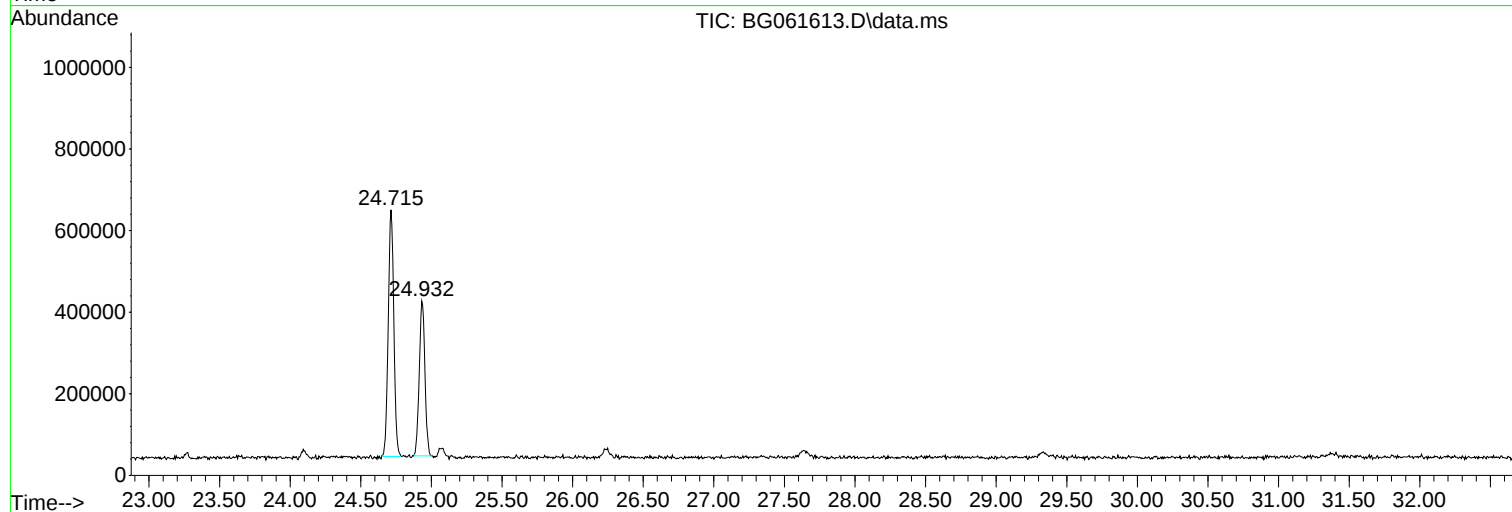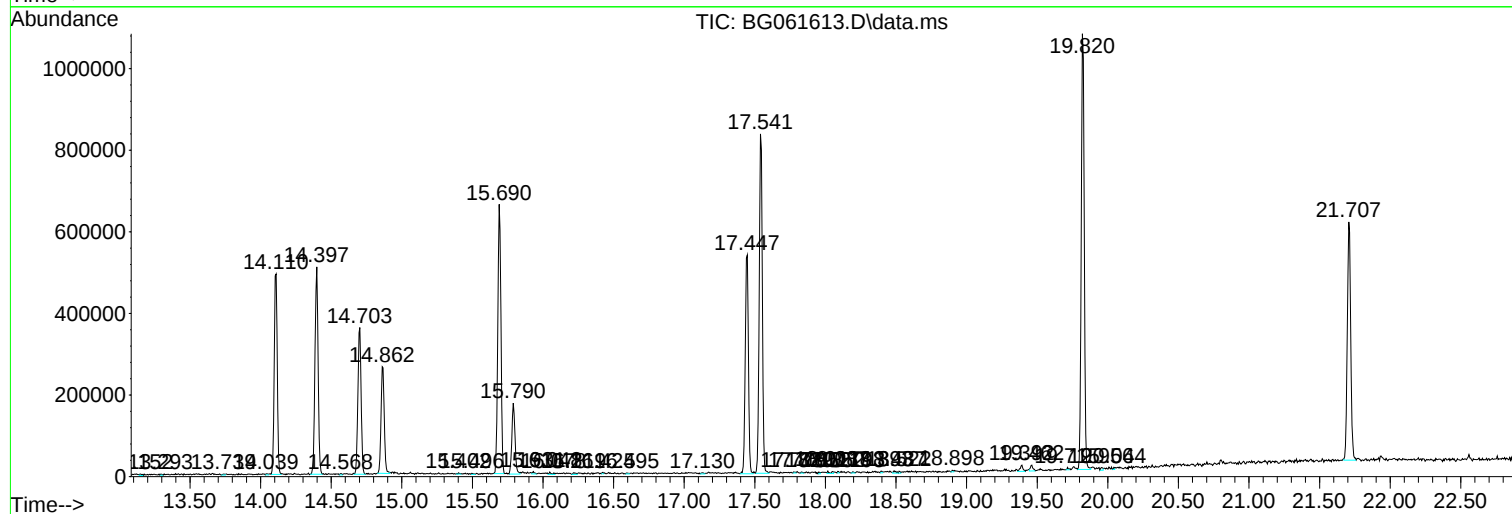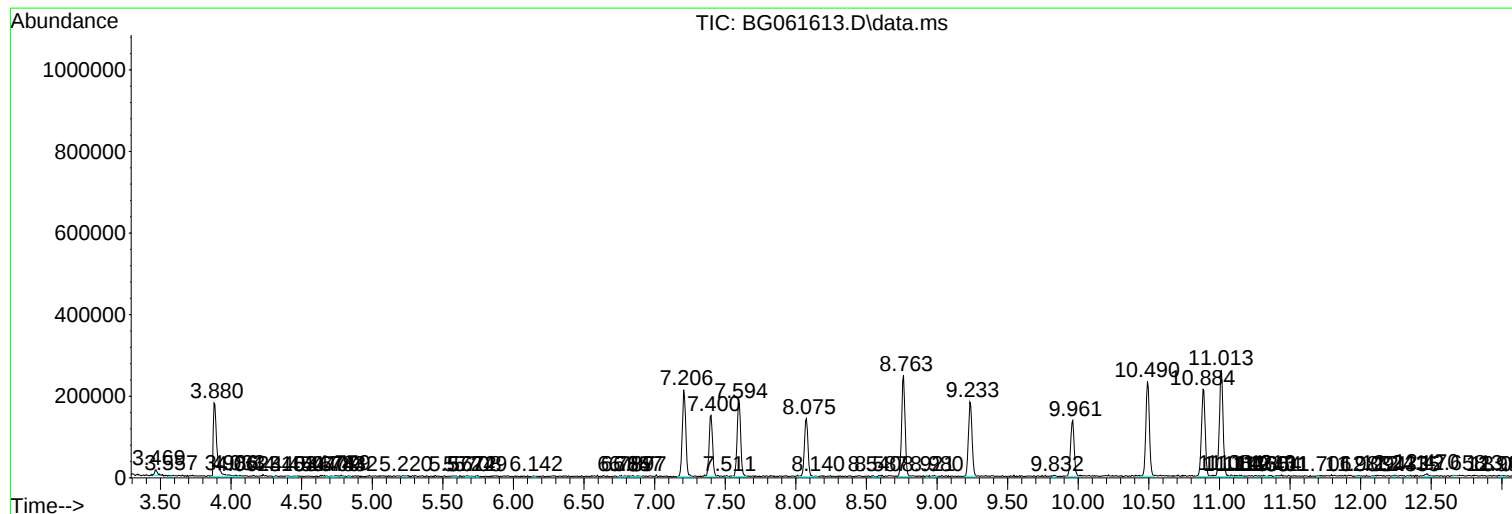

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
Data File : BG061613.D
Acq On : 21 Jun 2024 9:48
Operator : MA/JU
Sample : PB161409BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
Data File : BG061613.D
Acq On : 21 Jun 2024 9:48
Operator : MA/JU
Sample : PB161409BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc