

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
 Data File : BG061624.D
 Acq On : 21 Jun 2024 17:33
 Operator : MA/JU
 Sample : PB161409BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK409

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.470	27	31	37	rVB3	18971	28745	1.40%	0.135%
2	3.587	49	51	53	rVB2	6183	3811	0.19%	0.018%
3	3.887	98	102	111	rBV	287861	467324	22.71%	2.189%
4	4.216	156	158	161	rBV3	2852	3174	0.15%	0.015%
5	4.568	216	218	221	rVB3	3564	2765	0.13%	0.013%
6	5.038	295	298	301	rBV4	2044	3423	0.17%	0.016%
7	5.074	303	304	308	rVB3	2765	3014	0.15%	0.014%
8	5.168	317	320	324	rBV3	3426	4205	0.20%	0.020%
9	5.491	373	375	380	rBV4	2258	3694	0.18%	0.017%
10	5.896	442	444	449	rVB3	2440	3814	0.19%	0.018%
11	6.084	473	476	478	rVB3	3218	3679	0.18%	0.017%
12	6.108	478	480	482	rBV3	2581	2780	0.14%	0.013%
13	6.284	506	510	511	rBV2	2711	2866	0.14%	0.013%
14	6.372	524	525	531	rVB3	2710	2968	0.14%	0.014%
15	6.437	531	536	538	rBV	2262	3525	0.17%	0.017%
16	6.660	570	574	575	rVB3	3294	3520	0.17%	0.016%
17	6.678	575	577	579	rBV2	2850	2765	0.13%	0.013%
18	6.872	607	610	612	rVB2	2517	2783	0.14%	0.013%
19	7.030	632	637	638	rBV4	3234	3748	0.18%	0.018%
20	7.212	661	668	675	rBV	325424	550074	26.74%	2.576%
21	7.353	690	692	694	rBV	2587	3092	0.15%	0.014%
22	7.400	694	700	708	rVV	241312	390899	19.00%	1.831%
23	7.600	725	734	745	rBV	299719	518225	25.19%	2.427%
24	7.688	745	749	752	rVB3	2299	3874	0.19%	0.018%
25	7.741	755	758	760	rBV2	3938	4116	0.20%	0.019%
26	7.806	767	769	772	rBV2	2750	3994	0.19%	0.019%
27	8.076	809	815	823	rBV	226709	378581	18.40%	1.773%
28	8.282	847	850	852	rBV3	2406	2994	0.15%	0.014%
29	8.763	923	932	940	rBV2	404840	678290	32.97%	3.177%
30	8.881	950	952	958	rVB	2714	3192	0.16%	0.015%
31	8.975	966	968	973	rBV3	2900	3508	0.17%	0.016%
32	9.234	1005	1012	1023	rBV	296794	532434	25.88%	2.493%
33	9.892	1120	1124	1125	rBV3	2467	3439	0.17%	0.016%
34	9.962	1129	1136	1143	rBV	236434	419214	20.38%	1.963%
35	10.203	1175	1177	1180	rBV2	2314	3143	0.15%	0.015%
36	10.309	1192	1195	1200	rBV4	2498	3715	0.18%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
 Data File : BG061624.D
 Acq On : 21 Jun 2024 17:33
 Operator : MA/JU
 Sample : PB161409BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK409

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	10.379	1205	1207	1210	rBV2	4101	4099	0.20%	0.019%
38	10.491	1219	1226	1239	rVB	366935	664981	32.32%	3.114%
39	10.585	1239	1242	1243	rBV3	2936	3031	0.15%	0.014%
40	10.885	1286	1293	1300	rVB	337244	593809	28.86%	2.781%
41	11.014	1308	1315	1324	rBV	405956	712476	34.63%	3.337%
42	11.208	1345	1348	1350	rVB2	2635	3041	0.15%	0.014%
43	11.243	1350	1354	1355	rBV	3010	3122	0.15%	0.015%
44	11.319	1364	1367	1370	rVB2	3182	4637	0.23%	0.022%
45	11.355	1370	1373	1375	rBV2	2318	2935	0.14%	0.014%
46	11.877	1458	1462	1464	rVB	4179	4343	0.21%	0.020%
47	11.930	1468	1471	1473	rBV3	3931	3114	0.15%	0.015%
48	12.024	1486	1487	1490	rBV	2946	3257	0.16%	0.015%
49	12.365	1541	1545	1547	rBV2	2655	2935	0.14%	0.014%
50	12.447	1558	1559	1560	rBV	5567	3307	0.16%	0.015%
51	12.923	1637	1640	1641	rBV	2877	2792	0.14%	0.013%
52	13.135	1672	1676	1681	rBV3	2975	3172	0.15%	0.015%
53	13.317	1705	1707	1709	rVB	3999	2914	0.14%	0.014%
54	13.581	1750	1752	1755	rVB	3058	3048	0.15%	0.014%
55	13.664	1763	1766	1767	rBV	2792	3201	0.16%	0.015%
56	13.811	1789	1791	1794	rBV	1984	2810	0.14%	0.013%
57	13.981	1819	1820	1822	rBV2	3968	2797	0.14%	0.013%
58	14.104	1835	1841	1849	rBV	707998	1002923	48.75%	4.697%
59	14.204	1852	1858	1859	rBV2	3234	5459	0.27%	0.026%
60	14.392	1884	1890	1900	rVB	749286	1201637	58.40%	5.627%
61	14.474	1900	1904	1906	rVB2	3376	4358	0.21%	0.020%
62	14.592	1923	1924	1927	rBV2	5485	3596	0.17%	0.017%
63	14.698	1935	1942	1951	rVB	552687	874265	42.49%	4.094%
64	14.862	1964	1970	1979	rBV	400784	640942	31.15%	3.002%
65	14.944	1982	1984	1986	rVV2	3965	3497	0.17%	0.016%
66	15.009	1993	1995	2000	rVB	2221	3241	0.16%	0.015%
67	15.150	2016	2019	2020	rBV2	4949	4129	0.20%	0.019%
68	15.356	2051	2054	2055	rBV	2727	3049	0.15%	0.014%
69	15.497	2077	2078	2080	rVB2	5180	2936	0.14%	0.014%
70	15.597	2093	2095	2098	rVB2	3225	3186	0.15%	0.015%
71	15.632	2098	2101	2104	rBV3	5927	4935	0.24%	0.023%
72	15.691	2104	2111	2119	rBV	1012905	1499747	72.89%	7.024%
73	15.791	2123	2128	2134	rBV	295282	421295	20.48%	1.973%
74	15.896	2145	2146	2148	rBV2	4995	3517	0.17%	0.016%
75	15.926	2148	2151	2157	rVV6	5259	9160	0.45%	0.043%
76	16.026	2167	2168	2170	rVB	4740	2870	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
 Data File : BG061624.D
 Acq On : 21 Jun 2024 17:33
 Operator : MA/JU
 Sample : PB161409BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK409

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

77	16.055	2170	2173	2175	rBV2	3232	3796	0.18%	0.018%
78	16.161	2190	2191	2194	rBV3	2986	3400	0.17%	0.016%
79	16.331	2219	2220	2222	rBV	3620	3088	0.15%	0.014%
80	16.496	2244	2248	2253	rBV4	3686	5778	0.28%	0.027%
81	16.778	2292	2296	2297	rBV3	3366	3519	0.17%	0.016%
82	16.972	2327	2329	2332	rVB	6260	4886	0.24%	0.023%
83	17.007	2332	2335	2336	rBV2	4130	3497	0.17%	0.016%
84	17.236	2372	2374	2378	rVB4	3421	3338	0.16%	0.016%
85	17.442	2403	2409	2417	rVB	800380	1151831	55.98%	5.394%
86	17.541	2419	2426	2434	rVB2	1159571	1734603	84.31%	8.123%
87	17.677	2444	2449	2452	rBV4	8140	12591	0.61%	0.059%
88	17.806	2470	2471	2476	rVB3	5938	4951	0.24%	0.023%
89	18.041	2509	2511	2512	rBV	3960	2964	0.14%	0.014%
90	18.188	2534	2536	2539	rBV	3987	4271	0.21%	0.020%
91	18.329	2557	2560	2563	rBV4	9403	11712	0.57%	0.055%
92	19.040	2678	2681	2682	rBV	5636	5415	0.26%	0.025%
93	19.386	2735	2740	2744	rBV6	17483	27371	1.33%	0.128%
94	19.457	2748	2752	2757	rBV2	18688	29074	1.41%	0.136%
95	19.657	2782	2786	2787	rBV4	6699	8160	0.40%	0.038%
96	19.756	2801	2803	2806	rVB4	13977	12982	0.63%	0.061%
97	19.821	2808	2814	2820	rVV	1399328	1956908	95.11%	9.165%
98	21.707	3129	3135	3141	rVB	758561	1214558	59.03%	5.688%
99	24.710	3637	3646	3661	rVB	742999	2057477	100.00%	9.636%
100	24.933	3674	3684	3694	rBV2	465990	1306931	63.52%	6.121%




Sum of corrected areas: 21353051

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
Data File : BG061624.D
Acq On : 21 Jun 2024 17:33
Operator : MA/JU
Sample : PB161409BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

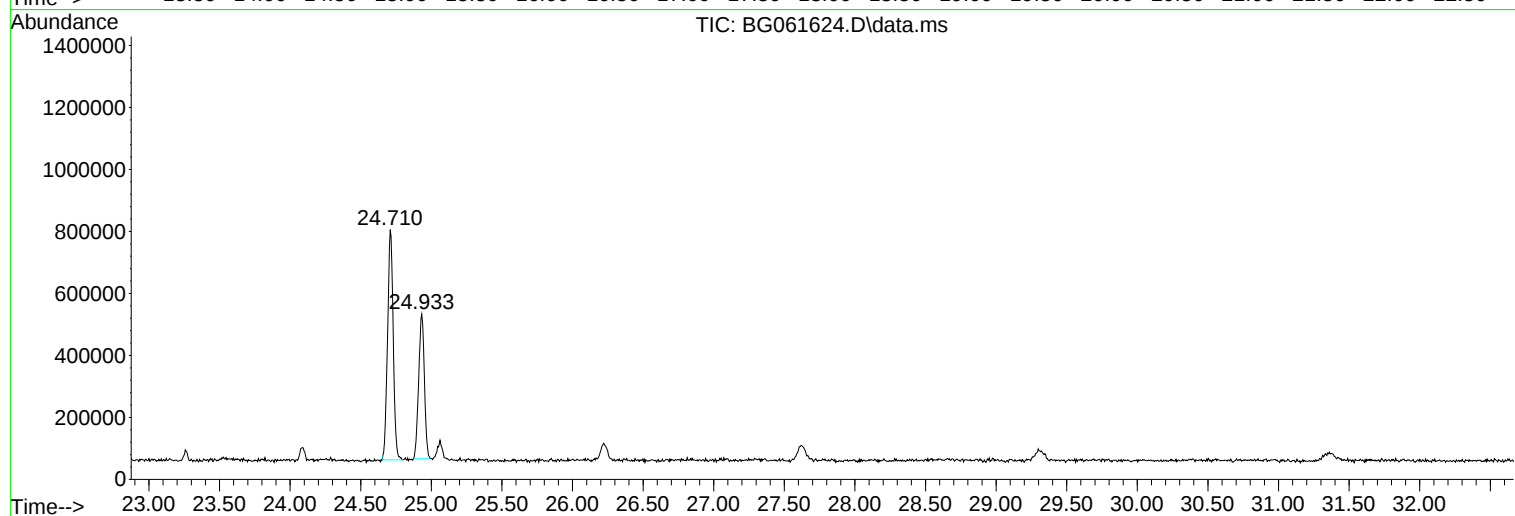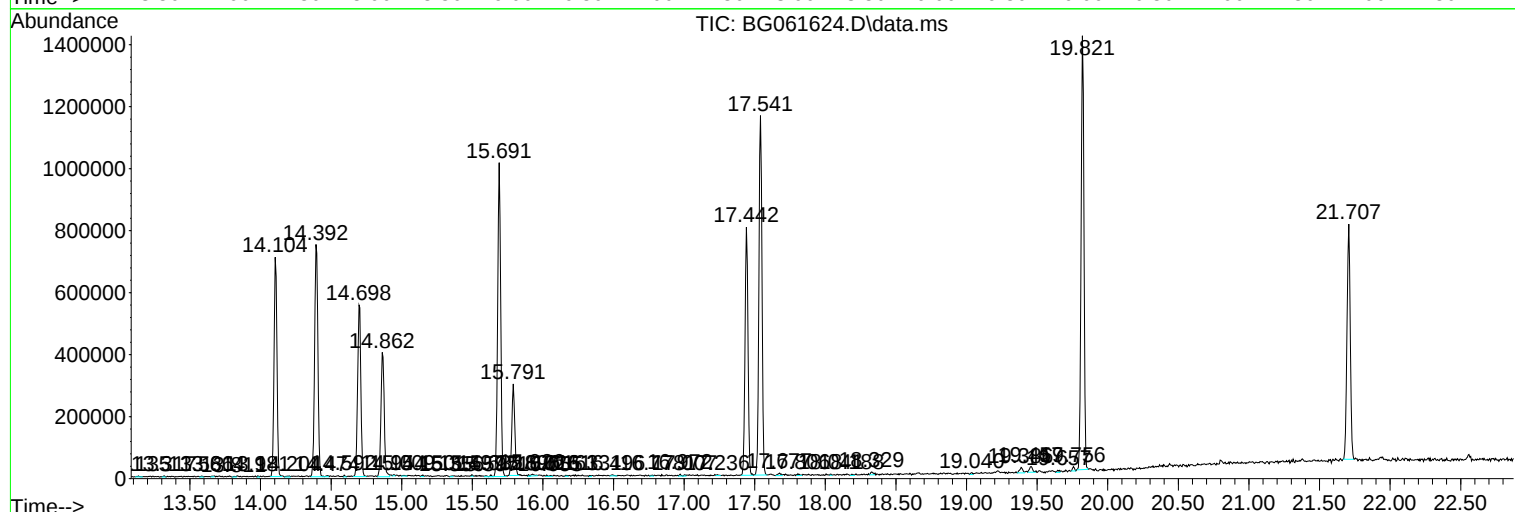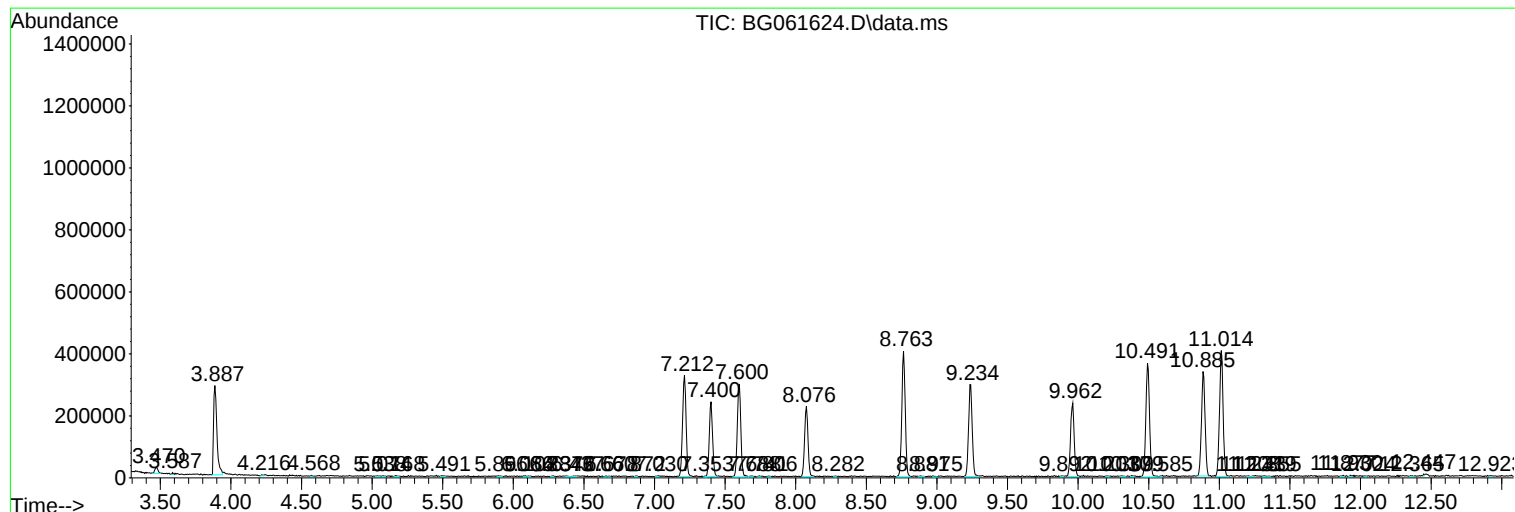

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
Data File : BG061624.D
Acq On : 21 Jun 2024 17:33
Operator : MA/JU
Sample : PB161409BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062124\
Data File : BG061624.D
Acq On : 21 Jun 2024 17:33
Operator : MA/JU
Sample : PB161409BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc