


Data Path : Z:\HPCHEM1\BNA_G\Data\BG062215\
 Data File : BG017738.D
 Acq On : 22 Jun 2015 9:45
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 06:05:07 2015

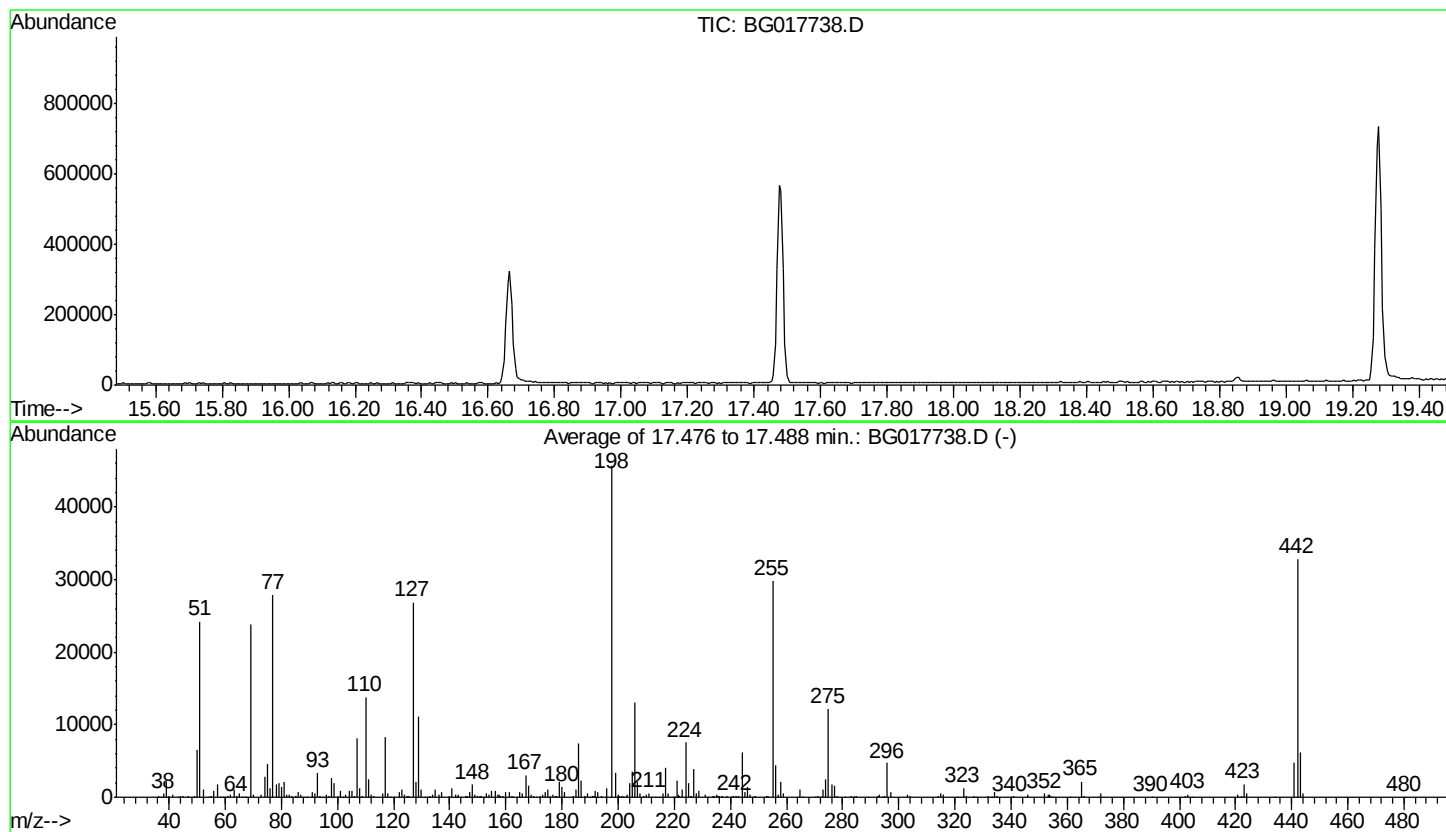

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	24253	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.3	23902	PASS
70	69	0.00	2	1.2	298	PASS
127	198	10	80	58.8	26858	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45706	PASS
199	198	5	9	7.5	3409	PASS
275	198	10	60	26.7	12201	PASS
365	198	1	100	4.7	2129	PASS
441	442	0.01	24	14.4	4736	PASS
442	198	50	100	71.9	32864	PASS
443	442	15	24	18.7	6152	PASS