
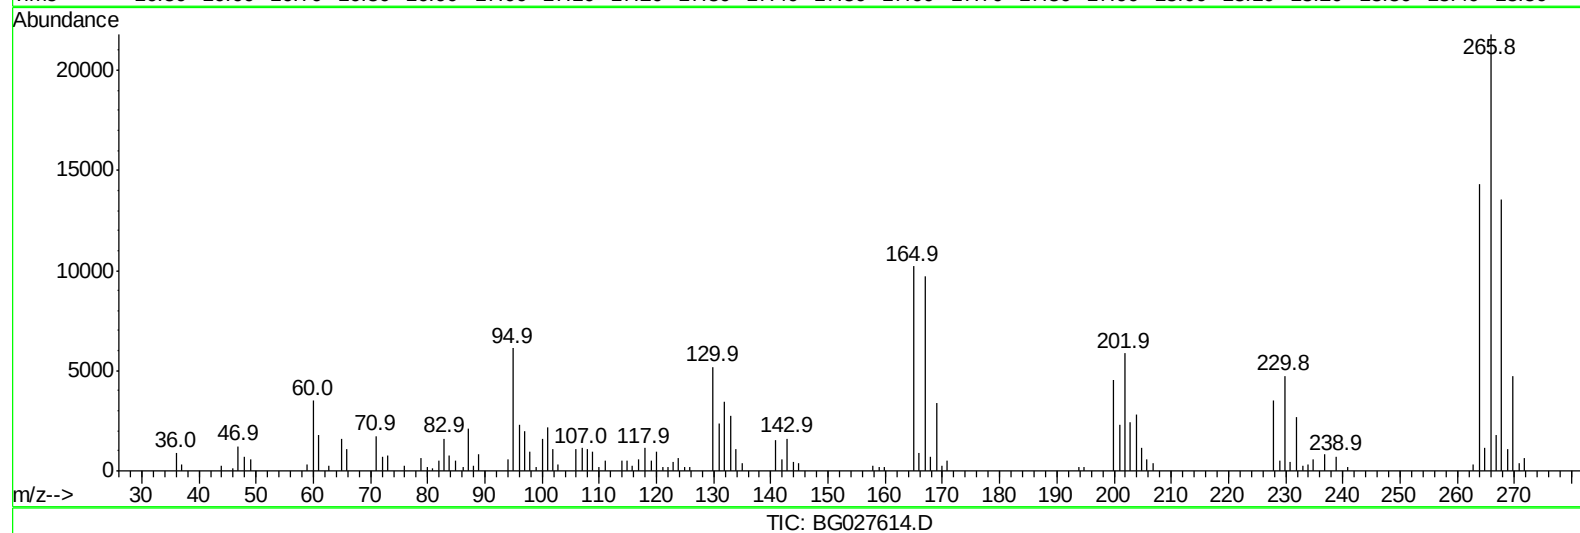


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062217\
Data File : BG027614.D
Acq On : 23 Jun 2017 2:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 07:39:06 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 18:52:15 2017
Response via : Initial Calibration

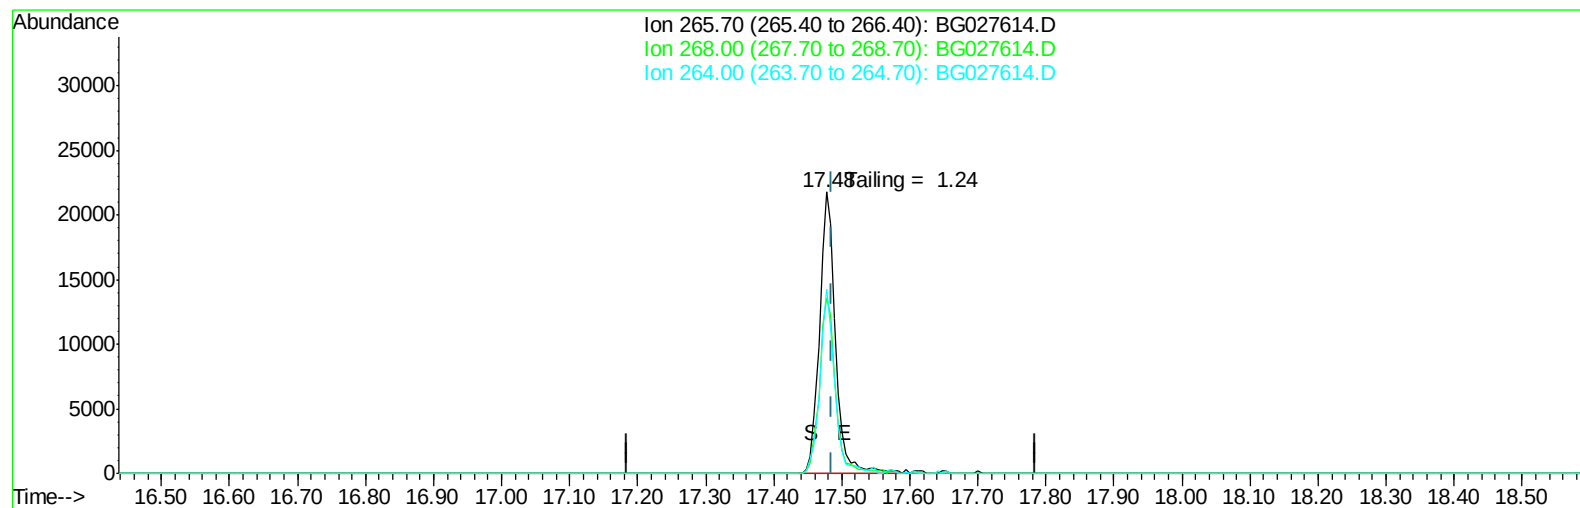

(69) Pentachlorophenol (C)



17.477min (-0.008) 0.00ng

response 35965

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.10
264.00	62.60	65.66
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062217\
Data File : BG027614.D
Acq On : 23 Jun 2017 2:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 07:39:06 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 18:52:15 2017
Response via : Initial Calibration

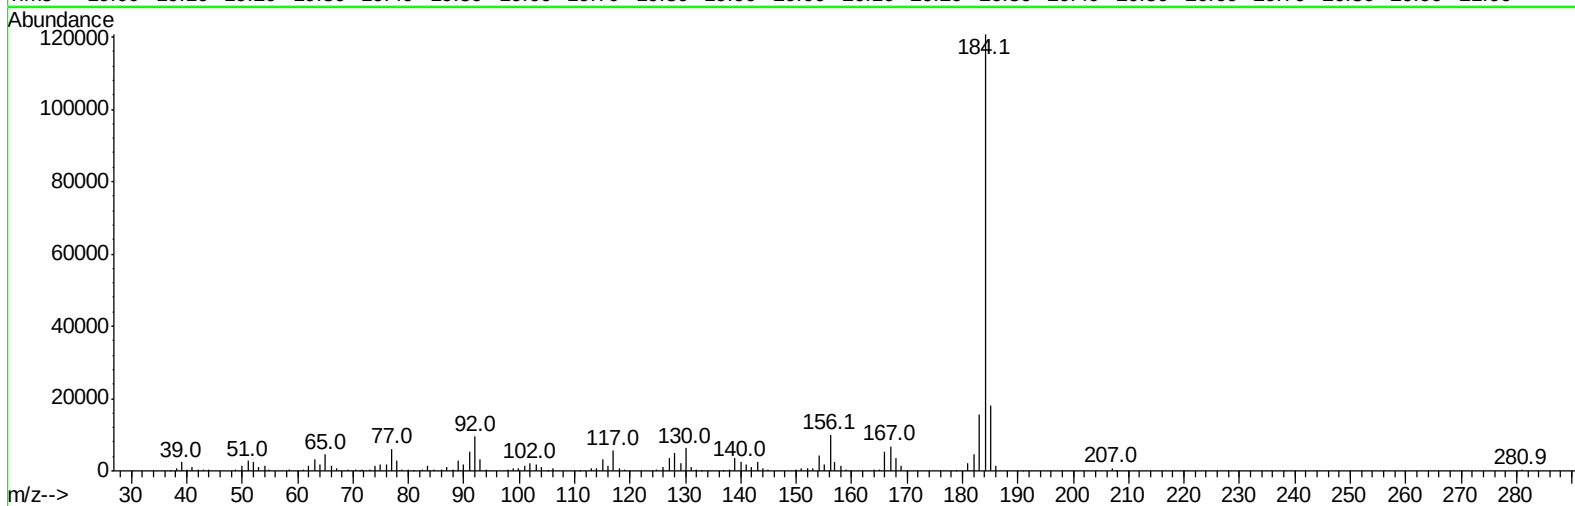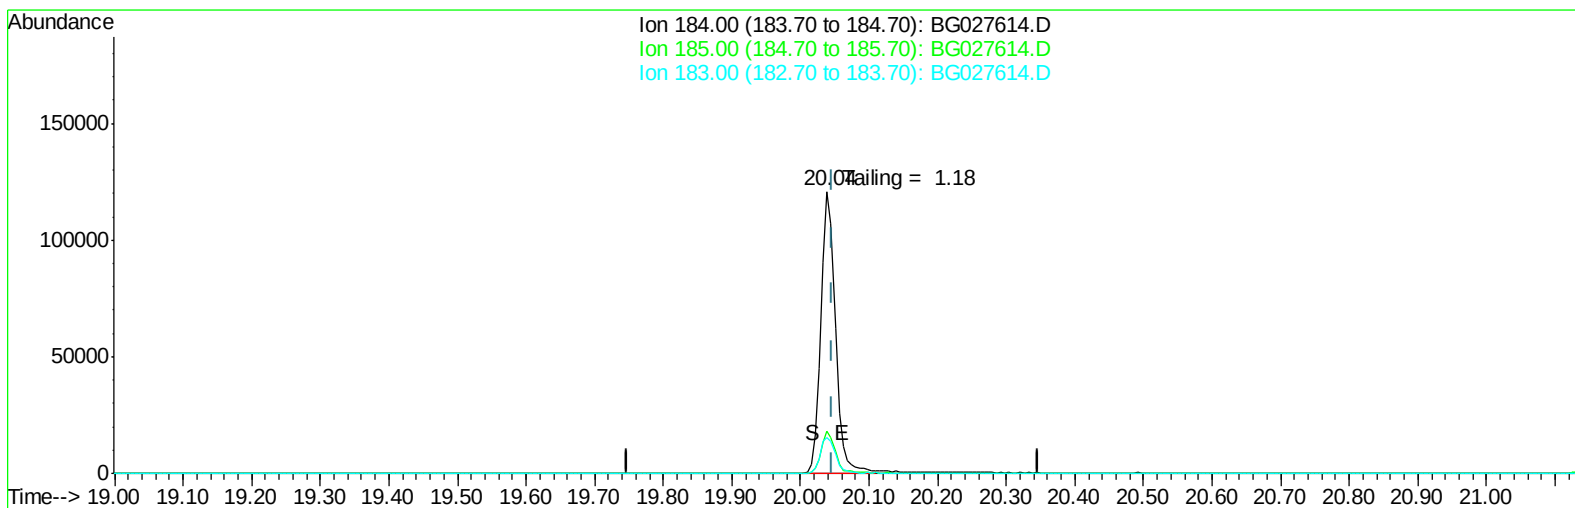

TIC: BG027614.D

(76) Benzidine

20.039min (-0.008) 0.00ng

response 179659

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.01
183.00	13.80	12.87
0.00	0.00	0.00