

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG062217\
 Data File : BG027623.D
 Acq On : 23 Jun 2017 9:15
 Operator : SJ/JU
 Sample : I3657-20
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-102S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.086	368	374	382	rBV	132616	224655	10.29%	3.024%
2	7.637	632	638	648	rVB	79250	147246	6.74%	1.982%
3	8.036	698	706	714	rBV	247993	458490	20.99%	6.172%
4	8.506	779	786	794	rVB	59738	101837	4.66%	1.371%
5	8.830	833	841	849	rBV	206075	386553	17.70%	5.204%
6	9.670	975	984	995	rBV	187458	360312	16.50%	4.851%
7	11.321	1256	1265	1273	rBV2	82472	158245	7.24%	2.130%
8	13.712	1663	1672	1679	rBV	583729	910628	41.69%	12.259%
9	15.087	1899	1906	1914	rVB2	145871	243591	11.15%	3.279%
10	16.573	2151	2159	2169	rBV	626727	1002516	45.90%	13.496%
11	17.837	2367	2374	2382	rBV	237061	378396	17.32%	5.094%
12	20.416	2806	2813	2820	rBV	1590191	2184281	100.00%	29.405%
13	22.202	3110	3117	3126	rBV	244758	463997	21.24%	6.246%
14	25.839	3724	3736	3748	rBV	124774	407530	18.66%	5.486%


Sum of corrected areas: 7428277

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG062217\
Data File : BG027623.D
Acq On : 23 Jun 2017 9:15
Operator : SJ/JU
Sample : I3657-20
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-102S

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

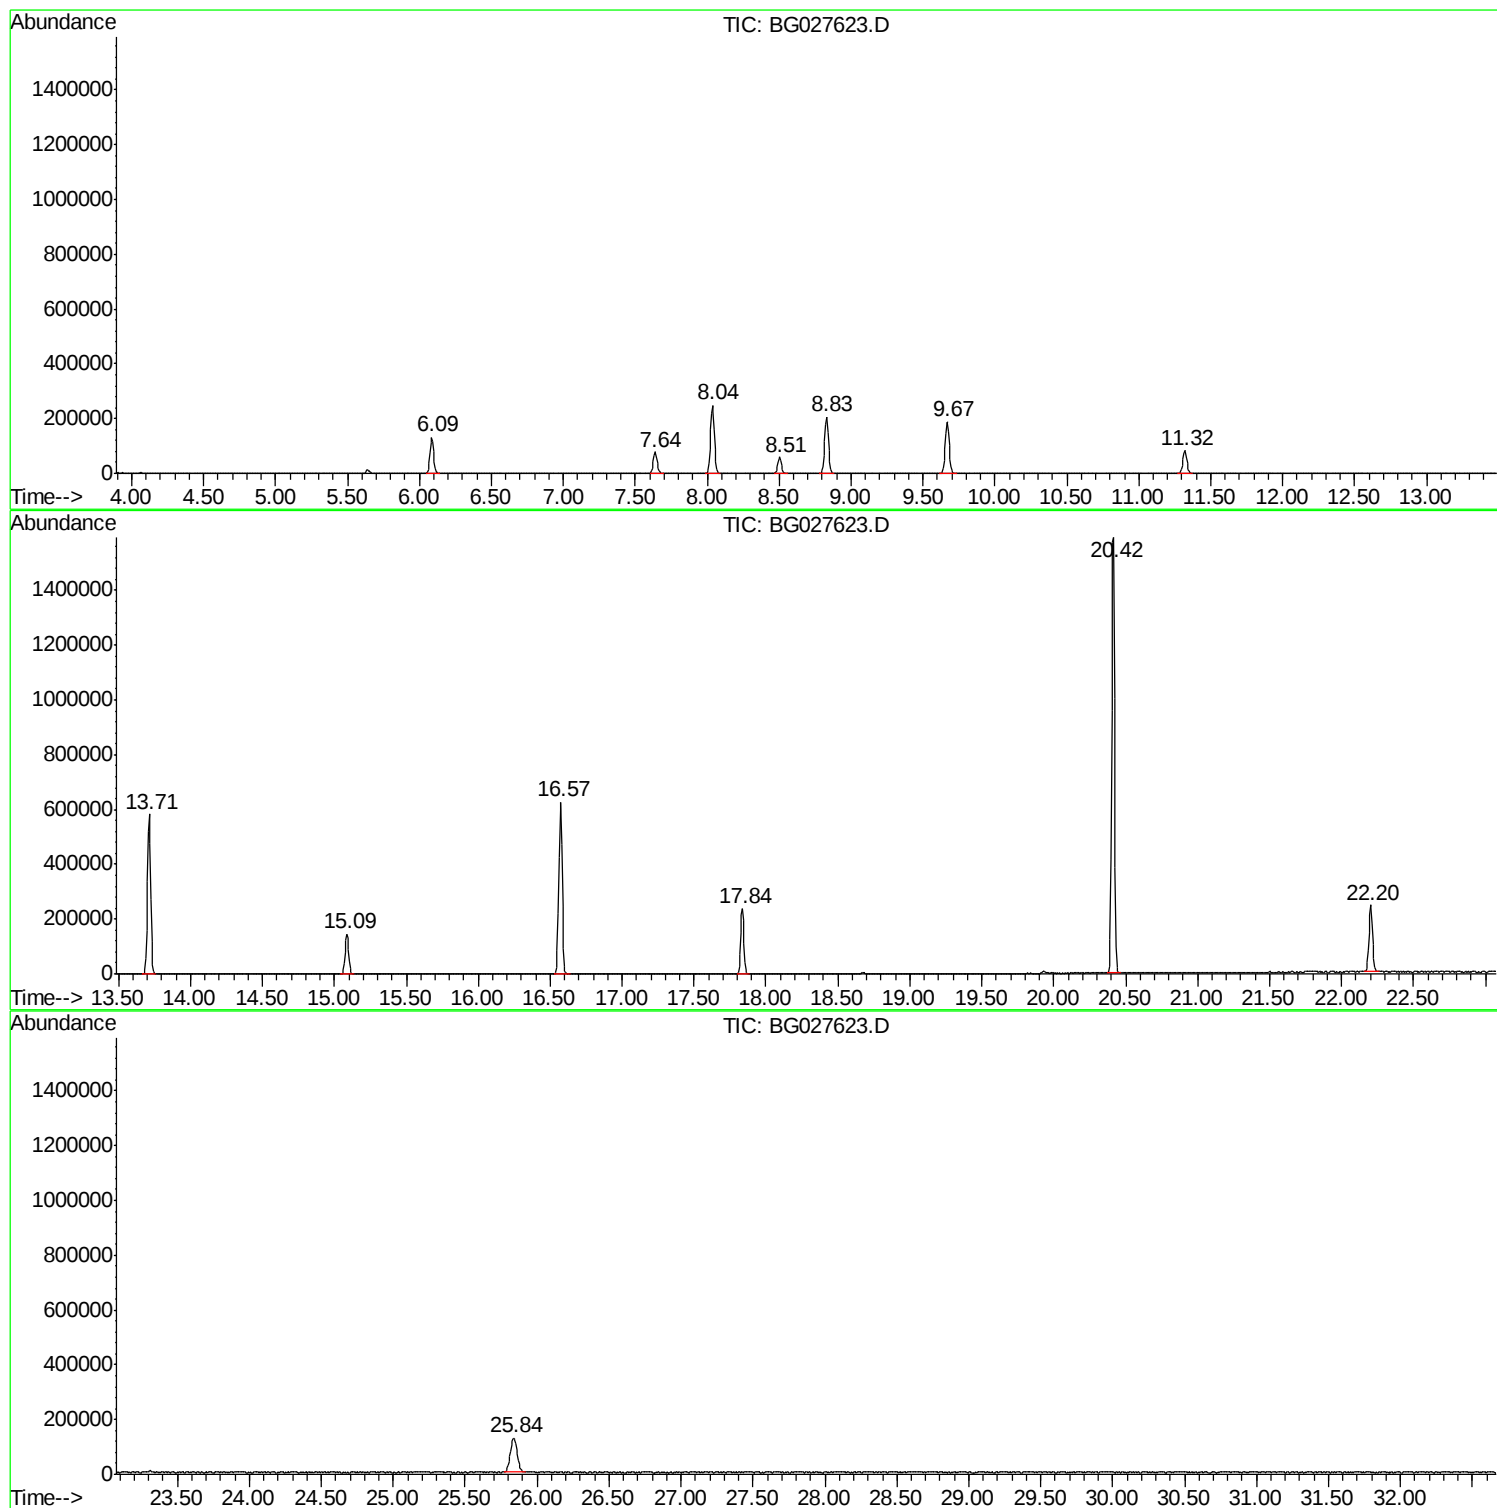

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG062217\
Data File : BG027623.D
Acq On : 23 Jun 2017 9:15
Operator : SJ/JU
Sample : I3657-20
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-102S










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown8.04 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.04	90.04 ng	458490	1,4-Dichlorobenzene-d4	8.51

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	27
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		Imidazole, 4,5-dicvano-1-methyl-	132	C6H4N4	019485-35-9	22
5		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	17

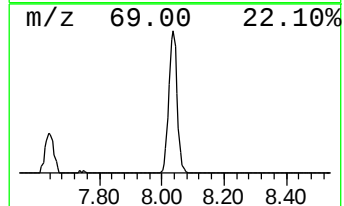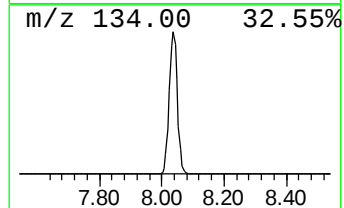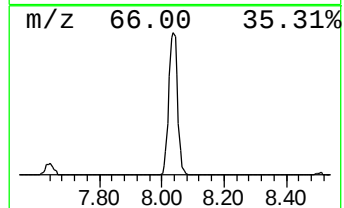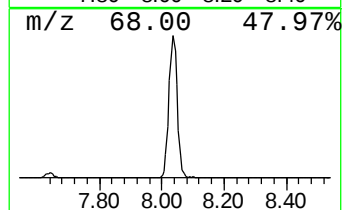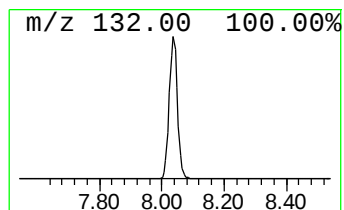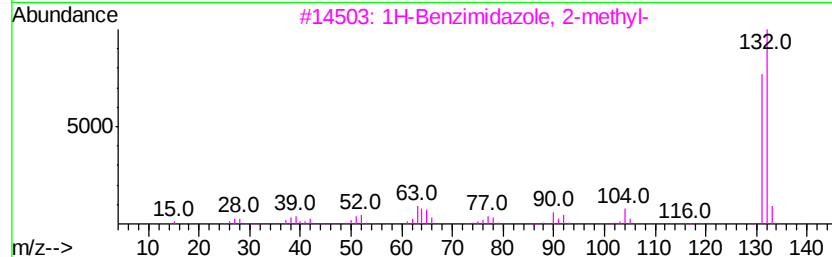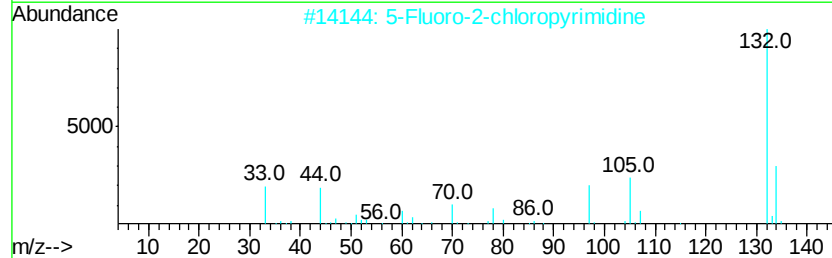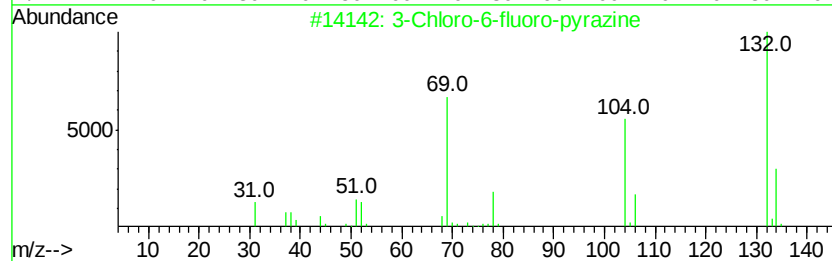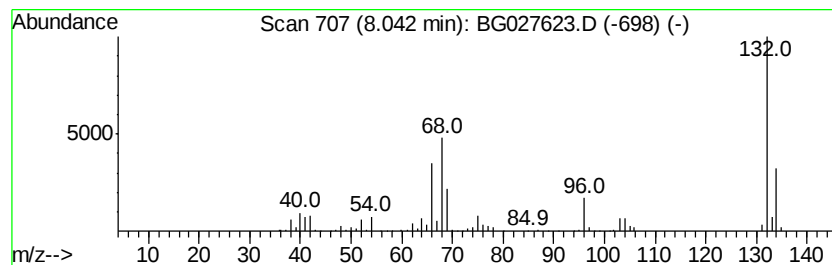

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG062217\
Data File : BG027623.D
Acq On : 23 Jun 2017 9:15
Operator : SJ/JU
Sample : I3657-20
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-102S

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.04	8.04	90.0	ng	458490	1	8.51	101837	20.0