

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG062217\
 Data File : BG027624.D
 Acq On : 23 Jun 2017 9:55
 Operator : SJ/JU
 Sample : I3657-22
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-102D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.088	367	374	383	rBV	154383	264770	9.81%	3.014%
2	7.639	630	638	648	rBB	96012	174380	6.46%	1.985%
3	8.032	697	705	716	rBV	296110	536427	19.87%	6.106%
4	8.502	778	785	794	rBB	61247	109884	4.07%	1.251%
5	8.831	833	841	850	rBB	248048	458522	16.99%	5.219%
6	9.666	975	983	992	rBV	222588	422335	15.65%	4.807%
7	11.323	1258	1265	1273	rVB	86515	164853	6.11%	1.877%
8	13.714	1664	1672	1683	rBV	671796	1092505	40.47%	12.436%
9	15.089	1898	1906	1914	rBB2	145728	254500	9.43%	2.897%
10	16.569	2151	2158	2170	rBV	756723	1200477	44.47%	13.665%
11	17.833	2365	2373	2381	rBV2	263789	409950	15.19%	4.667%
12	20.412	2806	2812	2819	rBV	2008194	2699332	100.00%	30.727%
13	22.204	3109	3117	3131	rVB	267053	513212	19.01%	5.842%
14	25.835	3721	3735	3749	rBV2	145128	483791	17.92%	5.507%


Sum of corrected areas: 8784938

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG062217\
Data File : BG027624.D
Acq On : 23 Jun 2017 9:55
Operator : SJ/JU
Sample : I3657-22
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-102D

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

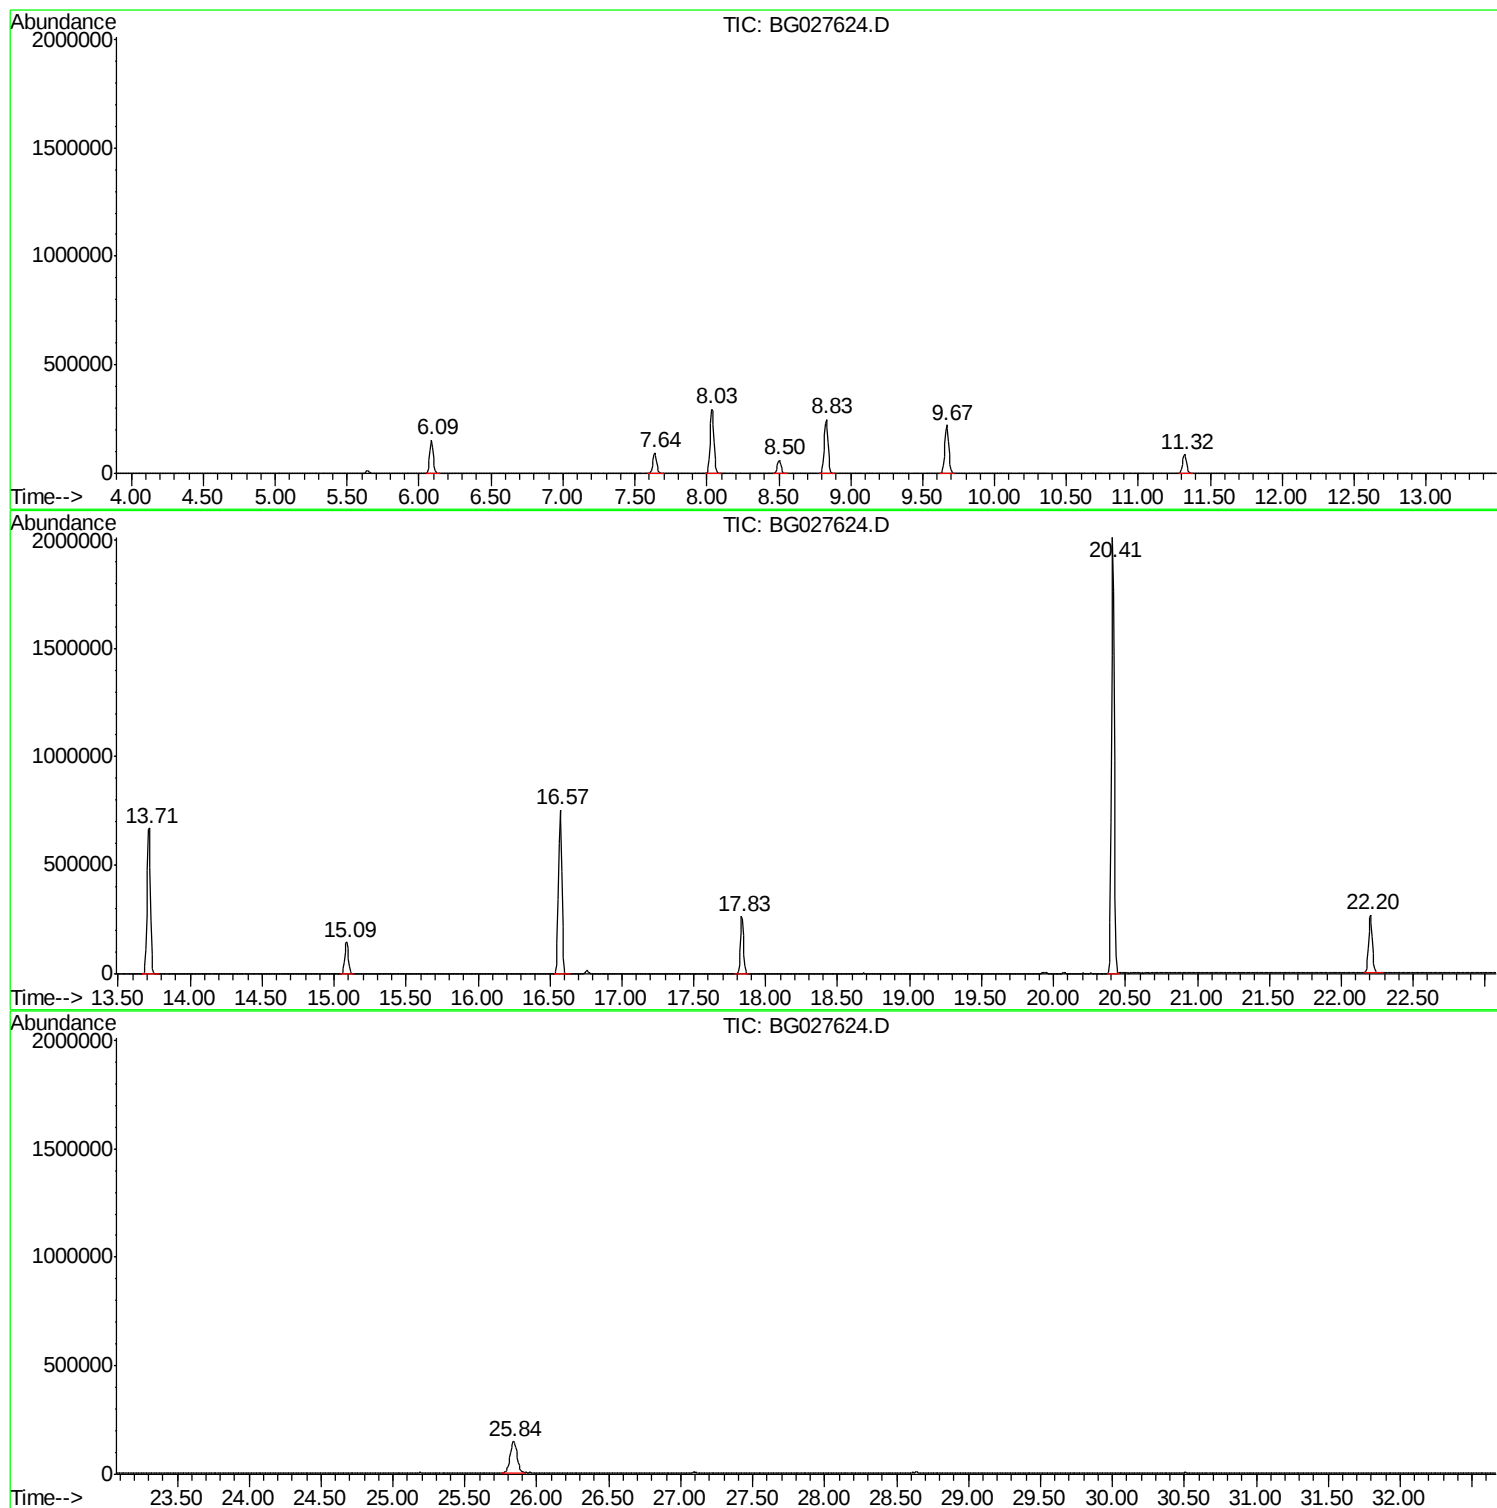

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG062217\
Data File : BG027624.D
Acq On : 23 Jun 2017 9:55
Operator : SJ/JU
Sample : I3657-22
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-102D










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown8.03 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.03	97.64 ng	536427	1,4-Dichlorobenzene-d4	8.50

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	35
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
5		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	14

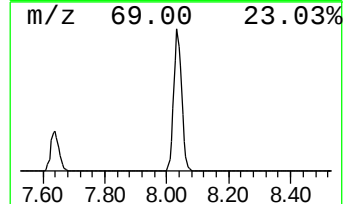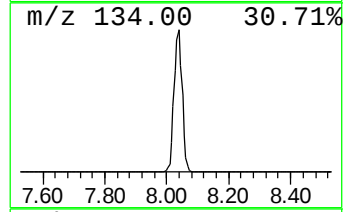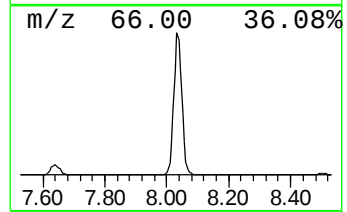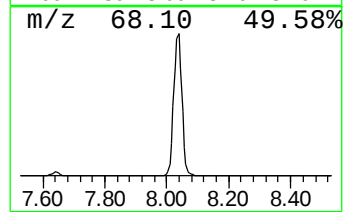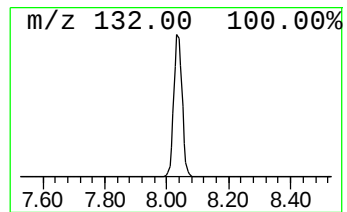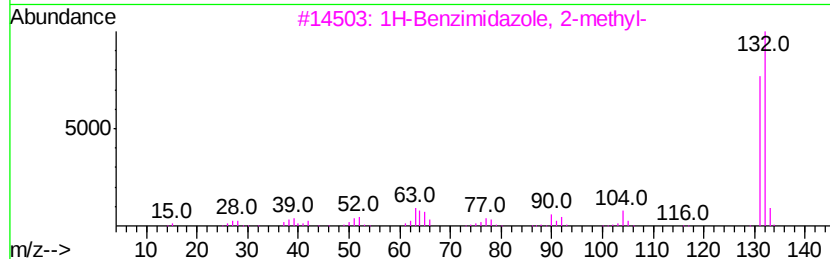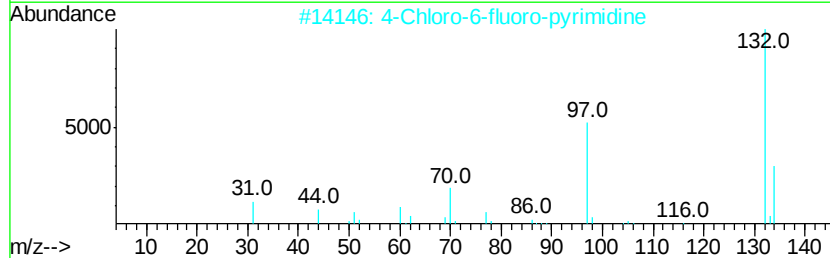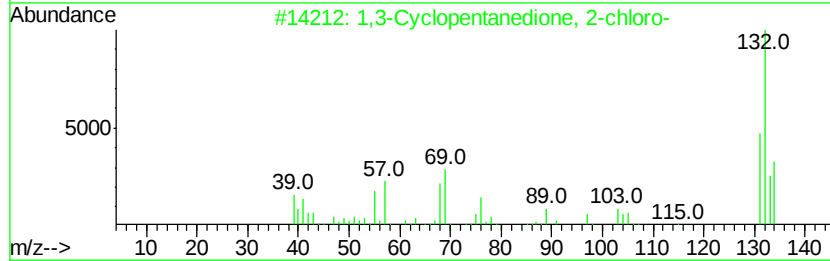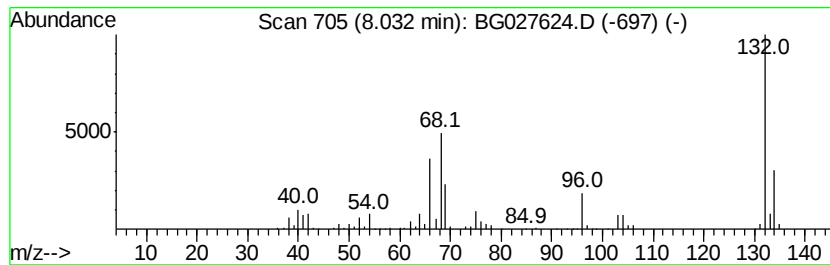

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG062217\
Data File : BG027624.D
Acq On : 23 Jun 2017 9:55
Operator : SJ/JU
Sample : I3657-22
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-102D

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.03	8.03	97.6	ng	536427	1	8.50	109884	20.0