

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG062217\
 Data File : BG027631.D
 Acq On : 23 Jun 2017 14:32
 Operator : SJ/JU
 Sample : I3657-13
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-103I

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.641	291	298	308	rBV	16001	27695	1.22%	0.328%
2	6.088	366	374	387	rVB	175911	299343	13.21%	3.541%
3	7.639	630	638	650	rBV	108350	202813	8.95%	2.399%
4	8.038	697	706	714	rBV	317673	571041	25.21%	6.755%
5	8.502	779	785	792	rBB	66950	118964	5.25%	1.407%
6	8.831	834	841	849	rBB	243311	445065	19.64%	5.265%
7	9.672	976	984	992	rBV	222492	425651	18.79%	5.035%
8	11.323	1255	1265	1274	rBB	97438	178495	7.88%	2.111%
9	13.714	1663	1672	1680	rBV	660505	1049527	46.33%	12.415%
10	14.519	1802	1809	1816	rBV	84788	122588	5.41%	1.450%
11	15.089	1899	1906	1913	rBV2	156126	264919	11.69%	3.134%
12	16.569	2151	2158	2171	rBV	702716	1136084	50.15%	13.439%
13	17.838	2366	2374	2381	rBV	243881	393457	17.37%	4.654%
14	18.673	2511	2516	2522	rBV3	25551	36988	1.63%	0.438%
15	19.930	2723	2730	2736	rBV3	17169	28840	1.27%	0.341%
16	20.412	2806	2812	2819	rBV	1693915	2265555	100.00%	26.799%
17	22.204	3109	3117	3126	rBV	249003	459639	20.29%	5.437%
18	25.835	3723	3735	3752	rVB2	131574	427131	18.85%	5.053%


Sum of corrected areas: 8453795

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG062217\
Data File : BG027631.D
Acq On : 23 Jun 2017 14:32
Operator : SJ/JU
Sample : I3657-13
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-103I

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

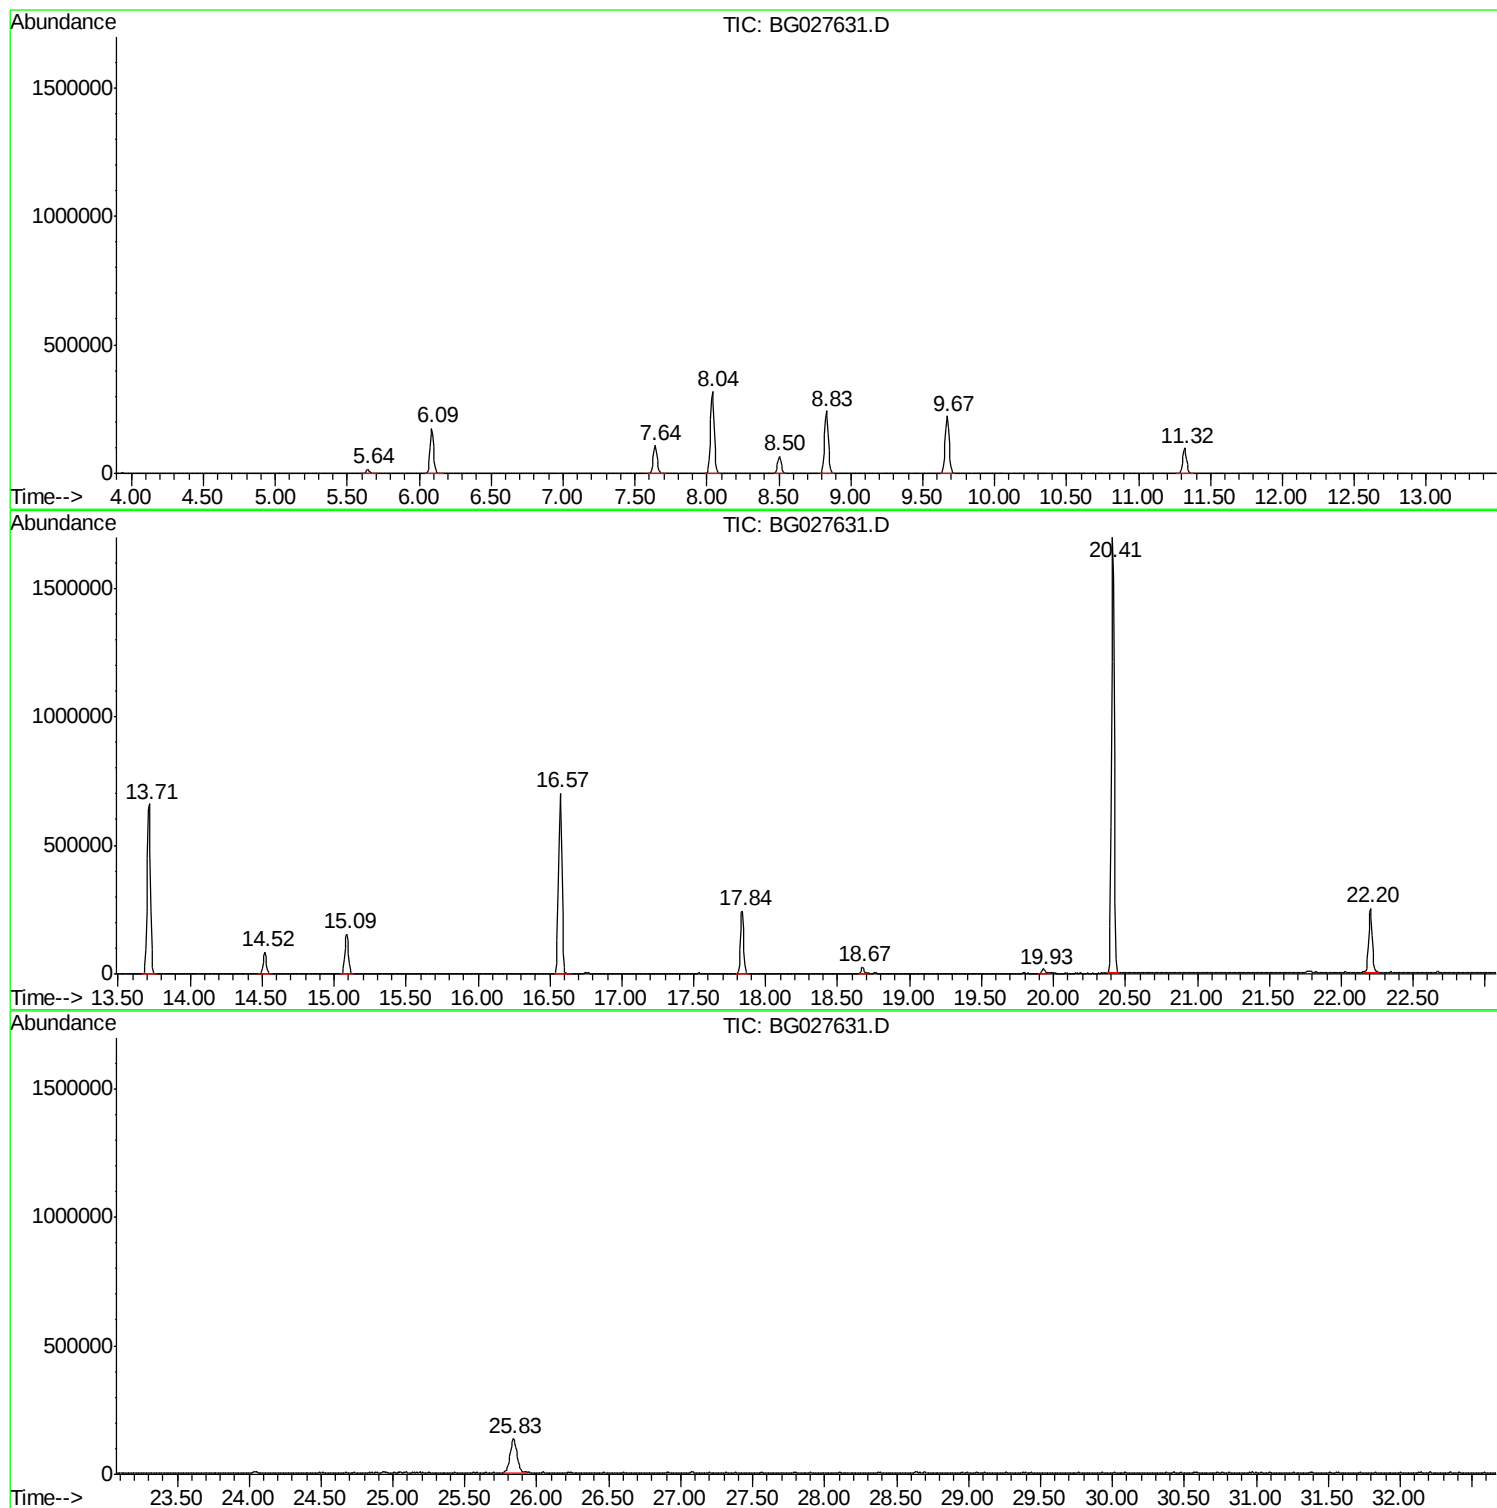

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG062217\
Data File : BG027631.D
Acq On : 23 Jun 2017 14:32
Operator : SJ/JU
Sample : I3657-13
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-103I










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.64 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.64	4.66 ng	27695	1,4-Dichlorobenzene-d4	8.51

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Oxirane, [(1-methylethoxy)methyl]-	116	C6H12O2	004016-14-2	43
2			Silane, trimethyl-	74	C3H10Si	000993-07-7	28
3			Guanidine	59	CH5N3	000113-00-8	9
4			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	9
5			2-Butanol, 1-chloro-	108	C4H9ClO	001873-25-2	9

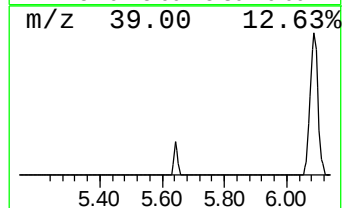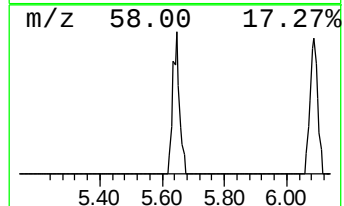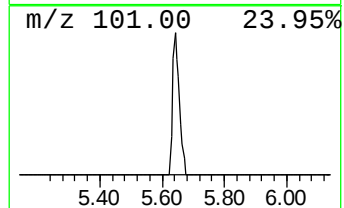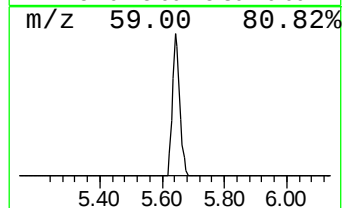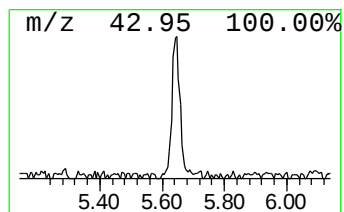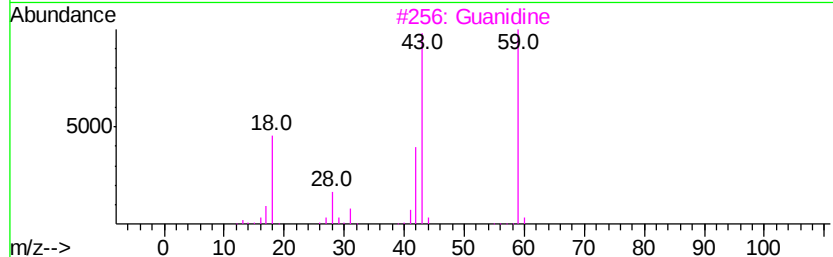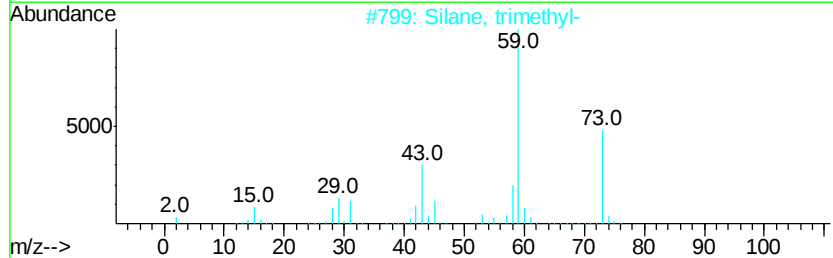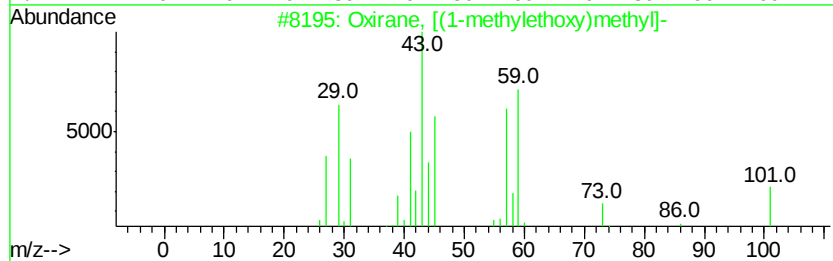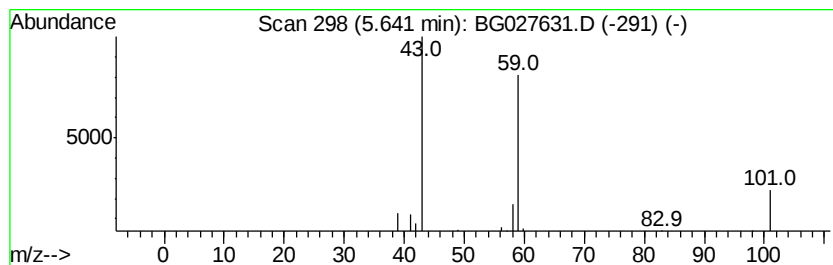

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG062217\
Data File : BG027631.D
Acq On : 23 Jun 2017 14:32
Operator : SJ/JU
Sample : I3657-13
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-103I










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown8.04 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.04	96.00 ng	571041	1,4-Dichlorobenzene-d4	8.51

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	35
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
4		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	25
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22

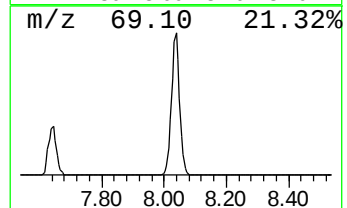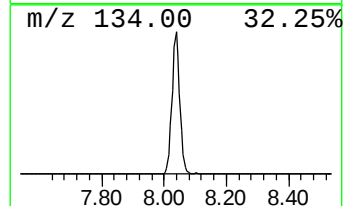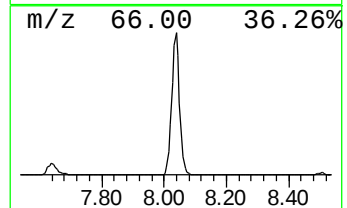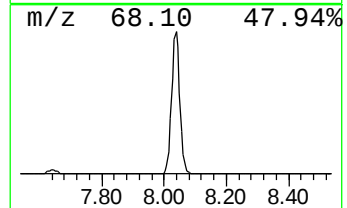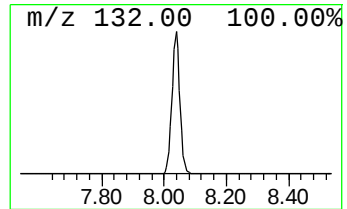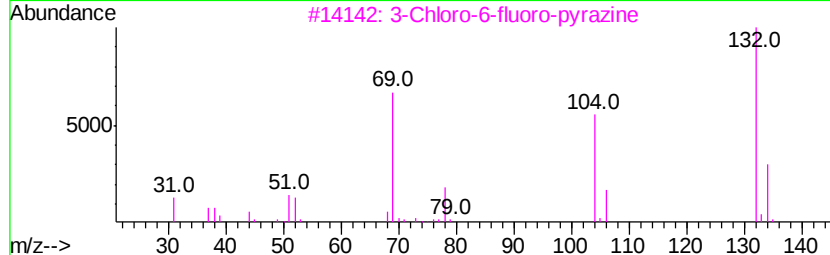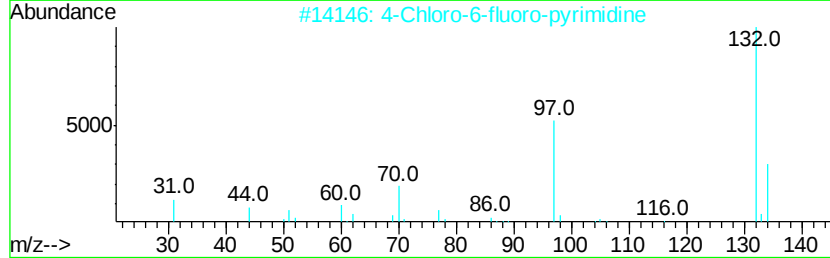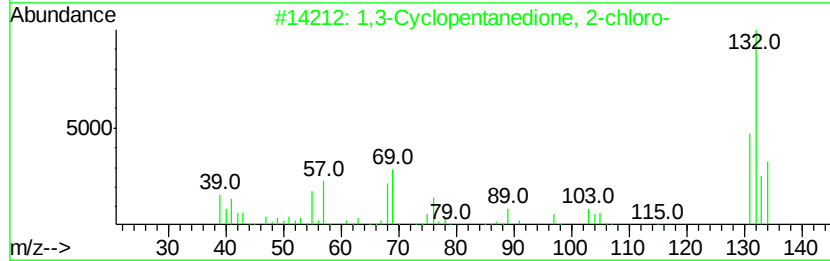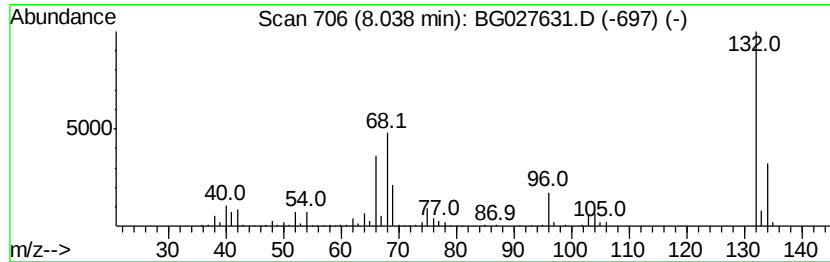

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG062217\
Data File : BG027631.D
Acq On : 23 Jun 2017 14:32
Operator : SJ/JU
Sample : I3657-13
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-103I

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.64	5.64	4.7	ng	27695	1	8.51	118964	20.0
unknown8.04	8.04	96.0	ng	571041	1	8.51	118964	20.0