


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG062217\
 Data File : BG027614.D
 Acq On : 23 Jun 2017 2:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 21 18:52:15 2017

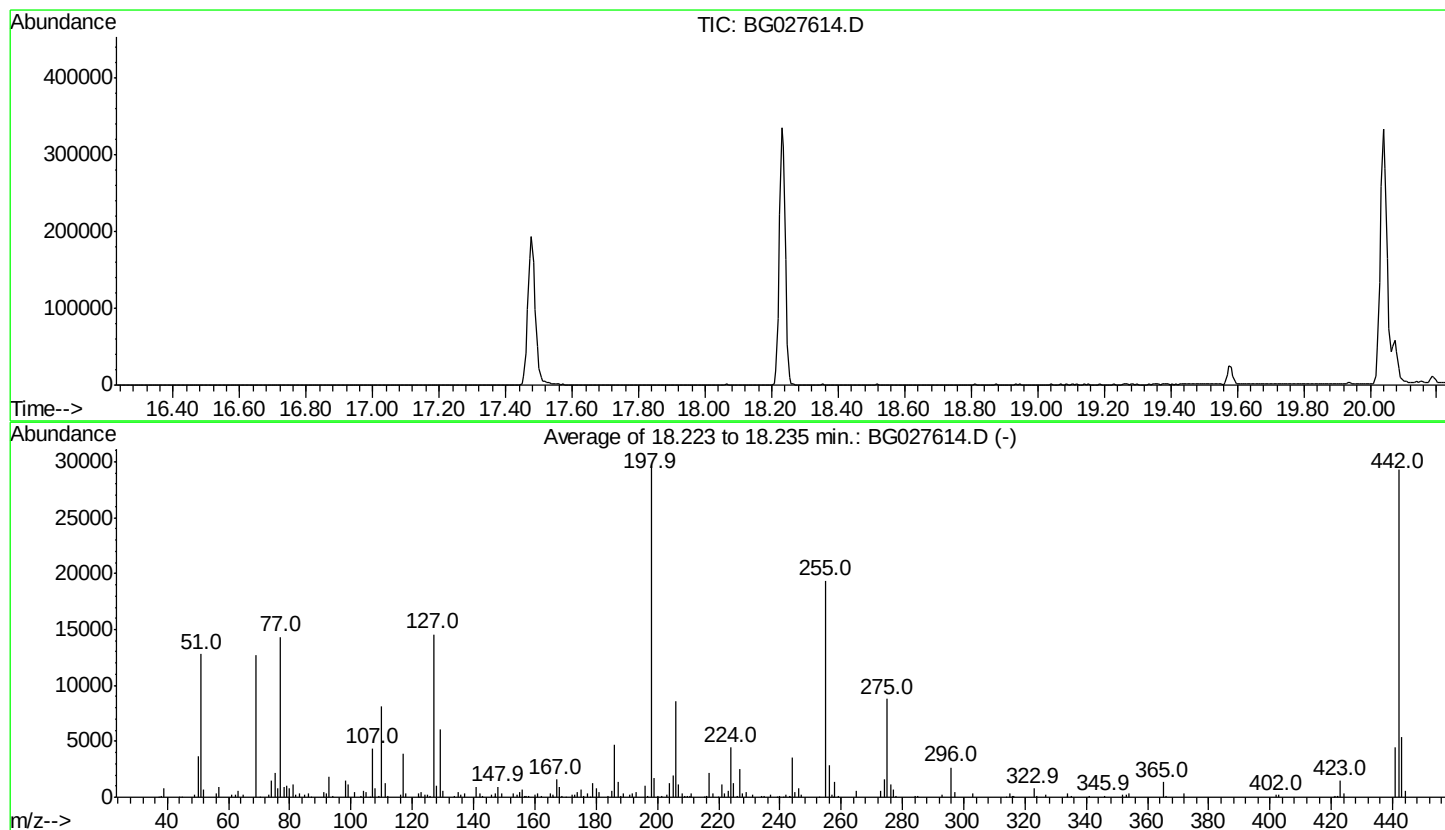

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	12789	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.0	12750	PASS
70	69	0.00	2	0.4	53	PASS
127	198	10	80	49.1	14554	PASS
197	198	0.00	2	0.4	118	PASS
198	198	100	100	100.0	29661	PASS
199	198	5	9	5.9	1763	PASS
275	198	10	60	29.6	8784	PASS
365	198	1	100	4.5	1337	PASS
441	442	0.01	24	15.1	4436	PASS
442	198	50	100	99.0	29368	PASS
443	442	15	24	18.4	5407	PASS