
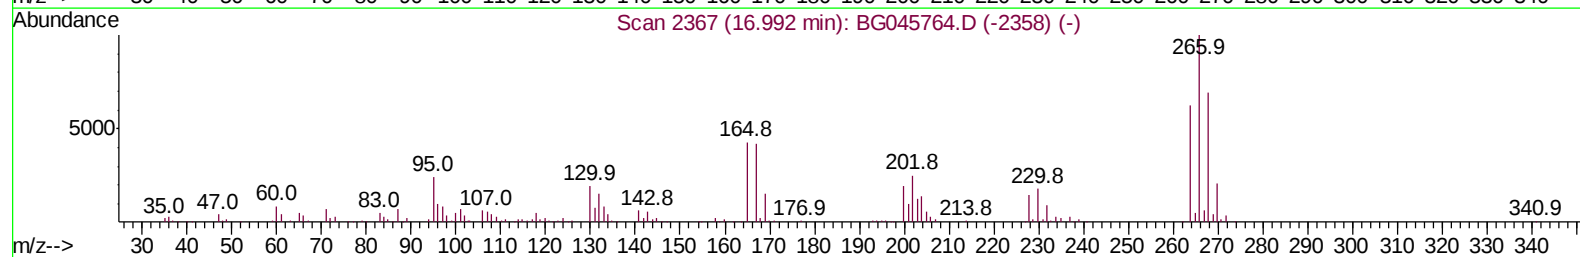
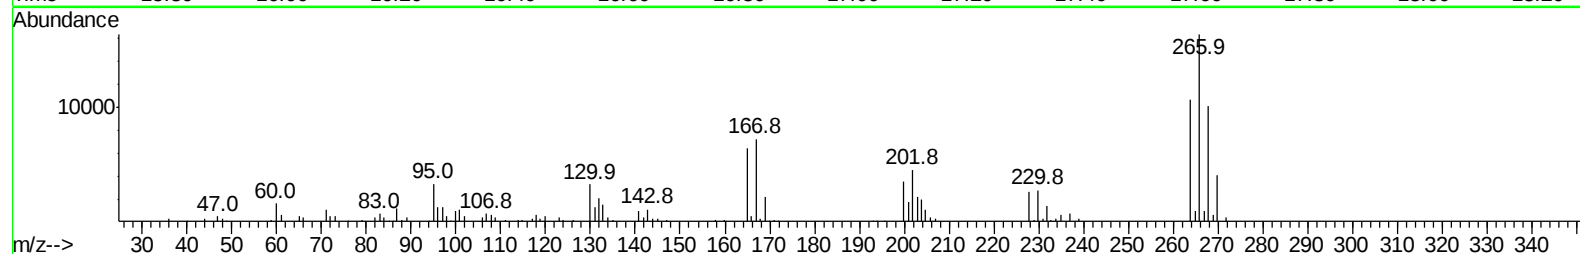


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062220\
Data File : BG045820.D
Acq On : 22 Jun 2020 9:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 08:09:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 18:34:19 2020
Response via : Initial Calibration

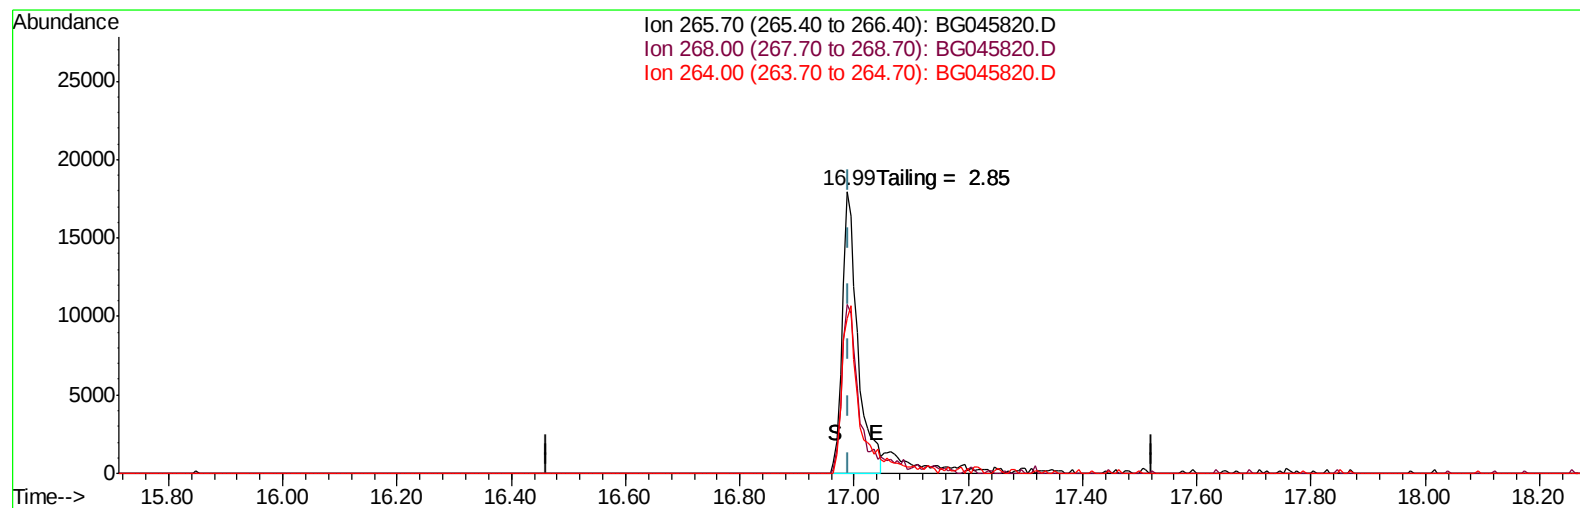

TIC: BG045820.D

(70) Pentachlorophenol (C)




16.988min (-0.004) 15098.91ng

response 34144

Ion	Exp%	Act%
265.70	100	100
268.00	69.20	60.08
264.00	62.20	55.22
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062220\
 Data File : BG045820.D
 Acq On : 22 Jun 2020 9:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 08:09:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 18:34:19 2020
 Response via : Initial Calibration

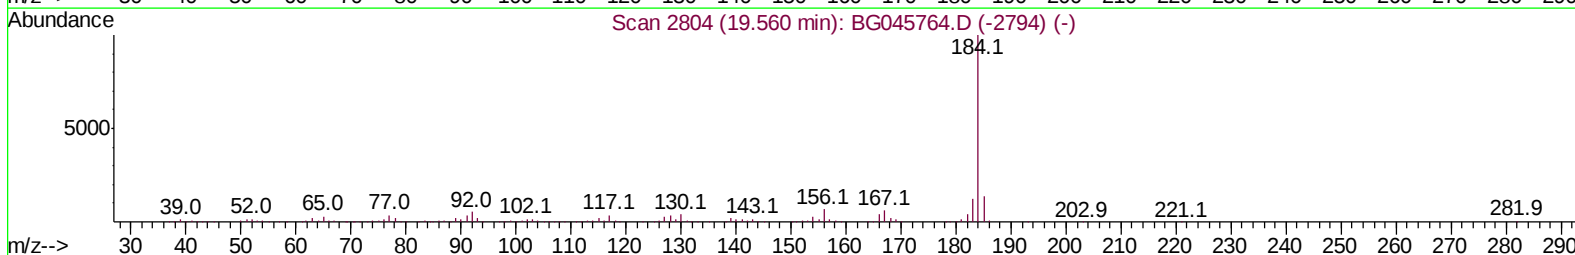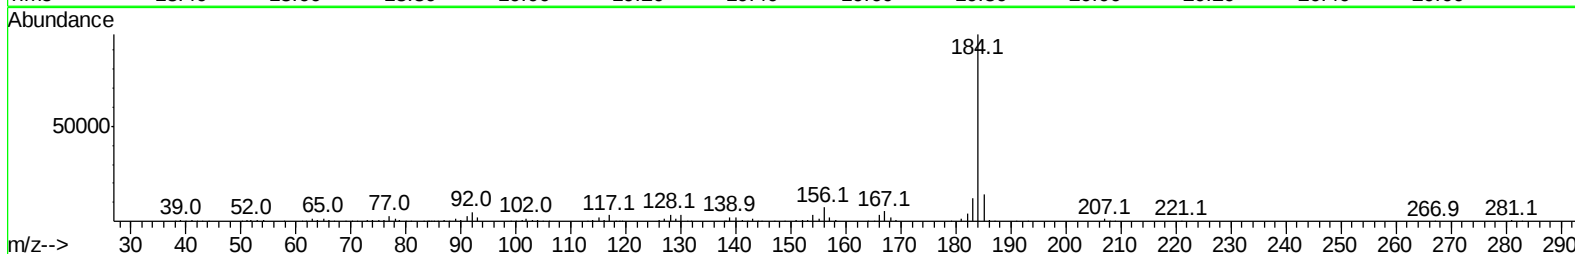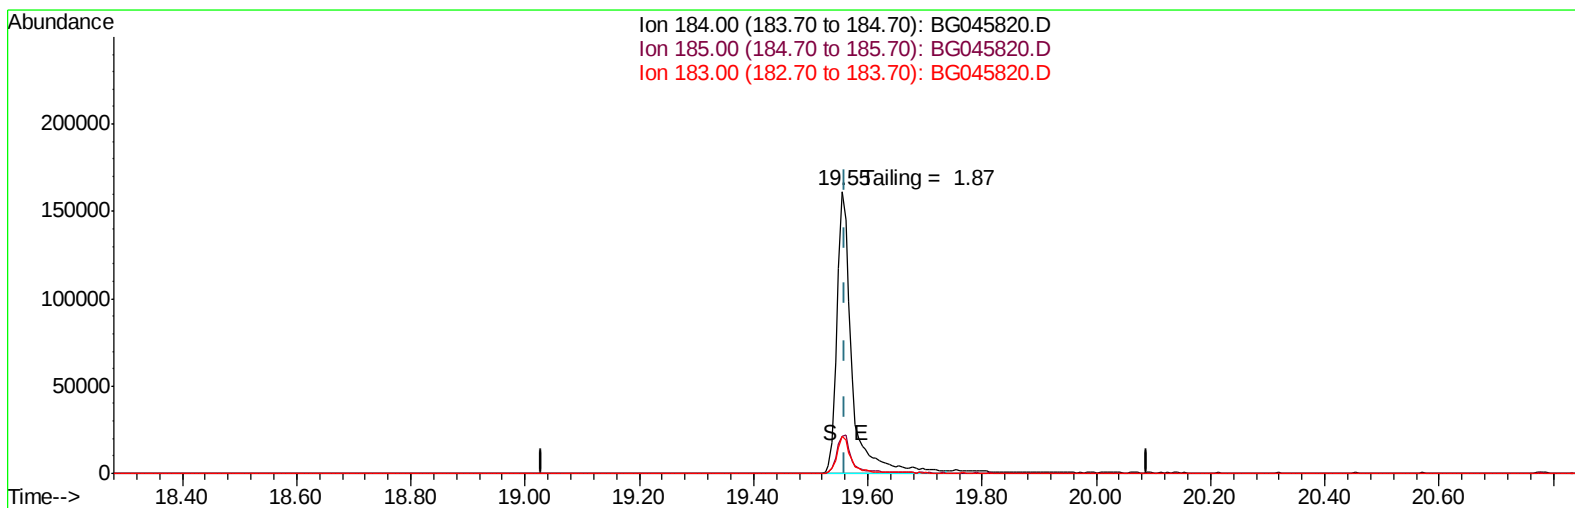

TIC: BG045820.D

(77) Benzidine

19.555min (-0.005) 180984.17ng

response 296418

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.41
183.00	12.10	13.13
0.00	0.00	0.00