
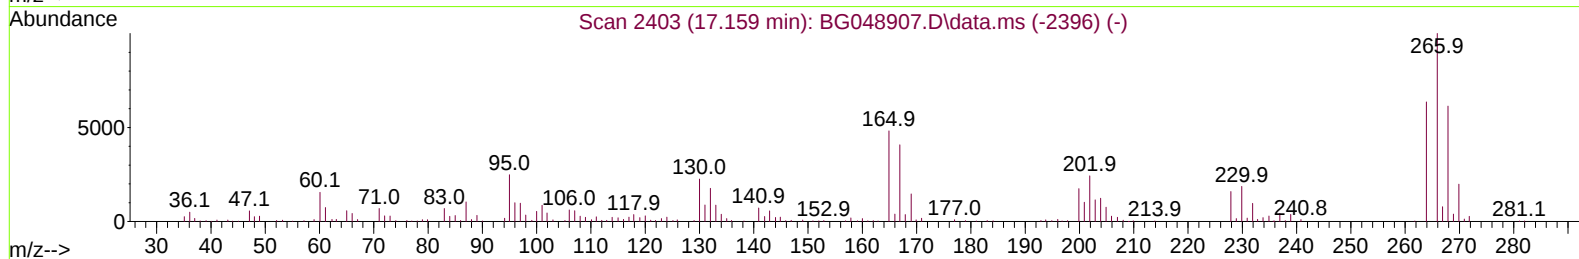
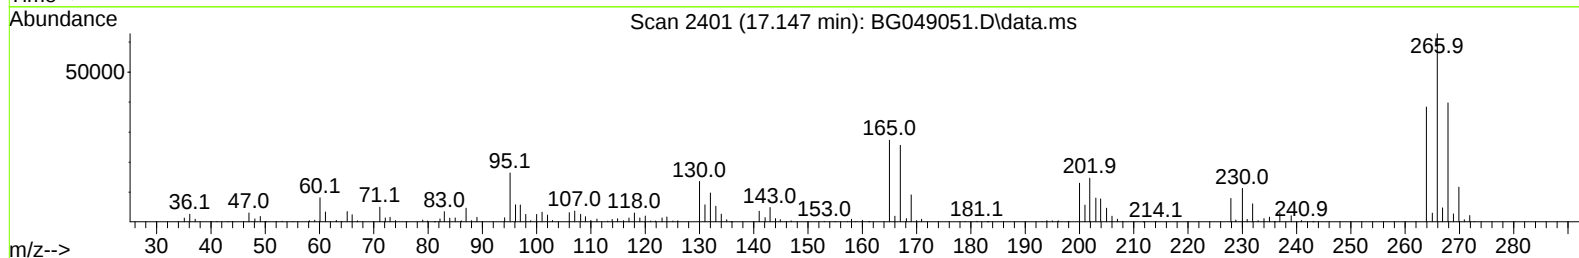


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062221\
Data File : BG049051.D
Acq On : 22 Jun 2021 21:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 07:57:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

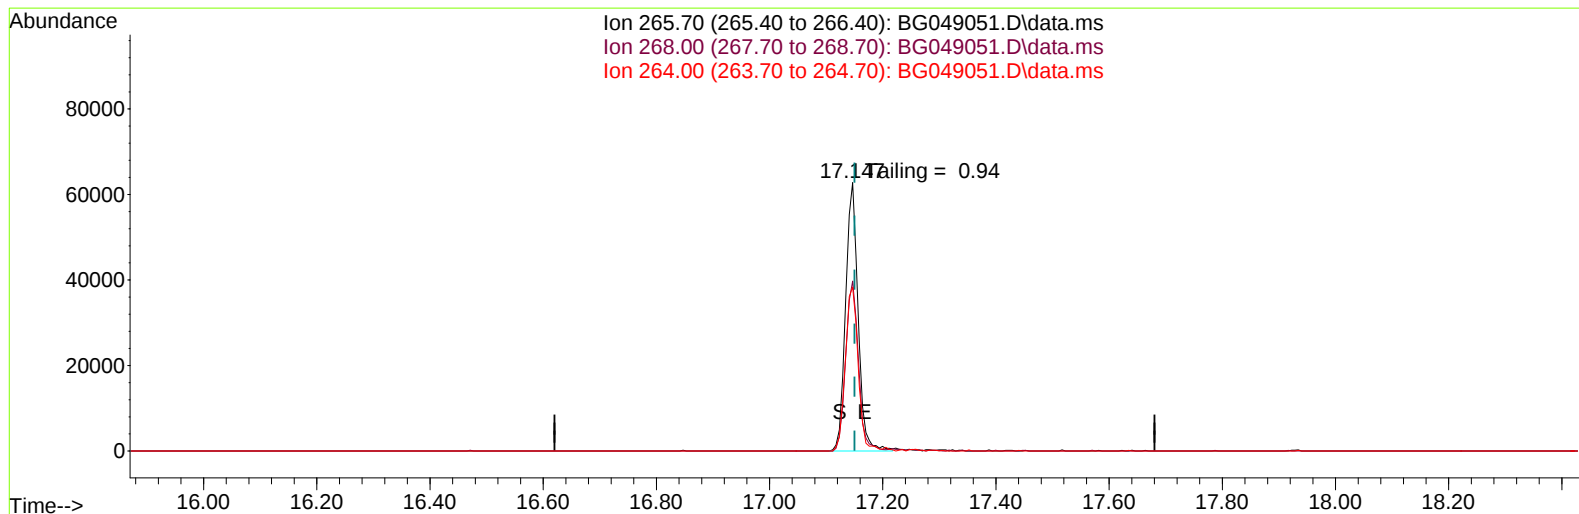

TIC: BG049051.D\data.ms

(70) Pentachlorophenol (C)




17.147min (-0.003) 109459.26 ng

response 97037

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.30
264.00	61.30	61.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062221\
Data File : BG049051.D
Acq On : 22 Jun 2021 21:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 07:57:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

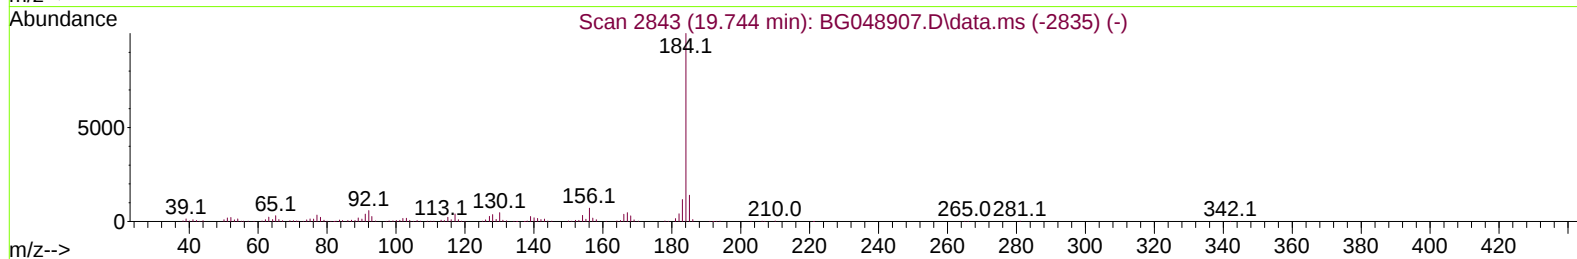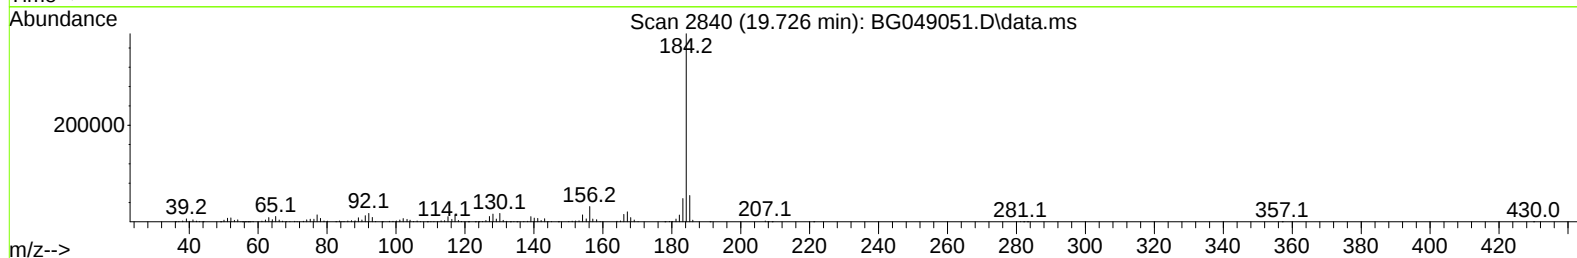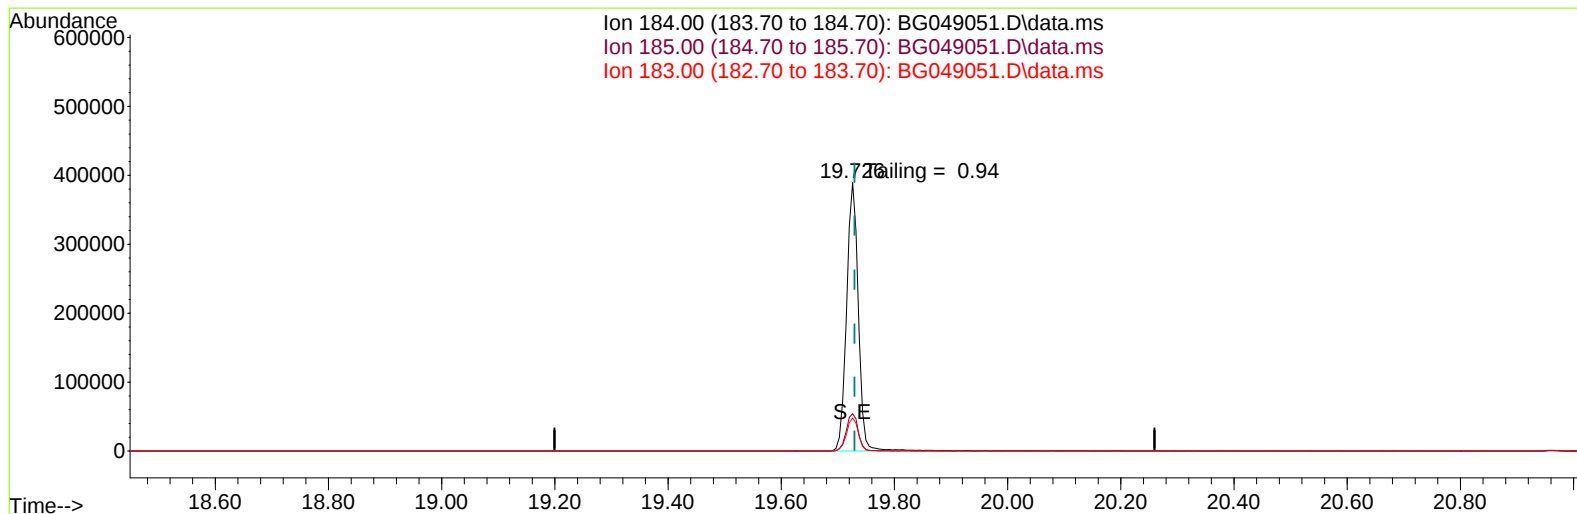

TIC: BG049051.D\data.ms

(77) Benzidine**19.726min (-0.003) 0.00 ng****response 555973**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.95
183.00	11.70	12.34
0.00	0.00	0.00