
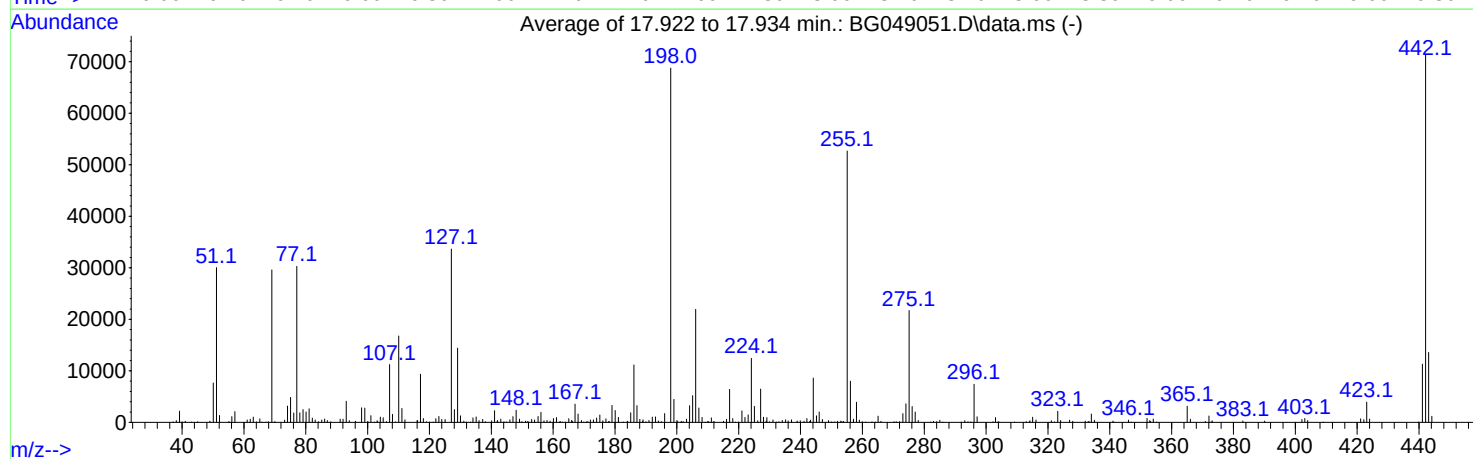


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062221\
 Data File : BG049051.D
 Acq On : 22 Jun 2021 21:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 16 12:04:50 2021

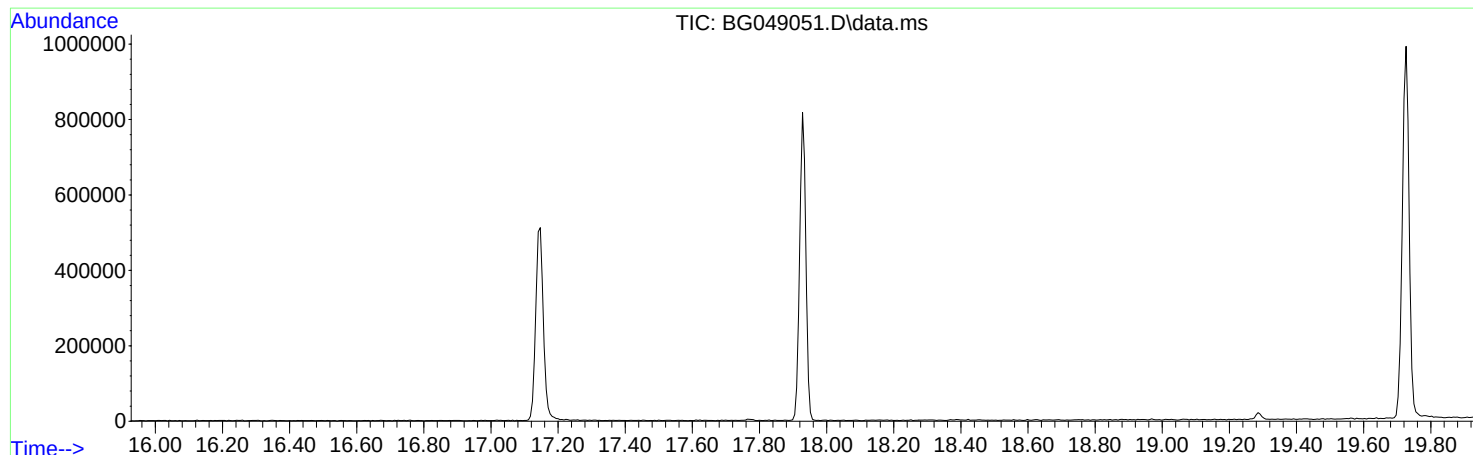




AutoFind: Scans 2533, 2534, 2535; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	30024	PASS
68	69	0.00	2	0.4	128	PASS
69	198	0.00	100	43.0	29589	PASS
70	69	0.00	2	0.3	88	PASS
127	198	10	80	48.9	33637	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68763	PASS
199	198	5	9	6.5	4484	PASS
275	198	10	60	31.6	21707	PASS
365	198	1	100	4.6	3155	PASS
441	198	0.01	100	16.5	11316	PASS
442	442	100	100	100.0	71397	PASS
443	442	15	24	19.0	13559	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062221\
Data File : BG049051.D
Acq On : 22 Jun 2021 21:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 23 07:57:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

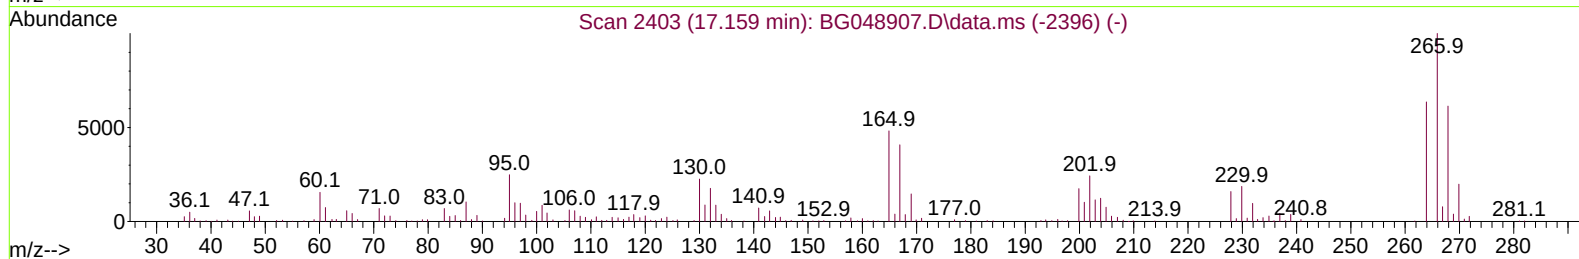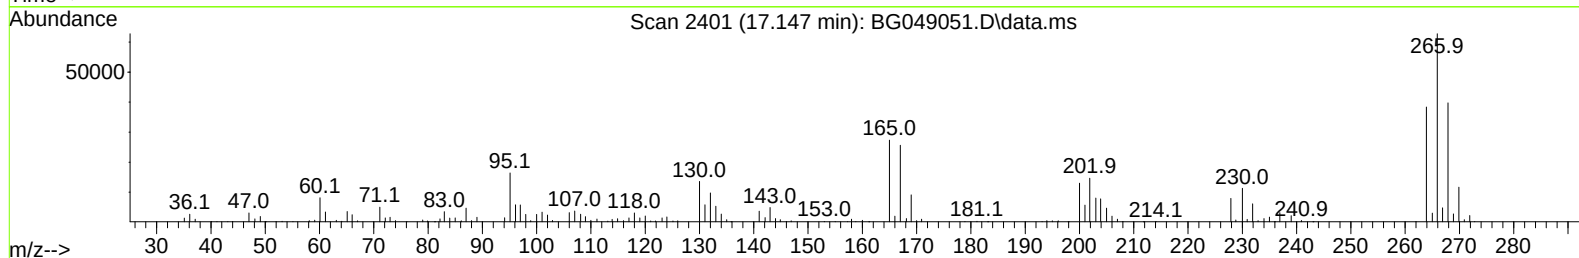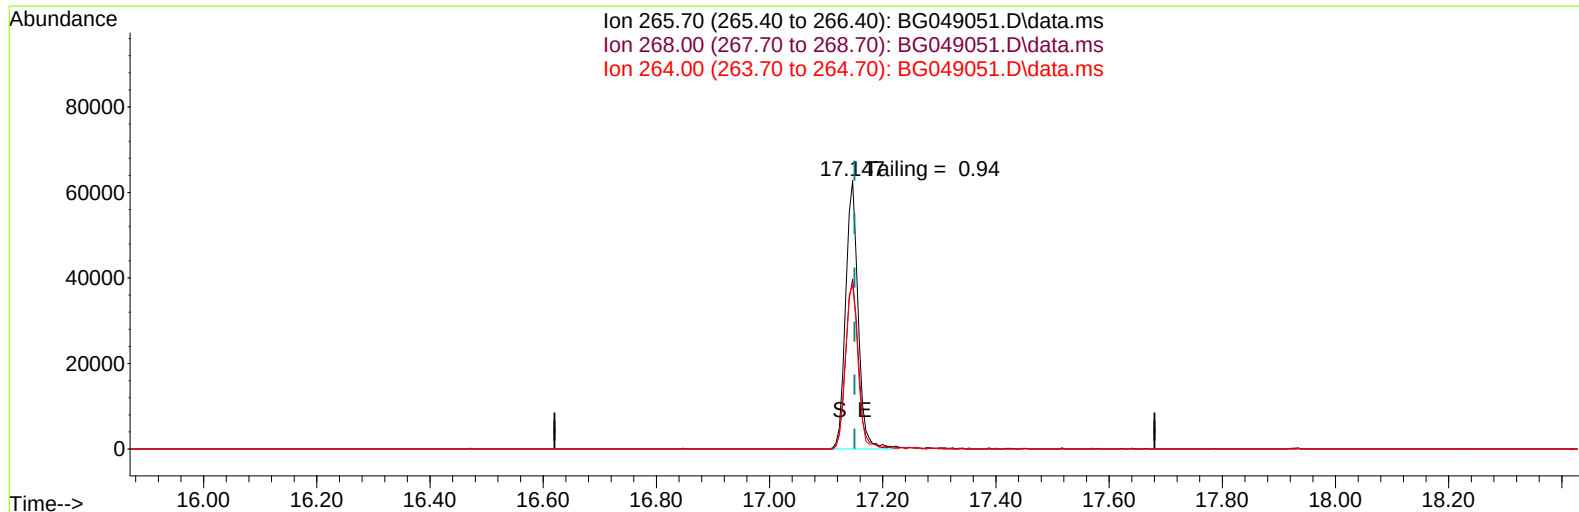

TIC: BG049051.D\data.ms

(70) Pentachlorophenol (C)

17.147min (-0.003) 109459.26 ng




response 97037

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.30
264.00	61.30	61.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062221\
Data File : BG049051.D
Acq On : 22 Jun 2021 21:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 23 07:57:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

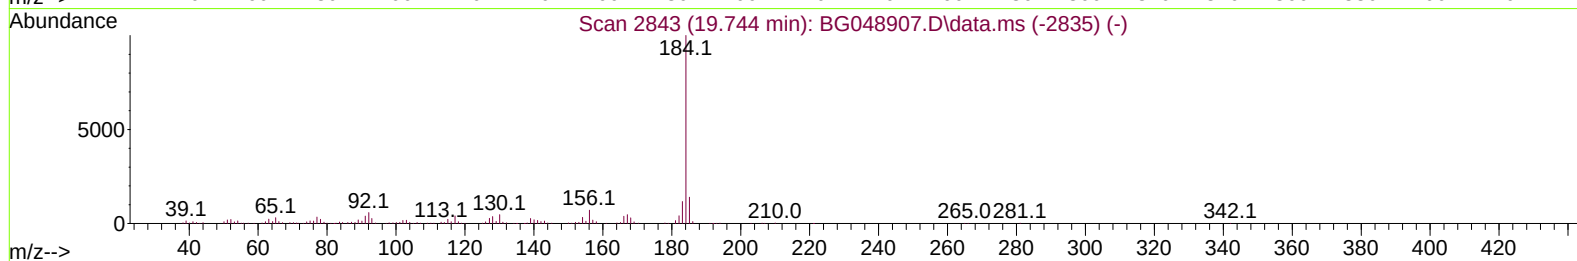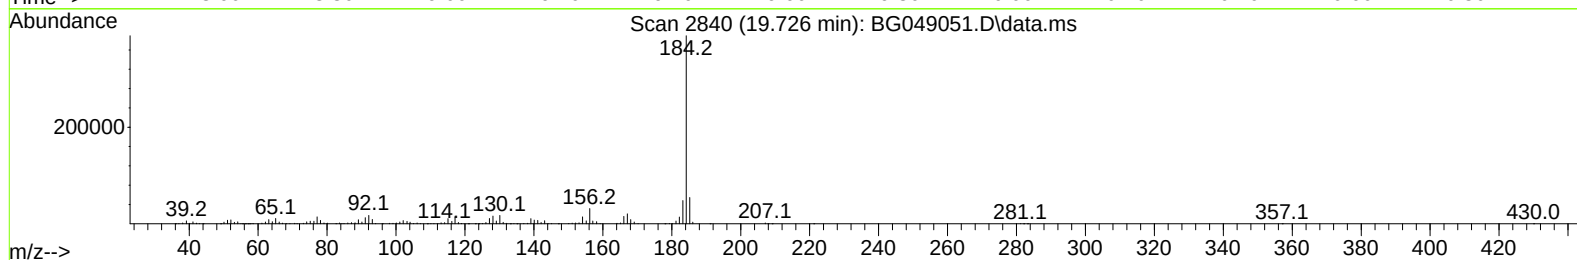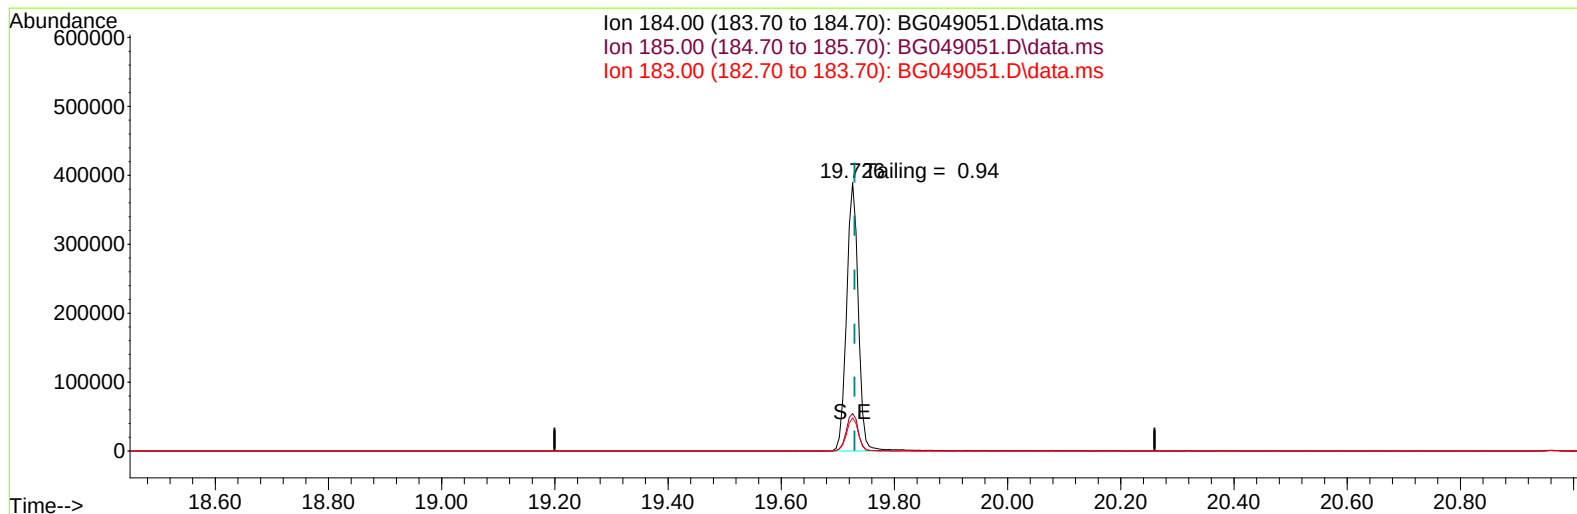

TIC: BG049051.D\data.ms

(77) Benzidine

19.726min (-0.003) 0.00 ng

response 555973

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.95
183.00	11.70	12.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/22/2021	BNA_G	BG049051.D
Compound Name	Response	Retention Time
DDT	259155	20.96
DDD	15699	20.519
DDE	362	20.014
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16061	275216	5.84