




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061646.D
Acq On : 22 Jun 2024 13:00
Operator : MA/JU
Sample : P2775-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4C96

Manual IntegrationsAPPROVED

Quant Time: Jun 22 13:48:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

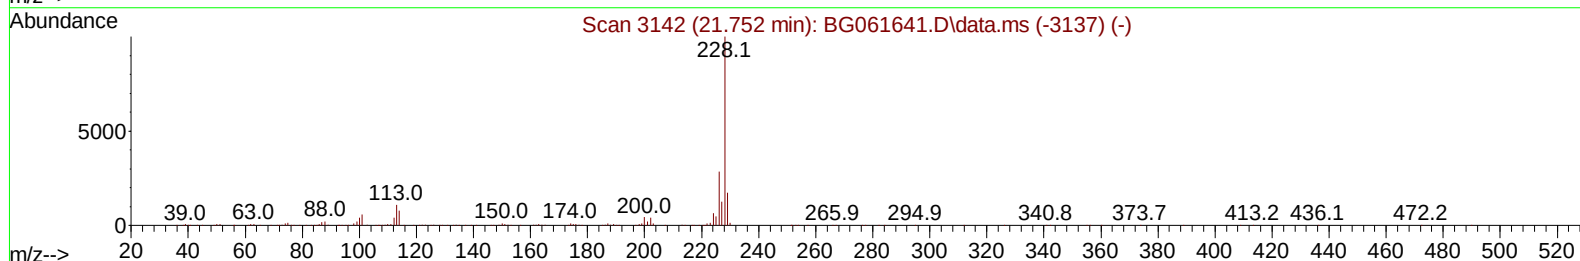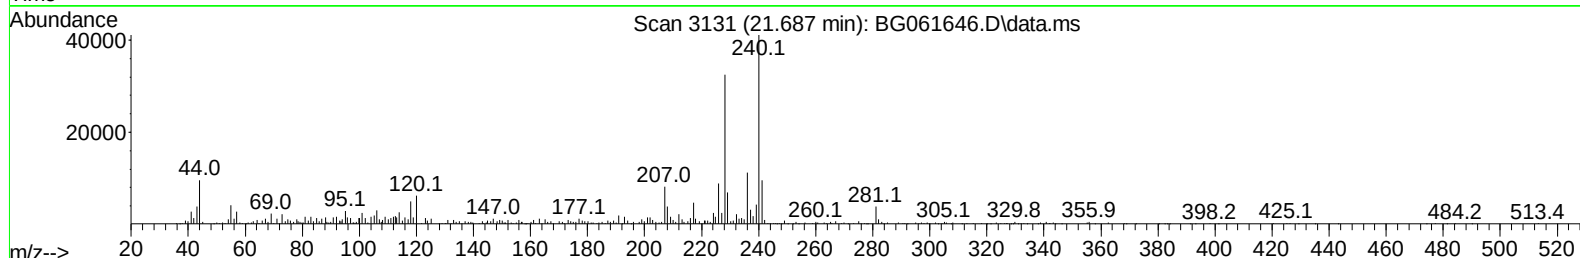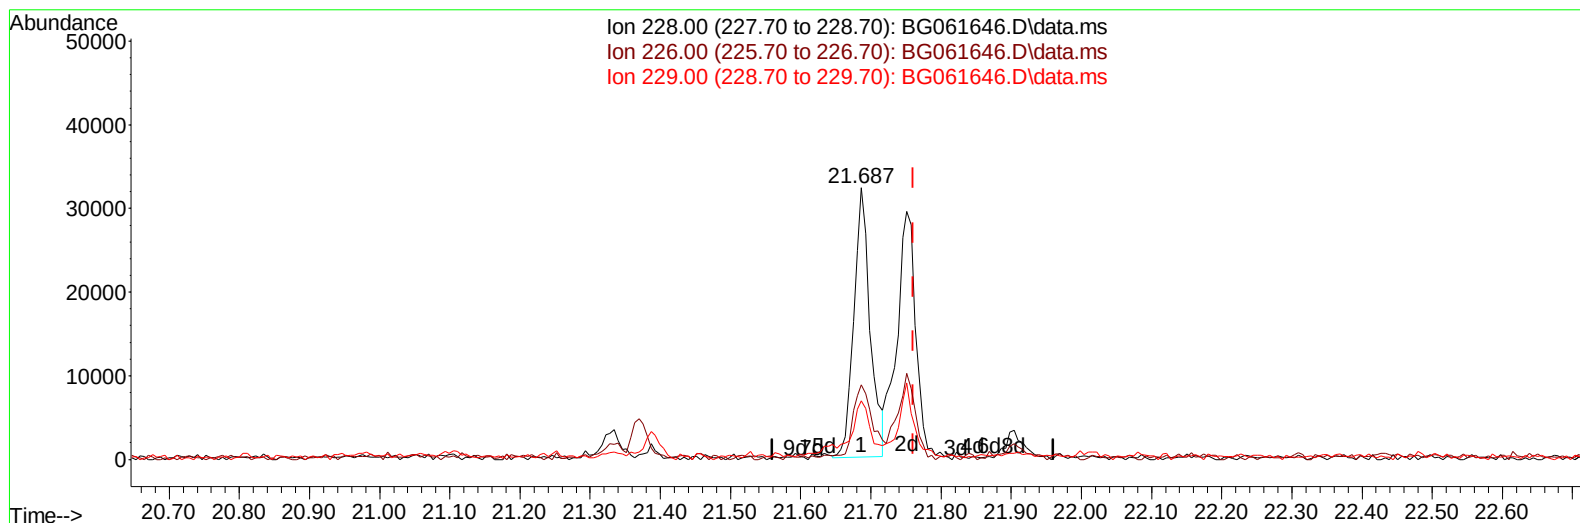

TIC: BG061646.D\data.ms

(87) Chrysene

21.687min (-0.074) 2.37 ng/u1

response 52363

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.20	27.54
229.00	20.60	21.58
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061646.D
Acq On : 22 Jun 2024 13:00
Operator : MA/JU
Sample : P2775-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4C96

Manual IntegrationsAPPROVED

Quant Time: Jun 22 13:48:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

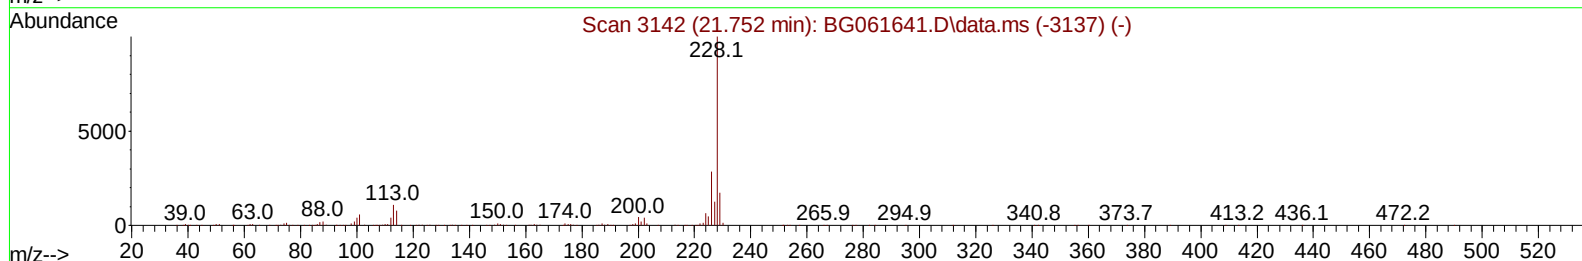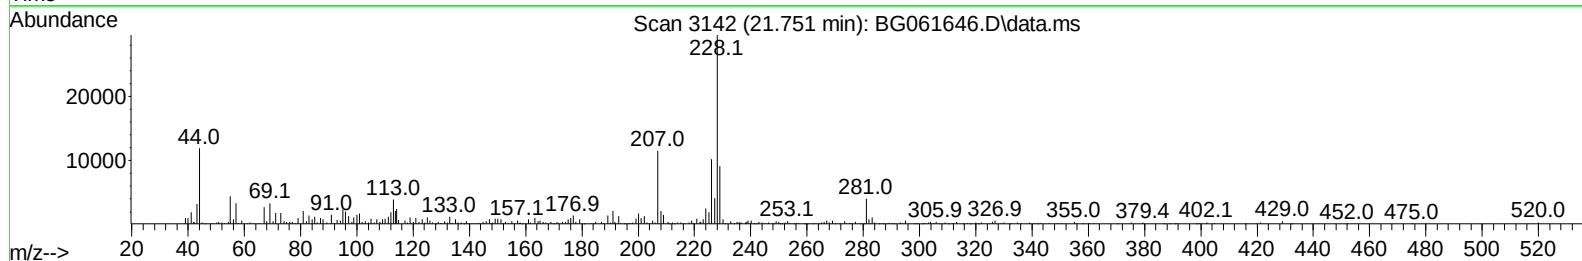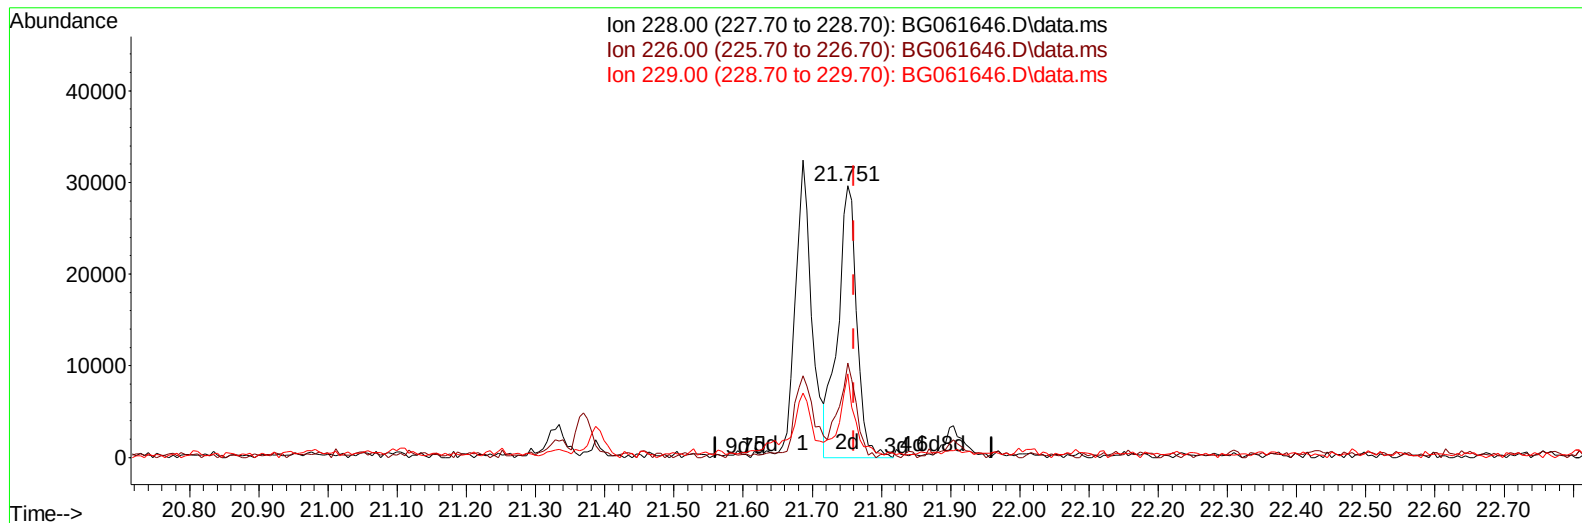

TIC: BG061646.D\data.ms

(87) Chrysene

21.751min (-0.009) 2.57 ng/ul m

response 56791

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.20	34.70
229.00	20.60	30.80#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061646.D
Acq On : 22 Jun 2024 13:00
Operator : MA/JU
Sample : P2775-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4C96

Manual IntegrationsAPPROVED

Quant Time: Jun 22 13:49:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

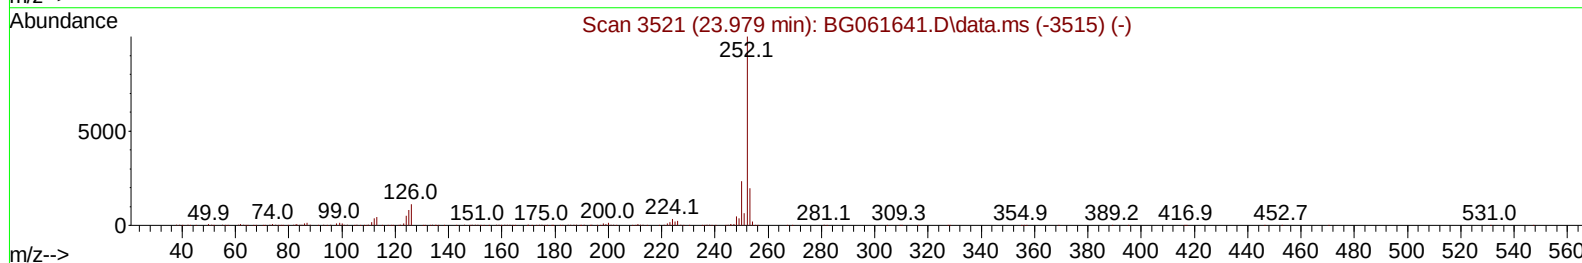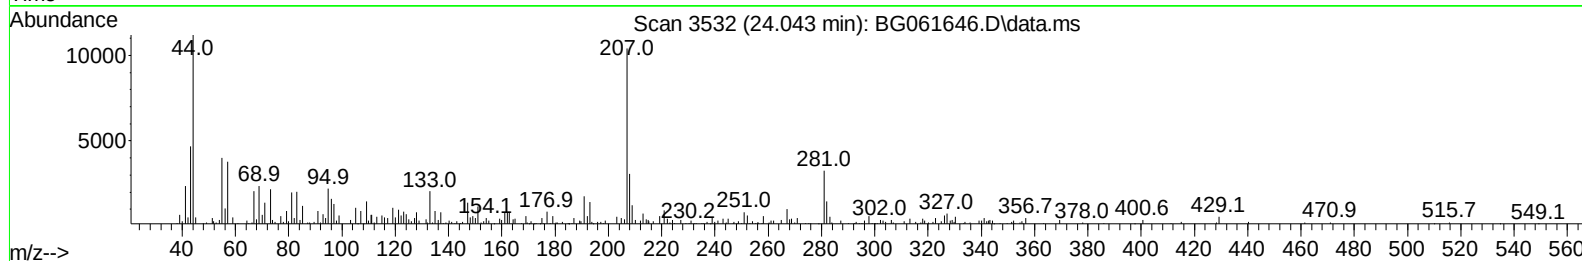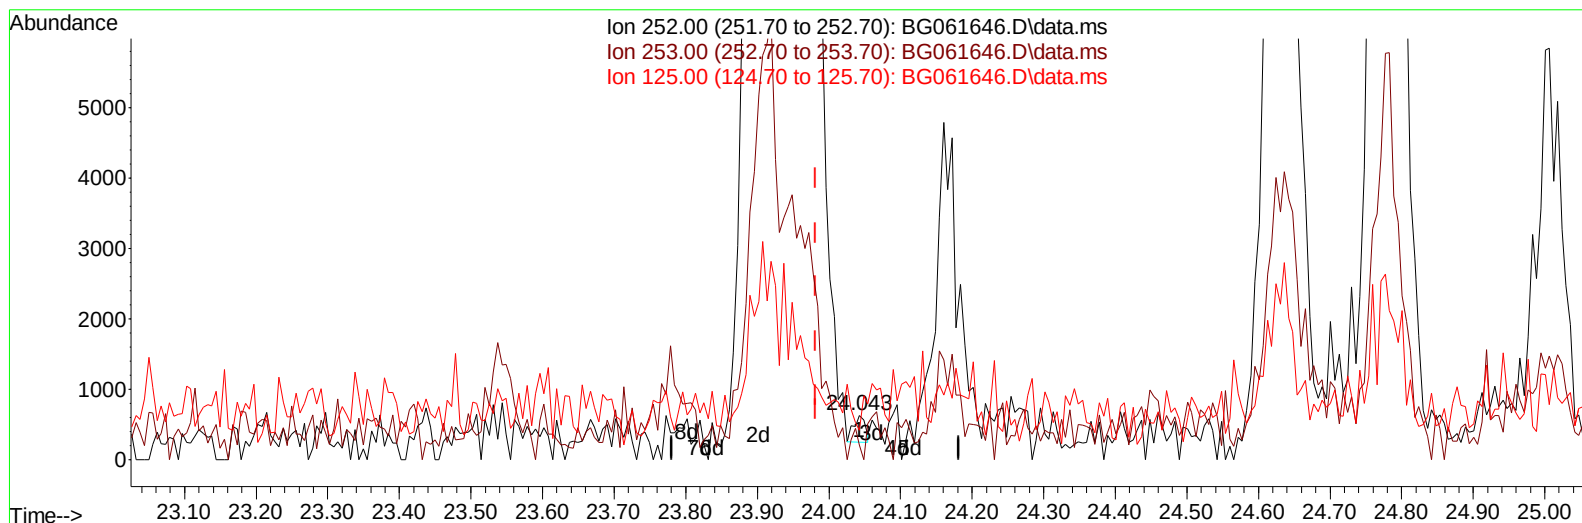

TIC: BG061646.D\data.ms

(91) Benzo(k)fluoranthene

24.043min (+ 0.062) 0.02 ng/u1

response 443

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.20	32.06#
125.00	7.70	65.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061646.D
Acq On : 22 Jun 2024 13:00
Operator : MA/JU
Sample : P2775-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4C96

Manual IntegrationsAPPROVED

Quant Time: Jun 22 13:49:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

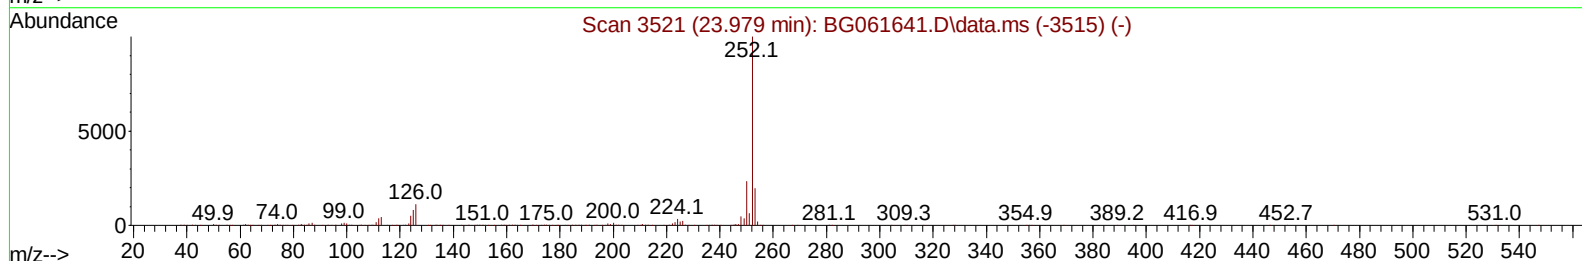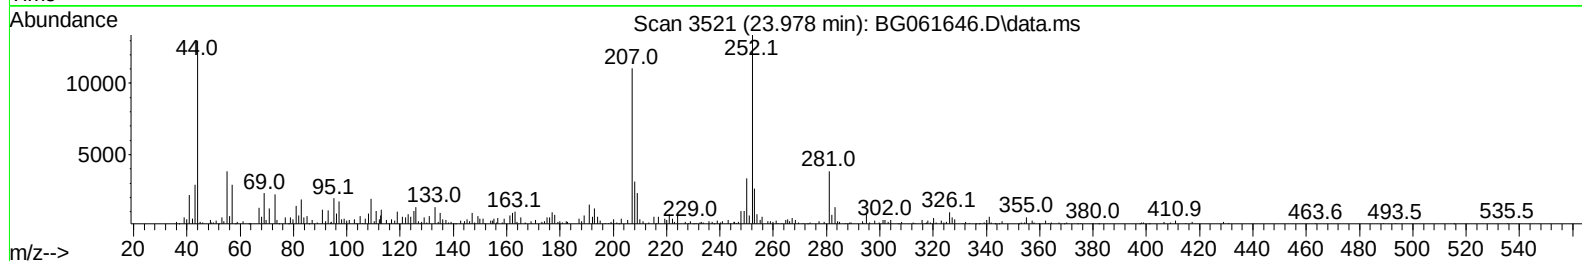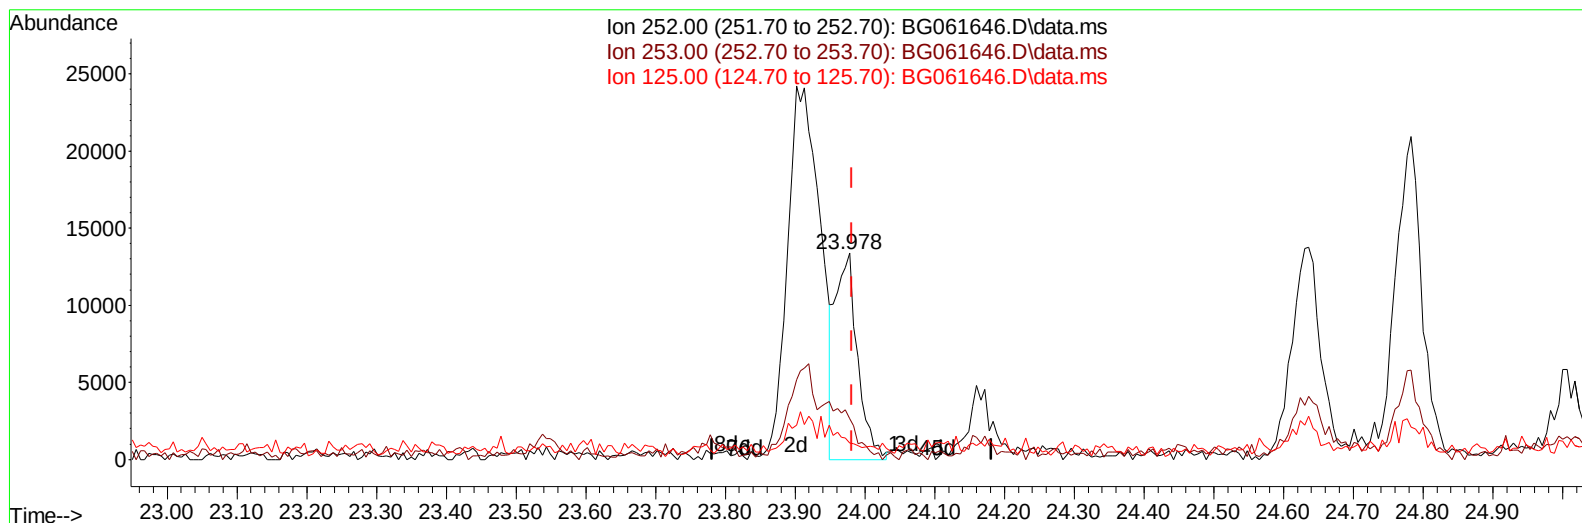

TIC: BG061646.D\data.ms

(91) Benzo(k)fluoranthene

23.978min (-0.003) 1.21 ng/u l m

response 29899

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.20	19.66
125.00	7.70	7.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061646.D
 Acq On : 22 Jun 2024 13:00
 Operator : MA/JU
 Sample : P2775-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4C96

Manual IntegrationsAPPROVED

Quant Time: Jun 22 13:49:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 05:03:55 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/24/2024

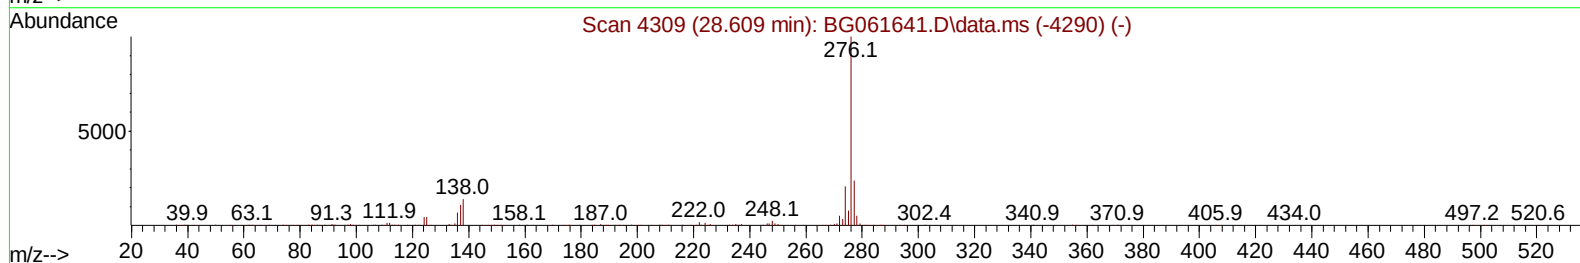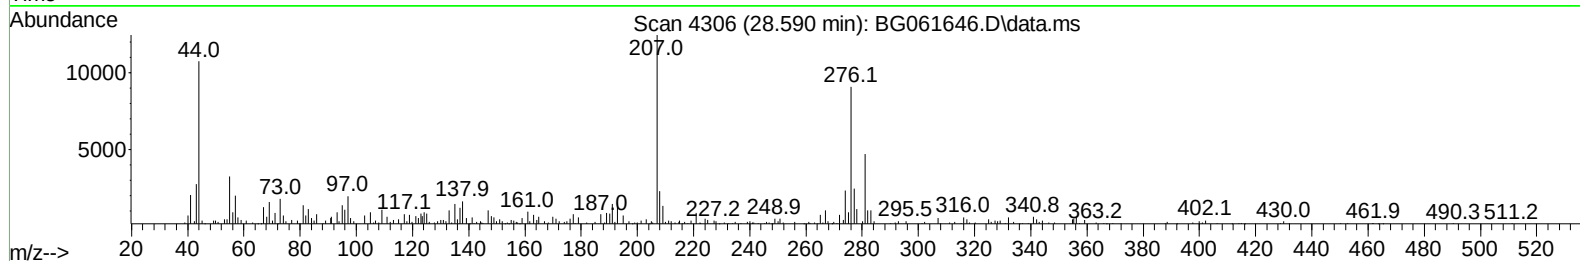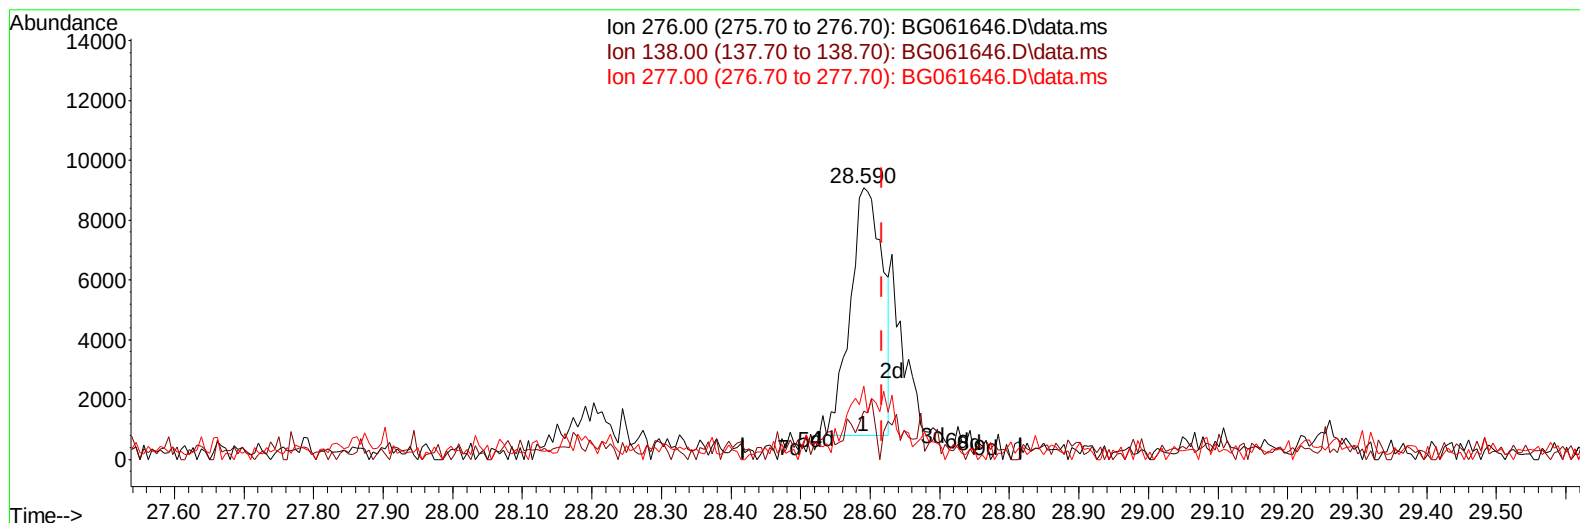

TIC: BG061646.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.590min (-0.027) 0.92 ng/u1

response 26680

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	15.30	17.85
277.00	24.60	26.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061646.D
Acq On : 22 Jun 2024 13:00
Operator : MA/JU
Sample : P2775-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4C96

Manual IntegrationsAPPROVED

Quant Time: Jun 22 13:49:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

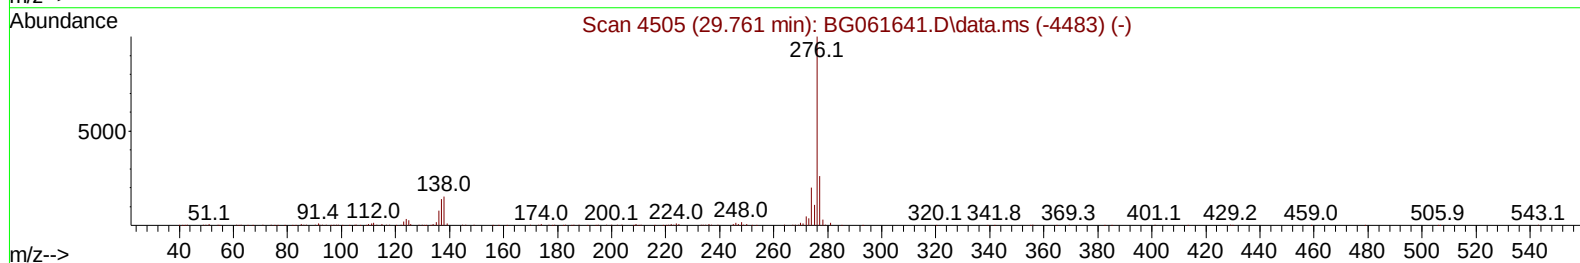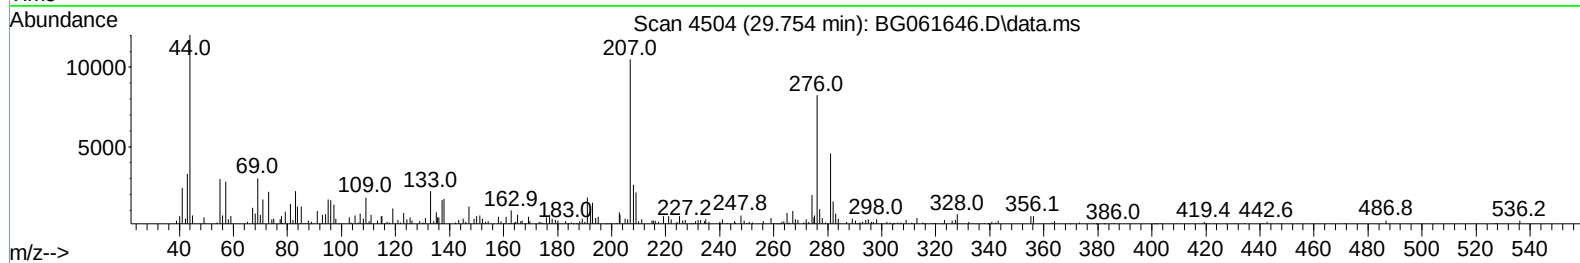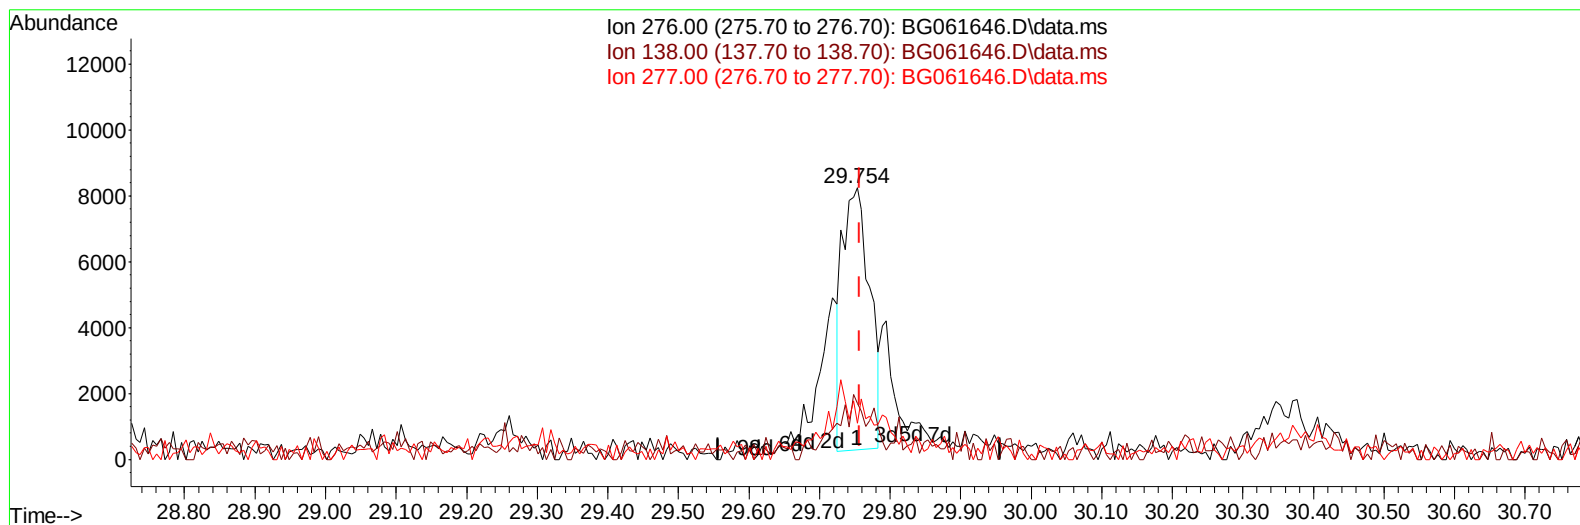

TIC: BG061646.D\data.ms

(96) Benzo(g,h,i)perylene

29.754min (-0.003) 0.92 ng/u1

response 21443

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	15.30	20.69#
277.00	23.20	13.24#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061646.D
Acq On : 22 Jun 2024 13:00
Operator : MA/JU
Sample : P2775-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4C96

Manual IntegrationsAPPROVED

Quant Time: Jun 22 13:49:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

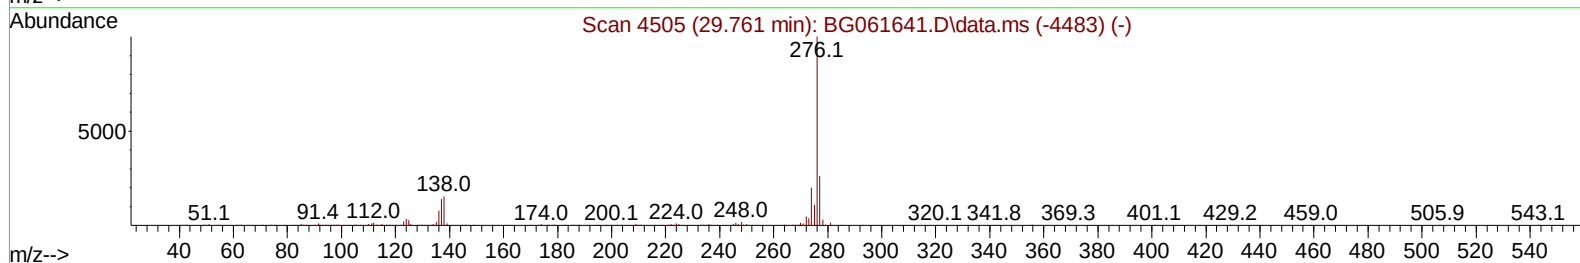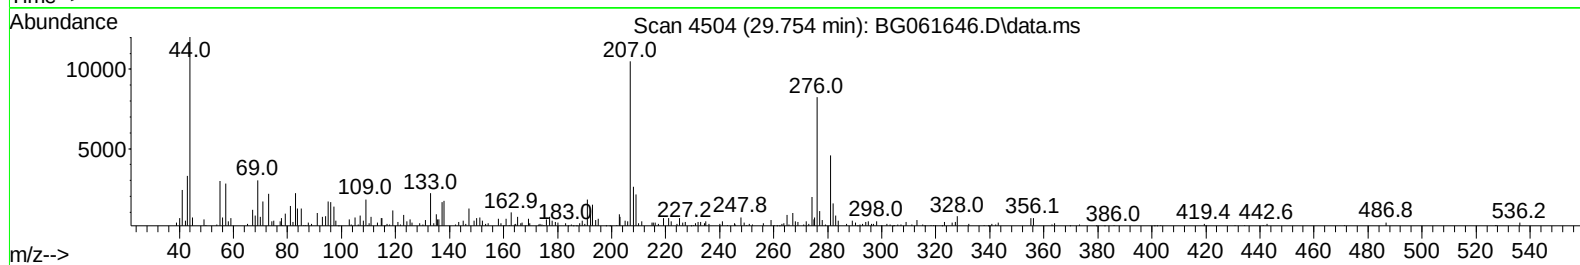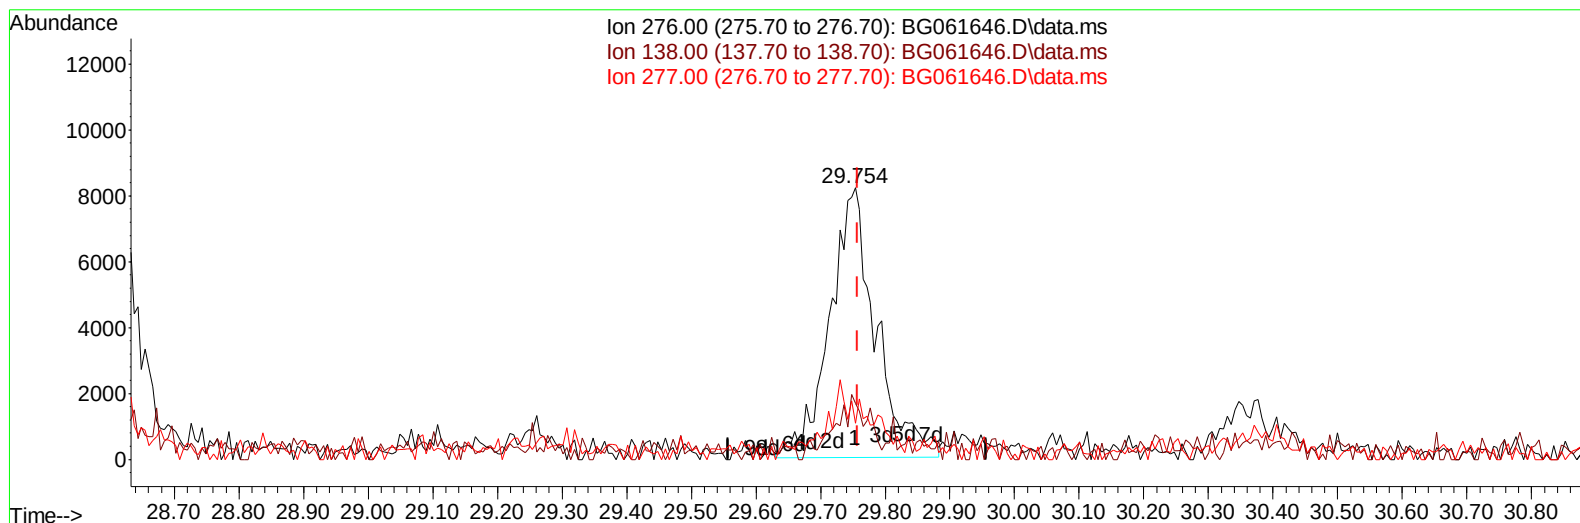

TIC: BG061646.D\data.ms

(96) Benzo(g,h,i)perylene

29.754min (-0.003) 1.73 ng/ul m

response 40338

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	15.30	20.69#
277.00	23.20	13.24#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061646.D
 Acq On : 22 Jun 2024 13:00
 Operator : MA/JU
 Sample : P2775-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4C96

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/24/2024

Quant Time: Jun 22 13:51:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 05:03:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.079	152	46493	20.000	ng/ul	0.00
20) Naphthalene-d8	10.888	136	237033	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.701	164	170435	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	382844	20.000	ng/ul	0.00
79) Chrysene-d12	21.704	240	333260	20.000	ng/ul	0.00
88) Perylene-d12	24.936	264	400007	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.473	96	8091	6.287	ng/uL	0.00
4) Pyridine-d5	3.884	84	126461	32.499	ng/ul	0.00
7) Phenol-d5	7.215	99	176531	34.976	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.398	67	101249	32.180	ng/ul	0.00
11) 2-Chlorophenol-d4	7.603	132	122972	35.504	ng/ul	0.00
15) 4-Methylphenol-d8	8.767	113	140992	36.135	ng/ul	0.00
21) Nitrobenzene-d5	9.242	128	62108	38.590	ng/ul	0.00
24) 2-Nitrophenol-d4	9.959	143	70731	43.392	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.500	165	137819	35.707	ng/ul	0.00
31) 4-Chloroaniline-d4	11.017	131	173006	29.606	ng/ul	0.00
46) Dimethylphthalate-d6	14.107	166	440835	33.611	ng/ul	0.00
49) Acenaphthylene-d8	14.395	160	513981	35.759	ng/ul	0.00
54) 4-Nitrophenol-d4	14.871	143	74774	33.196	ng/ul	0.00
60) Fluorene-d10	15.694	176	396957	34.572	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.794	200	47615	29.086	ng/ul	0.00
73) Anthracene-d10	17.544	188	623426	35.675	ng/ul	0.00
81) Pyrene-d10	19.824	212	676218	36.326	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.713	264	699110	36.593	ng/ul	0.00
Target Compounds						
					Qvalue	
72) Phenanthrene	17.486	178	63350	3.145	ng/ul	98
80) Fluoranthene	19.489	202	124371	5.758	ng/ul	97
82) Pyrene	19.848	202	107748	4.692	ng/ul	97
85) Benzo(a)anthracene	21.687	228	53180	2.273	ng/ul	98
87) Chrysene	21.751	228	56791m	2.566	ng/ul	
90) Benzo(b)fluoranthene	23.902	252	77278	3.214	ng/ul	97
91) Benzo(k)fluoranthene	23.978	252	29899m	1.209	ng/ul	
93) Benzo(a)pyrene	24.783	252	51965	2.245	ng/ul#	88
94) Indeno(1,2,3-cd)pyrene	28.590	276	43789m	1.518	ng/ul	
96) Benzo(g,h,i)perylene	29.754	276	40338m	1.735	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061646.D
Acq On : 22 Jun 2024 13:00
Operator : MA/JU
Sample : P2775-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4C96

Manual IntegrationsAPPROVED

Quant Time: Jun 22 13:51:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

