




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061648.D
Acq On : 22 Jun 2024 14:22
Operator : MA/JU
Sample : P2775-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4D59

Manual IntegrationsAPPROVED

Quant Time: Jun 22 15:02:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

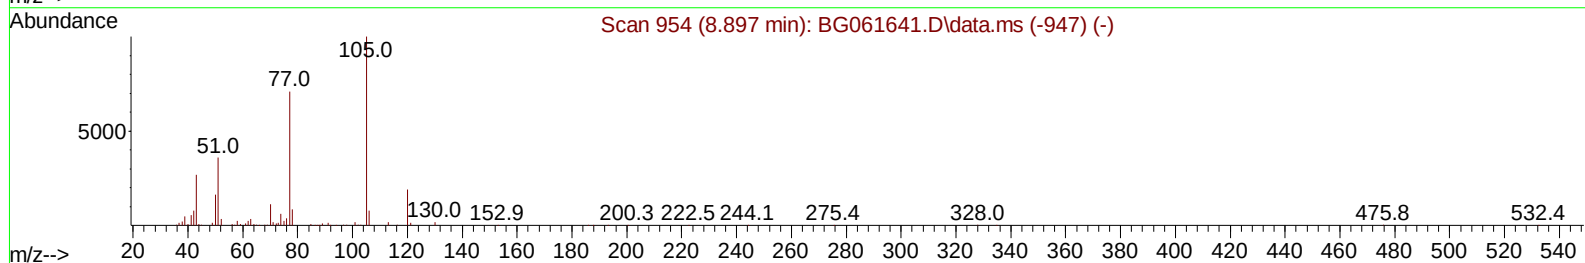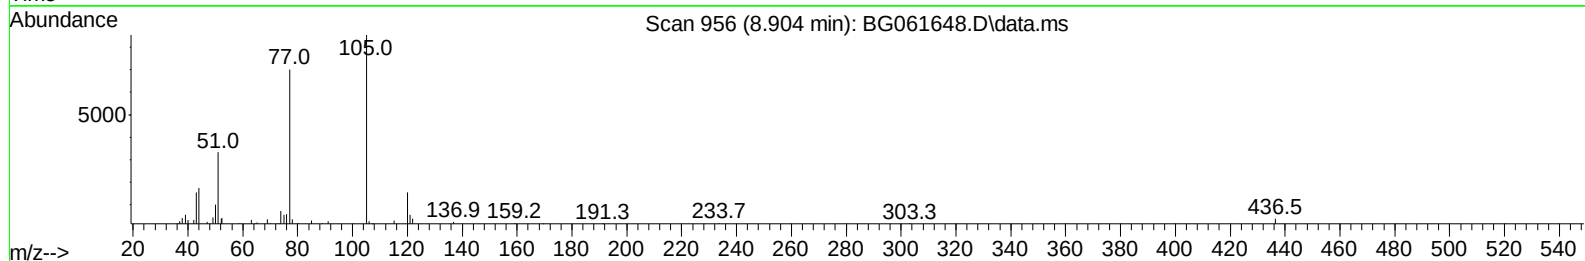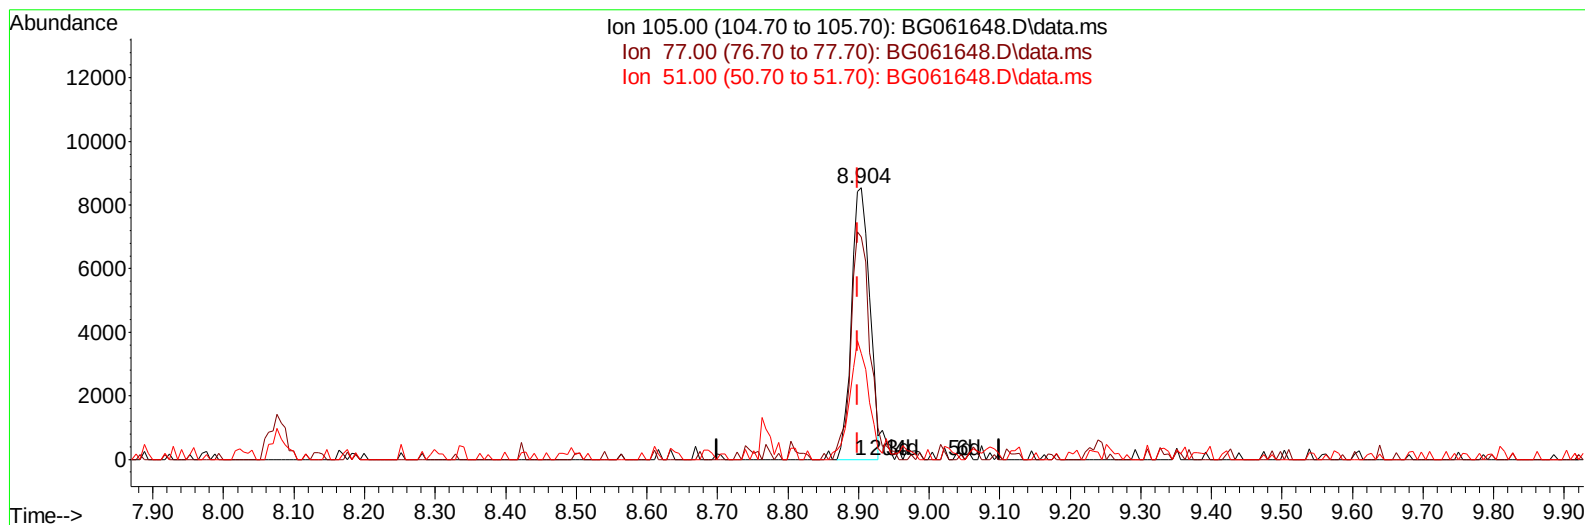

TIC: BG061648.D\data.ms

(16) Acetophenone

8.904min (+ 0.005) 2.06 ng/u1

response 15425

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	75.50	82.04
51.00	38.90	39.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061648.D
 Acq On : 22 Jun 2024 14:22
 Operator : MA/JU
 Sample : P2775-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4D59

Manual IntegrationsAPPROVED

Quant Time: Jun 22 15:02:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 05:03:55 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/24/2024

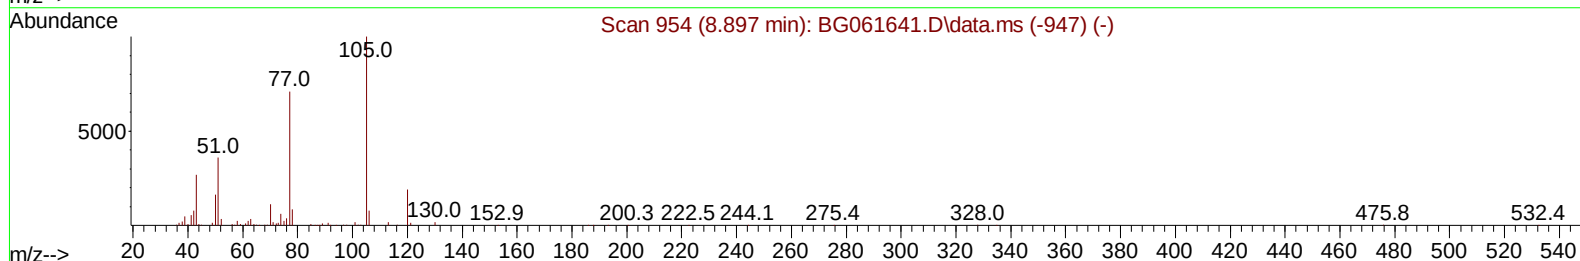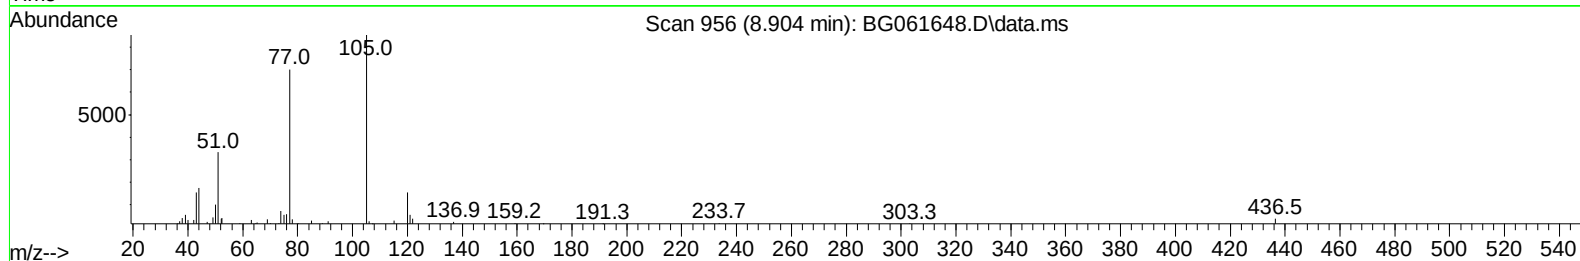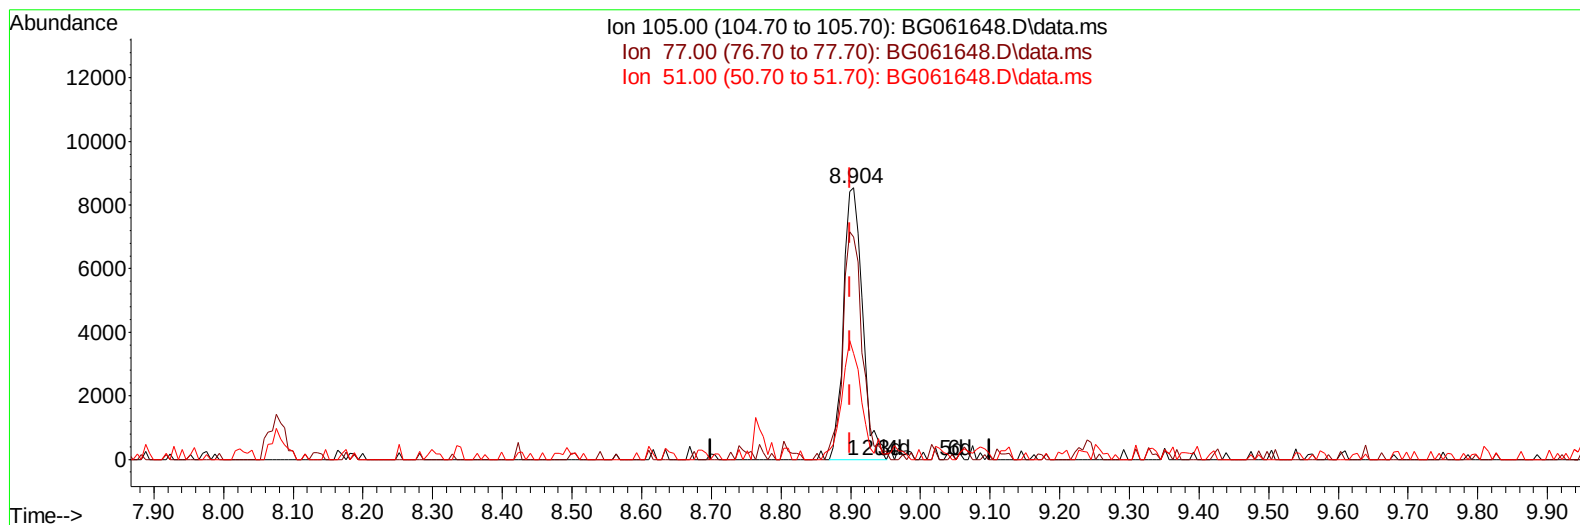

TIC: BG061648.D\data.ms

(16) Acetophenone

8.904min (+ 0.005) 2.14 ng/ul m

response 16027

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	75.50	82.04
51.00	38.90	39.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061648.D
Acq On : 22 Jun 2024 14:22
Operator : MA/JU
Sample : P2775-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4D59

Manual IntegrationsAPPROVED

Quant Time: Jun 22 14:58:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

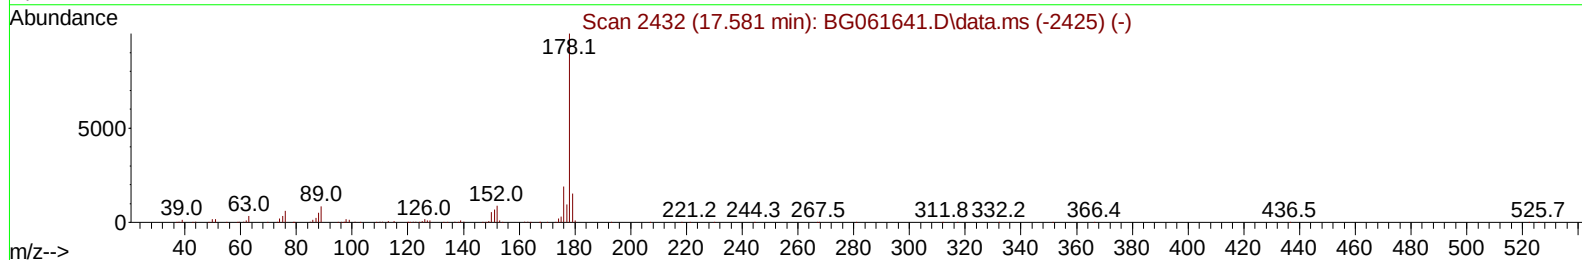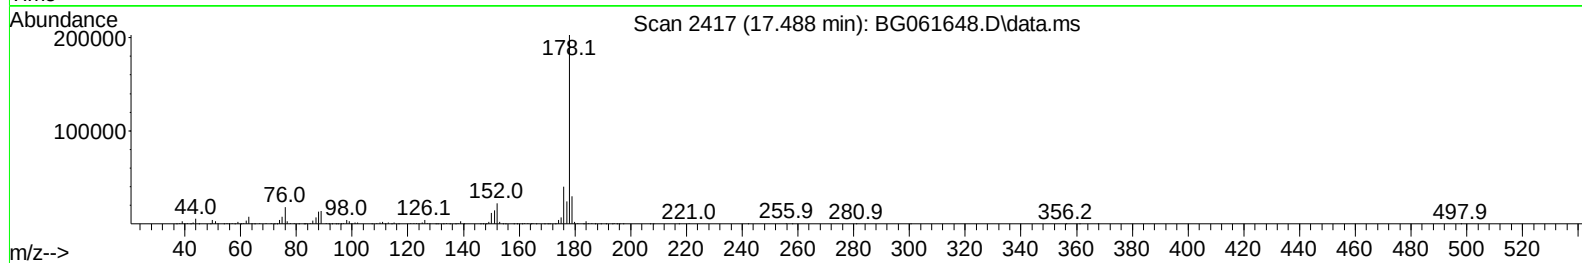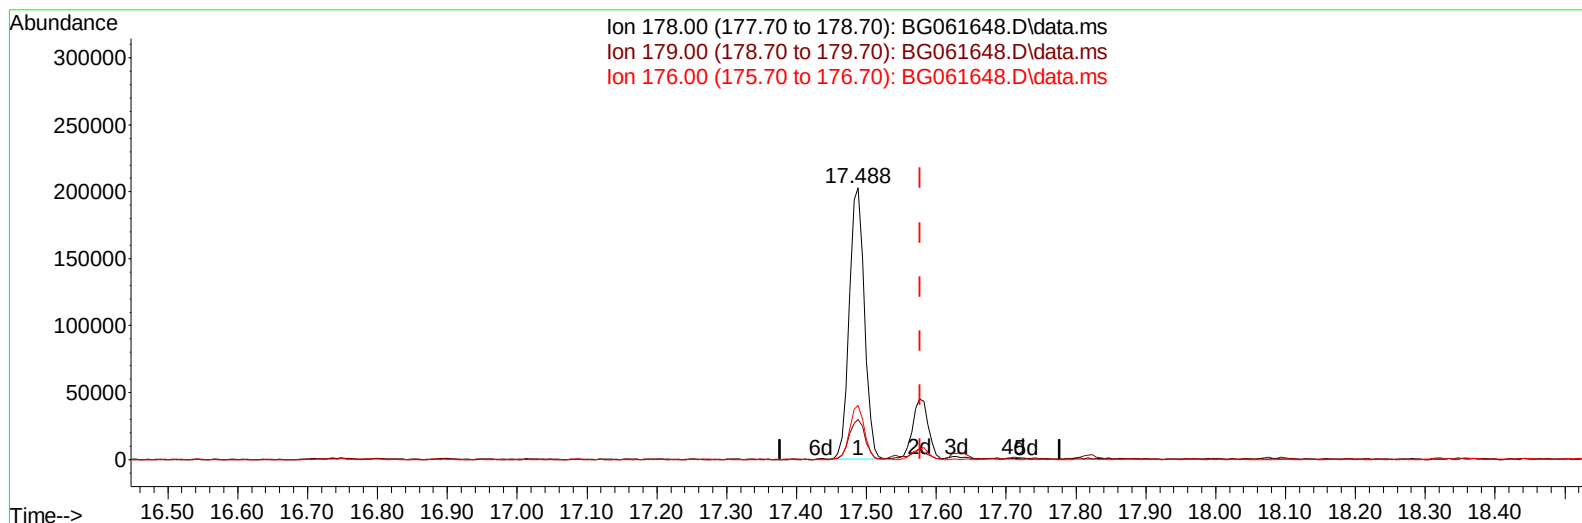

TIC: BG061648.D\data.ms

(74) Anthracene

17.488min (-0.089) 12.76 ng/u1

response 301384

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	14.30	14.82
176.00	18.40	19.87
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061648.D
Acq On : 22 Jun 2024 14:22
Operator : MA/JU
Sample : P2775-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4D59

Manual IntegrationsAPPROVED

Quant Time: Jun 22 14:58:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

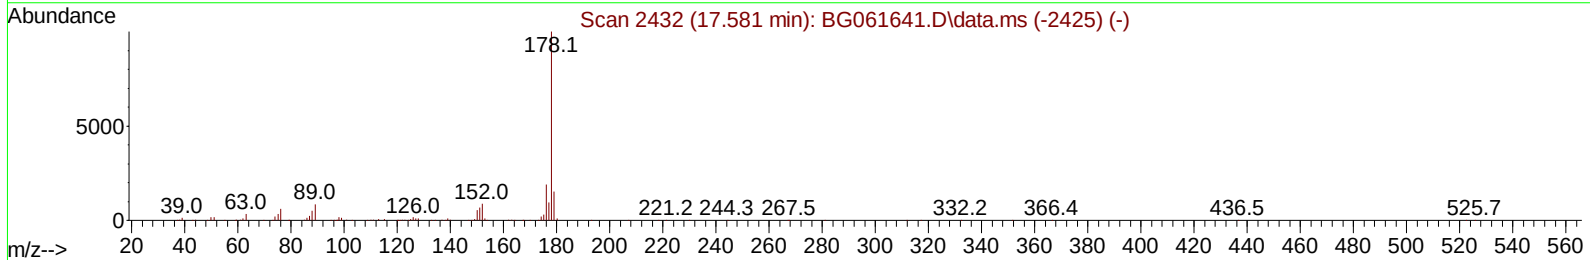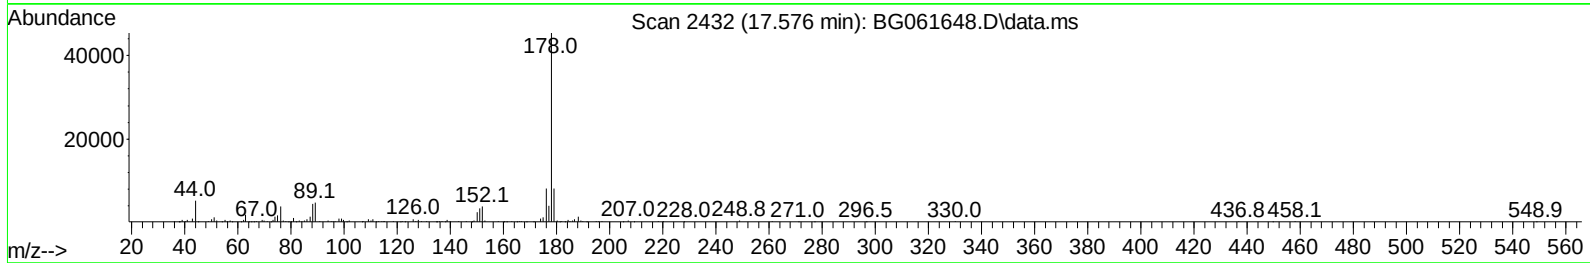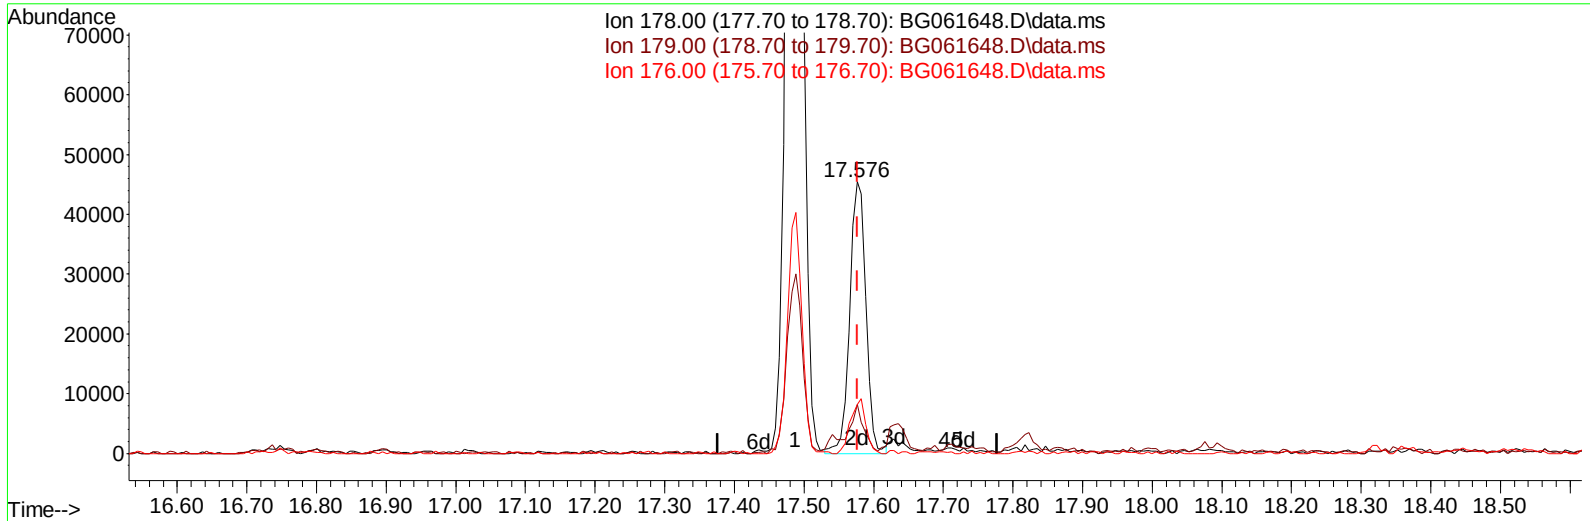

TIC: BG061648.D\data.ms

(74) Anthracene

17.576min (-0.001) 3.09 ng/ul m

response 72992

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	14.30	17.98#
176.00	18.40	17.96
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061648.D
 Acq On : 22 Jun 2024 14:22
 Operator : MA/JU
 Sample : P2775-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4D59

Manual IntegrationsAPPROVED

Quant Time: Jun 22 14:58:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 05:03:55 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/24/2024

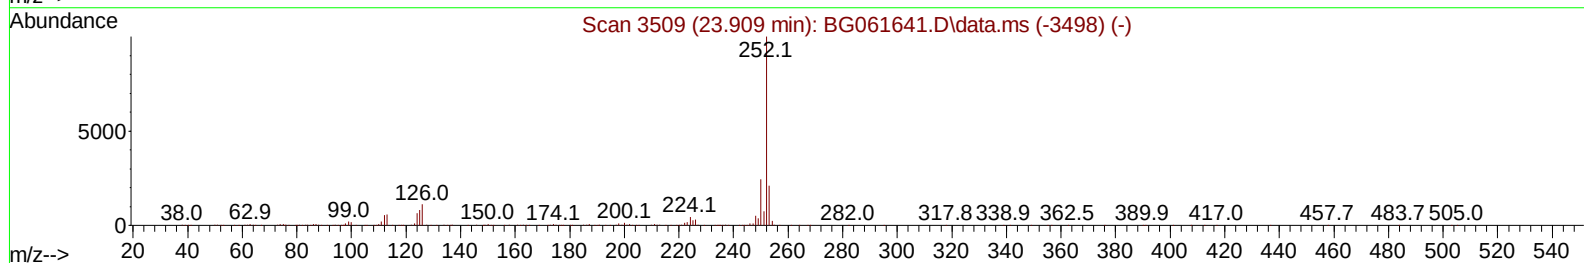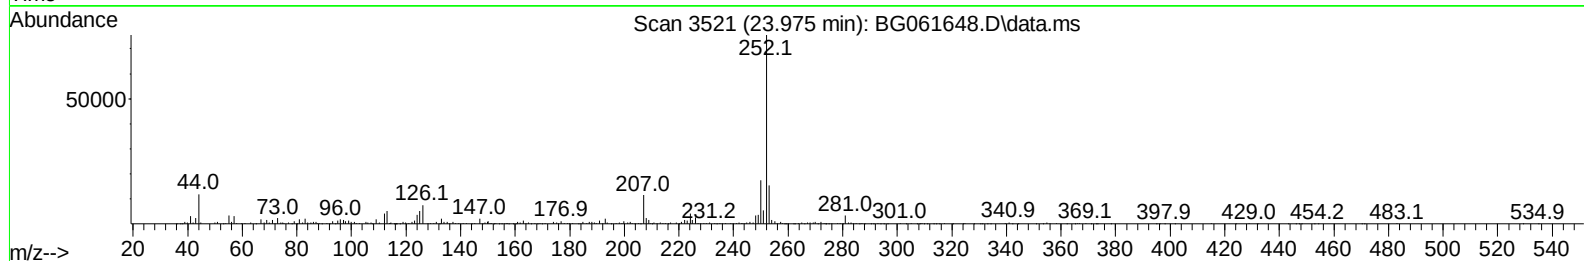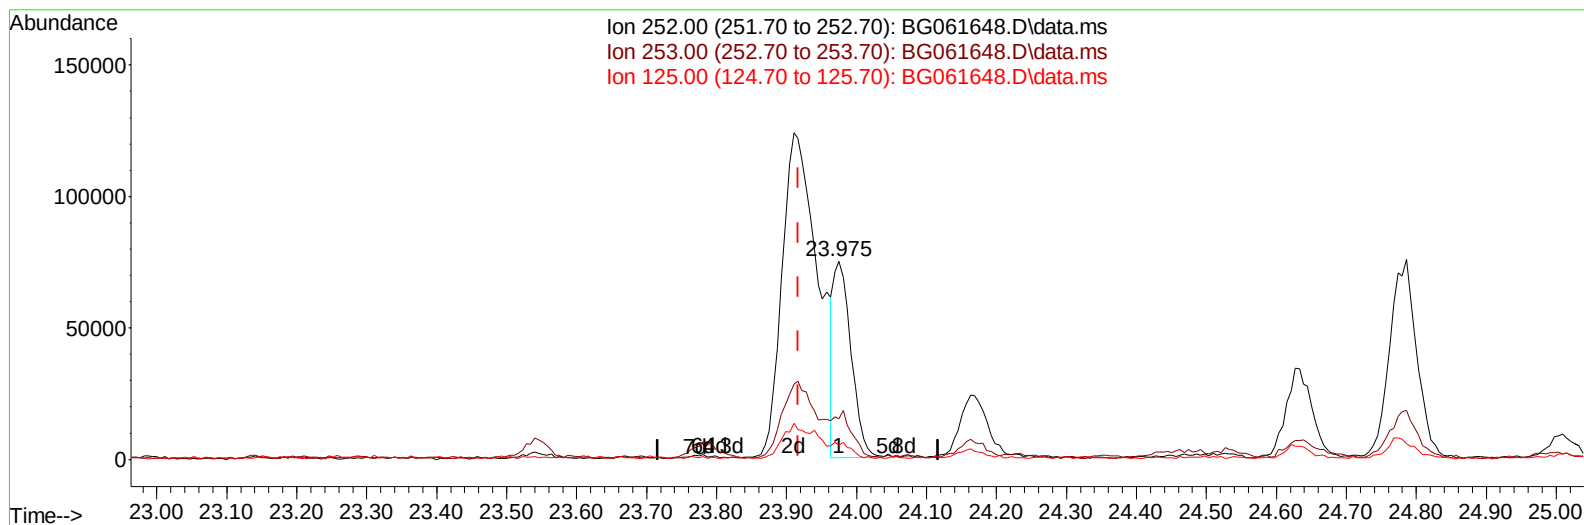

TIC: BG061648.D\data.ms

(90) Benzo(b)fluoranthene

23.975min (+ 0.058) 4.76 ng/u1

response 128838

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.20	20.56
125.00	8.80	7.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061648.D
Acq On : 22 Jun 2024 14:22
Operator : MA/JU
Sample : P2775-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4D59

Manual IntegrationsAPPROVED

Quant Time: Jun 22 14:58:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

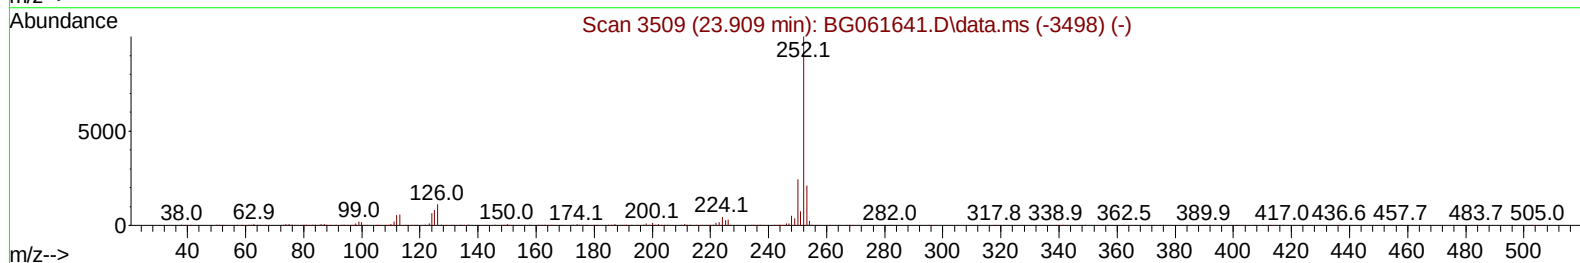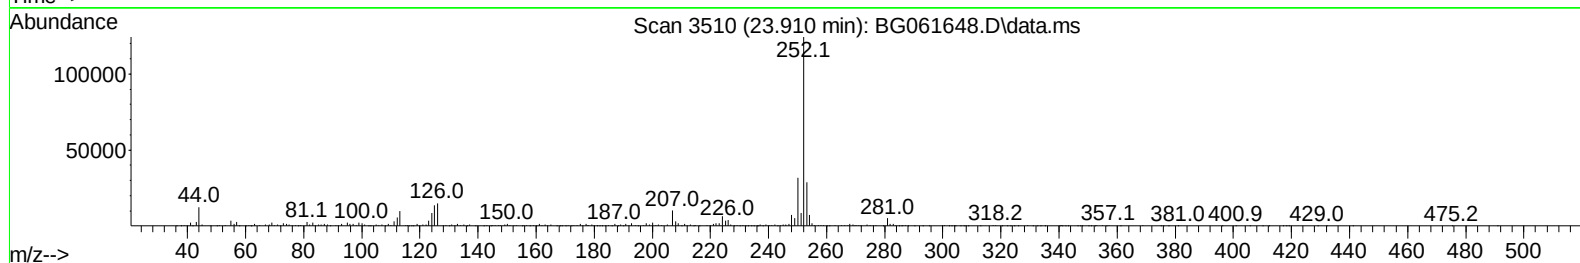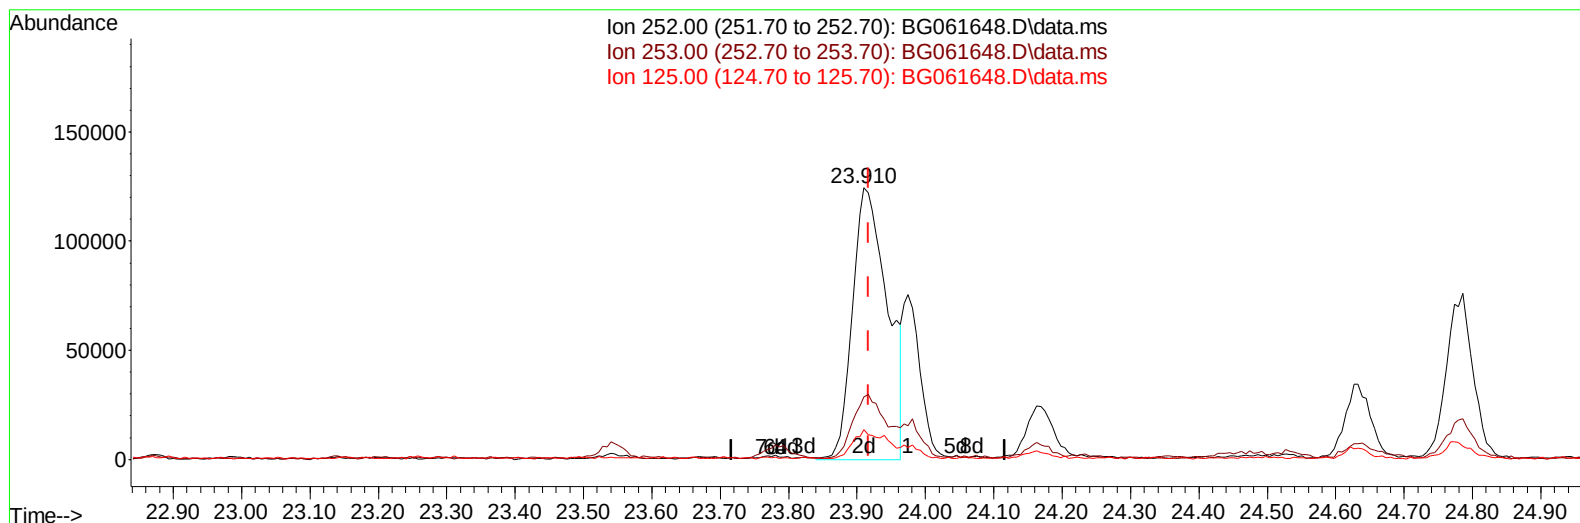

TIC: BG061648.D\data.ms

(90) Benzo(b)fluoranthene

23.910min (-0.006) 16.29 ng/ul m

response 440978

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.20	23.02
125.00	8.80	11.09#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061648.D
Acq On : 22 Jun 2024 14:22
Operator : MA/JU
Sample : P2775-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4D59

Manual IntegrationsAPPROVED

Quant Time: Jun 22 14:58:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

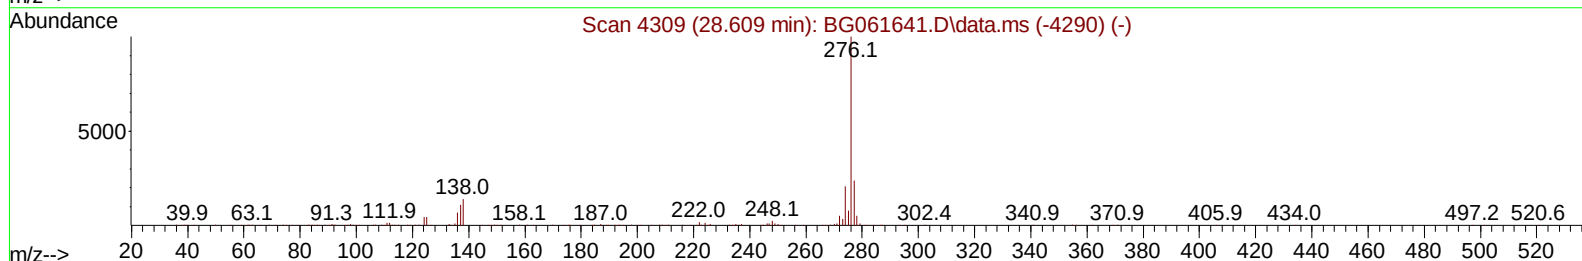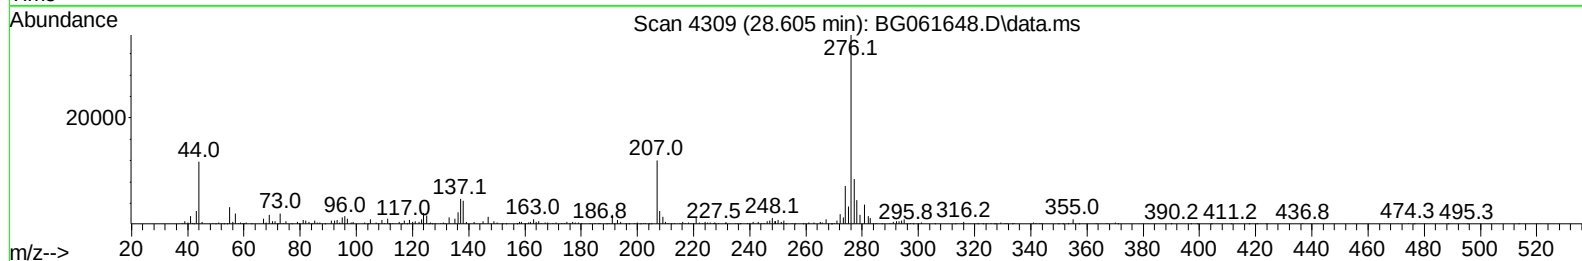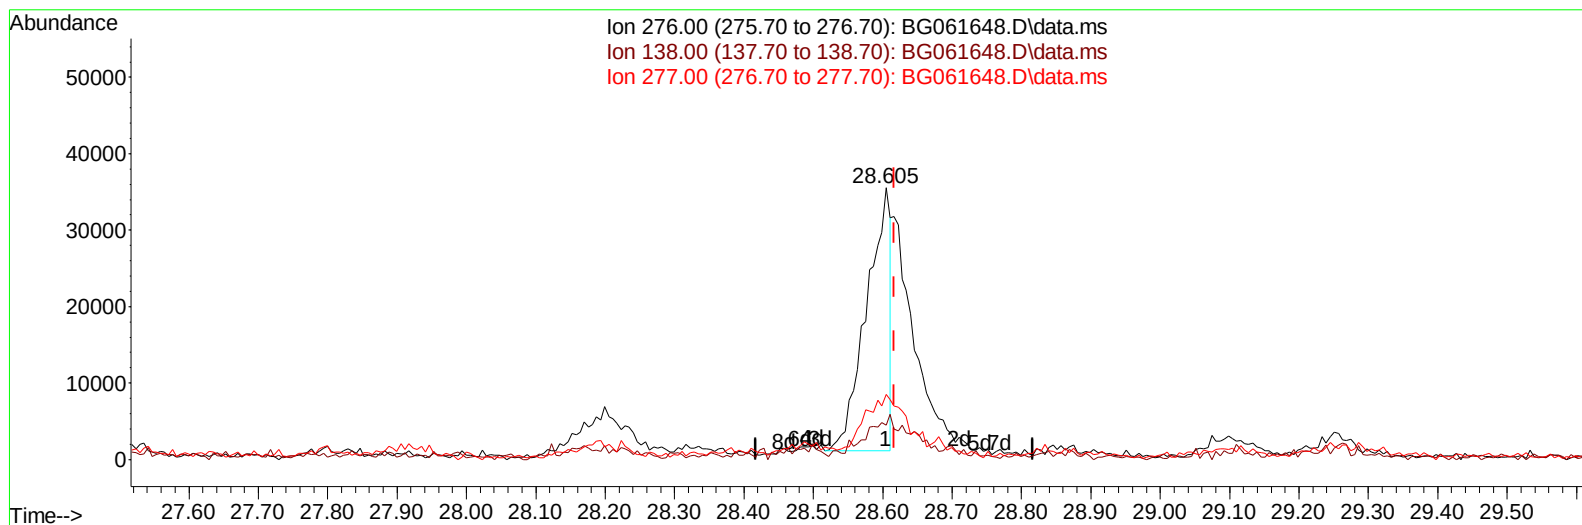

TIC: BG061648.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.605min (-0.012) 2.52 ng/u1

response 81964

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	15.30	12.67
277.00	24.60	23.90
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061648.D
Acq On : 22 Jun 2024 14:22
Operator : MA/JU
Sample : P2775-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4D59

Manual IntegrationsAPPROVED

Quant Time: Jun 22 14:58:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

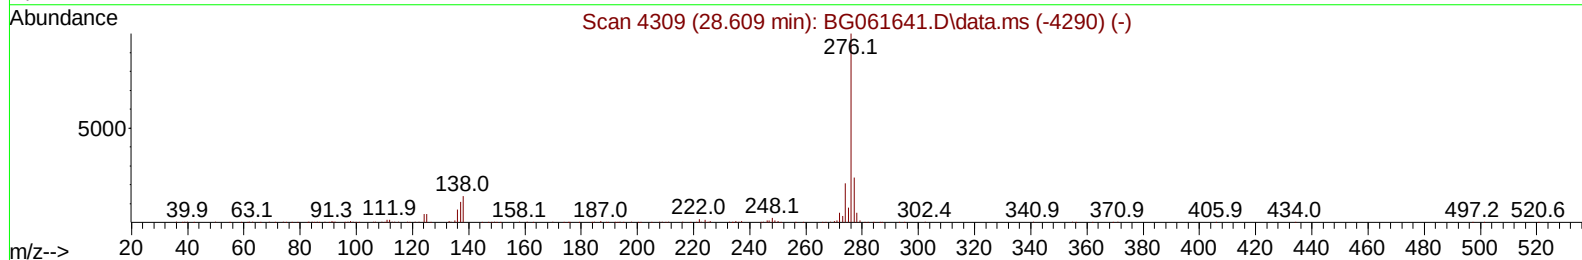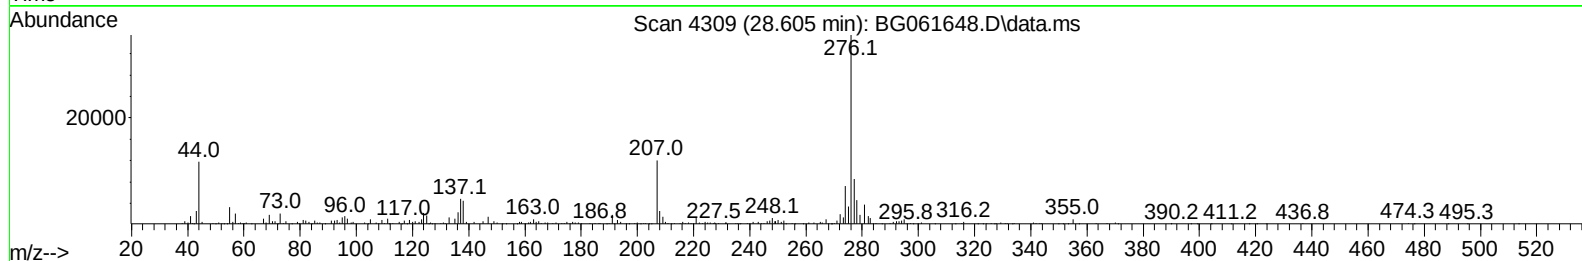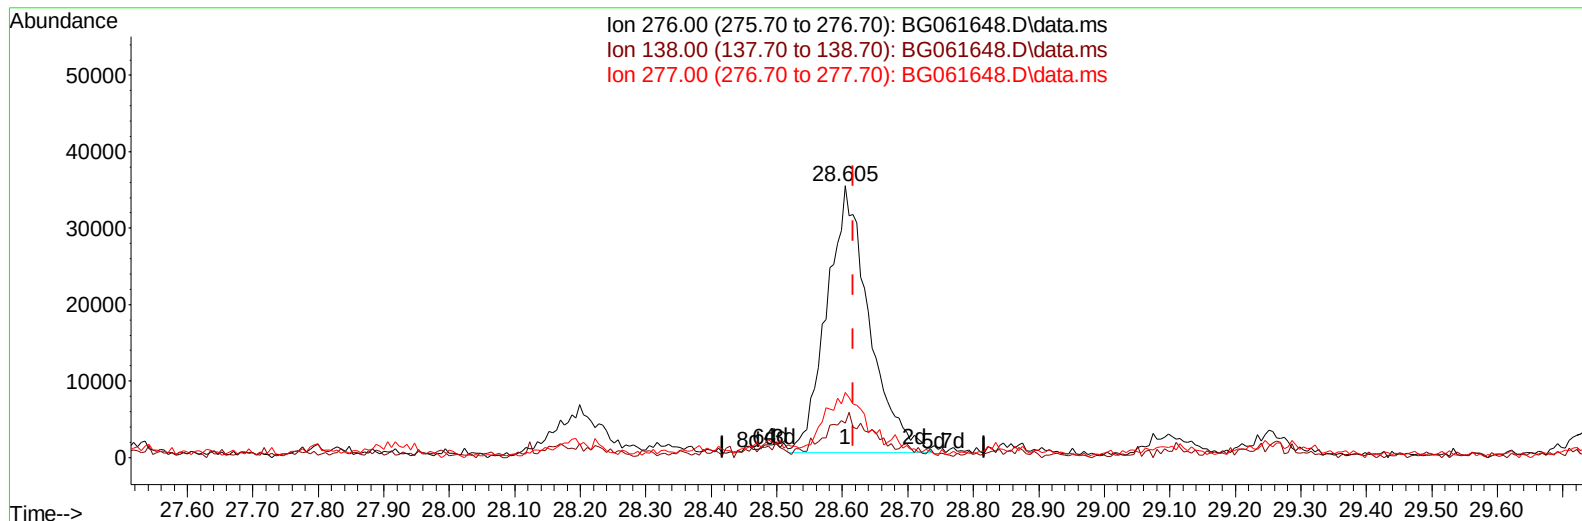

TIC: BG061648.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.605min (-0.012) 4.83 ng/ul m

response 156970

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	15.30	12.67
277.00	24.60	23.90
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061648.D
Acq On : 22 Jun 2024 14:22
Operator : MA/JU
Sample : P2775-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4D59

Manual IntegrationsAPPROVED

Quant Time: Jun 22 14:58:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

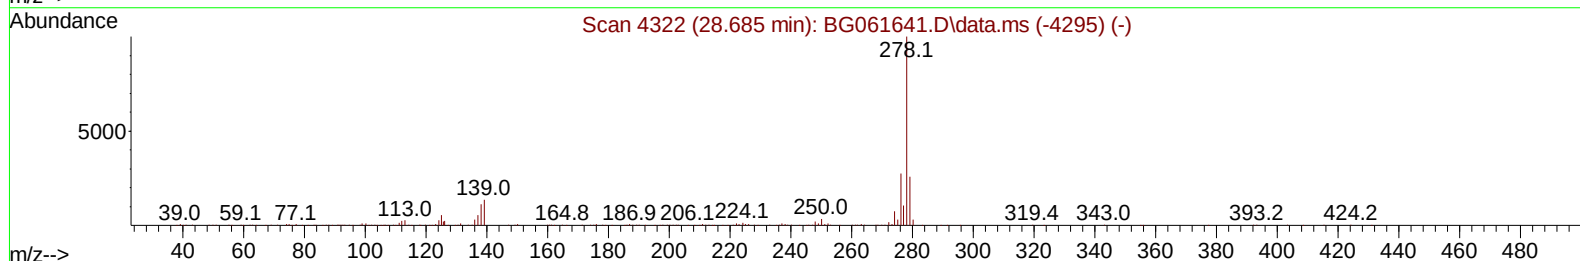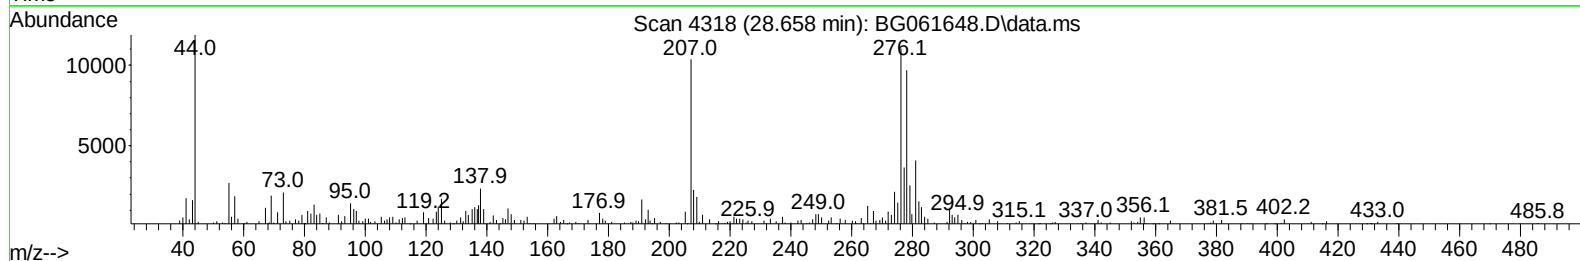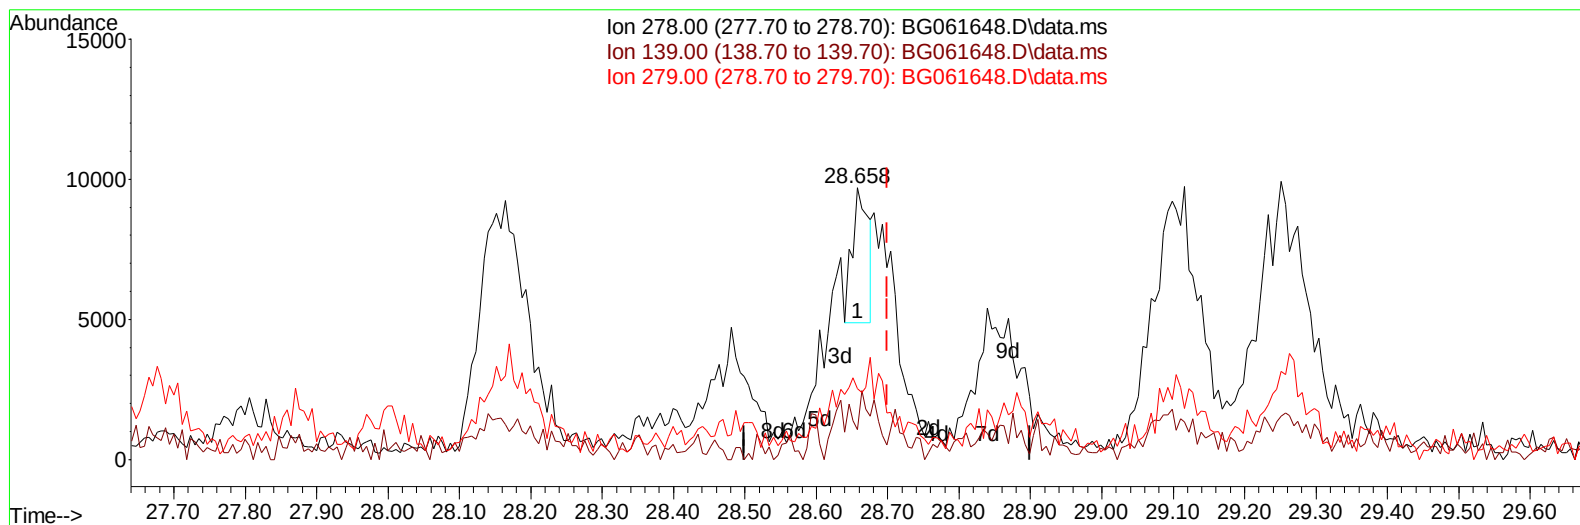

TIC: BG061648.D\data.ms

(95) Dibenzo(a,h)anthracene

28.658min (-0.042) 0.28 ng/u1

response 7547

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	11.40	10.91
279.00	23.30	26.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061648.D
Acq On : 22 Jun 2024 14:22
Operator : MA/JU
Sample : P2775-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4D59

Manual IntegrationsAPPROVED

Quant Time: Jun 22 14:58:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

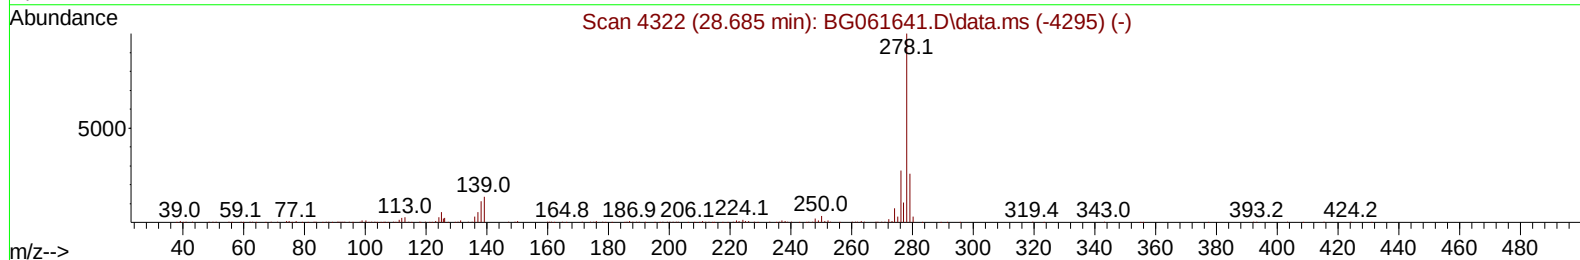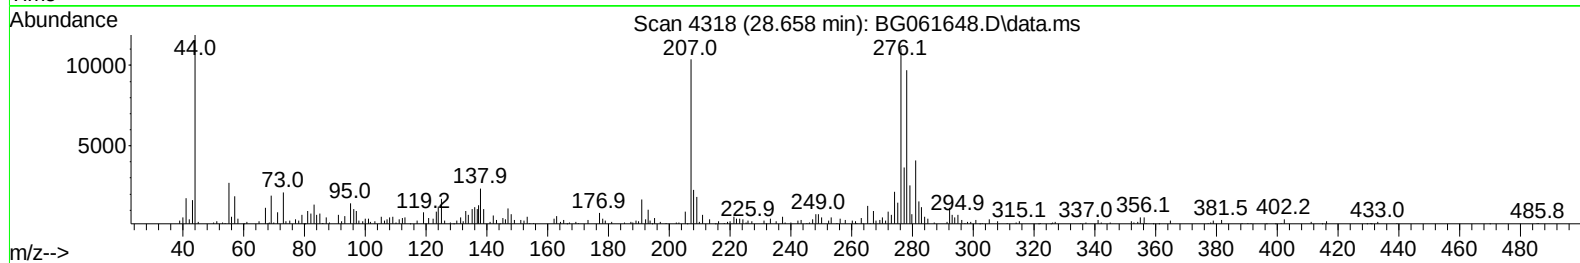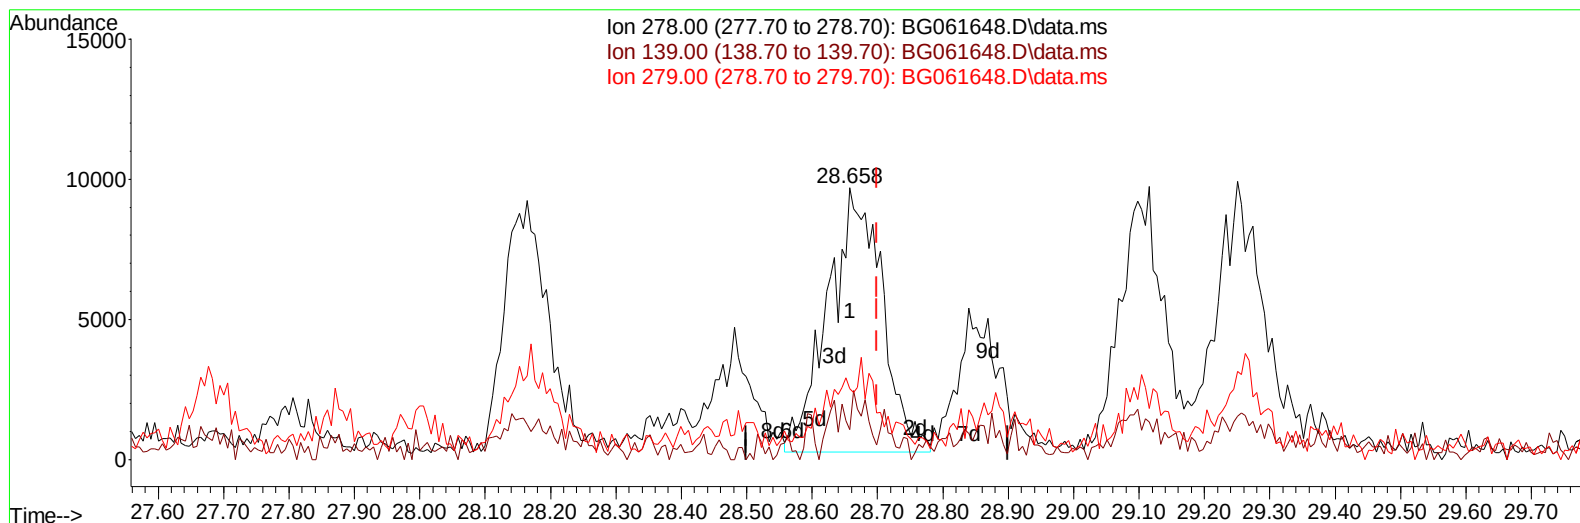

TIC: BG061648.D\data.ms

(95) Dibenzo(a,h)anthracene

28.658min (-0.042) 2.00 ng/ul m

response 53966

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	11.40	10.91
279.00	23.30	26.17
0.00	0.00	0.00