




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061665.D
 Acq On : 23 Jun 2024 2:02
 Operator : MA/JU
 Sample : PB161462BS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 05:03:55 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/24/2024

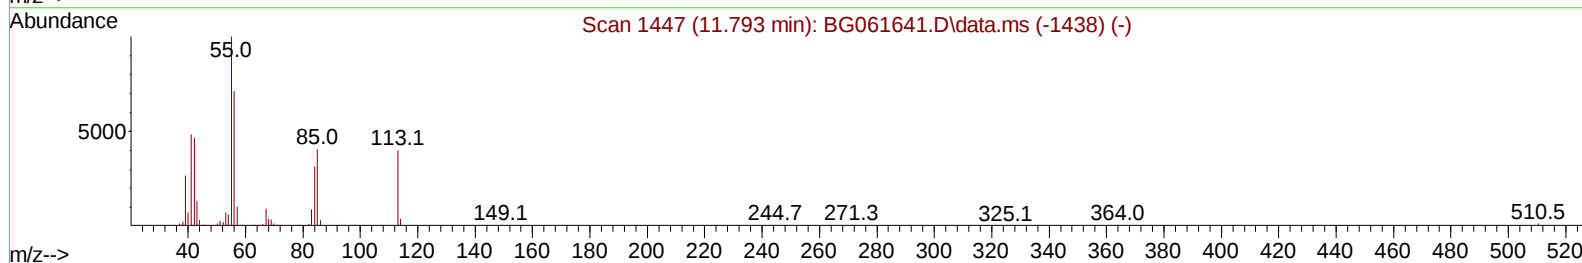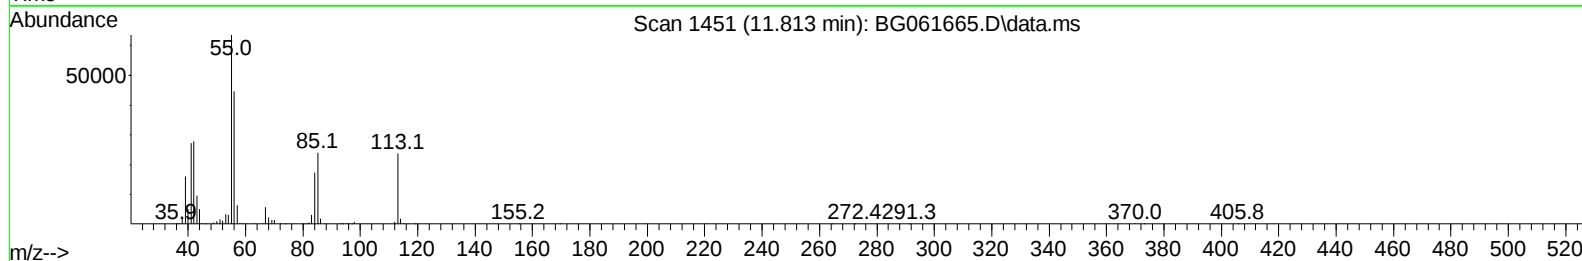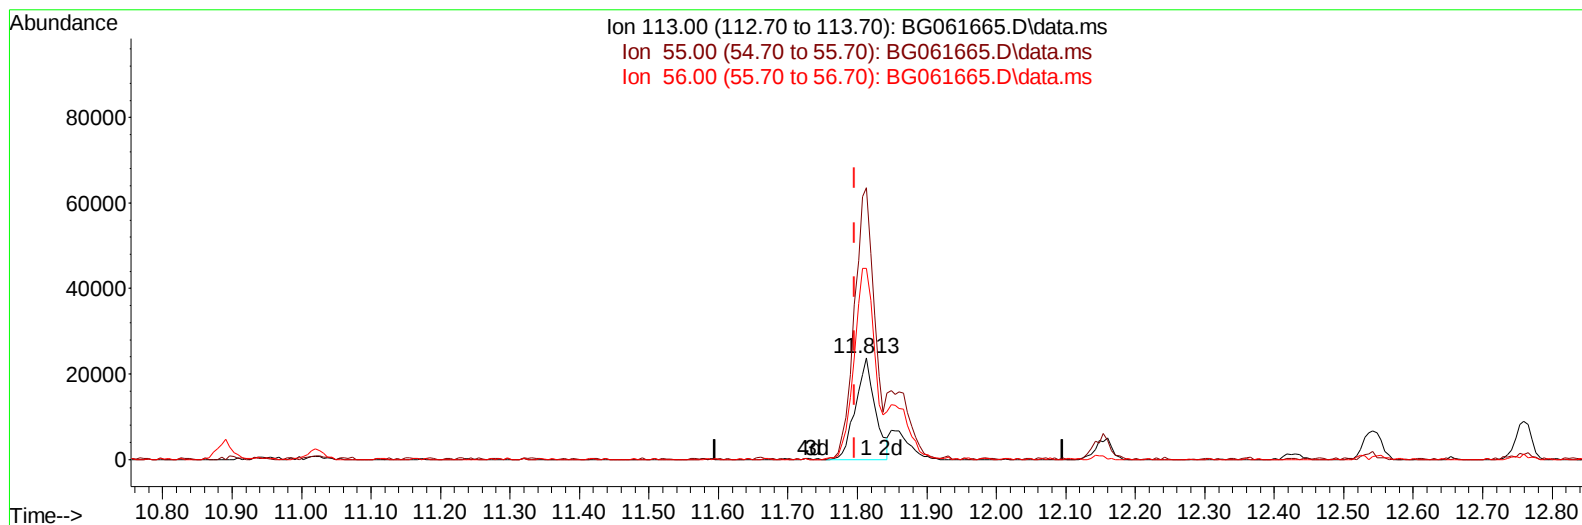

TIC: BG061665.D\data.ms

(34) Caprolactam

11.813min (+ 0.018) 19.72 ng/ul

response 46393

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	259.30	268.06
56.00	209.00	188.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061665.D
 Acq On : 23 Jun 2024 2:02
 Operator : MA/JU
 Sample : PB161462BS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 05:03:55 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/24/2024

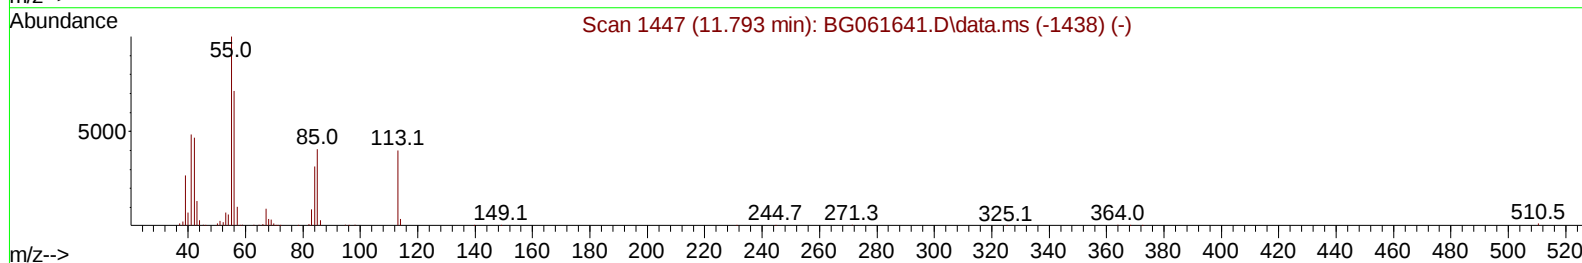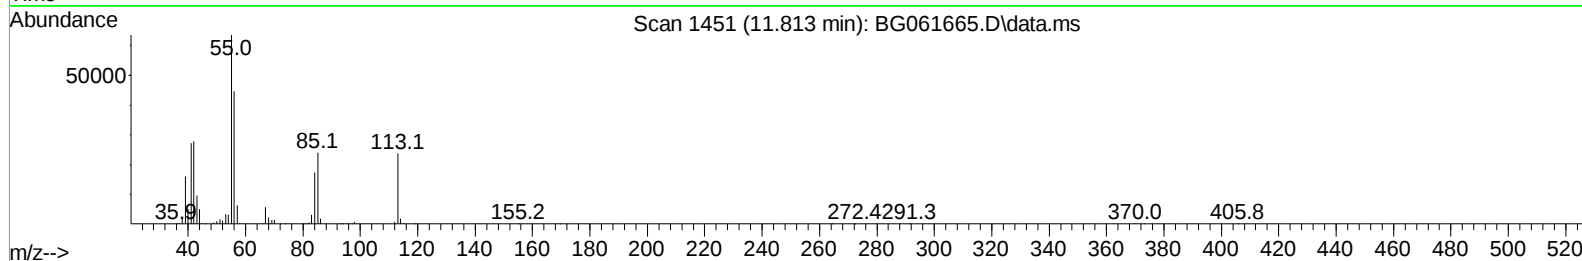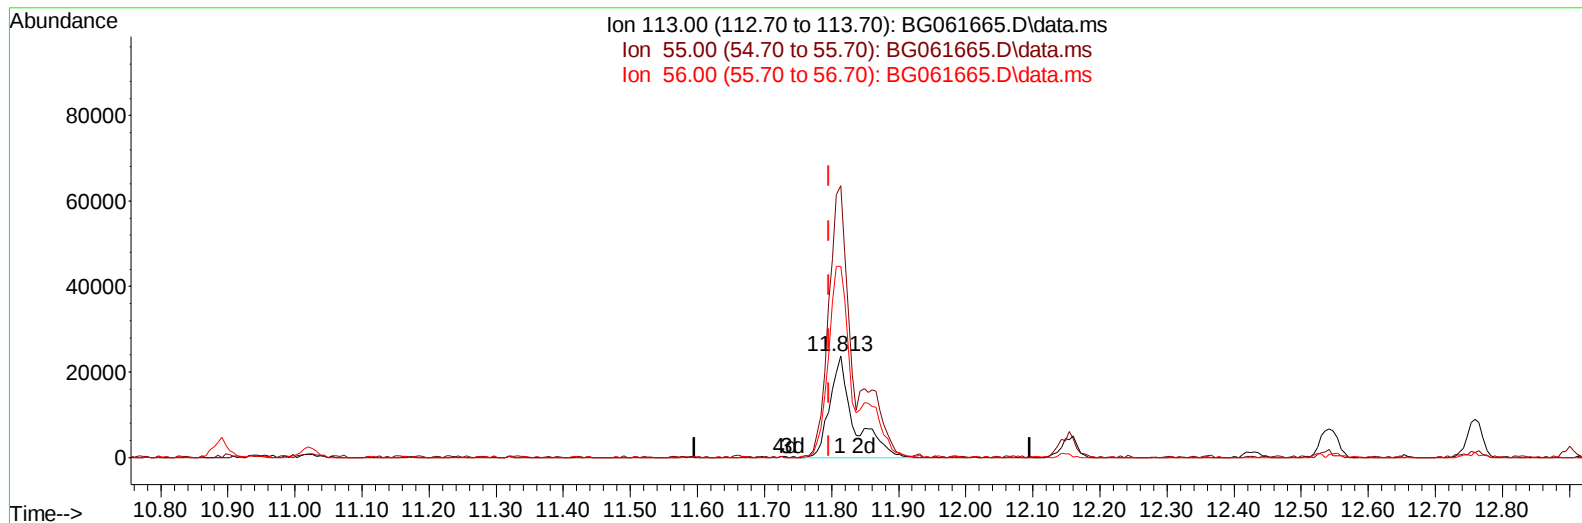

TIC: BG061665.D\data.ms

(34) Caprolactam

11.813min (+ 0.018) 25.30 ng/ul m

response 59537

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	259.30	268.06
56.00	209.00	188.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061665.D
Acq On : 23 Jun 2024 2:02
Operator : MA/JU
Sample : PB161462BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

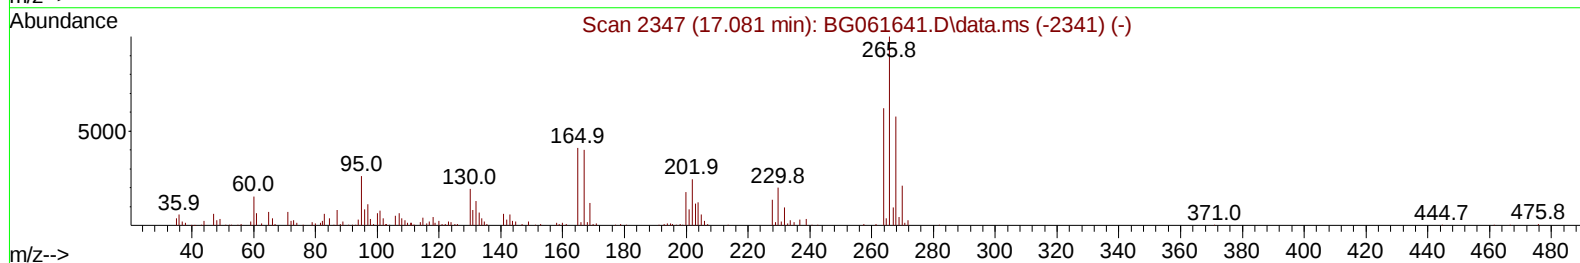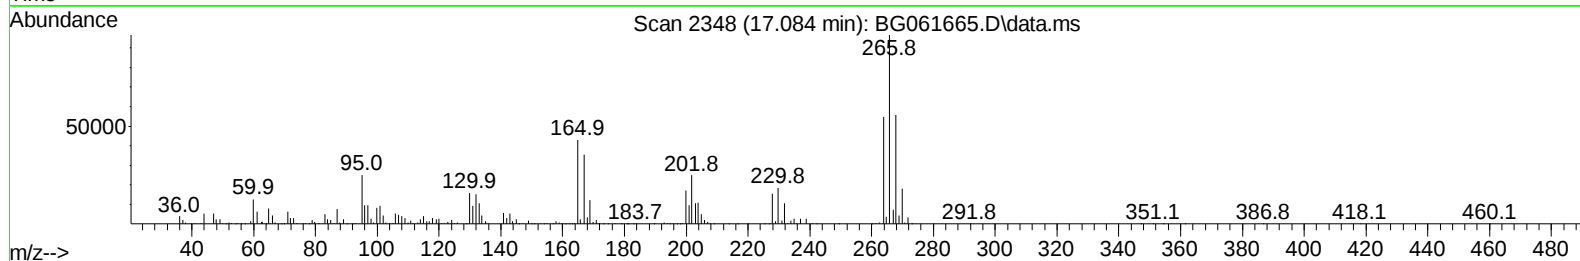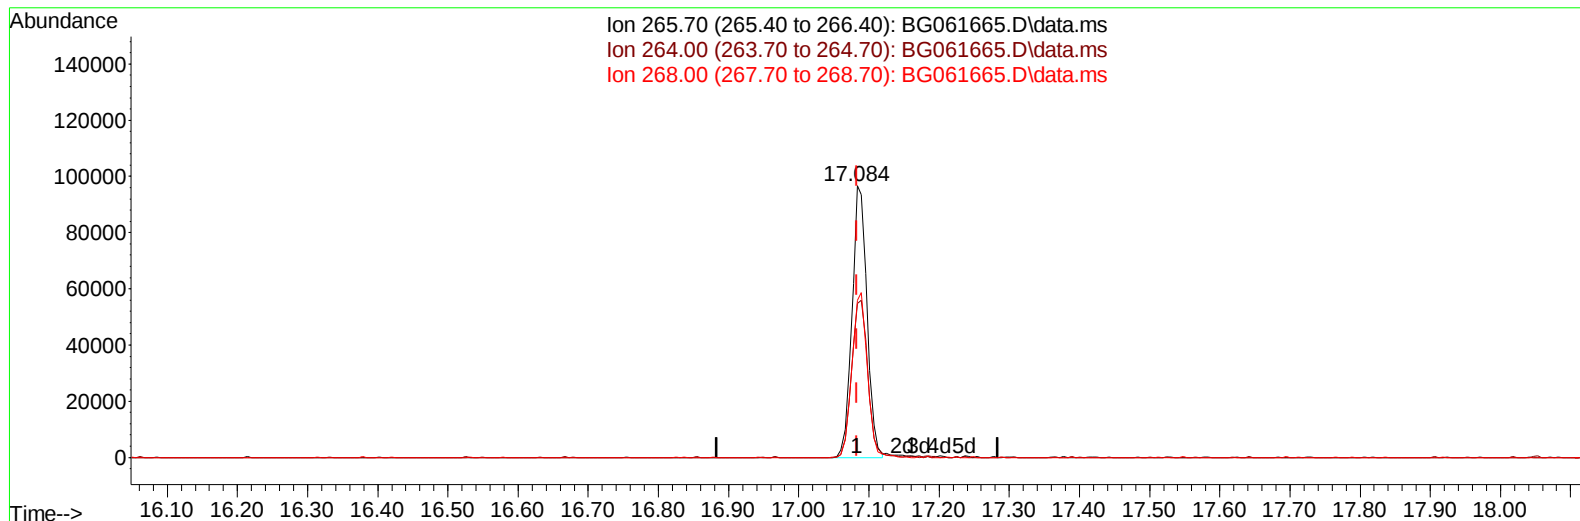

TIC: BG061665.D\data.ms

(71) Pentachlorophenol (C)

17.084min (+ 0.000) 33.53 ng/u1

response 143922

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	65.60	56.83
268.00	59.40	57.78
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061665.D
Acq On : 23 Jun 2024 2:02
Operator : MA/JU
Sample : PB161462BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

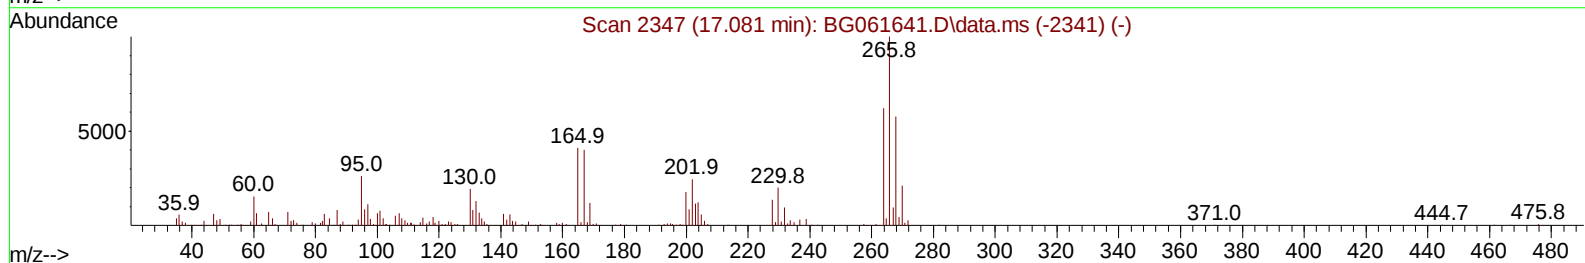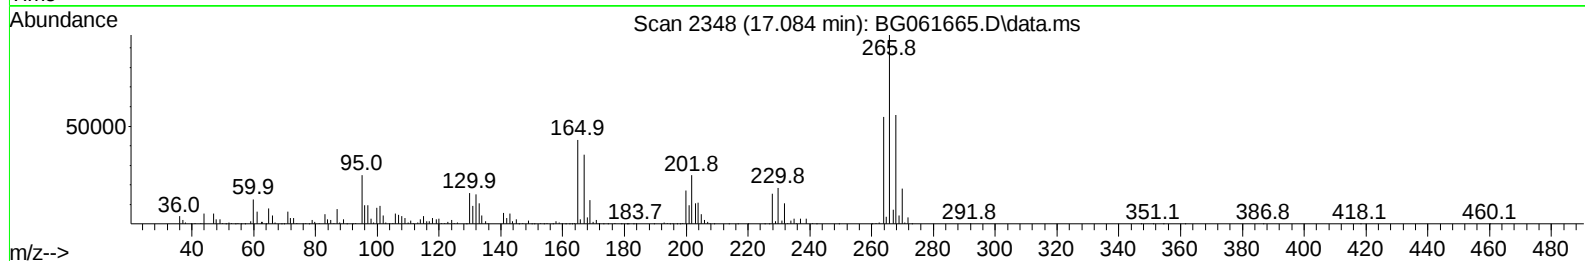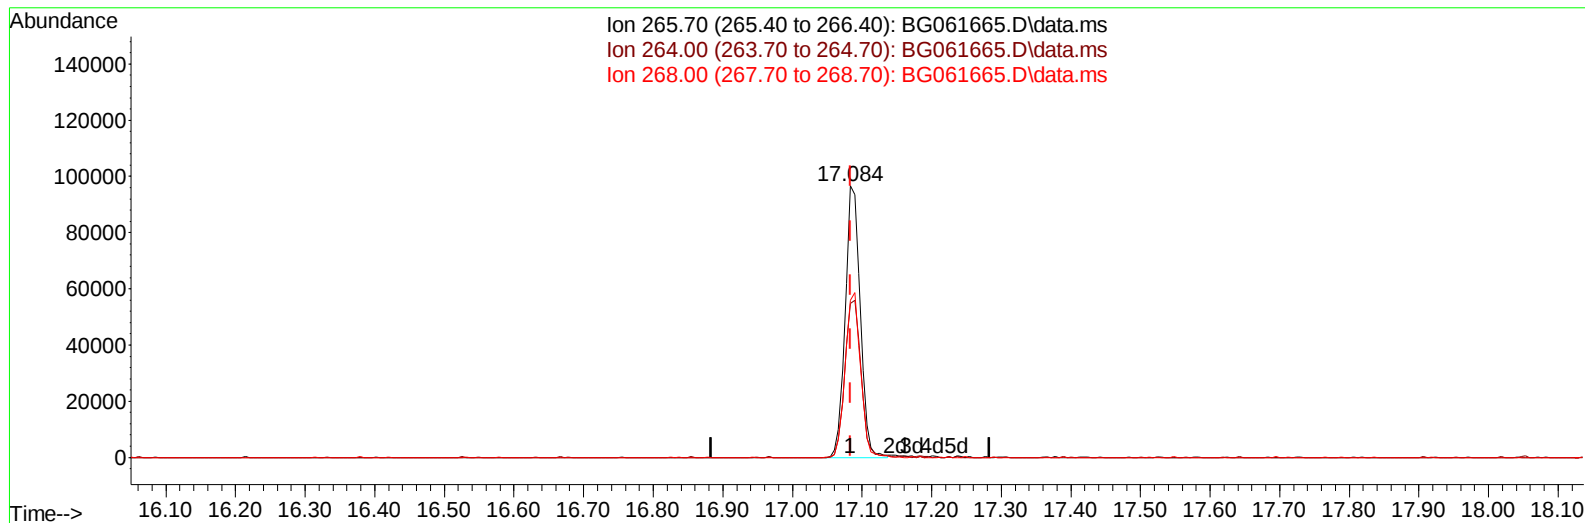

TIC: BG061665.D\data.ms

(71) Pentachlorophenol (C)

17.084min (+ 0.000) 33.79 ng/ul m

response 145052

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	65.60	56.83
268.00	59.40	57.78
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061665.D
Acq On : 23 Jun 2024 2:02
Operator : MA/JU
Sample : PB161462BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

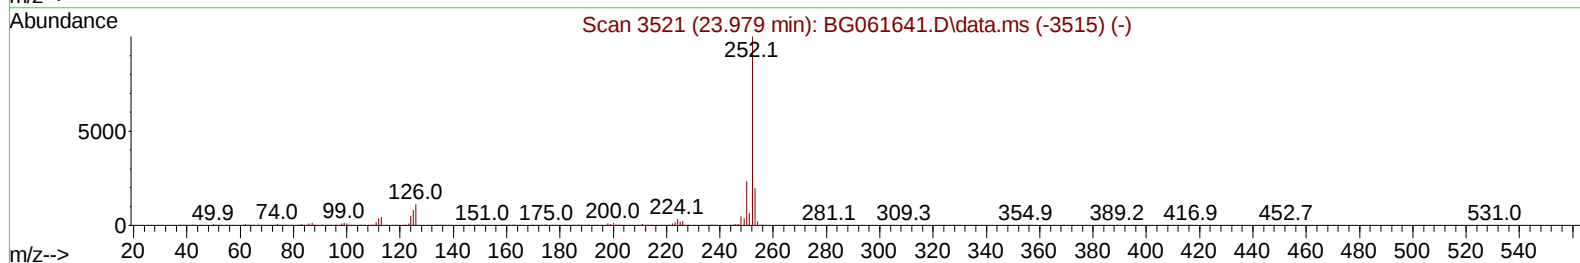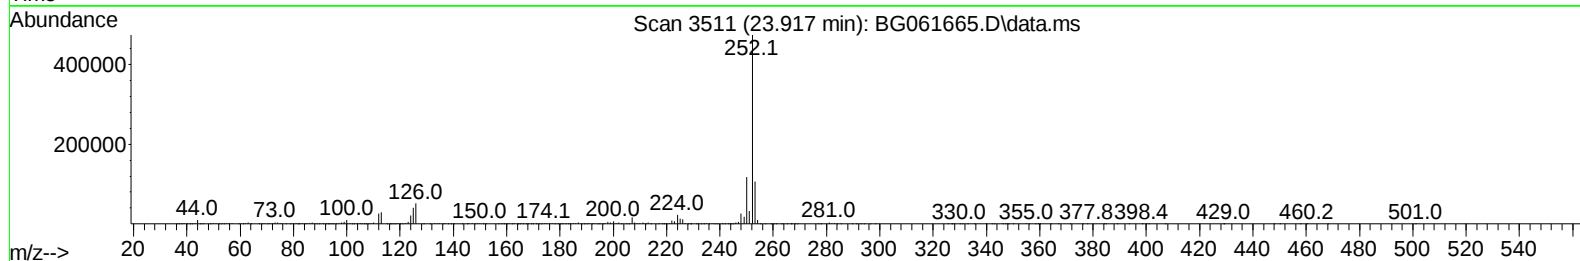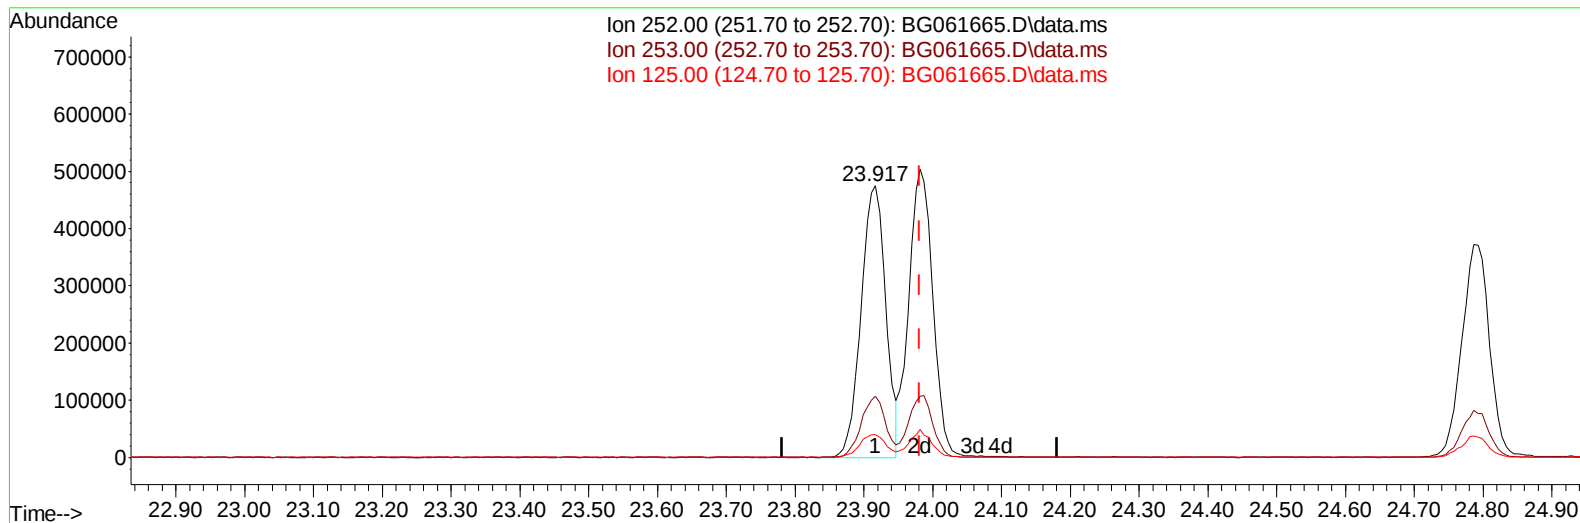

TIC: BG061665.D\data.ms

(91) Benzo(k)fluoranthene

23.917min (-0.065) 32.47 ng/u1

response 1183723

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.20	22.49
125.00	7.70	8.50
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061665.D
Acq On : 23 Jun 2024 2:02
Operator : MA/JU
Sample : PB161462BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

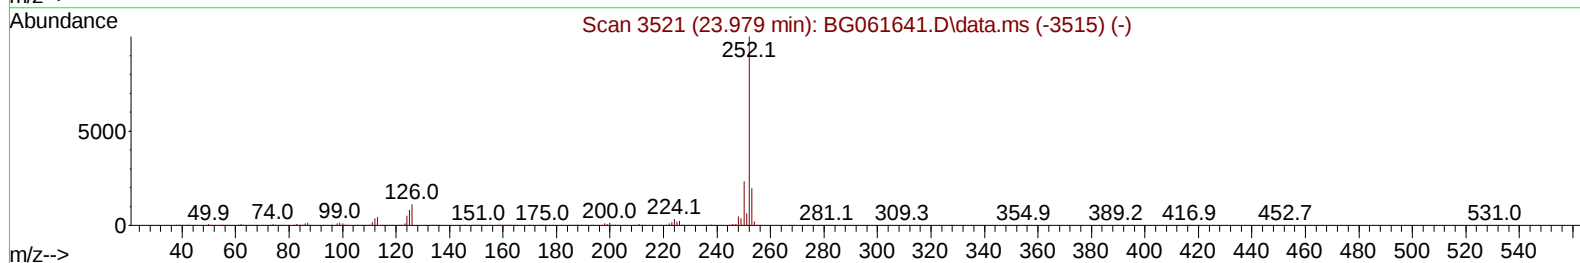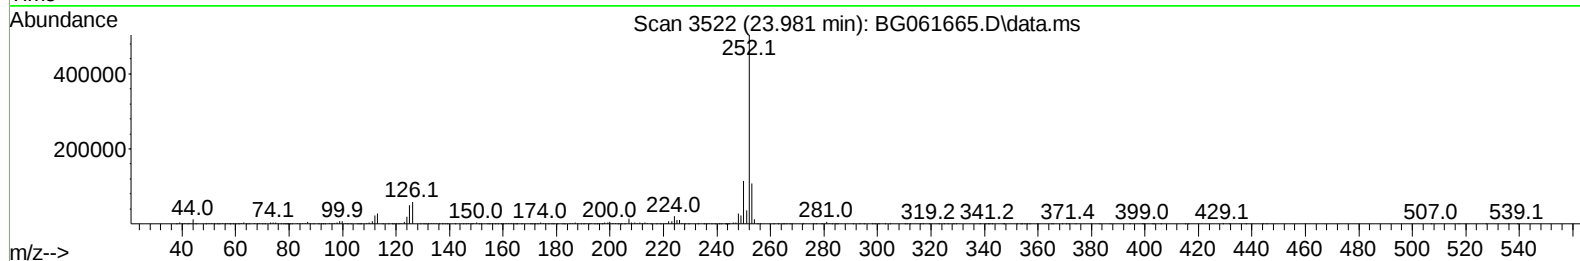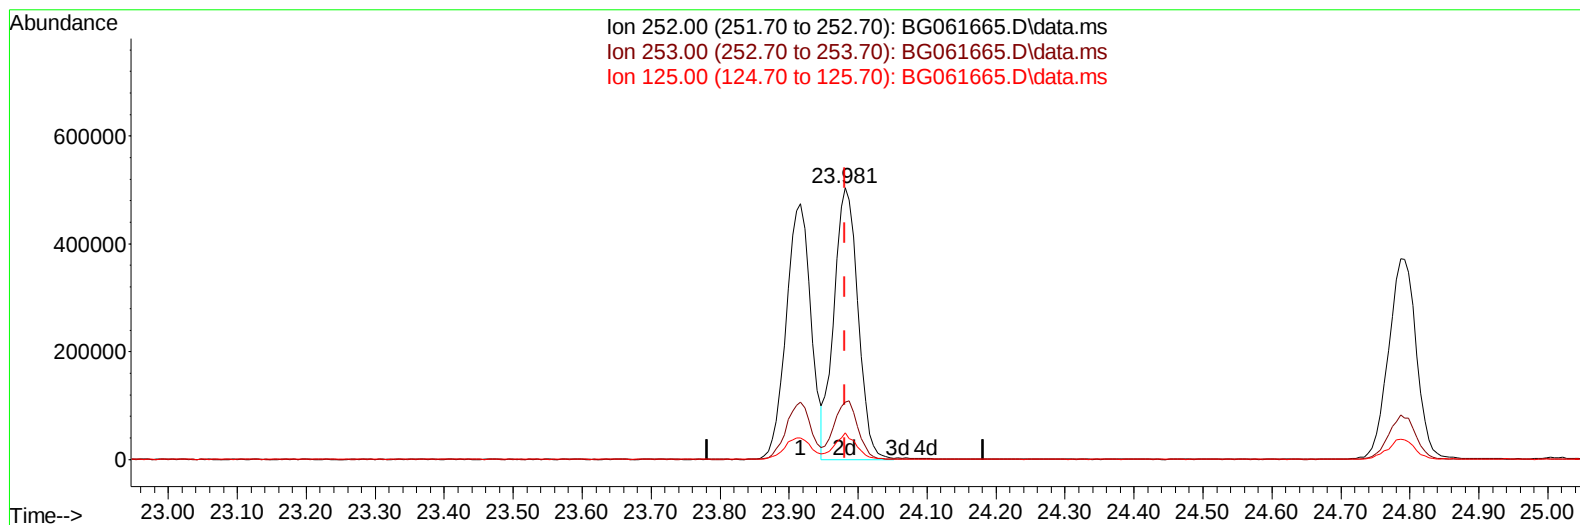

TIC: BG061665.D\data.ms

(91) Benzo(k)fluoranthene

23.981min (+ 0.000) 33.44 ng/ul m

response 1219201

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.20	21.22
125.00	7.70	9.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061665.D
 Acq On : 23 Jun 2024 2:02
 Operator : MA/JU
 Sample : PB161462BS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 05:03:55 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/24/2024

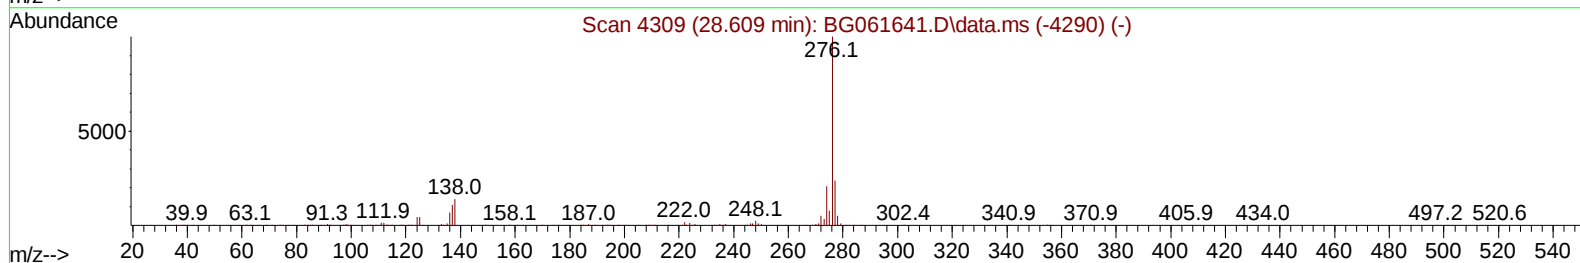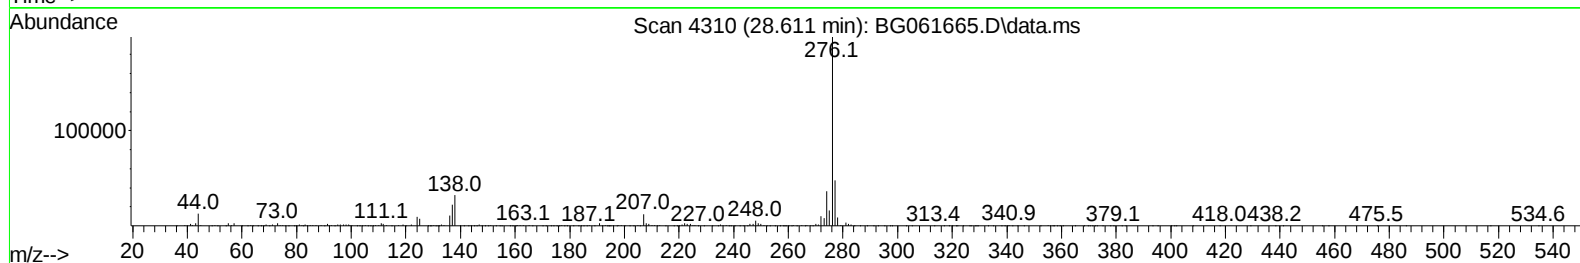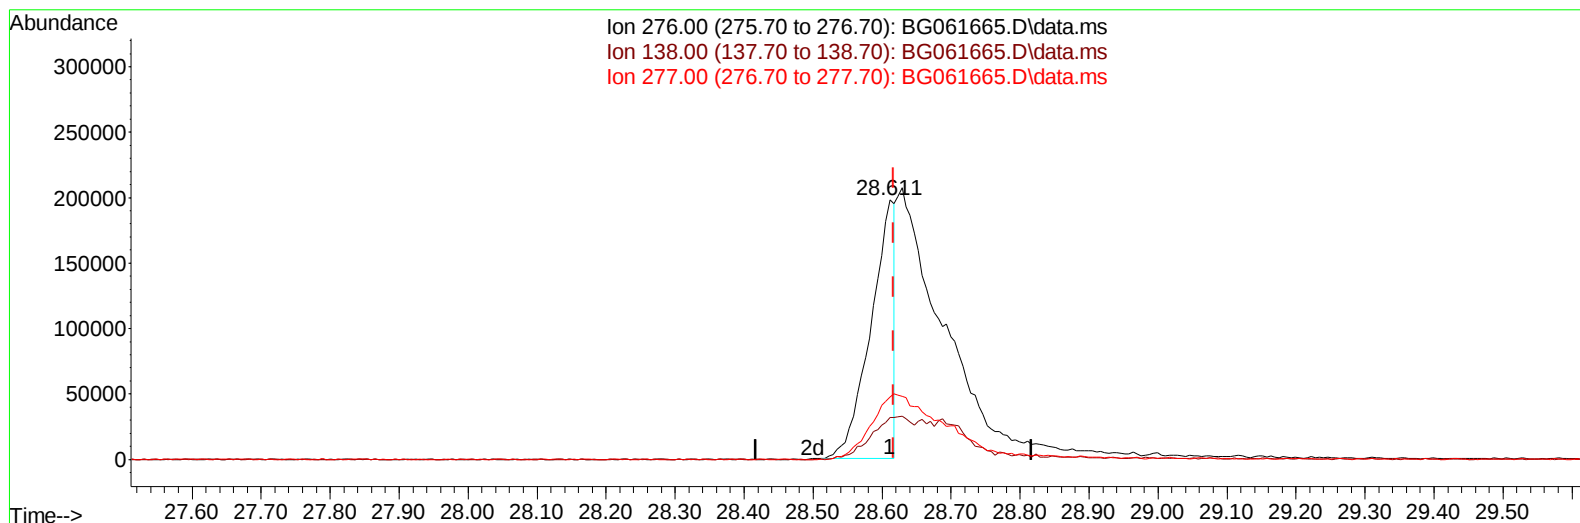

TIC: BG061665.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.611min (-0.006) 11.25 ng/u1

response 478196

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	15.30	16.30
277.00	24.60	24.15
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061665.D
Acq On : 23 Jun 2024 2:02
Operator : MA/JU
Sample : PB161462BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

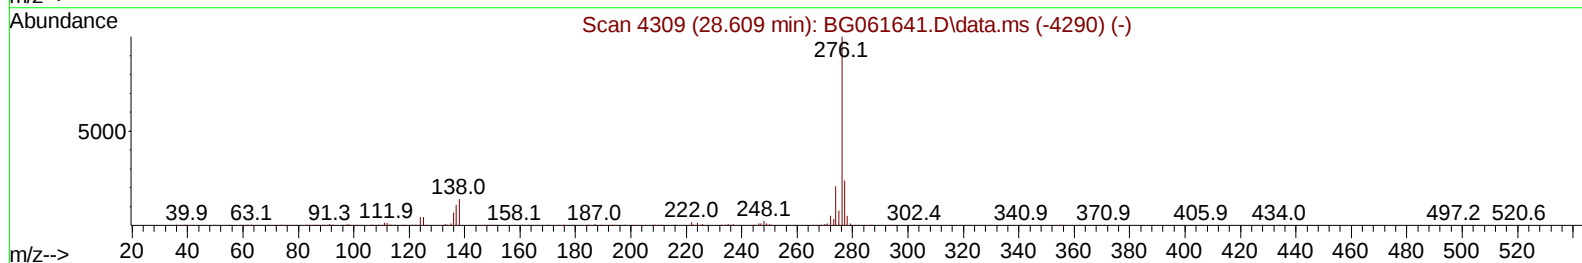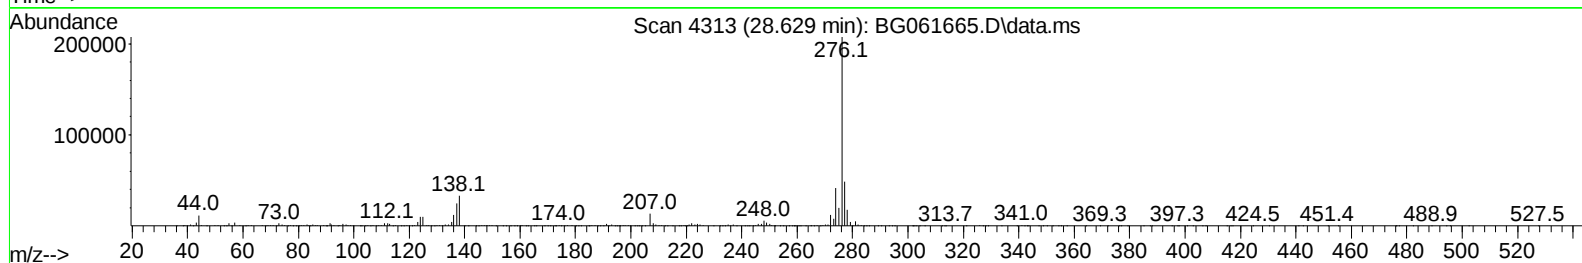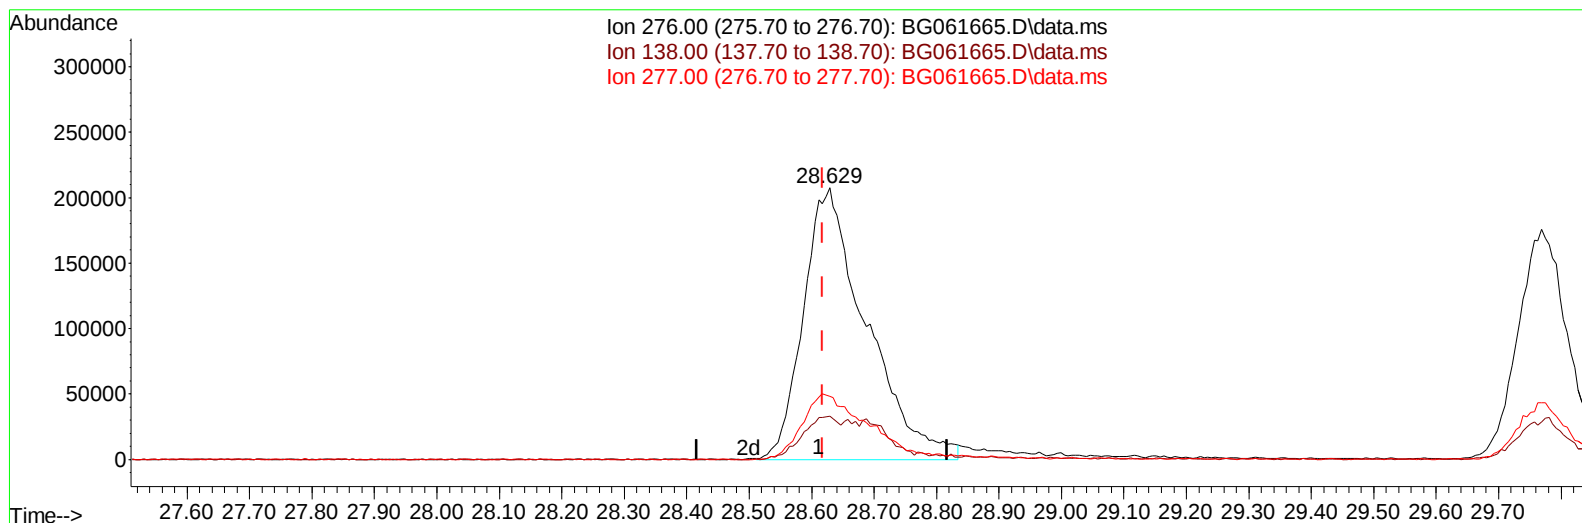

TIC: BG061665.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.629min (+ 0.012) 34.14 ng/ul m

response 1451984

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	15.30	16.04
277.00	24.60	23.29
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061665.D
Acq On : 23 Jun 2024 2:02
Operator : MA/JU
Sample : PB161462BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

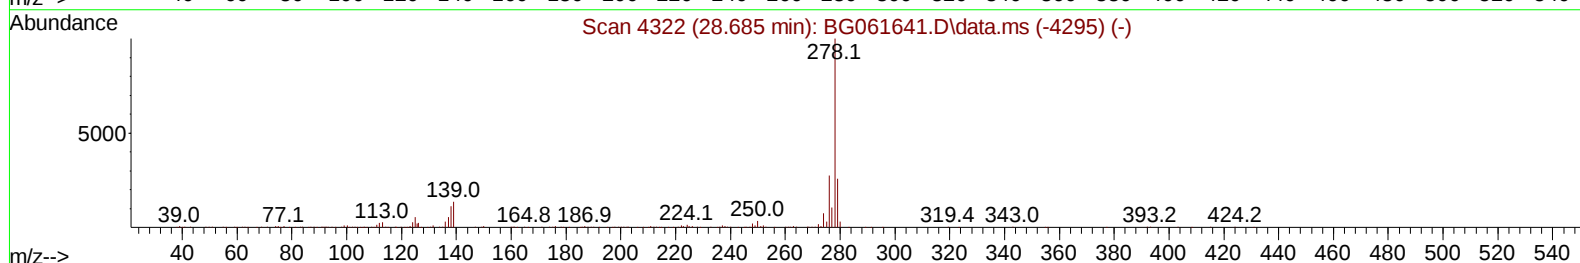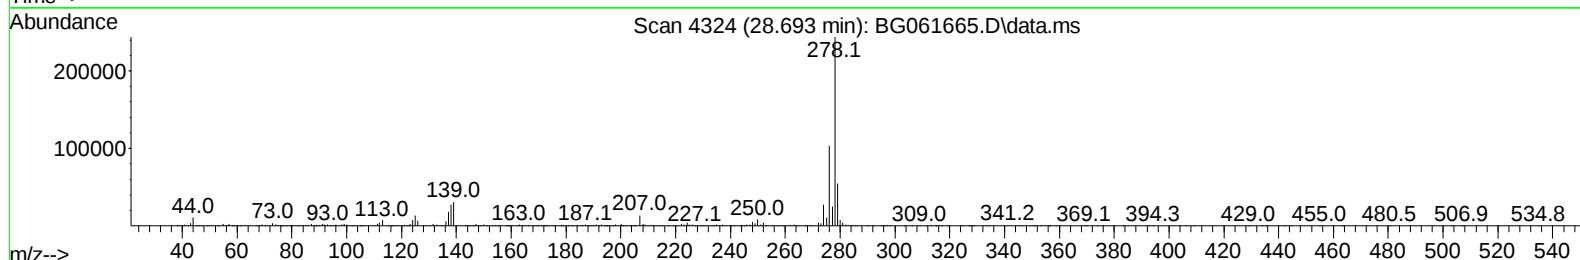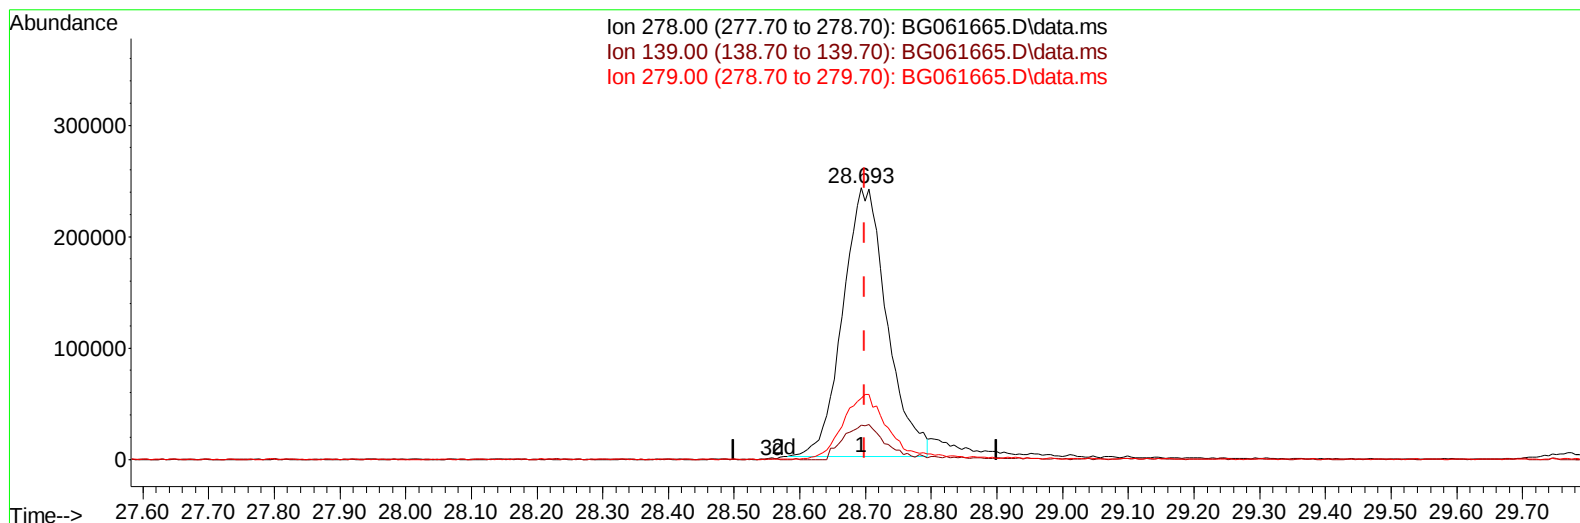

TIC: BG061665.D\data.ms

(95) Dibenzo(a,h)anthracene

28.693min (-0.006) 31.97 ng/u1

response 1130527

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	11.40	12.72
279.00	23.30	22.49
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061665.D
Acq On : 23 Jun 2024 2:02
Operator : MA/JU
Sample : PB161462BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

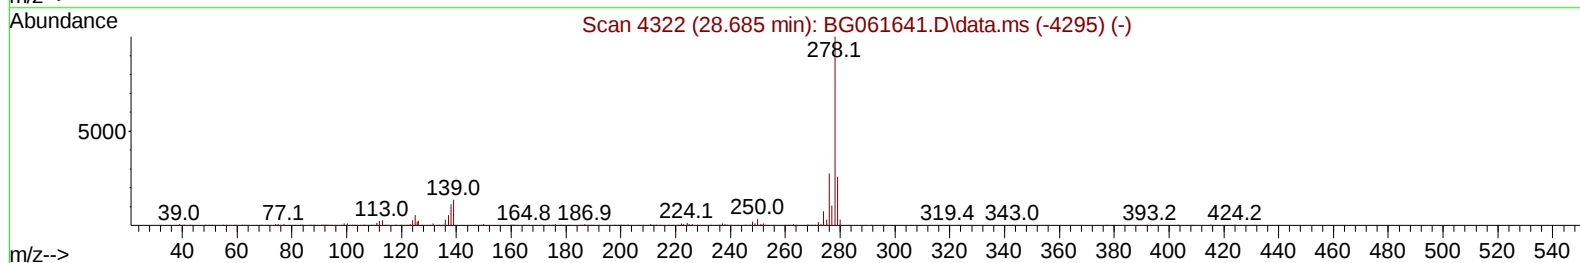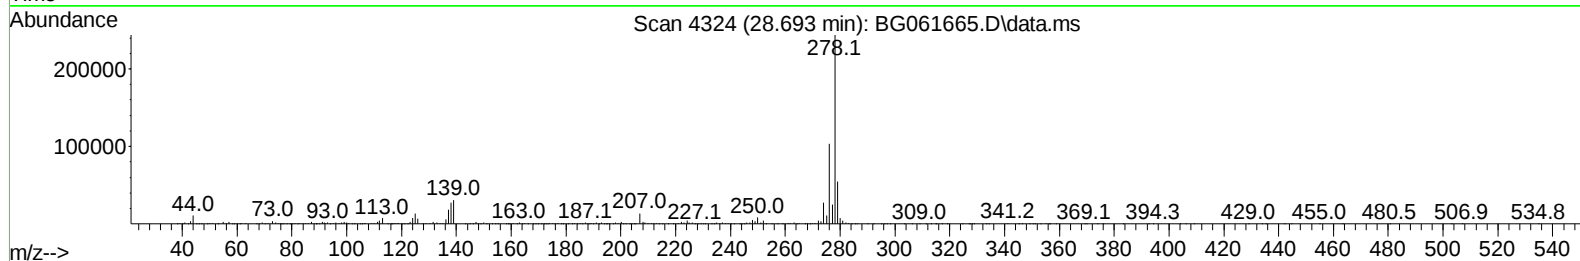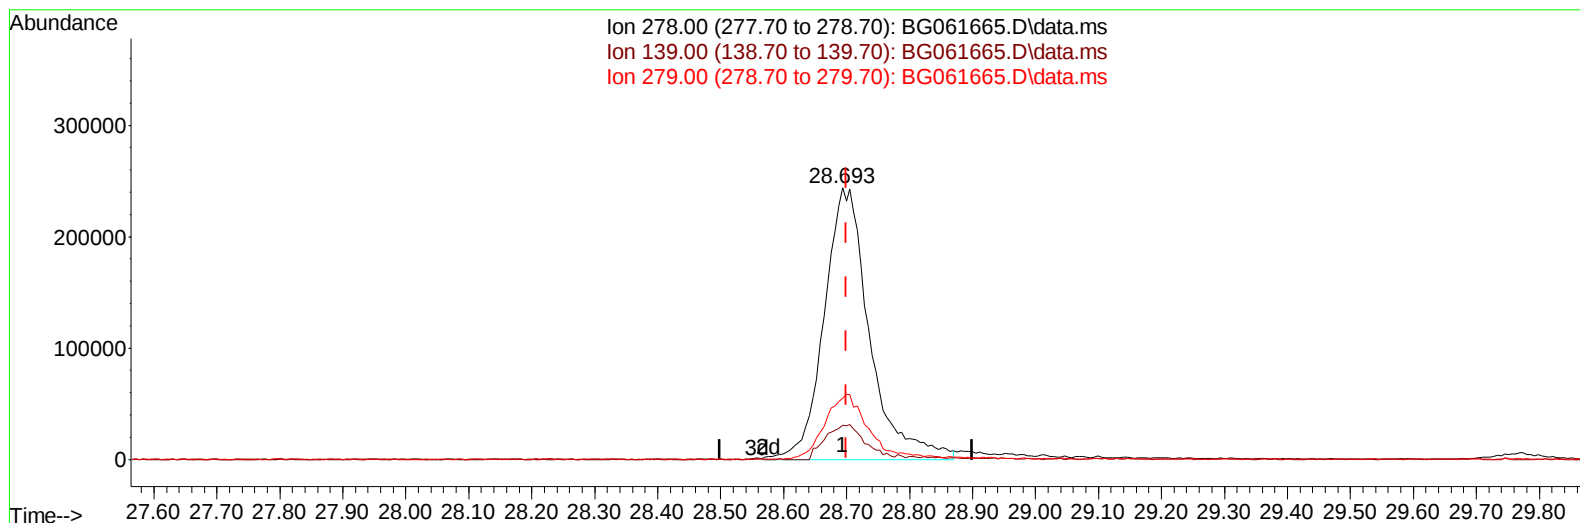

TIC: BG061665.D\data.ms

(95) Dibenzo(a,h)anthracene

28.693min (-0.006) 34.60 ng/u1 m

response 1223357

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	11.40	12.72
279.00	23.30	22.49
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061665.D
Acq On : 23 Jun 2024 2:02
Operator : MA/JU
Sample : PB161462BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

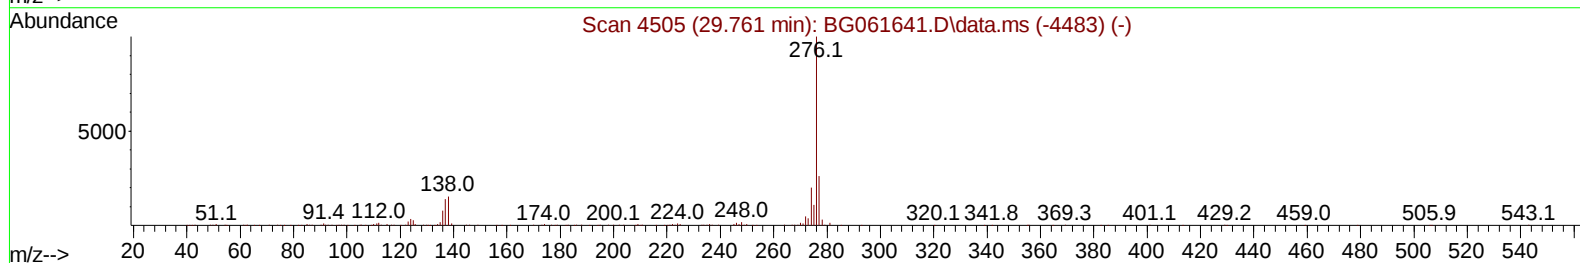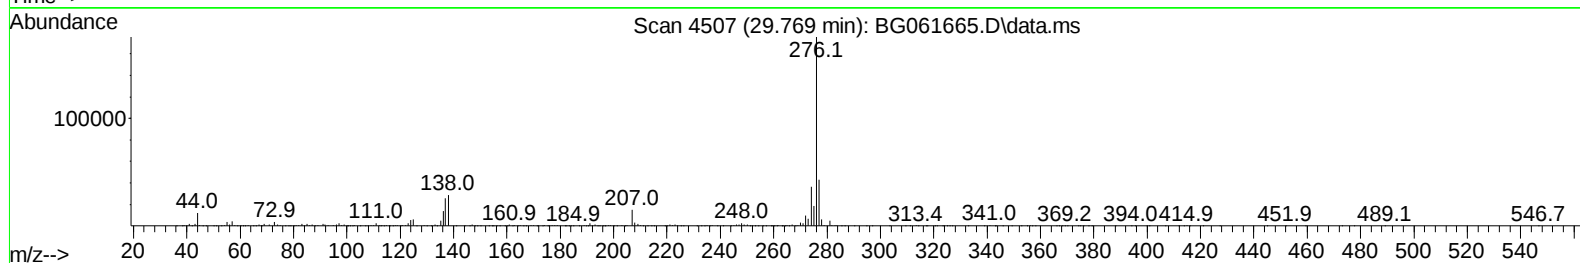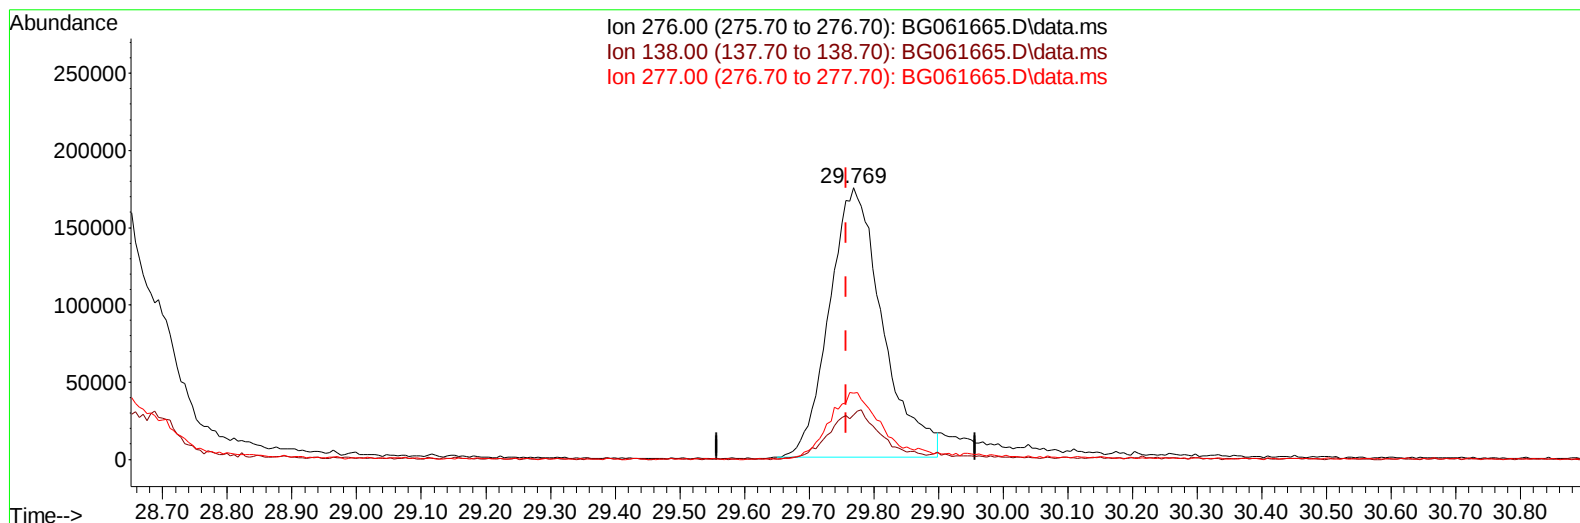

TIC: BG061665.D\data.ms

(96) Benzo(g,h,i)perylene

29.769min (+ 0.012) 29.06 ng/u1

response 996280

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	15.30	16.42
277.00	23.20	24.52
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061665.D
Acq On : 23 Jun 2024 2:02
Operator : MA/JU
Sample : PB161462BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:41:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 05:03:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/24/2024

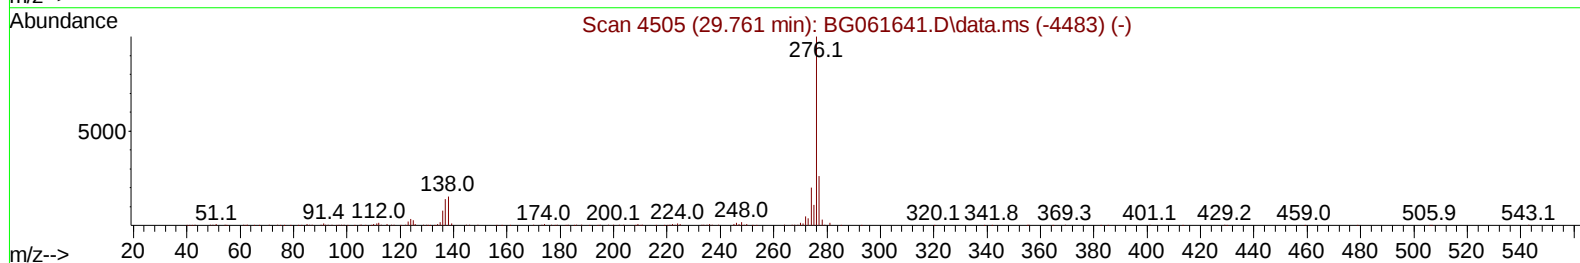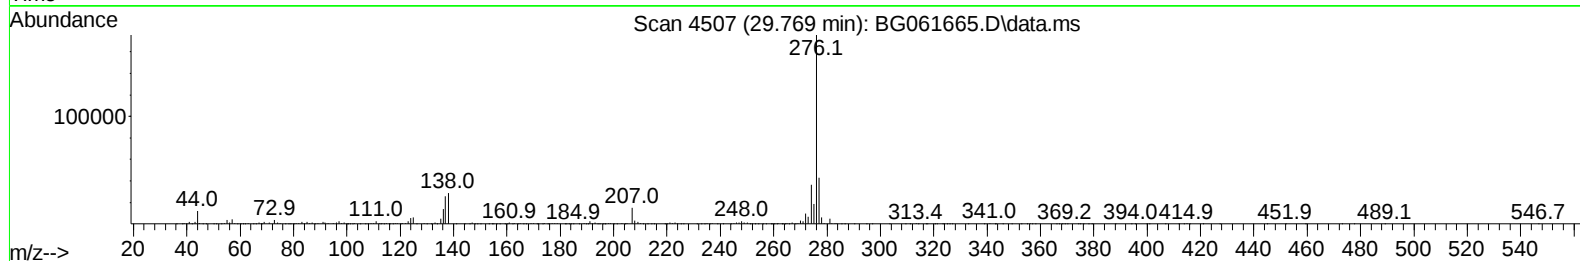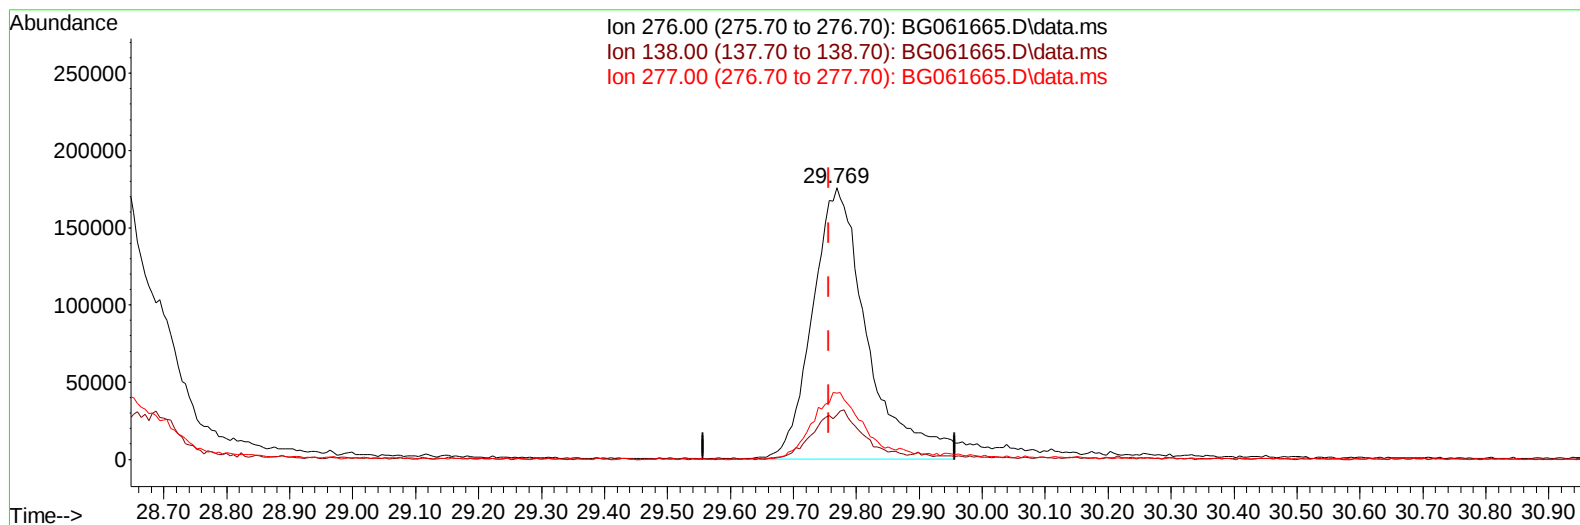

TIC: BG061665.D\data.ms

(96) Benzo(g,h,i)perylene

29.769min (+ 0.012) 30.97 ng/ul m

response 1061689

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	15.30	16.42
277.00	23.20	24.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061665.D
 Acq On : 23 Jun 2024 2:02
 Operator : MA/JU
 Sample : PB161462BS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:44:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 05:03:55 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/24/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.076	152	74688	20.000	ng/ul	0.00
20) Naphthalene-d8	10.891	136	381405	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.704	164	255272	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.448	188	563947	20.000	ng/ul	0.00
79) Chrysene-d12	21.713	240	495594	20.000	ng/ul	0.00
88) Perylene-d12	24.939	264	589670	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.464	96	11222	5.428	ng/uL	0.00
4) Pyridine-d5	3.887	84	155235	24.833	ng/ul	0.00
7) Phenol-d5	7.219	99	225901	27.861	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.401	67	132463	26.207	ng/ul	0.00
11) 2-Chlorophenol-d4	7.606	132	157407	28.290	ng/ul	0.00
15) 4-Methylphenol-d8	8.776	113	175560	28.009	ng/ul	0.01
21) Nitrobenzene-d5	9.246	128	77845	30.059	ng/ul	0.01
24) 2-Nitrophenol-d4	9.963	143	97299	37.096	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.503	165	180025	28.986	ng/ul	0.01
31) 4-Chloroaniline-d4	11.020	131	243613	25.908	ng/ul	0.00
46) Dimethylphthalate-d6	14.111	166	562413	28.630	ng/ul	0.00
49) Acenaphthylene-d8	14.398	160	662104	30.755	ng/ul	0.00
54) 4-Nitrophenol-d4	14.880	143	100943	29.920	ng/ul	0.01
60) Fluorene-d10	15.697	176	503558	29.281	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.803	200	85687	35.533	ng/ul	0.00
73) Anthracene-d10	17.548	188	766366	29.771	ng/ul	0.00
81) Pyrene-d10	19.822	212	840082	30.347	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.722	264	884668	31.412	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.505	88	24709	9.616	ng/uL#	81
5) Pyridine	3.911	79	162725	24.216	ng/ul	98
6) Benzaldehyde	7.213	77	90710	22.735	ng/ul	96
8) Phenol	7.248	94	273928	32.105	ng/ul	98
10) Bis(2-Chloroethyl)ether	7.495	93	186860	29.097	ng/ul#	96
12) 2-Chlorophenol	7.636	128	178322	31.945	ng/ul	89
13) 2-Methylphenol	8.511	108	191851	32.138	ng/ul	98
14) 2,2'-oxybis(1-Chloropr...	8.599	45	388525	29.612	ng/ul	96
16) Acetophenone	8.905	105	307149	29.759	ng/ul	90
17) N-Nitroso-di-n-propyla...	8.887	70	160915	29.023	ng/ul	98
18) 4-Methylphenol	8.840	108	212360	31.753	ng/ul	98
19) Hexachloroethane	9.163	117	72919	32.579	ng/ul#	88
22) Nitrobenzene	9.287	77	248544	33.315	ng/ul	96
23) Isophorone	9.810	82	491302	28.635	ng/ul	98
25) 2-Nitrophenol	9.998	139	106950	38.994	ng/ul#	75
26) 2,4-Dimethylphenol	10.051	107	214455	27.957	ng/ul	94
27) Bis(2-Chloroethoxy)met...	10.292	93	279916	28.840	ng/ul	96
29) 2,4-Dichlorophenol	10.527	162	192517	33.833	ng/ul	97
30) Naphthalene	10.944	128	653899	30.641	ng/ul	99
32) 4-Chloroaniline	11.044	127	235691	25.273	ng/ul	93
33) Hexachlorobutadiene	11.220	225	124897	31.776	ng/ul#	92
34) Caprolactam	11.813	113	59537m	25.303	ng/ul	
35) 4-Chloro-3-methylphenol	12.154	107	259009	32.550	ng/ul	96

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061665.D
 Acq On : 23 Jun 2024 2:02
 Operator : MA/JU
 Sample : PB161462BS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS462

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:44:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 05:03:55 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/24/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.542	142	467141	31.022	ng/ul	100
37) 1-Methylnaphthalene	12.759	142	485333	30.206	ng/ul	95
39) 1,2,4,5-Tetrachloroben...	12.900	216	256450	35.497	ng/ul	97
40) Hexachlorocyclopentadiene	12.877	237	72318	16.824	ng/ul#	92
41) 2,4,6-Trichlorophenol	13.135	196	169338	36.330	ng/ul	91
42) 2,4,5-Trichlorophenol	13.206	196	189582	37.316	ng/ul	91
43) 1,1'-Biphenyl	13.541	154	637497	34.475	ng/ul	98
44) 2-Chloronaphthalene	13.588	162	489503	34.463	ng/ul	98
45) 2-Nitroaniline	13.782	65	199538	41.037	ng/ul	98
47) Dimethylphthalate	14.158	163	592595	30.379	ng/ul	98
48) 2,6-Dinitrotoluene	14.275	165	130185	40.218	ng/ul#	87
50) Acenaphthylene	14.428	152	773243	32.176	ng/ul	97
51) 3-Nitroaniline	14.604	138	135850	40.981	ng/ul#	95
52) Acenaphthene	14.769	153	533181	32.037	ng/ul	98
53) 2,4-Dinitrophenol	14.804	184	61439	37.350	ng/ul#	87
55) 4-Nitrophenol	14.898	109	115661	33.198	ng/ul	98
56) Dibenzofuran	15.104	168	763350	32.777	ng/ul	89
57) 2,4-Dinitrotoluene	15.062	165	185633	38.634	ng/ul#	90
58) 2,3,4,6-Tetrachlorophenol	15.321	232	161741	32.468	ng/ul	97
59) Diethylphthalate	15.521	149	615837	30.653	ng/ul	96
61) Fluorene	15.750	166	612862	31.797	ng/ul	92
62) 4-Chlorophenyl-phenyle...	15.744	204	305961	31.977	ng/ul	97
63) 4-Nitroaniline	15.762	138	140563	40.025	ng/ul	94
66) 4,6-Dinitro-2-methylph...	15.820	198	97543	35.711	ng/ul#	87
67) N-Nitrosodiphenylamine	15.955	169	516479	35.415	ng/ul	93
68) 4-Bromophenyl-phenylether	16.637	248	207015	35.652	ng/ul	95
69) Hexachlorobenzene	16.743	284	240393	34.115	ng/ul	96
70) Atrazine	16.901	200	157533	27.044	ng/ul	94
71) Pentachlorophenol	17.084	266	145052m	33.792	ng/ul	
72) Phenanthrene	17.489	178	954977	32.188	ng/ul	99
74) Anthracene	17.583	178	964729	31.798	ng/ul	97
75) 1,2,3,4-Tetrachloroben...	13.505	216	269696	42.924	ng/uL	97
76) Pentachlorobenzene	15.015	250	254703	33.756	ng/uL	91
77) Carbazole	17.847	167	876302	34.017	ng/ul	99
78) Di-n-butylphthalate	18.411	149	1030326	33.441	ng/ul	100
80) Fluoranthene	19.493	202	1071814	33.369	ng/ul	99
82) Pyrene	19.851	202	1139937	33.377	ng/ul	98
83) Butylbenzylphthalate	20.744	149	460479	37.030	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.602	252	412738	39.387	ng/ul	98
85) Benzo(a)anthracene	21.690	228	1139513	32.756	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.614	149	660805	36.151	ng/ul	99
87) Chrysene	21.755	228	1077394	32.730	ng/ul	100
89) Di-n-octyl phthalate	22.842	149	1177975	37.876	ng/ul	100
90) Benzo(b)fluoranthene	23.917	252	1183723	33.394	ng/ul	99
91) Benzo(k)fluoranthene	23.981	252	1219201m	33.444	ng/ul	
93) Benzo(a)pyrene	24.786	252	1047338	30.691	ng/ul#	97
94) Indeno(1,2,3-cd)pyrene	28.629	276	1451984m	34.145	ng/ul	
95) Dibenzo(a,h)anthracene	28.693	278	1223357m	34.597	ng/ul	
96) Benzo(g,h,i)perylene	29.769	276	1061689m	30.972	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA_G

ClientSampleId :

SLCS462

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024

Supervised By :mohammad ahmed 06/24/2024

