

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061642.D
 Acq On : 22 Jun 2024 10:19
 Operator : MA/JU
 Sample : PB161446BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK446

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.467	25	30	35	rVB3	18643	27153	1.43%	0.132%
2	3.514	35	38	41	rBV4	2346	2850	0.15%	0.014%
3	3.649	60	61	66	rVB4	2918	3964	0.21%	0.019%
4	3.696	66	69	70	rBV2	3862	3959	0.21%	0.019%
5	3.884	97	101	117	rVV	270892	419881	22.09%	2.040%
6	4.225	156	159	163	rBV4	4037	6121	0.32%	0.030%
7	4.254	163	164	167	rVB2	4476	3668	0.19%	0.018%
8	4.295	167	171	172	rBV3	3726	4004	0.21%	0.019%
9	4.377	184	185	189	rVB3	2754	3220	0.17%	0.016%
10	4.413	189	191	194	rBV2	2907	3161	0.17%	0.015%
11	4.842	261	264	266	rBV	3316	3174	0.17%	0.015%
12	5.523	375	380	382	rBV2	2116	3211	0.17%	0.016%
13	5.917	445	447	450	rVB	3296	2563	0.13%	0.012%
14	5.976	454	457	459	rVB	3681	3129	0.16%	0.015%
15	6.839	603	604	608	rVB2	2724	2934	0.15%	0.014%
16	7.215	661	668	676	rVB	326294	555682	29.24%	2.700%
17	7.397	692	699	707	rBV	220697	353640	18.61%	1.718%
18	7.597	727	733	741	rBV	277713	477195	25.11%	2.319%
19	7.738	756	757	762	rVB3	2610	3294	0.17%	0.016%
20	7.779	762	764	768	rVV	2092	2840	0.15%	0.014%
21	7.844	770	775	777	rVB2	2700	4521	0.24%	0.022%
22	7.956	791	794	797	rVB	3018	3777	0.20%	0.018%
23	7.991	797	800	802	rBV	3367	3683	0.19%	0.018%
24	8.073	805	814	824	rBV	221842	386468	20.33%	1.878%
25	8.149	824	827	831	rBV2	3356	3578	0.19%	0.017%
26	8.261	841	846	848	rVB2	2582	2742	0.14%	0.013%
27	8.666	913	915	918	rBV2	3410	2587	0.14%	0.013%
28	8.766	925	932	940	rVB2	402044	664737	34.98%	3.230%
29	8.907	953	956	960	rVB2	2329	2570	0.14%	0.012%
30	9.242	1006	1013	1021	rVV	292654	512443	26.96%	2.490%
31	9.325	1025	1027	1030	rVB	3039	2815	0.15%	0.014%
32	9.377	1034	1036	1038	rBV	3265	3713	0.20%	0.018%
33	9.489	1048	1055	1057	rBV3	2016	3687	0.19%	0.018%
34	9.695	1087	1090	1092	rVB	3335	3250	0.17%	0.016%
35	9.959	1128	1135	1143	rBV2	239309	430088	22.63%	2.090%
36	10.159	1166	1169	1170	rBV2	3578	3429	0.18%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061642.D
 Acq On : 22 Jun 2024 10:19
 Operator : MA/JU
 Sample : PB161446BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK446

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	10.494	1218	1226	1236	rVB	387702	686240	36.11%	3.334%
38	10.588	1239	1242	1243	rVB	2591	2591	0.14%	0.013%
39	10.664	1251	1255	1256	rBV	2500	2897	0.15%	0.014%
40	10.887	1285	1293	1301	rVB	344605	616853	32.46%	2.997%
41	11.017	1308	1315	1325	rVB	406722	727364	38.27%	3.534%
42	11.293	1359	1362	1364	rBV2	3000	3232	0.17%	0.016%
43	11.587	1409	1412	1414	rBV2	2190	2898	0.15%	0.014%
44	11.657	1422	1424	1426	rVB	3457	2911	0.15%	0.014%
45	11.851	1455	1457	1460	rBV2	2427	2914	0.15%	0.014%
46	11.992	1479	1481	1484	rBV2	2489	2899	0.15%	0.014%
47	12.168	1509	1511	1516	rVV	3572	3957	0.21%	0.019%
48	12.403	1548	1551	1553	rBV2	2995	2803	0.15%	0.014%
49	12.462	1558	1561	1566	rVB3	8912	12660	0.67%	0.062%
50	12.674	1595	1597	1601	rBV2	3060	3667	0.19%	0.018%
51	13.167	1679	1681	1685	rBV	2859	2738	0.14%	0.013%
52	13.279	1697	1700	1702	rBV	2919	3177	0.17%	0.015%
53	13.743	1777	1779	1781	rBV	3039	2807	0.15%	0.014%
54	13.913	1806	1808	1811	rBV	2575	3030	0.16%	0.015%
55	14.043	1827	1830	1832	rVB2	4466	4284	0.23%	0.021%
56	14.107	1835	1841	1849	rVB	688313	994227	52.31%	4.831%
57	14.236	1861	1863	1864	rBV	2715	2646	0.14%	0.013%
58	14.401	1883	1891	1899	rBV2	753585	1221982	64.30%	5.937%
59	14.536	1910	1914	1915	rVB	3342	3845	0.20%	0.019%
60	14.548	1915	1916	1918	rBV	5515	3609	0.19%	0.018%
61	14.636	1929	1931	1933	rBV	2797	3084	0.16%	0.015%
62	14.701	1935	1942	1949	rVB	569013	909816	47.87%	4.421%
63	14.871	1964	1971	1978	rBV	390978	590390	31.06%	2.869%
64	15.071	2003	2005	2007	rVB	5158	4384	0.23%	0.021%
65	15.182	2022	2024	2027	rVB	2616	3008	0.16%	0.015%
66	15.259	2035	2037	2041	rVB2	3612	3296	0.17%	0.016%
67	15.300	2041	2044	2046	rBV2	3648	4471	0.24%	0.022%
68	15.359	2052	2054	2056	rVB2	5181	3517	0.19%	0.017%
69	15.382	2056	2058	2059	rBV	3441	3278	0.17%	0.016%
70	15.594	2093	2094	2099	rBV2	3748	4152	0.22%	0.020%
71	15.694	2104	2111	2118	rBV	1007993	1485376	78.16%	7.217%
72	15.793	2122	2128	2134	rBV	270865	389969	20.52%	1.895%
73	16.258	2206	2207	2210	rBV2	2642	2852	0.15%	0.014%
74	16.346	2219	2222	2224	rVB3	4129	3616	0.19%	0.018%
75	16.569	2258	2260	2262	rBV	3400	3168	0.17%	0.015%
76	16.710	2281	2284	2285	rBV2	2611	3130	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061642.D
 Acq On : 22 Jun 2024 10:19
 Operator : MA/JU
 Sample : PB161446BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK446

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

77	16.745	2288	2290	2292	rVV	4974	2678	0.14%	0.013%
78	17.057	2341	2343	2345	rVB	3495	2622	0.14%	0.013%
79	17.098	2349	2350	2352	rBV	4013	3063	0.16%	0.015%
80	17.227	2370	2372	2375	rBV3	3323	2883	0.15%	0.014%
81	17.286	2380	2382	2383	rVB2	5534	3004	0.16%	0.015%
82	17.315	2383	2387	2388	rBV2	2755	3248	0.17%	0.016%
83	17.444	2402	2409	2417	rVB	771562	1140008	59.98%	5.539%
84	17.544	2419	2426	2435	rVV	1094860	1632487	85.90%	7.932%
85	17.668	2445	2447	2449	rBV	4826	3955	0.21%	0.019%
86	18.126	2523	2525	2526	rBV	4197	2870	0.15%	0.014%
87	18.214	2538	2540	2543	rVB2	3323	2631	0.14%	0.013%
88	18.426	2574	2576	2579	rVB3	4178	4600	0.24%	0.022%
89	18.455	2579	2581	2582	rBV2	3860	3055	0.16%	0.015%
90	18.496	2585	2588	2589	rBV3	3851	4372	0.23%	0.021%
91	18.737	2627	2629	2632	rBV3	3975	4159	0.22%	0.020%
92	18.802	2638	2640	2642	rBV2	3595	3096	0.16%	0.015%
93	18.949	2664	2665	2669	rBV3	3938	3681	0.19%	0.018%
94	19.360	2733	2735	2736	rBV2	5153	3101	0.16%	0.015%
95	19.389	2737	2740	2744	rVB4	16191	20087	1.06%	0.098%
96	19.824	2808	2814	2821	rBV	1266410	1785246	93.94%	8.674%
97	20.035	2848	2850	2851	rBV2	8101	5982	0.31%	0.029%
98	21.704	3129	3134	3141	rVB2	692099	1137032	59.83%	5.525%
99	24.718	3637	3647	3657	rBV2	693600	1900510	100.00%	9.234%
100	24.936	3675	3684	3694	rVB2	460946	1253380	65.95%	6.090%




Sum of corrected areas: 20581219

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061642.D
Acq On : 22 Jun 2024 10:19
Operator : MA/JU
Sample : PB161446BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

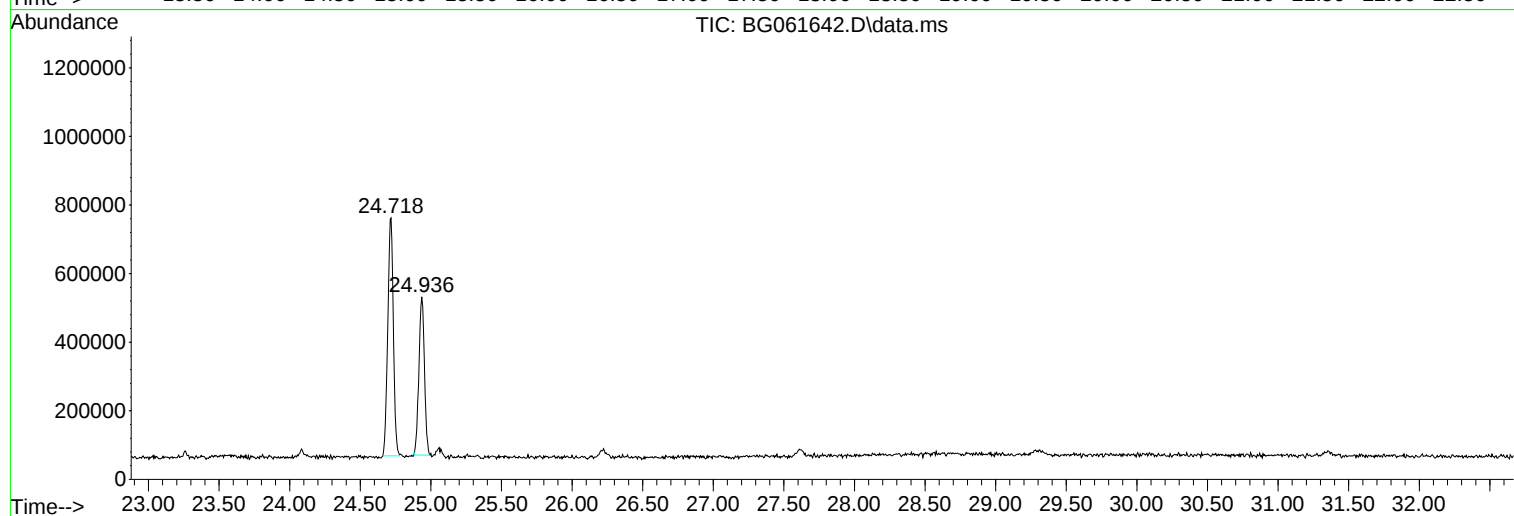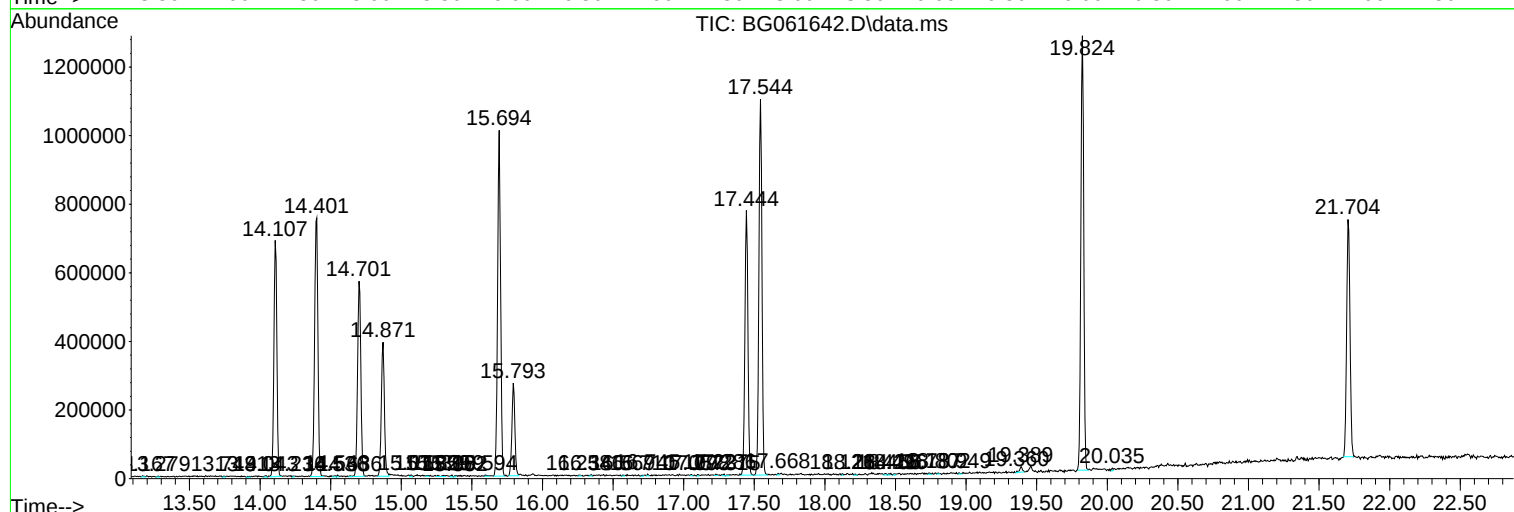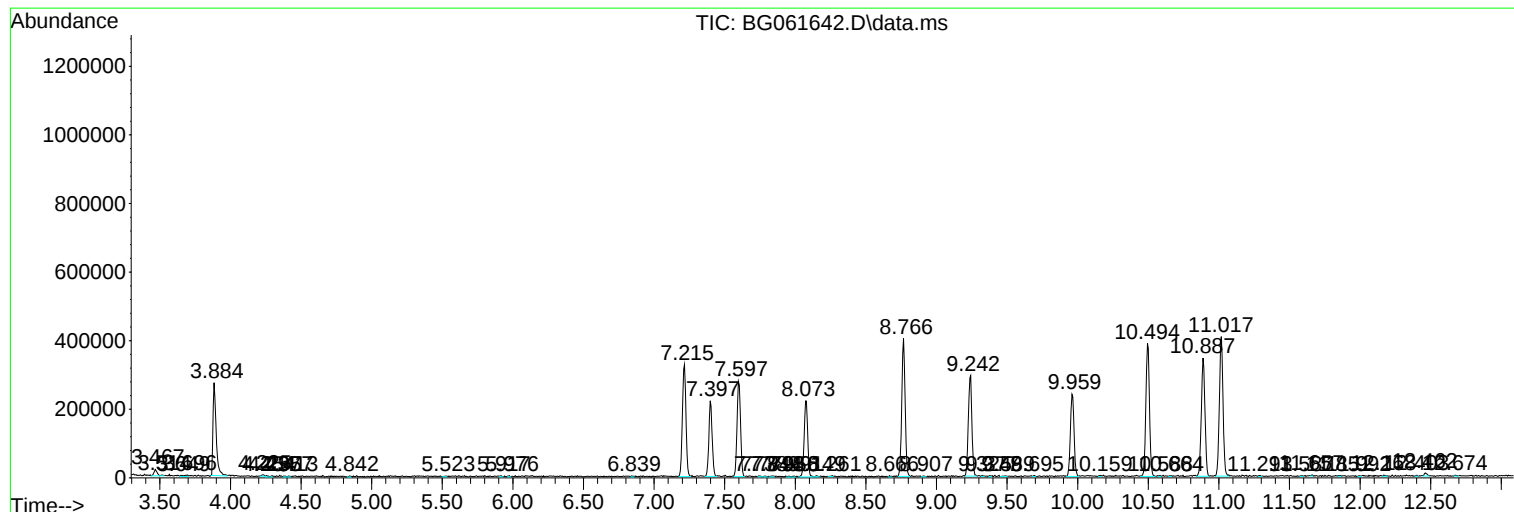

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061642.D
Acq On : 22 Jun 2024 10:19
Operator : MA/JU
Sample : PB161446BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061642.D
Acq On : 22 Jun 2024 10:19
Operator : MA/JU
Sample : PB161446BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------