

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061651.D
 Acq On : 22 Jun 2024 16:28
 Operator : MA/JU
 Sample : PB161462BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK462

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.467	26	30	35	rBV4	25102	39924	1.84%	0.165%
2	3.884	97	101	117	rBV	325894	533516	24.54%	2.206%
3	4.096	136	137	141	rVB2	3657	3344	0.15%	0.014%
4	4.231	157	160	164	rVB4	7394	9765	0.45%	0.040%
5	4.331	175	177	179	rBV3	5432	5422	0.25%	0.022%
6	4.460	196	199	200	rVB2	4139	3368	0.15%	0.014%
7	4.942	278	281	283	rBV3	3920	5205	0.24%	0.022%
8	4.989	286	289	291	rBV3	2070	3193	0.15%	0.013%
9	5.083	302	305	307	rVB2	2966	3158	0.15%	0.013%
10	5.242	331	332	337	rBV3	3026	4030	0.19%	0.017%
11	5.430	361	364	368	rBV5	2191	3226	0.15%	0.013%
12	5.577	387	389	392	rVB3	2913	3000	0.14%	0.012%
13	5.671	401	405	408	rBV6	2915	4918	0.23%	0.020%
14	5.823	429	431	435	rVB2	3621	3454	0.16%	0.014%
15	6.223	498	499	503	rVB4	4022	3218	0.15%	0.013%
16	6.334	514	518	521	rBV4	3544	4301	0.20%	0.018%
17	6.434	532	535	537	rVB3	3178	3694	0.17%	0.015%
18	6.511	545	548	551	rBV3	2991	3757	0.17%	0.016%
19	6.758	585	590	593	rBV3	3424	5473	0.25%	0.023%
20	6.852	603	606	607	rBV2	3118	3159	0.15%	0.013%
21	6.957	621	624	626	rBV3	2574	2972	0.14%	0.012%
22	7.216	661	668	677	rBV	394228	665469	30.61%	2.751%
23	7.398	692	699	706	rBV	265179	436665	20.09%	1.805%
24	7.598	726	733	740	rBV	348555	593095	27.28%	2.452%
25	7.827	767	772	774	rVB4	3823	3233	0.15%	0.013%
26	8.074	808	814	822	rBV	257055	434905	20.01%	1.798%
27	8.191	831	834	836	rVB2	3122	2888	0.13%	0.012%
28	8.250	841	844	845	rBV	3258	3038	0.14%	0.013%
29	8.315	851	855	857	rBV	2197	3242	0.15%	0.013%
30	8.362	860	863	866	rBV3	2914	3995	0.18%	0.017%
31	8.685	916	918	921	rVB	3846	3490	0.16%	0.014%
32	8.720	921	924	925	rBV2	3923	4598	0.21%	0.019%
33	8.767	925	932	942	rVB	473275	813831	37.44%	3.365%
34	8.884	950	952	955	rBV	2777	3909	0.18%	0.016%
35	8.949	961	963	968	rVB3	1759	3018	0.14%	0.012%
36	9.161	996	999	1002	rBV2	3502	3494	0.16%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061651.D
 Acq On : 22 Jun 2024 16:28
 Operator : MA/JU
 Sample : PB161462BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK462

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	9.237	1002	1012	1022	rVV	364899	637877	29.34%	2.637%
38	9.302	1022	1023	1028	rVB3	3862	4938	0.23%	0.020%
39	9.507	1055	1058	1060	rVB	4282	4942	0.23%	0.020%
40	9.537	1060	1063	1065	rBV	2845	3994	0.18%	0.017%
41	9.731	1092	1096	1098	rBV3	4125	4957	0.23%	0.020%
42	9.778	1101	1104	1106	rBV2	2787	2862	0.13%	0.012%
43	9.960	1128	1135	1144	rBV	302184	535569	24.64%	2.214%
44	10.148	1164	1167	1168	rBV	2900	3186	0.15%	0.013%
45	10.494	1219	1226	1236	rVB	457034	833068	38.32%	3.444%
46	10.888	1285	1293	1302	rBV	407184	712870	32.79%	2.947%
47	10.947	1302	1303	1306	rVB2	3853	3180	0.15%	0.013%
48	11.017	1306	1315	1325	rBV	494842	885993	40.76%	3.663%
49	11.123	1331	1333	1335	rBV	3049	2830	0.13%	0.012%
50	11.147	1335	1337	1342	rVB2	3235	4885	0.22%	0.020%
51	11.540	1401	1404	1407	rBV3	2195	3407	0.16%	0.014%
52	11.799	1446	1448	1450	rBV2	3869	3014	0.14%	0.012%
53	11.910	1464	1467	1470	rBV	2632	3030	0.14%	0.013%
54	11.969	1475	1477	1482	rBV4	3578	6163	0.28%	0.025%
55	12.010	1482	1484	1486	rVB2	4065	3070	0.14%	0.013%
56	12.451	1557	1559	1561	rBV2	7380	8504	0.39%	0.035%
57	12.686	1597	1599	1602	rBV	3137	4363	0.20%	0.018%
58	12.839	1623	1625	1628	rVB2	3128	3692	0.17%	0.015%
59	12.897	1632	1635	1637	rBV	3882	4095	0.19%	0.017%
60	13.221	1688	1690	1693	rBV4	2985	4084	0.19%	0.017%
61	13.273	1696	1699	1700	rBV2	2733	3342	0.15%	0.014%
62	13.315	1703	1706	1707	rBV2	3893	3387	0.16%	0.014%
63	13.367	1711	1715	1718	rBV	3628	5544	0.26%	0.023%
64	13.679	1765	1768	1770	rBV3	3057	3100	0.14%	0.013%
65	14.108	1834	1841	1848	rBV	852315	1204416	55.40%	4.980%
66	14.396	1883	1890	1898	rBV	935874	1463786	67.33%	6.052%
67	14.701	1936	1942	1949	rBV	654015	1025645	47.18%	4.240%
68	14.772	1951	1954	1957	rVB2	5180	5007	0.23%	0.021%
69	14.872	1965	1971	1981	rBV	462213	717851	33.02%	2.968%
70	14.936	1981	1982	1987	rVB4	4603	5584	0.26%	0.023%
71	15.083	2004	2007	2008	rBV	3369	2897	0.13%	0.012%
72	15.177	2021	2023	2024	rBV2	3201	2929	0.13%	0.012%
73	15.383	2056	2058	2061	rVB	3827	3933	0.18%	0.016%
74	15.483	2073	2075	2077	rBV	4009	4040	0.19%	0.017%
75	15.524	2081	2082	2084	rBV	4139	3398	0.16%	0.014%
76	15.694	2104	2111	2121	rVB	1172797	1788708	82.28%	7.395%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
 Data File : BG061651.D
 Acq On : 22 Jun 2024 16:28
 Operator : MA/JU
 Sample : PB161462BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK462

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

77	15.794	2122	2128	2138	rVV2	330590	487555	22.43%	2.016%
78	15.929	2149	2151	2153	rVB2	7062	4635	0.21%	0.019%
79	16.164	2187	2191	2192	rBV4	2963	3839	0.18%	0.016%
80	16.564	2256	2259	2261	rBV3	5689	6014	0.28%	0.025%
81	16.664	2273	2276	2277	rBV3	3992	3704	0.17%	0.015%
82	16.781	2294	2296	2299	rBV3	2776	3109	0.14%	0.013%
83	16.863	2308	2310	2313	rBV2	2798	3320	0.15%	0.014%
84	16.963	2324	2327	2328	rVB	3688	3126	0.14%	0.013%
85	16.987	2328	2331	2332	rBV2	4302	5395	0.25%	0.022%
86	17.198	2363	2367	2368	rBV3	3652	4671	0.21%	0.019%
87	17.310	2384	2386	2389	rVB2	2900	2953	0.14%	0.012%
88	17.392	2397	2400	2402	rBV2	4047	5554	0.26%	0.023%
89	17.445	2403	2409	2416	rVV	834541	1255754	57.76%	5.192%
90	17.545	2419	2426	2433	rVB2	1237712	1925459	88.57%	7.961%
91	17.651	2442	2444	2445	rBV	5390	3259	0.15%	0.013%
92	17.674	2445	2448	2454	rVB6	16317	28525	1.31%	0.118%
93	18.021	2505	2507	2508	rBV	3845	3201	0.15%	0.013%
94	18.326	2556	2559	2563	rBV4	9133	11811	0.54%	0.049%
95	19.825	2808	2814	2822	rVB	1452254	2078351	95.60%	8.593%
96	21.705	3128	3134	3143	rVB2	762908	1253212	57.65%	5.181%
97	24.713	3638	3646	3658	rVB	791342	2173941	100.00%	8.988%
98	24.936	3676	3684	3695	rVB2	481867	1360939	62.60%	5.627%




Sum of corrected areas: 24187434

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061651.D
Acq On : 22 Jun 2024 16:28
Operator : MA/JU
Sample : PB161462BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

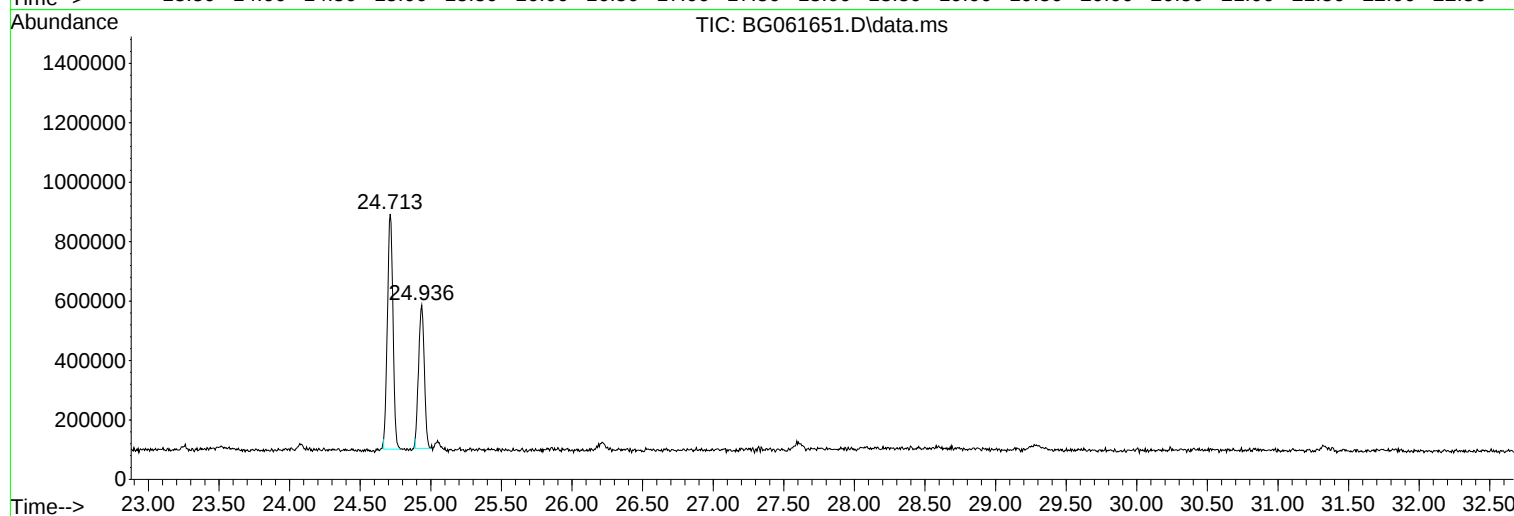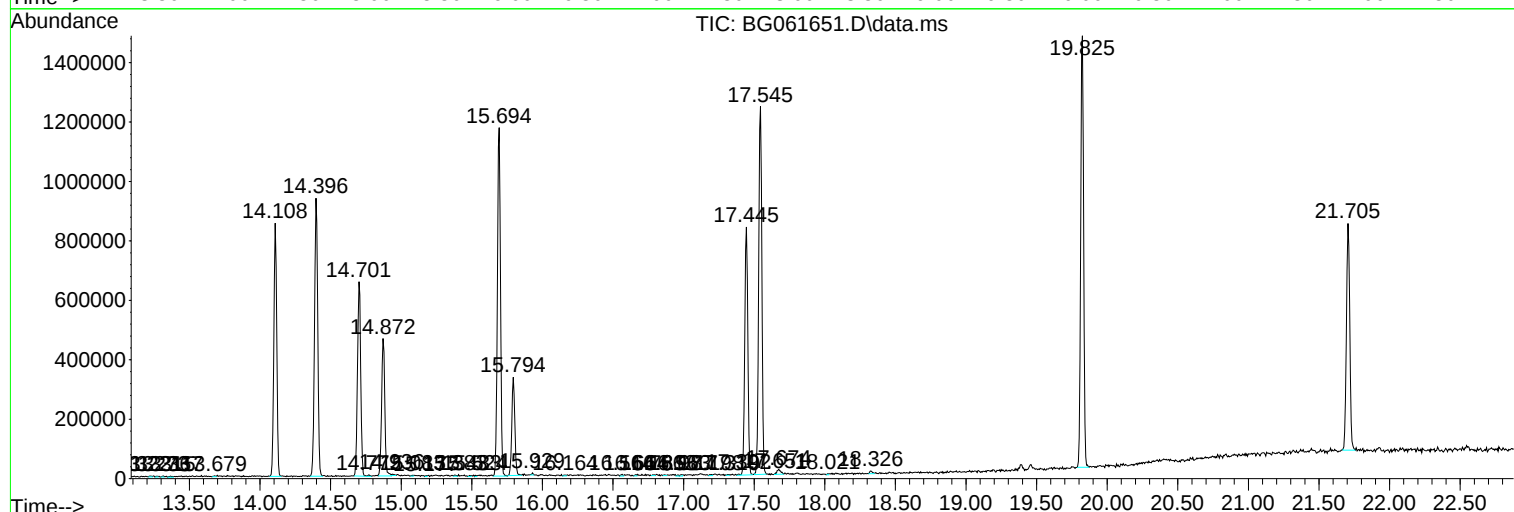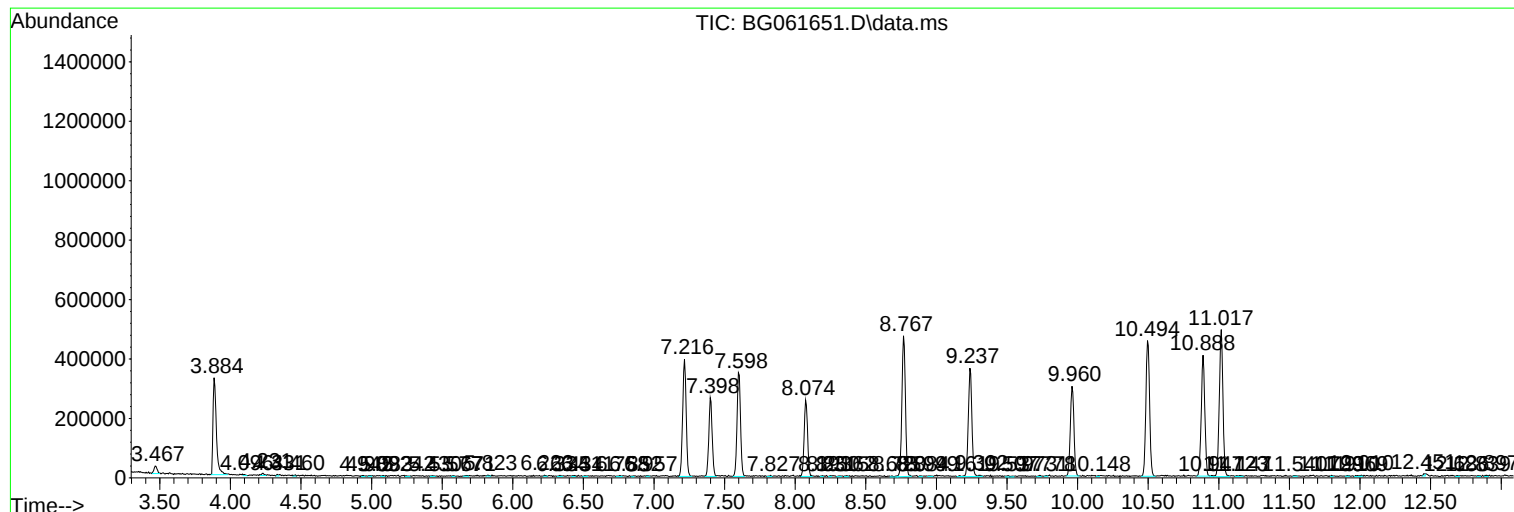

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061651.D
Acq On : 22 Jun 2024 16:28
Operator : MA/JU
Sample : PB161462BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062224\
Data File : BG061651.D
Acq On : 22 Jun 2024 16:28
Operator : MA/JU
Sample : PB161462BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------