


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062315\
 Data File : BG017756.D
 Acq On : 23 Jun 2015 10:25
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 06:05:07 2015

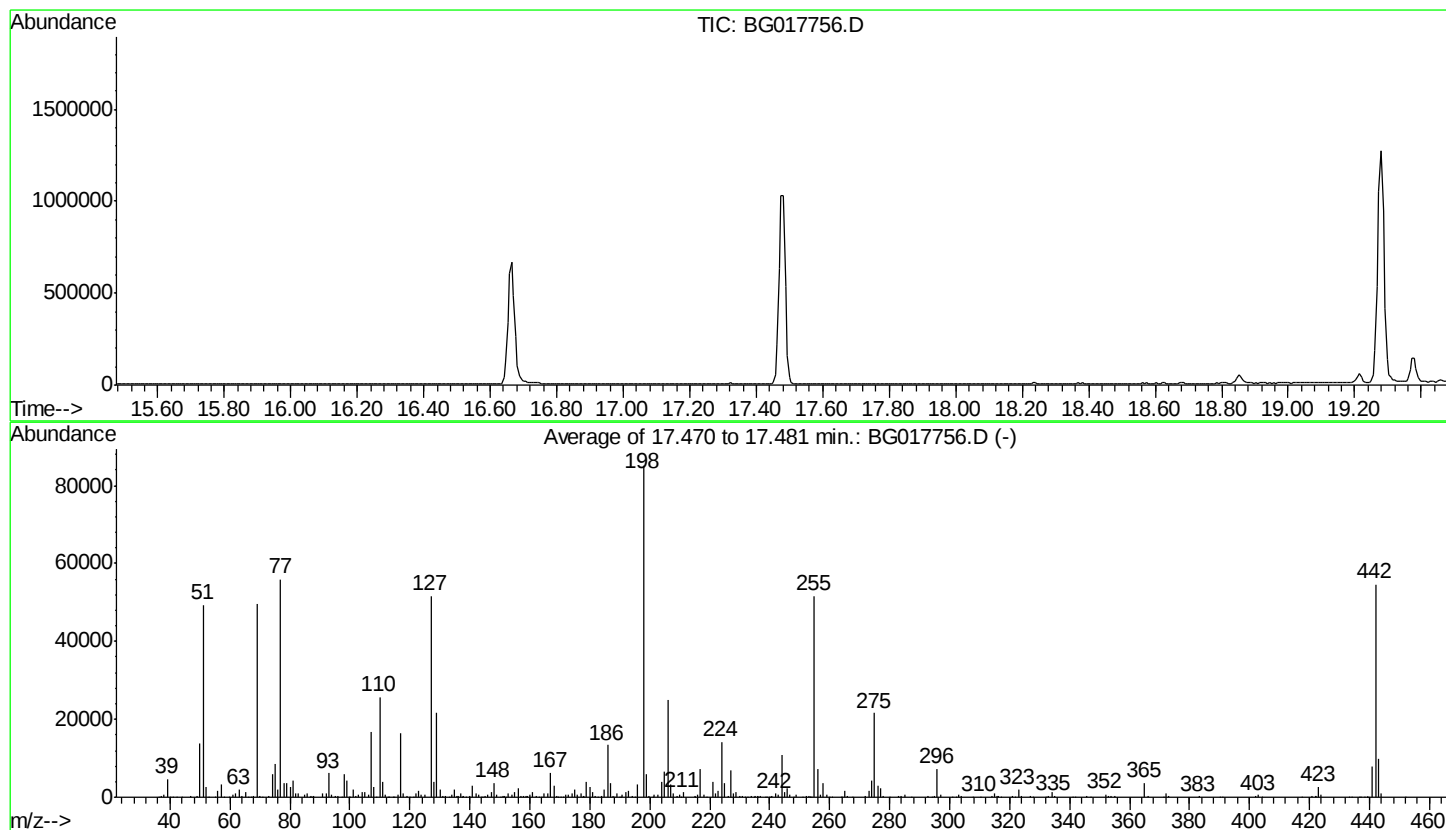

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.0	49359	PASS
68	69	0.00	2	0.9	472	PASS
69	198	0.00	100	58.4	49754	PASS
70	69	0.00	2	0.5	233	PASS
127	198	10	80	60.6	51610	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85128	PASS
199	198	5	9	7.1	6037	PASS
275	198	10	60	25.4	21628	PASS
365	198	1	100	4.4	3740	PASS
441	442	0.01	24	14.3	7779	PASS
442	198	50	100	64.1	54562	PASS
443	442	15	24	18.2	9912	PASS