

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062316\
 Data File : BG022510.D
 Acq On : 23 Jun 2016 8:29
 Operator : UM/SJ
 Sample : H3623-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 23 13:30:15 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 22 01:27:56 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.96	152	26074	20.00	ng	-0.03
21) Naphthalene-d8	10.79	136	140017	20.00	ng	-0.02
38) Acenaphthene-d10	14.62	164	85424	20.00	ng	-0.01
63) Phenanthrene-d10	17.36	188	187706	20.00	ng	-0.02
75) Chrysene-d12	21.62	240	118141	20.00	ng	-0.03
86) Perylene-d12	24.81	264	68909	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	261089	193.60	ng	-0.03
7) Phenol-d6	7.15	99	346571	163.45	ng	-0.03
23) Nitrobenzene-d5	9.14	82	222597	110.84	ng	-0.02
41) 2,4,6-Tribromophenol	16.11	330	132298	137.06	ng	-0.02
44) 2-Fluorobiphenyl	13.24	172	621917	110.95	ng	-0.01
78) Terphenyl-d14	19.96	244	671895	135.02	ng	-0.01
Target Compounds						
15) Benzyl Alcohol	8.28	79	2809	2.05	ng	Qvalue # 40

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062316\
Data File : BG022510.D
Acq On : 23 Jun 2016 8:29
Operator : UM/SJ
Sample : H3623-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 23 13:30:15 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:27:56 2016
Response via : Initial Calibration

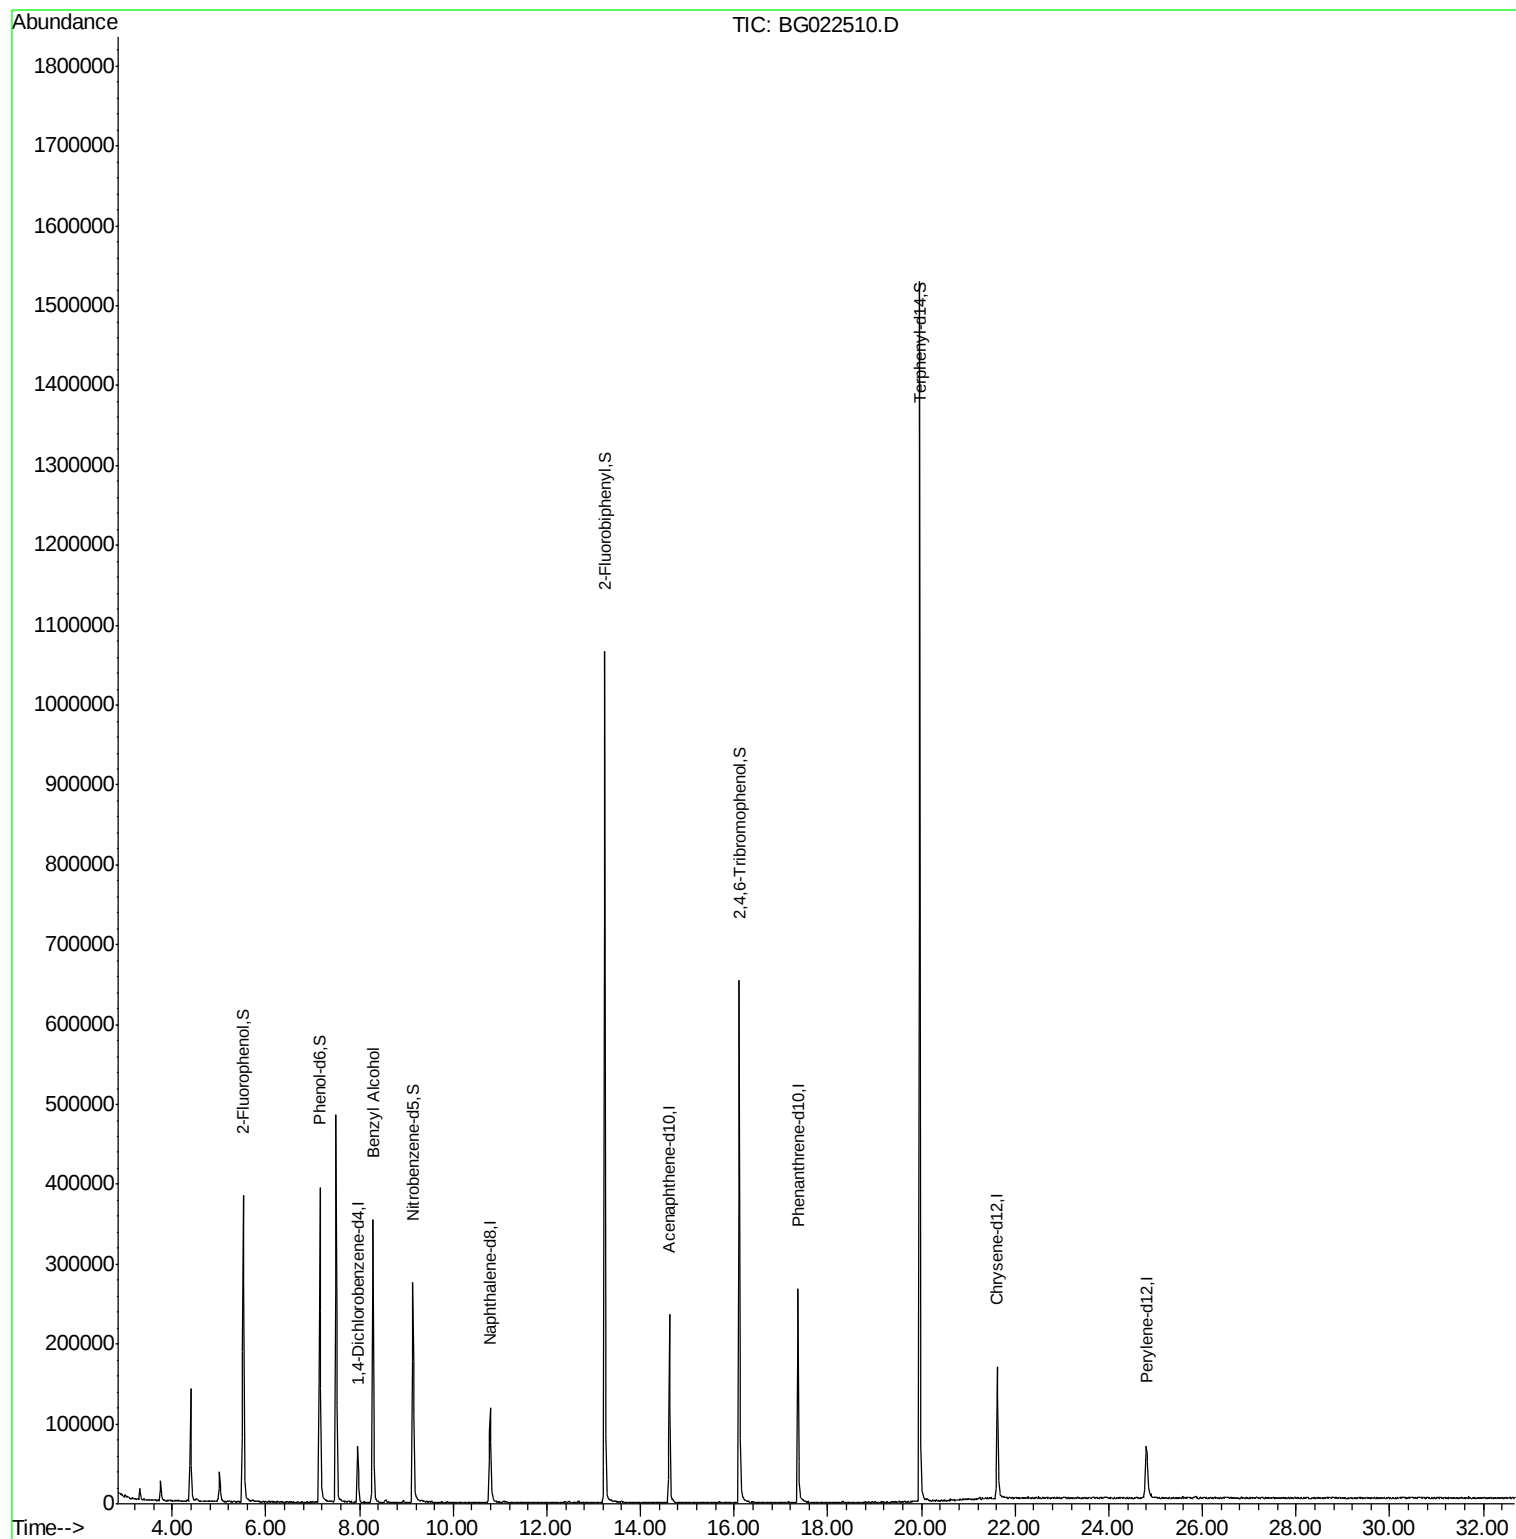




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.96 min Scan# 872
Delta R.T. -0.03 min
Lab File: BG022510.D
Acq: 23 Jun 2016 8:29

Instrument :
BNA_G
ClientSampled :

Tot Ion:152 Resp: 26074
Ion Ratio Lower Upper
152 100
150 145.5 130.1 195.1
115 57.9 62.2 93.2#

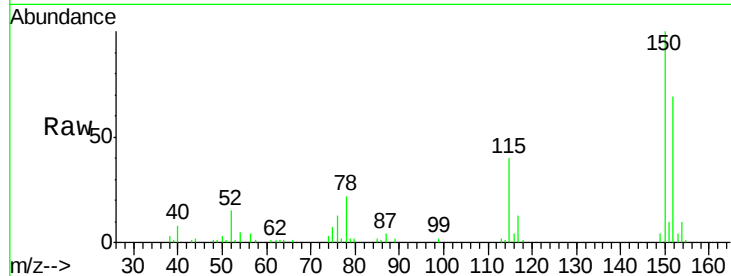


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

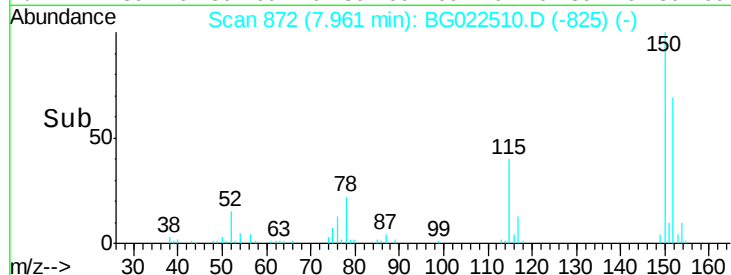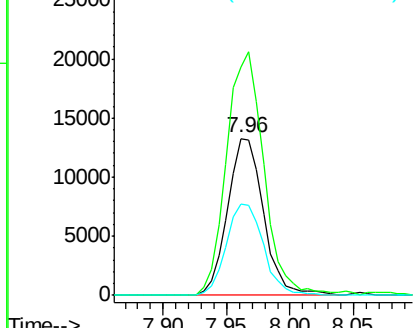



#5

2-Fluorophenol
Concen: 193.60 ng
RT: 5.51 min Scan# 455
Delta R.T. -0.03 min
Lab File: BG022510.D
Acq: 23 Jun 2016 8:29

Tgt Ion:112 Resp: 261089
Ion Ratio Lower Upper
112 100
64 48.1 51.1 76.7#
63 22.6 24.6 37.0#

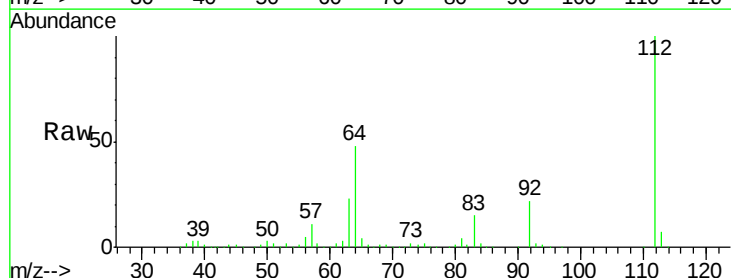

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

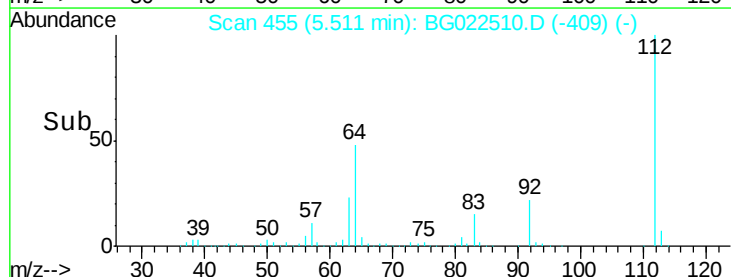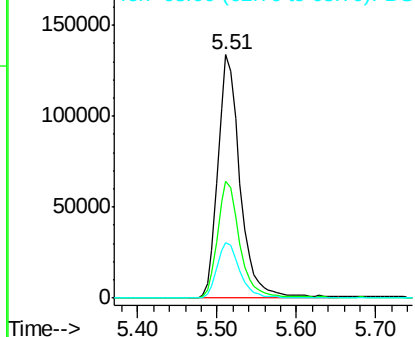



#7

Phenol-d6

Concen: 163.45 ng

RT: 7.15 min Scan# 734

Delta R.T. -0.03 min

Lab File: BG022510.D

Acq: 23 Jun 2016 8:29

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 346571

Ion Ratio Lower Upper




99 100

42 9.6 16.4 24.6#

71 23.3 25.0 37.4#

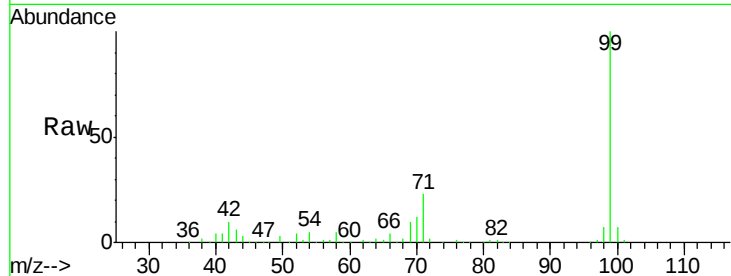

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

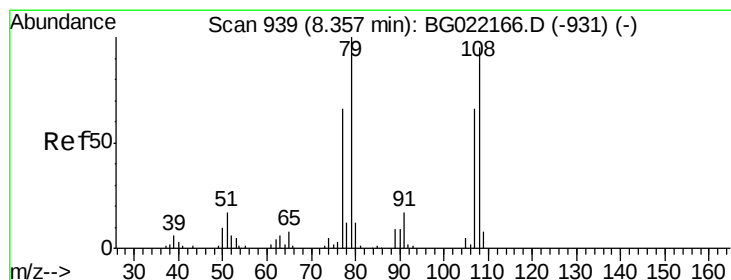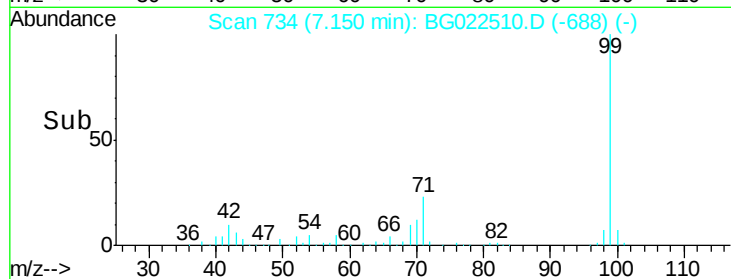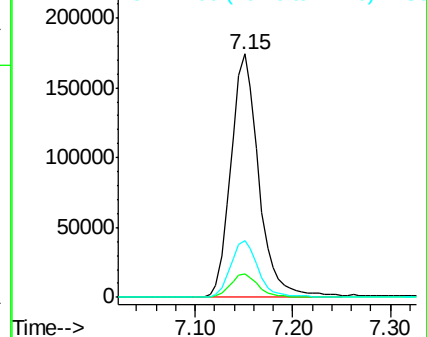

#15

Benzyl Alcohol

Concen: 2.05 ng

RT: 8.28 min Scan# 927

Delta R.T. 0.05 min

Lab File: BG022510.D

Acq: 23 Jun 2016 8:29


Tgt Ion: 79 Resp: 2809

Ion Ratio Lower Upper



79 100


108 38.9 59.4 89.0#

77 129.8 52.2 78.2#

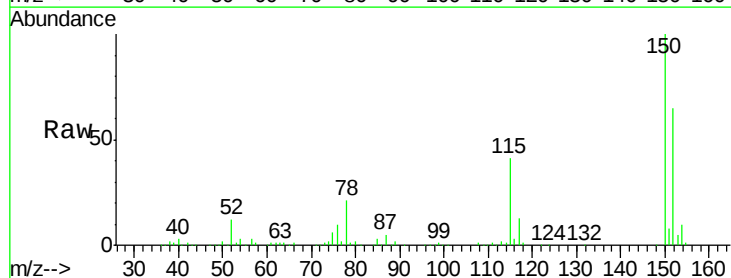

Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC



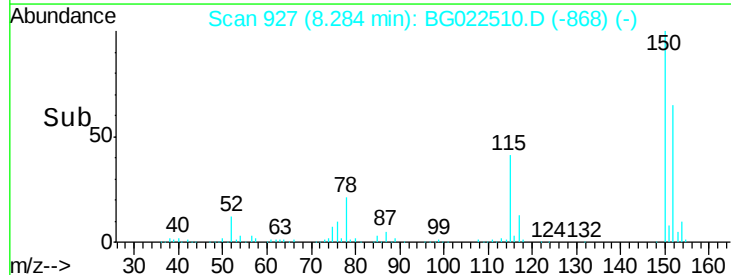
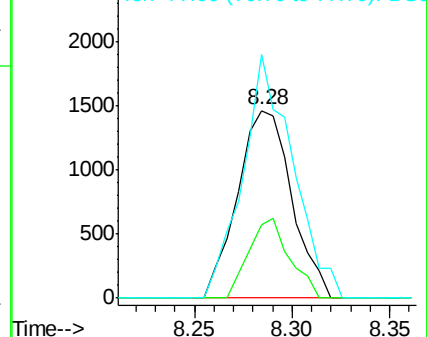


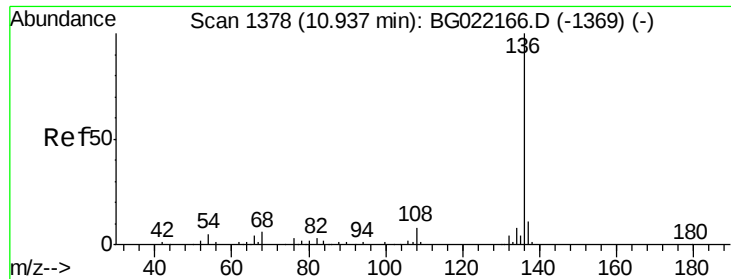

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.79 min Scan# 1353
Delta R.T. -0.02 min
Lab File: BG022510.D
Acq: 23 Jun 2016 8:29




Instrument :
BNA_G
ClientSampleId :


Tot Ion:136	Resp:	140017
Ion Ratio	Lower	Upper
136	100	
137	11.4	9.0 13.4
54	6.0	9.6 14.4#
68	6.5	6.4 9.6

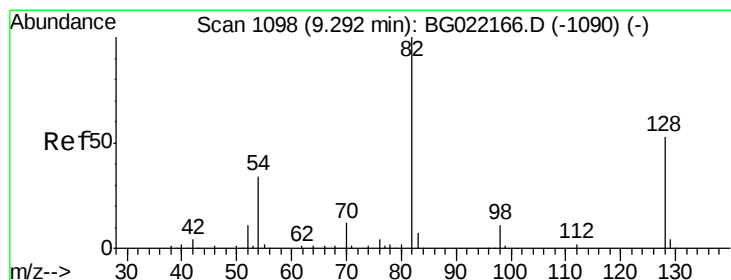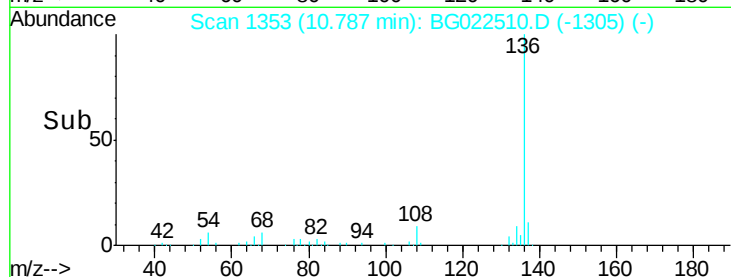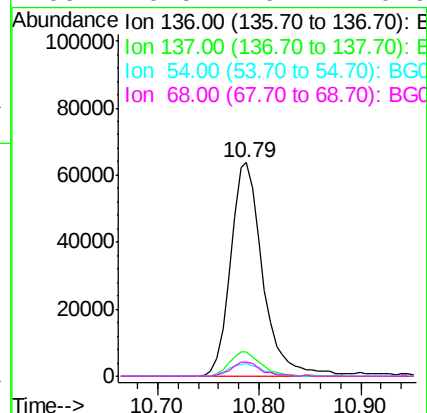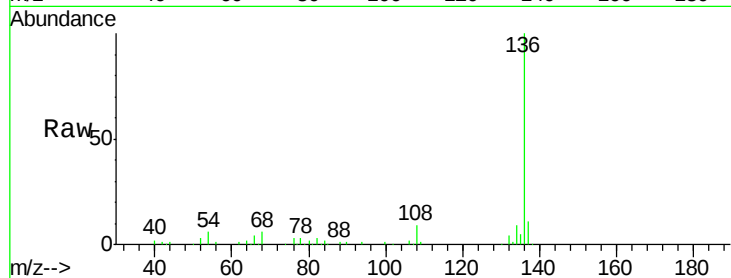

#23
Nitrobenzene-d5
Concen: 110.84 ng
RT: 9.14 min Scan# 1073
Delta R.T. -0.02 min
Lab File: BG022510.D
Acq: 23 Jun 2016 8:29

Tgt Ion: 82	Resp:	222597
Ion Ratio	Lower	Upper
82	100	
128	48.2	33.4 50.0
54	33.4	46.1 69.1#

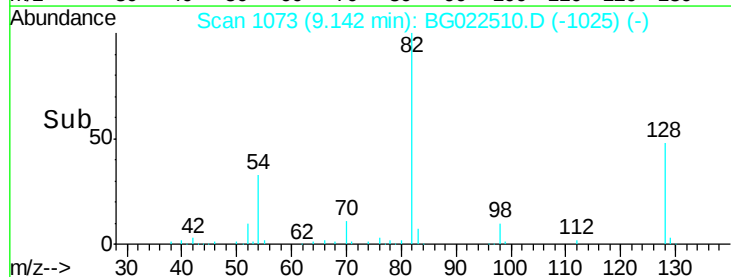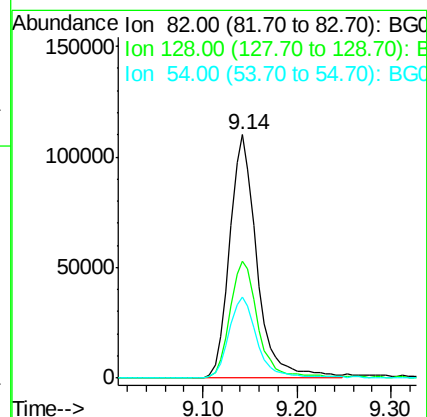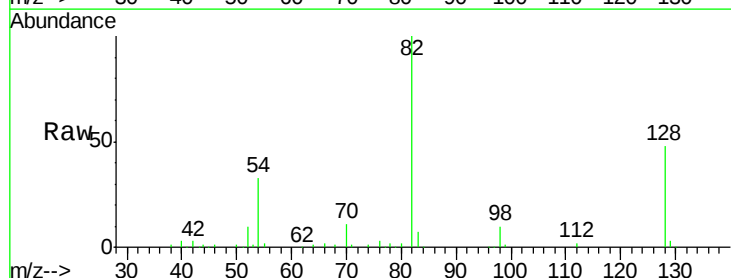

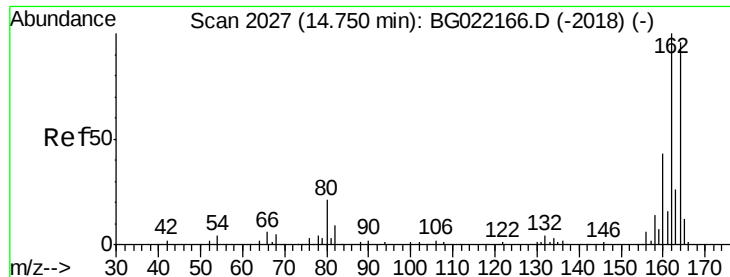

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.62 min Scan# 2005

Delta R.T. -0.01 min

Lab File: BG022510.D

Acq: 23 Jun 2016 8:29

Instrument :

BNA_G

ClientSampleId :


Tot Ion:164 Resp: 85424

Ion Ratio Lower Upper

164 100

162 108.0 78.0 117.0




160 48.9 32.9 49.3

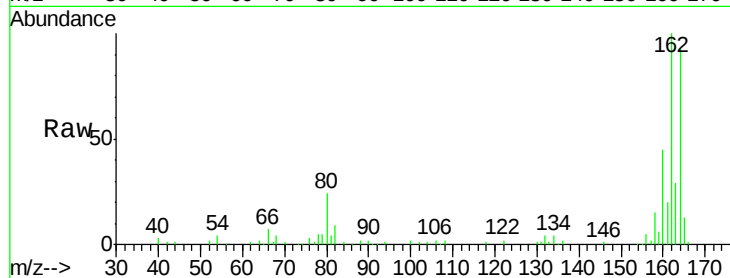

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

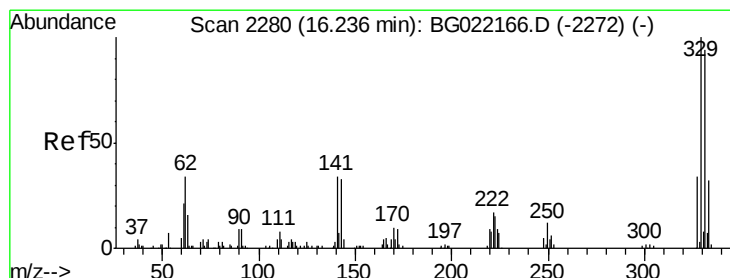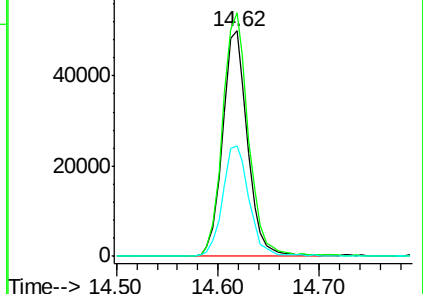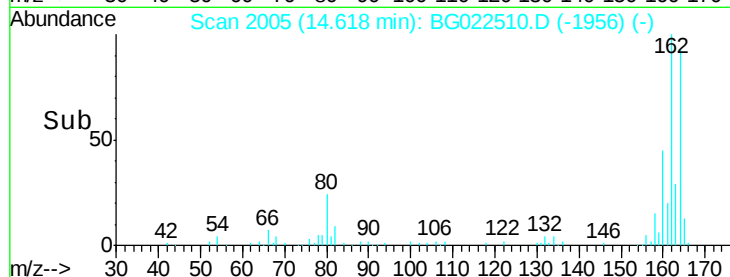

#41

2,4,6-Tribromophenol

Concen: 137.06 ng

RT: 16.11 min Scan# 2259

Delta R.T. -0.02 min

Lab File: BG022510.D

Acq: 23 Jun 2016 8:29


Tgt Ion:330 Resp: 132298

Ion Ratio Lower Upper

330 100

332 94.4 78.0 117.0



141 47.7 33.8 50.8

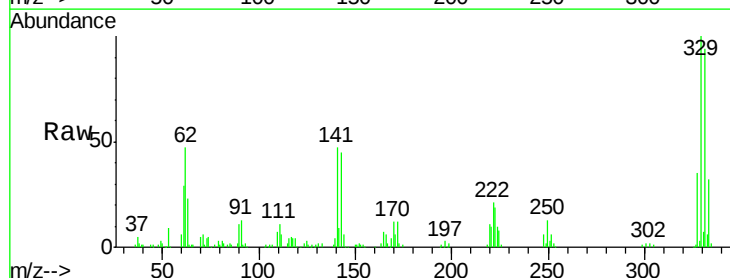


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

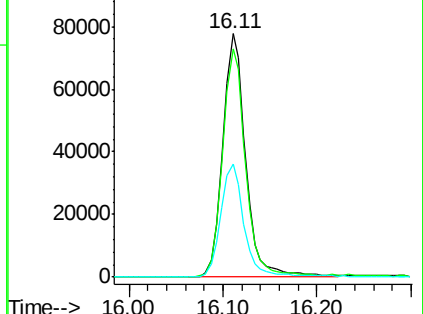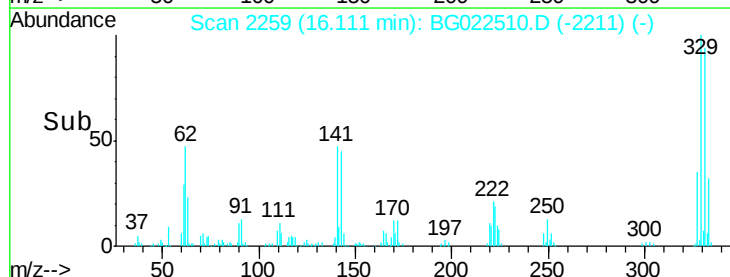


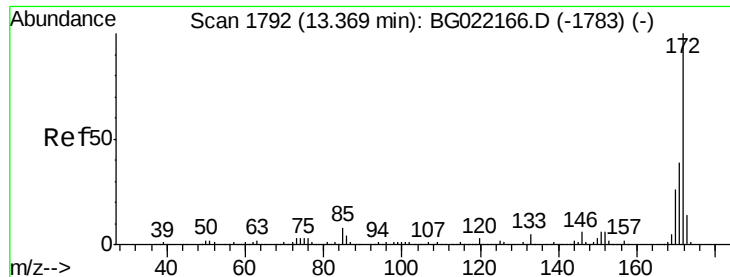




#44
 2-Fluorobiphenyl
 Concen: 110.95 ng
 RT: 13.24 min Scan# 1770
 Delta R.T. -0.01 min
 Lab File: BG022510.D
 Acq: 23 Jun 2016 8:29

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
172	100		
171	39.4	27.8	41.6
170	26.3	19.6	29.4

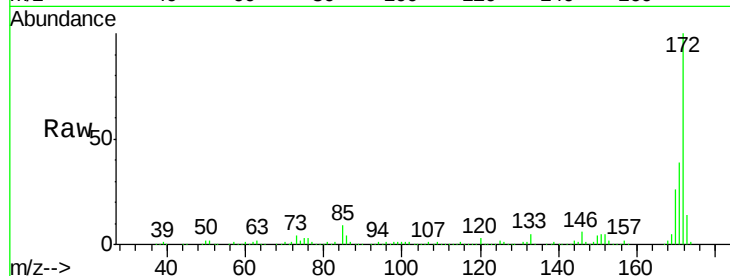


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

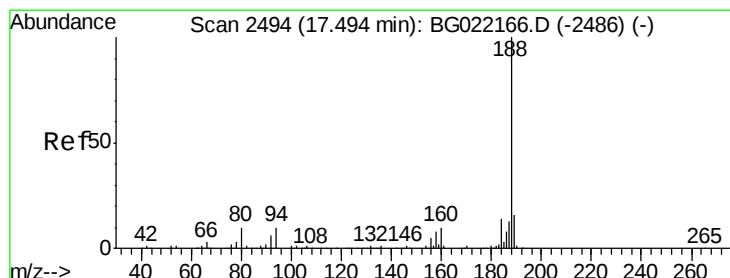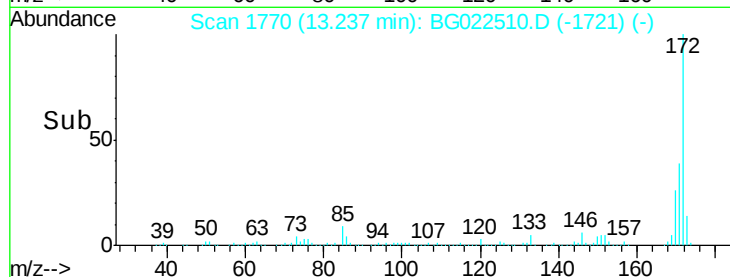
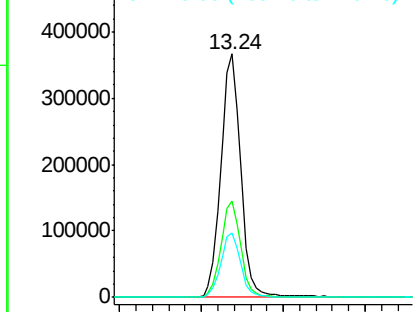


#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 17.36 min Scan# 2472
 Delta R.T. -0.02 min
 Lab File: BG022510.D
 Acq: 23 Jun 2016 8:29

Tgt Ion	Ratio	Lower	Upper
188	100		
94	11.2	7.5	11.3
80	12.5	8.6	13.0

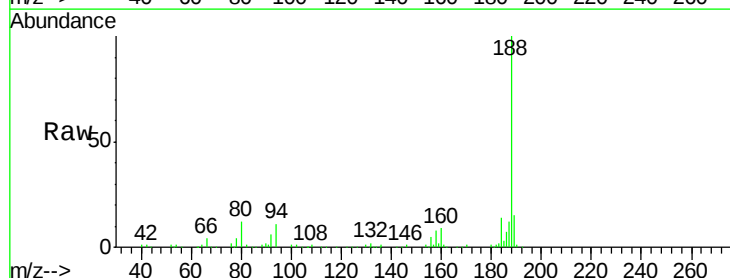

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BG0
 Ion 80.00 (79.70 to 80.70): BG0

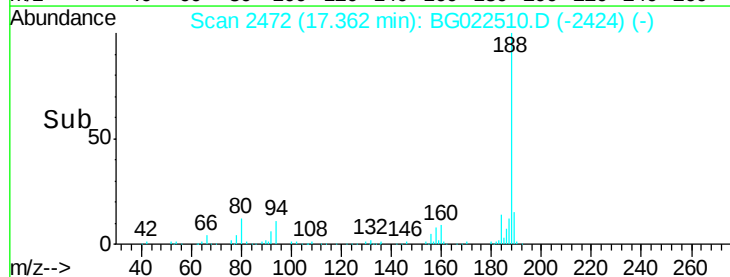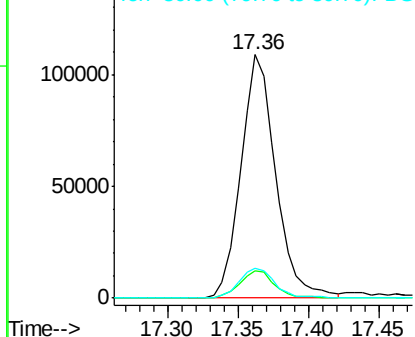



#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.62 min Scan# 3196

Delta R.T. -0.03 min

Lab File: BG022510.D

Acq: 23 Jun 2016 8:29

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 118141

Ion Ratio Lower Upper

240 100

120 16.6 8.4 12.6#




236 28.0 19.6 29.4

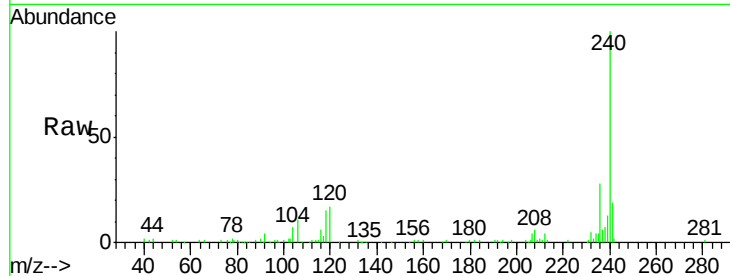

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

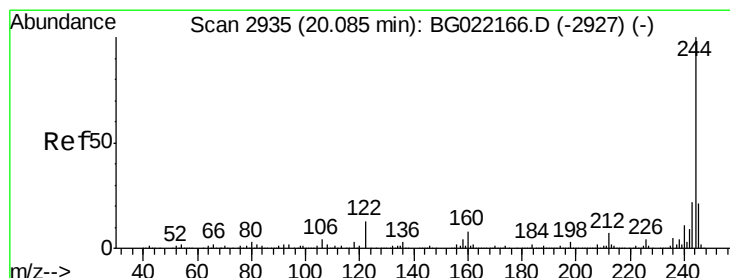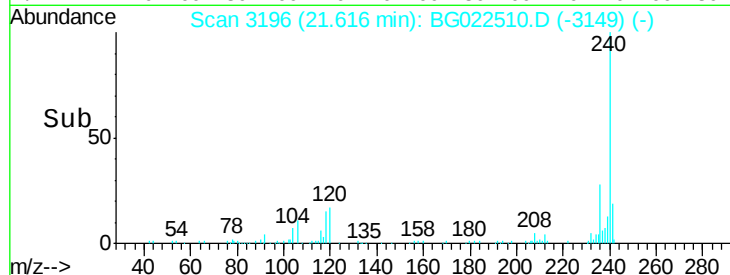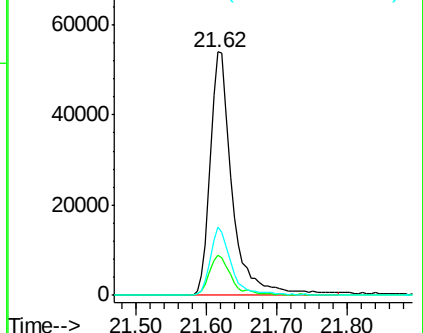

#78

Terphenyl-d14

Concen: 135.02 ng

RT: 19.96 min Scan# 2915

Delta R.T. -0.01 min

Lab File: BG022510.D

Acq: 23 Jun 2016 8:29


Tgt Ion:244 Resp: 671895

Ion Ratio Lower Upper

244 100

212 7.9 6.5 9.7



122 16.2 8.6 12.8#

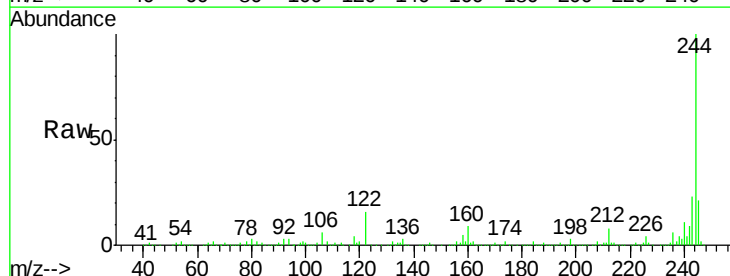


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

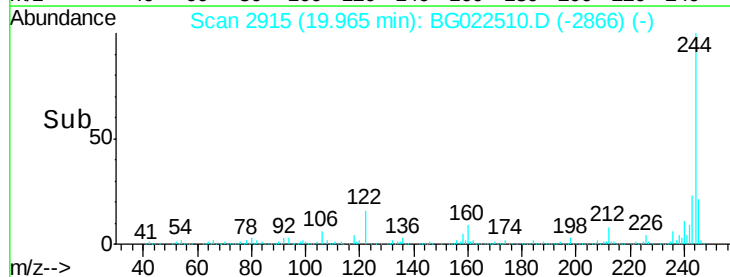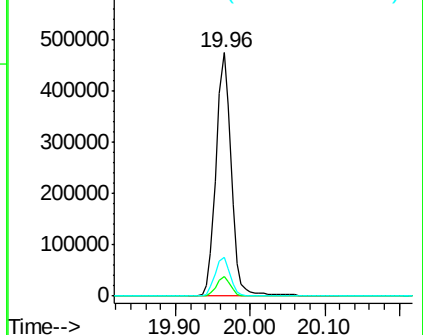


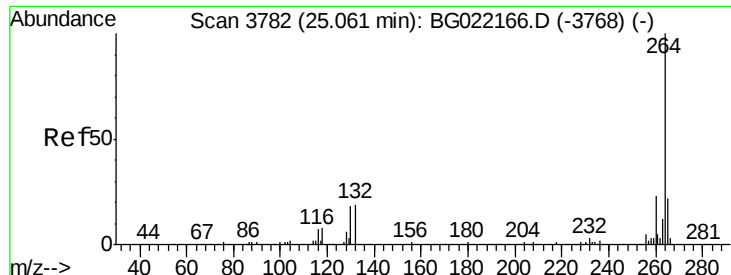

#86
Pervlene-d12
Concen: 20.00 ng
RT: 24.81 min Scan# 3739
Delta R.T. -0.03 min
Lab File: BG022510.D
Acq: 23 Jun 2016 8:29

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.5	20.2	30.4
265	21.3	17.8	26.8

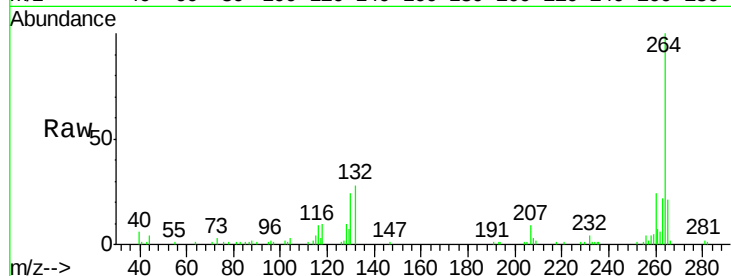

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

