


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062316\
Data File : BG022500.D
Acq On : 23 Jun 2016 1:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 22 01:27:56 2016

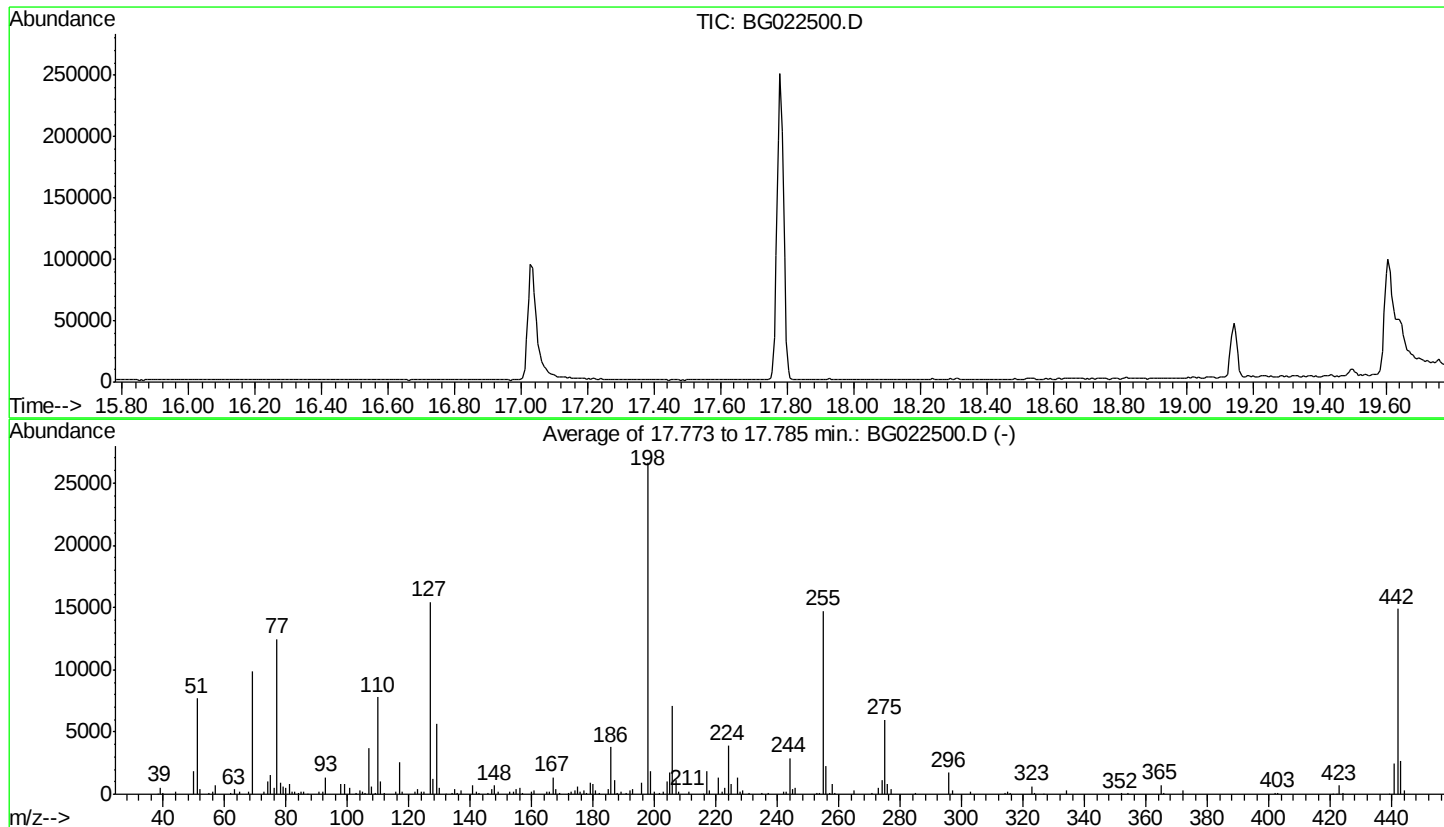

AutoFind: Scans 2542, 2543, 2544; Background Corrected with Scan 2535

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	7690	PASS
68	69	0.00	2	1.7	168	PASS
69	198	0.00	100	37.2	9900	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.1	15472	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26637	PASS
199	198	5	9	7.1	1895	PASS
275	198	10	60	22.4	5966	PASS
365	198	1	100	2.8	733	PASS
441	442	0.01	24	16.5	2460	PASS
442	198	50	100	55.9	14894	PASS
443	442	15	24	18.0	2683	PASS